

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014861.D
 Acq On : 10 Jun 2021 11:16
 Operator : CG/JU
 Sample : PB136905BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK905

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014861.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.211	18	21	28	rBB3	37347	63990	0.90%	0.100%
2	3.616	86	90	102	rBB	359708	634539	8.91%	0.995%
3	4.052	161	164	168	rBB6	7876	9029	0.13%	0.014%
4	4.981	319	322	328	rBB5	5770	12767	0.18%	0.020%
5	6.610	596	599	604	rBB4	6448	8280	0.12%	0.013%
6	6.869	637	643	654	rBV	807798	1267883	17.80%	1.988%
7	7.034	666	671	682	rBV	561191	912177	12.80%	1.430%
8	7.234	698	705	714	rVB	845099	1390064	19.51%	2.180%
9	7.699	778	784	793	rBV	754641	1232417	17.30%	1.933%
10	8.404	897	904	914	rBV	1055649	1747429	24.53%	2.740%
11	8.846	971	979	988	rBV	772828	1310377	18.39%	2.055%
12	9.569	1094	1102	1112	rBV2	658159	1086405	15.25%	1.704%
13	10.104	1186	1193	1202	rBB	1078576	1848398	25.94%	2.898%
14	10.369	1232	1238	1240	rBB4	5570	8360	0.12%	0.013%
15	10.481	1250	1257	1269	rVB	995407	1691704	23.74%	2.653%
16	10.616	1273	1280	1290	rBB	976622	1714960	24.07%	2.689%
17	12.087	1526	1530	1533	rBB4	13120	20222	0.28%	0.032%
18	12.304	1562	1567	1570	rBB5	5793	8829	0.12%	0.014%
19	13.757	1808	1814	1825	rBV	2142797	3117348	43.75%	4.888%
20	14.039	1854	1862	1871	rBV	2305570	3393630	47.63%	5.322%
21	14.351	1906	1915	1922	rBV	1597869	2431378	34.13%	3.813%
22	14.551	1944	1949	1959	rBB	664028	1087053	15.26%	1.705%
23	14.622	1959	1961	1965	rBB5	7972	9964	0.14%	0.016%
24	15.345	2077	2084	2091	rBV	2888362	4286231	60.16%	6.721%
25	15.463	2098	2104	2114	rBV2	806018	1121616	15.74%	1.759%
26	15.586	2118	2125	2131	rBB6	42741	71005	1.00%	0.111%
27	16.133	2213	2218	2224	rBB6	16571	22657	0.32%	0.036%
28	16.786	2324	2329	2331	rBB4	7862	9310	0.13%	0.015%
29	16.892	2343	2347	2350	rBB3	12984	14990	0.21%	0.024%
30	17.098	2374	2382	2393	rBV2	2123822	3149164	44.20%	4.938%
31	17.198	2393	2399	2409	rBV2	3229489	4791336	67.25%	7.513%
32	18.004	2533	2536	2541	rBB6	24937	33767	0.47%	0.053%
33	18.910	2688	2690	2693	rBB3	8620	8697	0.12%	0.014%
34	19.139	2725	2729	2734	rBB2	44188	59164	0.83%	0.093%
35	19.392	2766	2772	2777	rBB2	32853	47358	0.66%	0.074%
36	19.504	2784	2791	2798	rBV	4274078	6063586	85.10%	9.508%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014861.D
 Acq On : 10 Jun 2021 11:16
 Operator : CG/JU
 Sample : PB136905BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK905

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

37	19.786	2838	2839	2842	rBB3	9749	9529	0.13%	0.015%
38	20.633	2979	2983	2985	rBB5	7993	10618	0.15%	0.017%
39	20.757	2998	3004	3008	rBB8	12968	21919	0.31%	0.034%
40	20.869	3020	3023	3026	rBB5	8650	9418	0.13%	0.015%
41	21.027	3048	3050	3052	rBB3	15479	13751	0.19%	0.022%
42	21.057	3052	3055	3058	rBB5	9412	9016	0.13%	0.014%
43	21.298	3091	3096	3109	rBV	2943298	4063898	57.04%	6.373%
44	21.474	3120	3126	3129	rBB7	18209	34740	0.49%	0.054%
45	21.545	3136	3138	3140	rBB3	14245	11442	0.16%	0.018%
46	21.586	3143	3145	3146	rBB2	18615	8900	0.12%	0.014%
47	21.704	3163	3165	3167	rBB3	13529	10286	0.14%	0.016%
48	21.727	3167	3169	3171	rBB3	11708	9666	0.14%	0.015%
49	21.751	3171	3173	3174	rBB2	15033	8754	0.12%	0.014%
50	21.804	3179	3182	3184	rBB4	11839	10925	0.15%	0.017%
51	21.898	3193	3198	3203	rBB9	25626	43351	0.61%	0.068%
52	22.057	3224	3225	3227	rBB2	17472	10107	0.14%	0.016%
53	22.086	3227	3230	3232	rBB4	10552	8589	0.12%	0.013%
54	22.127	3234	3237	3238	rBB3	7980	10795	0.15%	0.017%
55	22.151	3240	3241	3244	rBB3	17178	13903	0.20%	0.022%
56	22.174	3244	3245	3251	rBB6	15600	24673	0.35%	0.039%
57	22.233	3253	3255	3258	rBB4	12713	13138	0.18%	0.021%
58	22.263	3258	3260	3262	rBB3	9521	8316	0.12%	0.013%
59	22.374	3273	3279	3283	rBB6	74563	95252	1.34%	0.149%
60	22.451	3290	3292	3296	rBB5	10375	11797	0.17%	0.018%
61	22.498	3298	3300	3301	rBB2	13144	9434	0.13%	0.015%
62	22.557	3309	3310	3312	rBB2	18813	10872	0.15%	0.017%
63	22.592	3312	3316	3319	rBB6	8110	12442	0.17%	0.020%
64	22.645	3323	3325	3328	rBB4	11419	13025	0.18%	0.020%
65	22.715	3333	3337	3338	rBB4	14650	11714	0.16%	0.018%
66	22.745	3338	3342	3344	rBB5	20130	21520	0.30%	0.034%
67	22.780	3347	3348	3349	rBB	20808	10218	0.14%	0.016%
68	22.815	3352	3354	3355	rBB2	13589	13925	0.20%	0.022%
69	22.886	3359	3366	3369	rBB5	114300	167784	2.35%	0.263%
70	22.915	3369	3371	3373	rBB3	20281	10119	0.14%	0.016%
71	22.945	3373	3376	3379	rBB5	15013	19059	0.27%	0.030%
72	22.986	3381	3383	3384	rBB2	12626	9655	0.14%	0.015%
73	23.039	3390	3392	3393	rBB2	16124	12793	0.18%	0.020%
74	23.057	3393	3395	3397	rBB3	19688	14520	0.20%	0.023%
75	23.080	3397	3399	3404	rBB6	13173	19078	0.27%	0.030%
76	23.192	3414	3418	3419	rBB4	18461	12979	0.18%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014861.D
 Acq On : 10 Jun 2021 11:16
 Operator : CG/JU
 Sample : PB136905BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK905

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

77	23.227	3420	3424	3425	rBB4	11437	12952	0.18%	0.020%
78	23.280	3429	3433	3435	rBB5	8984	13798	0.19%	0.022%
79	23.315	3437	3439	3440	rBB2	19019	9053	0.13%	0.014%
80	23.345	3440	3444	3447	rBB6	6624	8465	0.12%	0.013%
81	23.415	3447	3456	3472	rBB2	3452825	7124881	100.00%	11.173%
82	23.557	3472	3480	3495	rVB	2287246	4449759	62.45%	6.978%
83	23.757	3512	3514	3515	rBB2	15260	9254	0.13%	0.015%
84	23.792	3517	3520	3522	rBB4	17062	13880	0.19%	0.022%
85	23.827	3524	3526	3528	rBB2	26288	9932	0.14%	0.016%
86	23.851	3528	3530	3531	rBB2	15314	9512	0.13%	0.015%
87	23.862	3531	3532	3534	rBB2	18358	11237	0.16%	0.018%
88	23.886	3534	3536	3538	rBB3	14447	8498	0.12%	0.013%
89	23.927	3540	3543	3544	rBB3	10848	10005	0.14%	0.016%
90	23.939	3544	3545	3549	rVB4	15366	17801	0.25%	0.028%
91	23.974	3549	3551	3554	rBB4	14244	8674	0.12%	0.014%
92	23.998	3554	3555	3558	rBB3	15730	15381	0.22%	0.024%
93	24.115	3568	3575	3583	rBB4	218218	416427	5.84%	0.653%
94	24.180	3585	3586	3588	rBB2	13233	8716	0.12%	0.014%
95	24.215	3591	3592	3594	rBB2	14203	8277	0.12%	0.013%
96	24.280	3601	3603	3604	rBB2	13039	8738	0.12%	0.014%
97	24.351	3613	3615	3618	rBB4	13647	16418	0.23%	0.026%
98	24.480	3634	3637	3639	rBB4	9877	9769	0.14%	0.015%
99	24.533	3645	3646	3648	rBB2	22437	8779	0.12%	0.014%
100	24.557	3648	3650	3652	rBB3	19824	9917	0.14%	0.016%
101	24.604	3656	3658	3659	rBB2	17895	11071	0.16%	0.017%
102	24.621	3659	3661	3663	rBB3	12295	9695	0.14%	0.015%
103	24.698	3670	3674	3675	rBB4	21039	19234	0.27%	0.030%
104	24.868	3692	3703	3713	rBB8	171298	469108	6.58%	0.736%
105	24.945	3713	3716	3717	rBB3	23246	13005	0.18%	0.020%
106	24.998	3722	3725	3729	rBB5	11228	11030	0.15%	0.017%
107	25.033	3729	3731	3734	rBB4	17306	14266	0.20%	0.022%
108	25.068	3734	3737	3738	rBB3	19008	18417	0.26%	0.029%
109	25.098	3738	3742	3743	rBB4	9833	12263	0.17%	0.019%
110	25.115	3743	3745	3746	rBB2	26382	9914	0.14%	0.016%
111	25.133	3746	3748	3750	rBB3	27769	18474	0.26%	0.029%
112	25.162	3750	3753	3754	rBB3	28258	17427	0.24%	0.027%
113	25.221	3761	3763	3766	rBB4	14182	13600	0.19%	0.021%
114	25.257	3767	3769	3771	rBB3	19035	13810	0.19%	0.022%
115	25.321	3779	3780	3784	rBB4	28046	18884	0.27%	0.030%
116	25.362	3785	3787	3790	rBB4	13263	11393	0.16%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014861.D
 Acq On : 10 Jun 2021 11:16
 Operator : CG/JU
 Sample : PB136905BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK905

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

117	25.457	3802	3803	3805	rBB2	17164	9470	0.13%	0.015%
118	25.486	3805	3808	3811	rBB5	15631	14304	0.20%	0.022%
119	25.515	3811	3813	3818	rBB6	15639	23801	0.33%	0.037%
120	25.645	3829	3835	3839	rBB9	13887	26499	0.37%	0.042%
121	25.686	3839	3842	3845	rBB5	8579	10061	0.14%	0.016%
122	25.715	3845	3847	3848	rBB2	12160	8425	0.12%	0.013%
123	25.762	3848	3855	3864	rBB2	111057	303070	4.25%	0.475%
124	25.874	3872	3874	3875	rBB2	21495	8591	0.12%	0.013%
125	25.892	3875	3877	3879	rBB3	15845	12010	0.17%	0.019%
126	25.927	3881	3883	3885	rBB3	19760	9374	0.13%	0.015%
127	25.945	3885	3886	3888	rBB2	17283	8172	0.11%	0.013%
128	26.033	3899	3901	3904	rBB4	17312	13348	0.19%	0.021%
129	26.062	3904	3906	3908	rBB2	20484	16334	0.23%	0.026%
130	26.133	3917	3918	3921	rBB3	15007	12154	0.17%	0.019%
131	26.186	3924	3927	3929	rBB4	14531	15898	0.22%	0.025%
132	26.245	3935	3937	3938	rBB	17497	8653	0.12%	0.014%
133	26.268	3938	3941	3942	rBB2	13170	10298	0.14%	0.016%
134	26.292	3942	3945	3946	rBB3	13035	9515	0.13%	0.015%
135	26.304	3946	3947	3949	rBB2	19885	10400	0.15%	0.016%
136	26.327	3949	3951	3952	rBB2	10933	9040	0.13%	0.014%
137	26.392	3960	3962	3963	rBB2	18759	11049	0.16%	0.017%
138	26.409	3963	3965	3968	rBB4	17412	18539	0.26%	0.029%
139	26.451	3968	3972	3973	rBB4	13067	12043	0.17%	0.019%
140	26.515	3981	3983	3987	rBB5	12805	14912	0.21%	0.023%
141	26.568	3989	3992	3996	rBB6	33914	34659	0.49%	0.054%
142	26.609	3998	3999	4004	rBB5	5057	8848	0.12%	0.014%
143	26.668	4008	4009	4010	rBB	23581	9417	0.13%	0.015%
144	26.739	4019	4021	4022	rBB2	13142	8682	0.12%	0.014%
145	26.756	4022	4024	4025	rBB2	8535	8800	0.12%	0.014%
146	26.798	4026	4031	4032	rBB5	19239	50192	0.70%	0.079%
147	26.909	4048	4050	4051	rBB2	14594	8381	0.12%	0.013%
148	27.003	4062	4066	4069	rBB6	20388	21901	0.31%	0.034%
149	27.156	4088	4092	4095	rBB6	8494	11294	0.16%	0.018%
150	27.398	4131	4133	4134	rBB2	11414	8376	0.12%	0.013%
151	27.433	4138	4139	4140	rBB	15577	7287	0.10%	0.011%
152	27.603	4166	4168	4170	rBB3	14095	11464	0.16%	0.018%
153	27.656	4174	4177	4178	rBB2	12356	9772	0.14%	0.015%
154	27.674	4178	4180	4185	rBB6	13099	15736	0.22%	0.025%
155	27.733	4188	4190	4192	rBB3	12078	8197	0.12%	0.013%
156	27.786	4197	4199	4201	rBB3	14323	13051	0.18%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014861.D
 Acq On : 10 Jun 2021 11:16
 Operator : CG/JU
 Sample : PB136905BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK905

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

157	27.803	4201	4202	4207	rBB4	5654	10956	0.15%	0.017%
158	27.945	4224	4226	4228	rBB3	13144	8825	0.12%	0.014%
159	28.015	4237	4238	4240	rBB2	23826	16559	0.23%	0.026%
160	28.033	4240	4241	4245	rBB4	11580	10833	0.15%	0.017%
161	28.150	4257	4261	4263	rBB5	11799	8386	0.12%	0.013%
162	28.186	4265	4267	4269	rBB3	21137	18122	0.25%	0.028%
163	28.303	4284	4287	4288	rBB3	17315	9020	0.13%	0.014%
164	28.315	4288	4289	4291	rBB2	32507	16361	0.23%	0.026%
165	28.403	4302	4304	4306	rBB3	14906	10141	0.14%	0.016%
166	28.450	4308	4312	4314	rBB4	27389	30167	0.42%	0.047%
167	28.486	4314	4318	4319	rBB4	7499	12379	0.17%	0.019%
168	28.498	4319	4320	4323	rBB3	20395	10612	0.15%	0.017%
169	28.521	4323	4324	4326	rBB2	18369	9188	0.13%	0.014%
170	28.539	4326	4327	4333	rBB6	18898	18157	0.25%	0.028%
171	28.609	4335	4339	4341	rBB4	14388	11695	0.16%	0.018%
172	28.650	4344	4346	4347	rBB2	26448	10028	0.14%	0.016%
173	28.662	4347	4348	4351	rBB3	12913	11445	0.16%	0.018%
174	28.692	4351	4353	4356	rBB3	11296	13749	0.19%	0.022%
175	28.739	4359	4361	4364	rBB4	11935	9458	0.13%	0.015%
176	28.768	4364	4366	4367	rBB2	23599	13093	0.18%	0.021%
177	28.786	4367	4369	4371	rBB3	11665	8453	0.12%	0.013%
178	28.803	4371	4372	4374	rBB2	16818	8543	0.12%	0.013%
179	28.839	4374	4378	4381	rBB5	19423	16486	0.23%	0.026%
180	28.909	4387	4390	4392	rBV3	20370	20873	0.29%	0.033%
181	28.939	4394	4395	4398	rBB3	26482	20257	0.28%	0.032%
182	28.974	4398	4401	4402	rBB3	17231	14862	0.21%	0.023%
183	29.027	4408	4410	4411	rBB2	21236	9421	0.13%	0.015%
184	29.050	4411	4414	4415	rBB3	10588	8833	0.12%	0.014%
185	29.068	4415	4417	4420	rBB4	12983	13709	0.19%	0.021%
186	29.103	4420	4423	4424	rBB3	9974	9816	0.14%	0.015%
187	29.145	4426	4430	4432	rBB4	19319	19812	0.28%	0.031%
188	29.168	4432	4434	4438	rBB5	16227	19602	0.28%	0.031%
189	29.233	4444	4445	4447	rBB2	20134	9671	0.14%	0.015%
190	29.262	4447	4450	4451	rBB3	26051	20073	0.28%	0.031%
191	29.280	4451	4453	4456	rBB3	29326	21864	0.31%	0.034%
192	29.339	4460	4463	4466	rBB5	22418	18430	0.26%	0.029%
193	29.374	4466	4469	4470	rBB3	14564	9247	0.13%	0.015%




Sum of corrected areas: 63770861

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014861.D
Acq On : 10 Jun 2021 11:16
Operator : CG/JU
Sample : PB136905BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK905

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

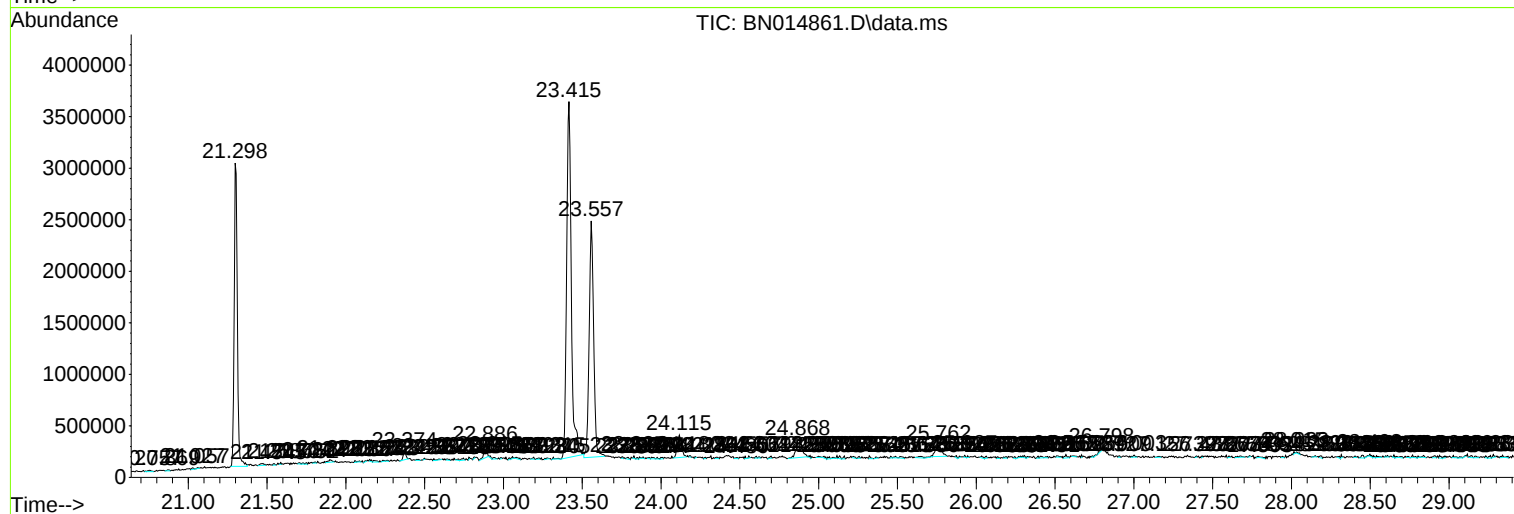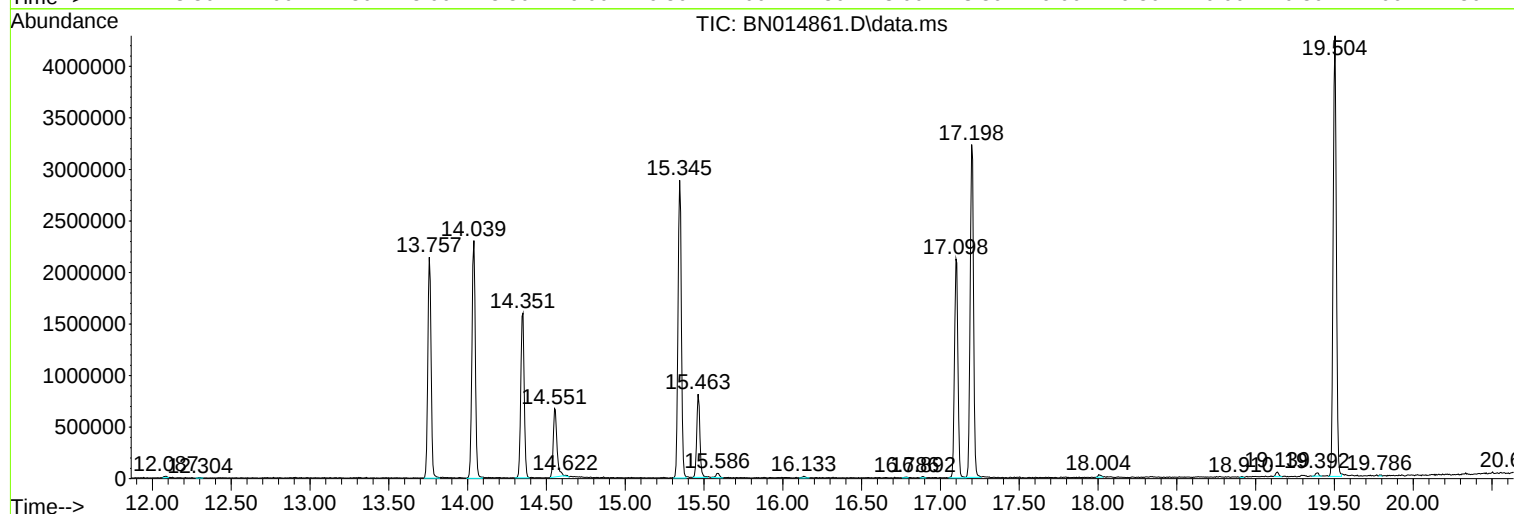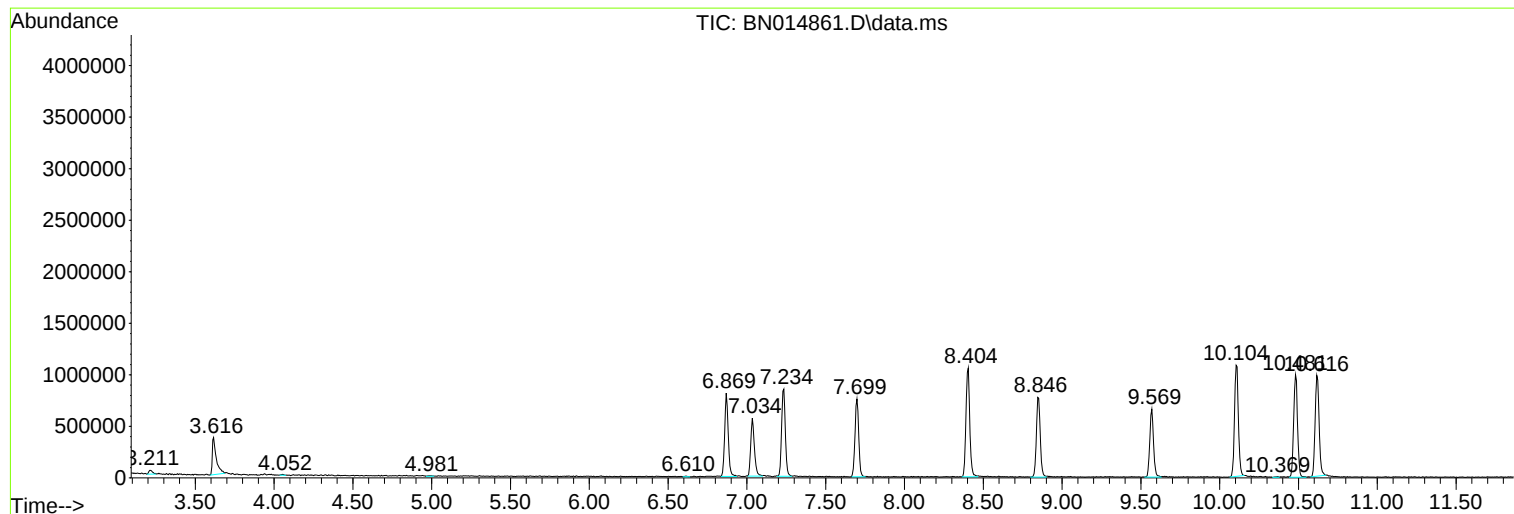

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014861.D
Acq On : 10 Jun 2021 11:16
Operator : CG/JU
Sample : PB136905BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK905










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
24.868	2.11 ng/ul	469108	Perylene-d12	23.557

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Nonadecane	268	C19H40	000629-92-5	90
2			Disulfide, di-tert-dodecyl	402	C24H50S2	027458-90-8	76
3			Hentriacontane	437	C31H64	000630-04-6	72
4			2-methylhexacosane	380	C27H56	1000376-72-7	72
5			Hentriacontane	437	C31H64	000630-04-6	72

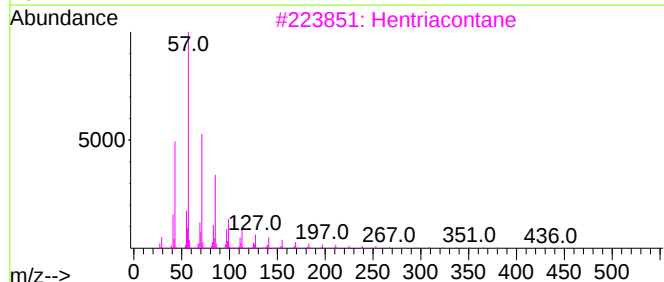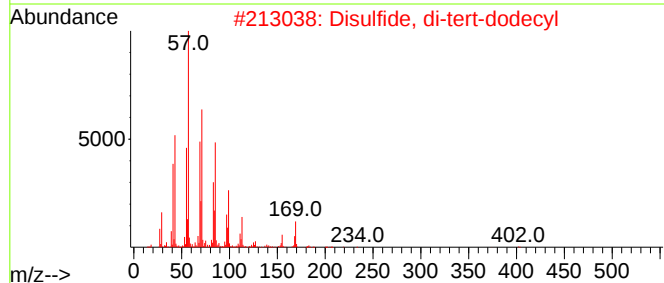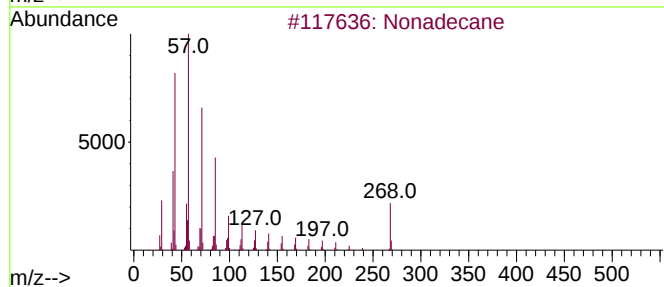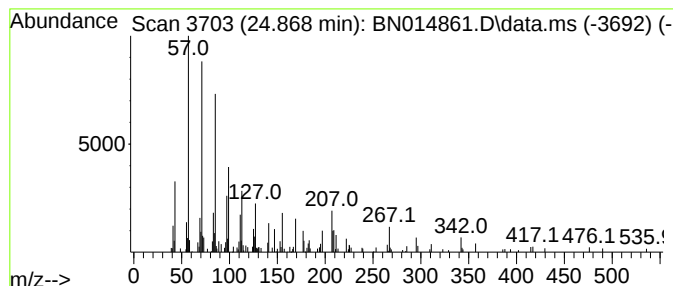

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014861.D
Acq On : 10 Jun 2021 11:16
Operator : CG/JU
Sample : PB136905BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK905

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	24.868	2.1	ng/ul	469108	6	23.557	4449760	20.0