

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014863.D
 Acq On : 10 Jun 2021 14:00
 Operator : CG/JU
 Sample : M2618-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG5R0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014863.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	18	22	28	rBB4	35580	44048	1.08%	0.085%
2	3.846	124	129	135	rBB	39243	59887	1.47%	0.116%
3	4.834	291	297	306	rVB2	52782	97526	2.40%	0.189%
4	6.875	635	644	652	rBB2	590746	997347	24.50%	1.928%
5	7.040	666	672	682	rBB	402644	671606	16.50%	1.298%
6	7.234	697	705	712	rBV	684525	1037257	25.48%	2.005%
7	7.698	776	784	792	rBV	641391	1020835	25.08%	1.973%
8	8.404	898	904	915	rBV	780829	1289229	31.67%	2.492%
9	8.522	918	924	932	rBB	100250	165708	4.07%	0.320%
10	8.851	973	980	990	rBV2	595505	981239	24.11%	1.897%
11	9.569	1094	1102	1110	rBB2	502174	834796	20.51%	1.614%
12	10.110	1188	1194	1202	rBV	864960	1449635	35.62%	2.802%
13	10.275	1217	1222	1232	rBB7	13699	33267	0.82%	0.064%
14	10.486	1250	1258	1265	rBV	830653	1404403	34.50%	2.715%
15	10.622	1273	1281	1293	rBB	692670	1189159	29.22%	2.299%
16	13.763	1808	1815	1824	rVB	1430495	2070199	50.86%	4.002%
17	14.039	1856	1862	1872	rVB	1650970	2403992	59.06%	4.647%
18	14.351	1909	1915	1923	rBV	1351116	2024025	49.73%	3.913%
19	14.563	1945	1951	1962	rBB2	434640	753960	18.52%	1.458%
20	15.351	2078	2085	2091	rBV	2058594	3046674	74.85%	5.890%
21	15.469	2098	2105	2113	rBV2	265218	423562	10.41%	0.819%
22	15.586	2118	2125	2130	rBB9	29812	44641	1.10%	0.086%
23	16.921	2348	2352	2357	rBB8	34581	55541	1.36%	0.107%
24	17.104	2377	2383	2388	rBB	1676484	2350001	57.74%	4.543%
25	17.145	2388	2390	2393	rBB	72995	73262	1.80%	0.142%
26	17.204	2395	2400	2405	rBB	2237579	3189696	78.37%	6.166%
27	17.939	2522	2525	2528	rBB5	28244	31793	0.78%	0.061%
28	18.010	2533	2537	2538	rBB4	34274	39779	0.98%	0.077%
29	18.480	2614	2617	2621	rBB6	53295	65405	1.61%	0.126%
30	18.539	2624	2627	2631	rBB6	29535	39582	0.97%	0.077%
31	18.586	2631	2635	2636	rBB4	50127	55013	1.35%	0.106%
32	18.633	2641	2643	2646	rBB4	43100	35499	0.87%	0.069%
33	18.910	2685	2690	2693	rBB7	40473	47218	1.16%	0.091%
34	19.027	2707	2710	2712	rBB4	49404	52135	1.28%	0.101%
35	19.051	2712	2714	2716	rBB3	41255	36793	0.90%	0.071%
36	19.080	2716	2719	2720	rBB3	44571	41031	1.01%	0.079%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014863.D
 Acq On : 10 Jun 2021 14:00
 Operator : CG/JU
 Sample : M2618-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG5R0

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

37	19.168	2729	2734	2738	rBB	237969	301067	7.40%	0.582%
38	19.233	2741	2745	2749	rBB7	59777	72730	1.79%	0.141%
39	19.310	2753	2758	2761	rBB7	40094	73019	1.79%	0.141%
40	19.392	2768	2772	2773	rBB4	32739	32194	0.79%	0.062%
41	19.462	2781	2784	2786	rBB4	42568	43582	1.07%	0.084%
42	19.509	2786	2792	2802	rBB	2560096	4070199	100.00%	7.868%
43	19.698	2820	2824	2825	rBB4	51972	59724	1.47%	0.115%
44	19.727	2825	2829	2830	rBB4	51465	59810	1.47%	0.116%
45	19.774	2835	2837	2838	rBB2	56733	35769	0.88%	0.069%
46	19.833	2845	2847	2849	rBB3	52290	34742	0.85%	0.067%
47	19.862	2849	2852	2855	rBB5	53366	50981	1.25%	0.099%
48	19.933	2859	2864	2867	rBB7	48080	72106	1.77%	0.139%
49	20.039	2876	2882	2884	rBB7	90432	137385	3.38%	0.266%
50	20.074	2884	2888	2889	rBB4	65873	68451	1.68%	0.132%
51	20.092	2889	2891	2892	rBB2	54386	35548	0.87%	0.069%
52	20.127	2895	2897	2899	rBB3	75322	46132	1.13%	0.089%
53	20.204	2907	2910	2912	rBB4	57003	42544	1.05%	0.082%
54	20.262	2918	2920	2922	rBB3	57145	54831	1.35%	0.106%
55	20.304	2922	2927	2928	rBB5	62378	63419	1.56%	0.123%
56	20.386	2935	2941	2942	rBB6	38833	51129	1.26%	0.099%
57	20.421	2944	2947	2948	rBB3	41322	30998	0.76%	0.060%
58	20.439	2948	2950	2952	rBB3	63853	48487	1.19%	0.094%
59	20.492	2957	2959	2961	rBB3	73457	61004	1.50%	0.118%
60	20.551	2964	2969	2970	rBB5	36676	60284	1.48%	0.117%
61	20.562	2970	2971	2974	rBB3	68176	47601	1.17%	0.092%
62	20.586	2974	2975	2976	rBB	89452	37068	0.91%	0.072%
63	20.621	2978	2981	2982	rBB3	87957	103876	2.55%	0.201%
64	20.645	2982	2985	2990	rBB7	76073	104112	2.56%	0.201%
65	20.721	2995	2998	2999	rBB3	39324	33475	0.82%	0.065%
66	20.756	2999	3004	3006	rBB6	80634	115242	2.83%	0.223%
67	20.792	3006	3010	3011	rBB4	52804	48157	1.18%	0.093%
68	20.898	3026	3028	3030	rBB3	56255	38807	0.95%	0.075%
69	20.945	3033	3036	3038	rBB4	94418	61079	1.50%	0.118%
70	20.992	3040	3044	3045	rBB4	43419	86424	2.12%	0.167%
71	21.009	3045	3047	3048	rBB2	57622	35576	0.87%	0.069%
72	21.027	3049	3050	3052	rBB2	67640	50518	1.24%	0.098%
73	21.086	3057	3060	3061	rBB3	69839	51151	1.26%	0.099%
74	21.121	3061	3066	3068	rBB6	130668	180277	4.43%	0.348%
75	21.162	3071	3073	3074	rBB2	45776	54085	1.33%	0.105%
76	21.174	3074	3075	3077	rBB2	96410	52290	1.28%	0.101%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014863.D
 Acq On : 10 Jun 2021 14:00
 Operator : CG/JU
 Sample : M2618-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG5R0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

77	21.233	3083	3085	3087	rBB2	106366	72226	1.77%	0.140%
78	21.304	3091	3097	3101	rBB	1872520	2531854	62.20%	4.894%
79	21.333	3101	3102	3106	rBB3	62256	50970	1.25%	0.099%
80	21.380	3108	3110	3111	rBB2	48683	41861	1.03%	0.081%
81	21.409	3113	3115	3117	rBB3	59944	40466	0.99%	0.078%
82	21.433	3117	3119	3121	rBB3	59230	59316	1.46%	0.115%
83	21.468	3121	3125	3129	rBB7	117633	127255	3.13%	0.246%
84	21.527	3131	3135	3136	rBB4	38683	84255	2.07%	0.163%
85	21.539	3136	3137	3141	rBB4	89853	54685	1.34%	0.106%
86	21.580	3141	3144	3145	rBB3	81331	45412	1.12%	0.088%
87	21.592	3145	3146	3149	rBB3	121422	72352	1.78%	0.140%
88	21.621	3149	3151	3156	rBB6	151672	180914	4.44%	0.350%
89	21.662	3156	3158	3161	rBB4	124587	111445	2.74%	0.215%
90	21.704	3161	3165	3166	rBB4	44056	59813	1.47%	0.116%
91	21.715	3166	3167	3171	rVB4	96790	98062	2.41%	0.190%
92	21.792	3178	3180	3182	rBB3	61302	56744	1.39%	0.110%
93	21.880	3191	3195	3196	rBB4	68455	37491	0.92%	0.072%
94	21.903	3196	3199	3200	rBB3	102561	93098	2.29%	0.180%
95	21.921	3200	3202	3205	rBB4	66346	32392	0.80%	0.063%
96	21.986	3209	3213	3214	rBB4	27711	73379	1.80%	0.142%
97	22.045	3220	3223	3224	rBB3	57169	58751	1.44%	0.114%
98	22.062	3224	3226	3229	rBB4	105032	86423	2.12%	0.167%
99	22.086	3229	3230	3232	rBB2	101206	40651	1.00%	0.079%
100	22.109	3232	3234	3236	rBB3	49200	31494	0.77%	0.061%
101	22.174	3239	3245	3246	rBB6	65429	113899	2.80%	0.220%
102	22.192	3246	3248	3252	rBB5	76995	93624	2.30%	0.181%
103	22.221	3252	3253	3255	rBB2	67030	40521	1.00%	0.078%
104	22.262	3258	3260	3263	rBB4	71123	38885	0.96%	0.075%
105	22.303	3266	3267	3273	rBB6	84915	86320	2.12%	0.167%
106	22.345	3273	3274	3277	rBB3	47871	41923	1.03%	0.081%
107	22.380	3277	3280	3285	rBB7	135964	206441	5.07%	0.399%
108	22.421	3285	3287	3288	rBB2	53242	35243	0.87%	0.068%
109	22.451	3290	3292	3294	rBB3	66063	41883	1.03%	0.081%
110	22.509	3299	3302	3305	rBB5	32813	35616	0.88%	0.069%
111	22.545	3307	3308	3314	rBB6	50346	53769	1.32%	0.104%
112	22.609	3318	3319	3322	rBB3	49960	33795	0.83%	0.065%
113	22.668	3326	3329	3330	rBB3	102352	69810	1.72%	0.135%
114	22.703	3333	3335	3339	rBB5	48788	67819	1.67%	0.131%
115	22.739	3339	3341	3346	rBB6	138979	155962	3.83%	0.301%
116	22.792	3349	3350	3356	rBB6	44311	51858	1.27%	0.100%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014863.D
 Acq On : 10 Jun 2021 14:00
 Operator : CG/JU
 Sample : M2618-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG5R0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

117	22.839	3356	3358	3361	rBB4	55203	64132	1.58%	0.124%
118	22.886	3364	3366	3367	rBB2	65189	104281	2.56%	0.202%
119	22.933	3371	3374	3376	rBB4	74758	65364	1.61%	0.126%
120	22.992	3381	3384	3385	rBB3	47680	59812	1.47%	0.116%
121	23.068	3395	3397	3398	rBB2	55844	44939	1.10%	0.087%
122	23.092	3400	3401	3404	rBB3	91668	59915	1.47%	0.116%
123	23.298	3435	3436	3441	rBB5	38462	78390	1.93%	0.152%
124	23.421	3450	3457	3462	rBB	1750815	3063774	75.27%	5.923%
125	23.462	3462	3464	3469	rBB6	111227	139640	3.43%	0.270%
126	23.562	3475	3481	3491	rBB2	1301952	2643710	64.95%	5.111%
127	23.780	3514	3518	3521	rBB6	58827	72471	1.78%	0.140%
128	23.827	3525	3526	3529	rBB3	46104	42929	1.05%	0.083%
129	23.856	3529	3531	3533	rBB3	63720	51487	1.26%	0.100%
130	23.909	3535	3540	3544	rBB8	83855	142092	3.49%	0.275%
131	24.009	3555	3557	3559	rBB3	40697	31805	0.78%	0.061%
132	24.050	3561	3564	3565	rBB3	58733	55405	1.36%	0.107%
133	24.068	3565	3567	3568	rBB2	48468	35065	0.86%	0.068%
134	24.121	3568	3576	3584	rBB2	296159	674284	16.57%	1.303%
135	24.197	3587	3589	3595	rBB7	52842	79510	1.95%	0.154%
136	24.339	3612	3613	3616	rBB3	39180	30813	0.76%	0.060%
137	24.433	3625	3629	3633	rBB7	62497	100349	2.47%	0.194%
138	24.486	3637	3638	3641	rBB3	62764	49097	1.21%	0.095%
139	24.562	3648	3651	3652	rBB3	46367	37950	0.93%	0.073%
140	24.574	3652	3653	3660	rBB7	79138	122717	3.02%	0.237%
141	24.703	3673	3675	3678	rBB4	34800	36896	0.91%	0.071%
142	24.745	3680	3682	3684	rBB3	51637	60561	1.49%	0.117%
143	24.809	3691	3693	3695	rBB3	67161	38367	0.94%	0.074%
144	24.933	3712	3714	3715	rBB2	42257	35876	0.88%	0.069%
145	24.962	3715	3719	3720	rBB4	44724	43060	1.06%	0.083%
146	24.980	3720	3722	3731	rBB10	29775	116756	2.87%	0.226%
147	25.097	3741	3742	3744	rBB2	62968	38943	0.96%	0.075%
148	25.174	3751	3755	3758	rBB6	65956	74838	1.84%	0.145%
149	25.215	3760	3762	3764	rBB3	61325	36449	0.90%	0.070%
150	25.439	3798	3800	3803	rBB4	49120	45594	1.12%	0.088%
151	25.527	3812	3815	3817	rBB4	72321	47313	1.16%	0.091%
152	25.644	3833	3835	3836	rBB2	36644	33555	0.82%	0.065%
153	25.762	3850	3855	3860	rBB9	139578	219499	5.39%	0.424%
154	25.850	3865	3870	3872	rBB6	91890	108138	2.66%	0.209%
155	25.874	3872	3874	3876	rBB3	44730	33800	0.83%	0.065%
156	26.039	3899	3902	3907	rBB7	76485	91393	2.25%	0.177%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014863.D
 Acq On : 10 Jun 2021 14:00
 Operator : CG/JU
 Sample : M2618-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG5R0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

157	26.086	3907	3910	3911	rBB3	34002	50002	1.23%	0.097%
158	26.109	3911	3914	3915	rBB3	36131	36229	0.89%	0.070%
159	26.197	3926	3929	3930	rBB3	44613	44449	1.09%	0.086%
160	26.227	3933	3934	3939	rBB5	59683	59541	1.46%	0.115%
161	26.268	3940	3941	3944	rBB3	47370	33860	0.83%	0.065%
162	26.327	3947	3951	3953	rBB5	61725	69196	1.70%	0.134%
163	26.350	3953	3955	3959	rBB5	59537	55586	1.37%	0.107%
164	26.456	3972	3973	3976	rBB3	64193	41023	1.01%	0.079%
165	26.503	3979	3981	3983	rBB3	66862	44189	1.09%	0.085%
166	26.662	3998	4008	4009	rBB10	33006	111323	2.74%	0.215%
167	26.686	4009	4012	4013	rBB3	62347	51014	1.25%	0.099%
168	26.715	4013	4017	4019	rBB5	44643	60907	1.50%	0.118%
169	26.768	4023	4026	4027	rBB3	55601	32736	0.80%	0.063%
170	26.809	4027	4033	4040	rBB3	135847	311244	7.65%	0.602%
171	26.880	4044	4045	4050	rBB5	54949	43591	1.07%	0.084%
172	26.927	4052	4053	4055	rBB2	48046	32851	0.81%	0.064%
173	26.950	4055	4057	4059	rBB3	64061	53048	1.30%	0.103%
174	26.986	4059	4063	4066	rBB6	57329	61082	1.50%	0.118%
175	27.039	4071	4072	4079	rBB7	39022	64709	1.59%	0.125%
176	27.086	4079	4080	4085	rBB5	45311	43744	1.07%	0.085%
177	27.180	4095	4096	4098	rBB2	49899	33034	0.81%	0.064%
178	27.203	4098	4100	4102	rBB3	37028	42142	1.04%	0.081%
179	27.233	4102	4105	4106	rVV3	60317	51123	1.26%	0.099%
180	27.291	4113	4115	4118	rBB4	52865	42169	1.04%	0.082%
181	27.327	4118	4121	4122	rBB3	39865	32334	0.79%	0.063%
182	27.386	4129	4131	4134	rBB4	55091	46754	1.15%	0.090%
183	27.438	4137	4140	4142	rBB4	60523	43997	1.08%	0.085%
184	27.486	4145	4148	4151	rBB5	52721	54590	1.34%	0.106%
185	27.597	4165	4167	4168	rBV2	49915	32594	0.80%	0.063%
186	27.656	4175	4177	4180	rBB4	61786	80172	1.97%	0.155%
187	27.962	4226	4229	4232	rBB5	31882	31199	0.77%	0.060%
188	28.056	4242	4245	4247	rBB4	50090	45980	1.13%	0.089%
189	28.286	4282	4284	4286	rBB3	57108	40294	0.99%	0.078%
190	28.456	4311	4313	4316	rBB4	30490	30724	0.75%	0.059%
191	28.515	4320	4323	4324	rBB3	42654	32650	0.80%	0.063%
192	28.638	4339	4344	4349	rBV9	55255	137260	3.37%	0.265%
193	28.768	4361	4366	4368	rBB6	73647	100938	2.48%	0.195%
194	28.891	4381	4387	4388	rBV6	63015	101782	2.50%	0.197%
195	28.903	4388	4389	4394	rBB5	45087	68409	1.68%	0.132%
196	29.021	4407	4409	4412	rBB4	31211	38057	0.94%	0.074%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014863.D
Acq On : 10 Jun 2021 14:00
Operator : CG/JU
Sample : M2618-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG5R0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Title : SVOA CALIBRATION

197	29.068	4412	4417	4420	rBB7	55440	96548	2.37%	0.187%
198	29.115	4422	4425	4431	rBB8	51036	72211	1.77%	0.140%
199	29.215	4438	4442	4446	rBB7	45916	52495	1.29%	0.101%
200	29.344	4459	4464	4465	rBB5	24450	40566	1.00%	0.078%

Sum of corrected areas: 51729608

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014863.D
Acq On : 10 Jun 2021 14:00
Operator : CG/JU
Sample : M2618-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG5R0










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
24.121	5.10 ng/ul	674284	Perylene-d12	23.562

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetratriacontane	479	C34H70	014167-59-0	92
2			Heneicosane	296	C21H44	000629-94-7	70
3			Nonacosane	408	C29H60	000630-03-5	70
4			Docosane	310	C22H46	000629-97-0	70
5			Hexadecane	226	C16H34	000544-76-3	62

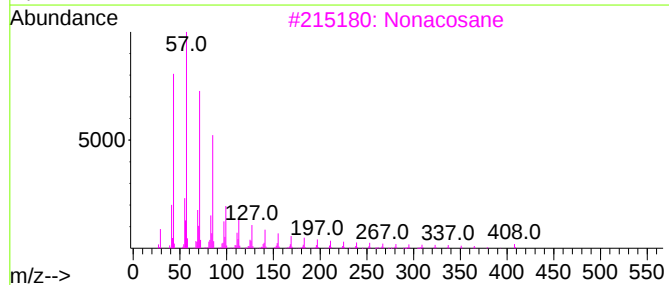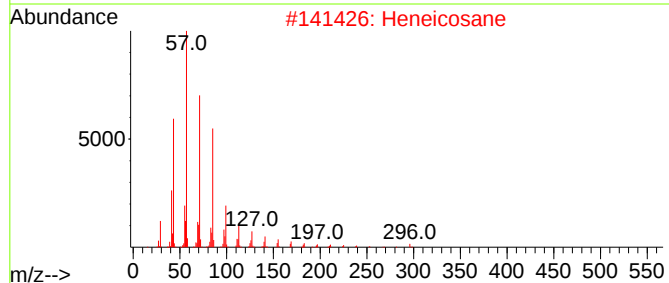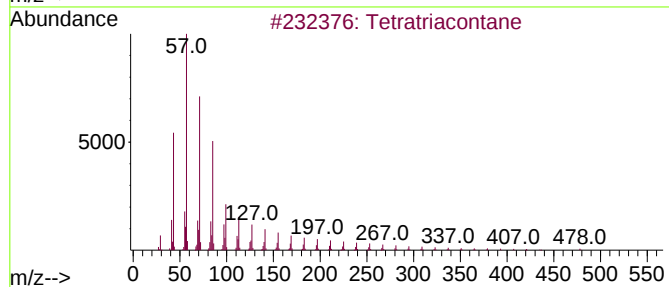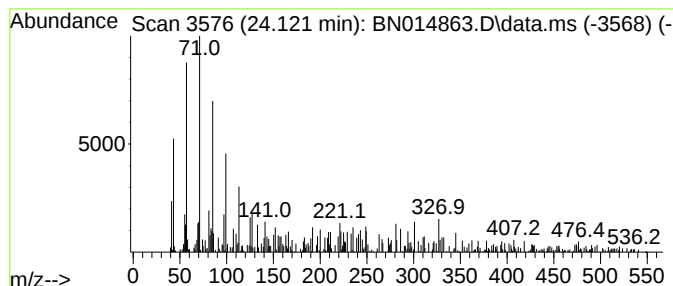

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014863.D
Acq On : 10 Jun 2021 14:00
Operator : CG/JU
Sample : M2618-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG5R0










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
26.809	2.35 ng/ul	311244	Perylene-d12	23.562

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-(3-Acetamidophenyl)-3-(2,2,2-t...	438	C16H21Cl3N4O2S	294658-29-0	47		
2	Sulfone, [2-isobutyl-5-(4-morpho...	350	C17H22N2O4S	1000300-55-3	47		
3	5-[(2,4-Dinitrophenyl)hydrazono]...	282	C11H14N4O5	001831-56-7	47		
4	Pentanal, 5-hydroxy-, (2,4-dinit...	282	C11H14N4O5	003638-33-3	38		
5	Butane-1,4-diol, 2,2-dimethylpen...	314	C18H34O4	1000163-75-6	38		

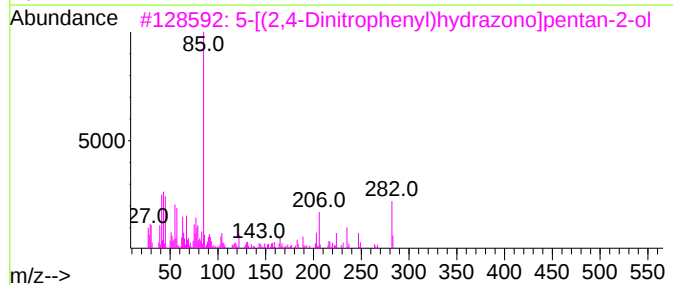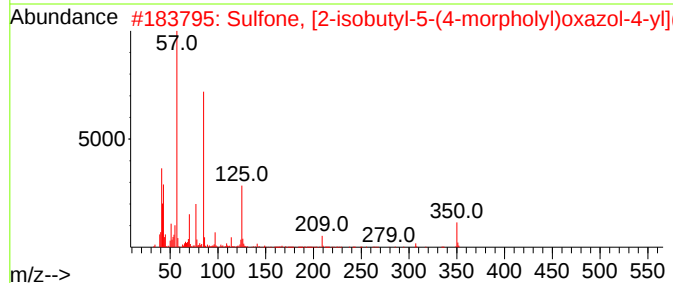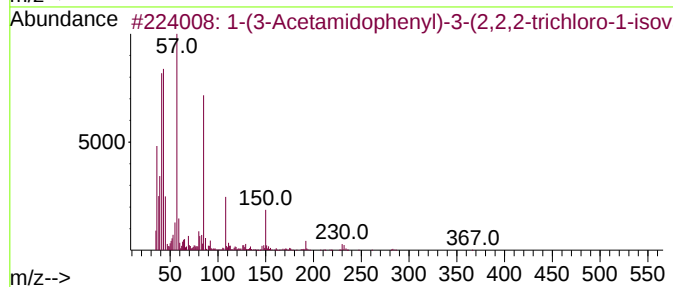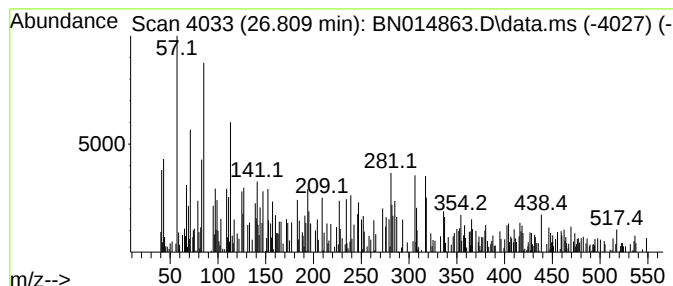

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014863.D
Acq On : 10 Jun 2021 14:00
Operator : CG/JU
Sample : M2618-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG5R0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	24.121	5.1	ng/u1	674284	6	23.562	2643710	20.0
unknown-01	26.809	2.4	ng/u1	311244	6	23.562	2643710	20.0