

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014866.D
 Acq On : 10 Jun 2021 16:32
 Operator : CG/JU
 Sample : M2618-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG5S6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014866.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	18	23	28	rBB6	24766	38784	1.36%	0.078%
2	3.846	123	129	135	rBB	43886	65844	2.31%	0.132%
3	4.028	157	160	169	rBB7	13676	33233	1.17%	0.066%
4	4.828	291	296	303	rBB	58953	90306	3.17%	0.180%
5	6.569	588	592	597	rBB3	21270	29330	1.03%	0.059%
6	6.875	636	644	652	rBB	551495	874773	30.69%	1.748%
7	7.034	666	671	679	rBB	347984	560564	19.66%	1.120%
8	7.234	699	705	713	rBV	607109	971305	34.07%	1.941%
9	7.699	777	784	790	rBB	677110	1080103	37.89%	2.159%
10	8.404	897	904	914	rBB2	708941	1141906	40.06%	2.282%
11	8.851	973	980	992	rBB	553095	919990	32.27%	1.839%
12	9.569	1096	1102	1112	rBV2	458024	788172	27.65%	1.575%
13	10.110	1187	1194	1203	rBV	809508	1333809	46.79%	2.666%
14	10.487	1250	1258	1271	rBV	920402	1530230	53.68%	3.058%
15	10.622	1274	1281	1291	rBB	628872	1086692	38.12%	2.172%
16	13.245	1721	1727	1732	rBB6	24583	46347	1.63%	0.093%
17	13.763	1804	1815	1824	rBB	1318497	1892562	66.39%	3.782%
18	14.039	1856	1862	1877	rVB	1421526	2229745	78.22%	4.456%
19	14.351	1908	1915	1922	rBV	1407711	2139094	75.04%	4.275%
20	14.563	1945	1951	1962	rBB	344382	606989	21.29%	1.213%
21	15.351	2077	2085	2092	rBB	1969959	2765685	97.02%	5.527%
22	15.475	2099	2106	2113	rBB4	128409	201854	7.08%	0.403%
23	16.757	2319	2324	2330	rBB10	23288	47566	1.67%	0.095%
24	16.880	2335	2345	2349	rBB10	47921	95184	3.34%	0.190%
25	16.922	2349	2352	2357	rBB7	23187	38413	1.35%	0.077%
26	17.104	2378	2383	2388	rBB	1728737	2407477	84.45%	4.811%
27	17.145	2388	2390	2394	rBB	240358	232653	8.16%	0.465%
28	17.204	2395	2400	2405	rBB2	2102200	2850692	100.00%	5.697%
29	17.304	2412	2417	2423	rBB10	25580	46901	1.65%	0.094%
30	17.422	2433	2437	2441	rBB7	32612	46175	1.62%	0.092%
31	17.945	2522	2526	2528	rBB5	20926	34039	1.19%	0.068%
32	17.986	2528	2533	2535	rBB5	36690	57914	2.03%	0.116%
33	18.033	2535	2541	2546	rBB5	76978	148651	5.21%	0.297%
34	18.169	2562	2564	2569	rBB6	69458	105142	3.69%	0.210%
35	18.222	2569	2573	2576	rBB6	30571	38640	1.36%	0.077%
36	18.380	2598	2600	2603	rBB4	57924	55820	1.96%	0.112%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014866.D
 Acq On : 10 Jun 2021 16:32
 Operator : CG/JU
 Sample : M2618-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG5S6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

37	18.492	2615	2619	2622	rBB6	48597	74231	2.60%	0.148%
38	18.627	2638	2642	2646	rBB7	24181	34818	1.22%	0.070%
39	18.910	2688	2690	2693	rBB4	43291	40057	1.41%	0.080%
40	19.045	2711	2713	2720	rBB8	49849	96111	3.37%	0.192%
41	19.174	2730	2735	2739	rBB	669179	870792	30.55%	1.740%
42	19.239	2741	2746	2749	rBB7	35617	51707	1.81%	0.103%
43	19.398	2769	2773	2774	rBB4	28209	39584	1.39%	0.079%
44	19.422	2774	2777	2779	rVB4	38039	40363	1.42%	0.081%
45	19.451	2779	2782	2785	rBV5	57902	50030	1.76%	0.100%
46	19.510	2787	2792	2796	rBB	2134125	2837383	99.53%	5.670%
47	19.716	2823	2827	2828	rBB4	43132	54455	1.91%	0.109%
48	19.857	2847	2851	2854	rBB6	45332	56620	1.99%	0.113%
49	19.886	2854	2856	2859	rBB4	48696	31960	1.12%	0.064%
50	20.033	2878	2881	2886	rBB7	96909	108864	3.82%	0.218%
51	20.098	2888	2892	2895	rBB6	30731	32966	1.16%	0.066%
52	20.139	2895	2899	2903	rBB7	45302	48003	1.68%	0.096%
53	20.198	2903	2909	2912	rBB7	97874	166749	5.85%	0.333%
54	20.298	2920	2926	2927	rBB6	28080	42449	1.49%	0.085%
55	20.345	2933	2934	2937	rBB3	58039	32487	1.14%	0.065%
56	20.386	2937	2941	2944	rBB6	63576	100362	3.52%	0.201%
57	20.416	2944	2946	2948	rBB3	66244	47128	1.65%	0.094%
58	20.451	2948	2952	2955	rBB6	53025	62290	2.19%	0.124%
59	20.710	2993	2996	2997	rBB3	35183	39203	1.38%	0.078%
60	20.763	3002	3005	3006	rBB3	29819	35288	1.24%	0.071%
61	20.851	3017	3020	3021	rBB3	45658	32346	1.13%	0.065%
62	20.945	3033	3036	3038	rBB4	42961	46913	1.65%	0.094%
63	21.004	3041	3046	3047	rBB4	64527	81321	2.85%	0.163%
64	21.039	3047	3052	3055	rBB6	116714	196568	6.90%	0.393%
65	21.080	3057	3059	3060	rBB2	49029	40661	1.43%	0.081%
66	21.116	3060	3065	3069	rBB8	101873	146951	5.15%	0.294%
67	21.192	3075	3078	3079	rBB3	62031	63645	2.23%	0.127%
68	21.233	3081	3085	3089	rBB	487622	527765	18.51%	1.055%
69	21.310	3090	3098	3102	rBB2	1995897	2740079	96.12%	5.476%
70	21.345	3102	3104	3108	rBB	166831	145362	5.10%	0.291%
71	21.421	3112	3117	3120	rBB7	78916	145245	5.10%	0.290%
72	21.474	3120	3126	3128	rBB7	63027	126696	4.44%	0.253%
73	21.510	3128	3132	3135	rBB6	67322	83546	2.93%	0.167%
74	21.539	3135	3137	3138	rBB2	42256	39408	1.38%	0.079%
75	21.627	3149	3152	3154	rBB4	66546	59474	2.09%	0.119%
76	21.686	3158	3162	3164	rBB5	52501	62084	2.18%	0.124%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014866.D
 Acq On : 10 Jun 2021 16:32
 Operator : CG/JU
 Sample : M2618-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG5S6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

77	21.727	3166	3169	3171	rBB4	72905	55798	1.96%	0.112%
78	21.804	3179	3182	3184	rBB4	37335	39638	1.39%	0.079%
79	21.868	3188	3193	3196	rBB6	91964	99731	3.50%	0.199%
80	21.921	3198	3202	3206	rBB7	162041	230279	8.08%	0.460%
81	22.015	3216	3218	3222	rBB5	57931	52046	1.83%	0.104%
82	22.057	3222	3225	3228	rBB5	70057	69399	2.43%	0.139%
83	22.086	3228	3230	3232	rBB3	43879	39193	1.37%	0.078%
84	22.121	3232	3236	3237	rBB4	35531	40283	1.41%	0.081%
85	22.257	3257	3259	3260	rBB2	45510	32937	1.16%	0.066%
86	22.380	3276	3280	3286	rBB8	151353	216776	7.60%	0.433%
87	22.486	3292	3298	3303	rBB10	95662	195587	6.86%	0.391%
88	22.527	3303	3305	3307	rBB3	51470	41601	1.46%	0.083%
89	22.604	3317	3318	3320	rBB2	56071	32463	1.14%	0.065%
90	22.639	3322	3324	3326	rBB3	86030	56791	1.99%	0.113%
91	22.674	3326	3330	3332	rBB5	66049	91090	3.20%	0.182%
92	22.727	3337	3339	3342	rBB4	45507	39522	1.39%	0.079%
93	22.763	3342	3345	3347	rBB4	83227	89290	3.13%	0.178%
94	22.792	3347	3350	3351	rBB3	46821	41676	1.46%	0.083%
95	22.804	3351	3352	3354	rBB2	62349	38497	1.35%	0.077%
96	22.827	3355	3356	3359	rBB3	42951	30798	1.08%	0.062%
97	22.898	3359	3368	3373	rBB4	335643	782904	27.46%	1.565%
98	22.933	3373	3374	3381	rBB7	36970	37979	1.33%	0.076%
99	23.004	3383	3386	3389	rBB5	55398	61766	2.17%	0.123%
100	23.074	3396	3398	3400	rBB3	59194	60552	2.12%	0.121%
101	23.145	3408	3410	3413	rBB4	53412	29902	1.05%	0.060%
102	23.180	3415	3416	3417	rBB	63675	35221	1.24%	0.070%
103	23.204	3417	3420	3421	rBB3	54185	34117	1.20%	0.068%
104	23.227	3421	3424	3426	rBB4	34994	36366	1.28%	0.073%
105	23.268	3429	3431	3433	rBB3	59542	53584	1.88%	0.107%
106	23.304	3436	3437	3441	rBB4	49026	58399	2.05%	0.117%
107	23.374	3445	3449	3452	rBB5	118869	171327	6.01%	0.342%
108	23.427	3452	3458	3463	rBB	1576435	2679250	93.99%	5.354%
109	23.468	3463	3465	3470	rBB3	163213	201052	7.05%	0.402%
110	23.574	3476	3483	3492	rBB2	1384890	2755205	96.65%	5.506%
111	23.680	3498	3501	3502	rBB3	81864	50509	1.77%	0.101%
112	23.698	3502	3504	3507	rBB4	42651	37642	1.32%	0.075%
113	23.727	3507	3509	3510	rBB2	62160	38877	1.36%	0.078%
114	23.780	3516	3518	3520	rBB3	59730	50355	1.77%	0.101%
115	23.798	3520	3521	3527	rBB6	26988	33953	1.19%	0.068%
116	23.892	3533	3537	3539	rBB5	31388	39533	1.39%	0.079%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014866.D
 Acq On : 10 Jun 2021 16:32
 Operator : CG/JU
 Sample : M2618-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG5S6

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

117	23.933	3541	3544	3546	rBB4	57229	50818	1.78%	0.102%
118	23.980	3551	3552	3554	rBB2	51072	31397	1.10%	0.063%
119	24.027	3557	3560	3561	rBB3	34587	41376	1.45%	0.083%
120	24.062	3565	3566	3571	rBB5	60881	40969	1.44%	0.082%
121	24.133	3571	3578	3583	rBB5	257661	599048	21.01%	1.197%
122	24.192	3586	3588	3589	rBB2	73541	32222	1.13%	0.064%
123	24.204	3589	3590	3593	rBB3	52044	41647	1.46%	0.083%
124	24.251	3597	3598	3600	rBB2	72321	37122	1.30%	0.074%
125	24.286	3600	3604	3605	rBB4	29122	34311	1.20%	0.069%
126	24.309	3605	3608	3609	rBB3	34116	32494	1.14%	0.065%
127	24.380	3619	3620	3624	rBB4	25310	36627	1.28%	0.073%
128	24.427	3624	3628	3629	rBB4	49650	69072	2.42%	0.138%
129	24.515	3642	3643	3645	rBB2	50091	30350	1.06%	0.061%
130	24.551	3645	3649	3651	rBB5	43783	37223	1.31%	0.074%
131	24.574	3651	3653	3656	rBB4	71730	64776	2.27%	0.129%
132	24.645	3661	3665	3666	rBB4	58094	51764	1.82%	0.103%
133	24.804	3690	3692	3694	rBB3	70626	50412	1.77%	0.101%
134	24.851	3697	3700	3701	rBB3	40515	38789	1.36%	0.078%
135	24.880	3701	3705	3714	rBB3	204656	463122	16.25%	0.926%
136	24.992	3723	3724	3726	rBB2	56506	37635	1.32%	0.075%
137	25.062	3734	3736	3738	rBB3	38898	29986	1.05%	0.060%
138	25.127	3745	3747	3752	rBB6	57072	68296	2.40%	0.136%
139	25.162	3752	3753	3755	rBB2	42255	30988	1.09%	0.062%
140	25.198	3757	3759	3762	rBB4	57291	55928	1.96%	0.112%
141	25.233	3762	3765	3767	rBB4	41898	57100	2.00%	0.114%
142	25.268	3767	3771	3772	rBB4	54256	46884	1.64%	0.094%
143	25.286	3772	3774	3775	rBB2	89117	57984	2.03%	0.116%
144	25.309	3775	3778	3781	rBB5	78283	110504	3.88%	0.221%
145	25.392	3789	3792	3796	rBB6	46367	63921	2.24%	0.128%
146	25.427	3796	3798	3801	rBB4	59020	37773	1.33%	0.075%
147	25.533	3815	3816	3819	rBB3	36524	33174	1.16%	0.066%
148	25.598	3823	3827	3828	rBB4	29624	38536	1.35%	0.077%
149	25.774	3852	3857	3862	rVB9	153817	322868	11.33%	0.645%
150	25.845	3865	3869	3873	rBB7	67573	101678	3.57%	0.203%
151	26.004	3895	3896	3899	rBB3	56507	43156	1.51%	0.086%
152	26.104	3911	3913	3918	rBB6	45040	58612	2.06%	0.117%
153	26.203	3926	3930	3931	rBB4	16866	37204	1.31%	0.074%
154	26.215	3931	3932	3936	rBB4	47706	43989	1.54%	0.088%
155	26.274	3940	3942	3945	rBB4	56838	31619	1.11%	0.063%
156	26.321	3945	3950	3951	rBB5	75036	120616	4.23%	0.241%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014866.D
 Acq On : 10 Jun 2021 16:32
 Operator : CG/JU
 Sample : M2618-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG5S6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

157	26.421	3964	3967	3968	rBB3	41857	38832	1.36%	0.078%
158	26.498	3977	3980	3981	rBB3	40879	32338	1.13%	0.065%
159	26.509	3981	3982	3986	rBB4	51663	35421	1.24%	0.071%
160	26.545	3986	3988	3989	rBB2	51592	33768	1.18%	0.067%
161	26.615	3998	4000	4004	rBB5	32991	33827	1.19%	0.068%
162	26.651	4004	4006	4008	rBB3	50982	35683	1.25%	0.071%
163	26.715	4016	4017	4020	rBB3	50290	33050	1.16%	0.066%
164	26.803	4028	4032	4035	rBB6	62869	88111	3.09%	0.176%
165	26.886	4045	4046	4048	rBB2	63994	35616	1.25%	0.071%
166	27.009	4065	4067	4070	rBB4	47586	41846	1.47%	0.084%
167	27.103	4080	4083	4085	rBB4	55192	53207	1.87%	0.106%
168	27.186	4093	4097	4100	rBB6	58370	82227	2.88%	0.164%
169	27.221	4100	4103	4105	rBB4	48660	38648	1.36%	0.077%
170	27.262	4108	4110	4112	rBB3	45285	34819	1.22%	0.070%
171	27.286	4112	4114	4116	rBB3	58643	46675	1.64%	0.093%
172	27.333	4119	4122	4124	rBB4	34308	33857	1.19%	0.068%
173	27.374	4127	4129	4131	rBB3	50005	37224	1.31%	0.074%
174	27.498	4148	4150	4153	rBB4	44855	50397	1.77%	0.101%
175	27.809	4201	4203	4204	rBB2	36047	33143	1.16%	0.066%
176	27.839	4204	4208	4210	rBB5	50656	38101	1.34%	0.076%
177	27.874	4212	4214	4219	rBB6	46250	56588	1.99%	0.113%
178	28.045	4240	4243	4244	rBB3	55919	41518	1.46%	0.083%
179	28.062	4244	4246	4247	rBB2	65354	37955	1.33%	0.076%
180	28.150	4259	4261	4262	rBB2	51616	30361	1.07%	0.061%
181	28.298	4284	4286	4289	rBB4	50472	35040	1.23%	0.070%
182	28.345	4291	4294	4296	rBB4	43927	46997	1.65%	0.094%
183	28.550	4325	4329	4330	rBB4	51419	41611	1.46%	0.083%
184	28.627	4340	4342	4344	rBB3	38164	29814	1.05%	0.060%
185	28.650	4344	4346	4348	rBB3	45461	33536	1.18%	0.067%
186	28.692	4348	4353	4356	rBB7	41327	62560	2.19%	0.125%
187	28.815	4369	4374	4376	rBB6	46020	44740	1.57%	0.089%
188	28.850	4378	4380	4383	rBB4	47292	53247	1.87%	0.106%
189	28.886	4383	4386	4390	rBB6	82499	115276	4.04%	0.230%
190	28.968	4397	4400	4401	rBV3	46294	37027	1.30%	0.074%
191	29.062	4414	4416	4420	rBB5	72701	76214	2.67%	0.152%
192	29.109	4420	4424	4426	rBB5	43811	55966	1.96%	0.112%
193	29.174	4433	4435	4437	rBB3	50493	31558	1.11%	0.063%
194	29.197	4437	4439	4441	rBB3	47367	29491	1.03%	0.059%
195	29.239	4443	4446	4448	rBB4	39410	48207	1.69%	0.096%
196	29.262	4448	4450	4453	rBB4	43673	36941	1.30%	0.074%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014866.D
Acq On : 10 Jun 2021 16:32
Operator : CG/JU
Sample : M2618-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG5S6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Title : SVOA CALIBRATION

197	29.297	4453	4456	4458	rBB4	73281	48382	1.70%	0.097%
198	29.333	4459	4462	4465	rBB5	27223	29381	1.03%	0.059%




Sum of corrected areas: 50037626

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014866.D
Acq On : 10 Jun 2021 16:32
Operator : CG/JU
Sample : M2618-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG5S6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

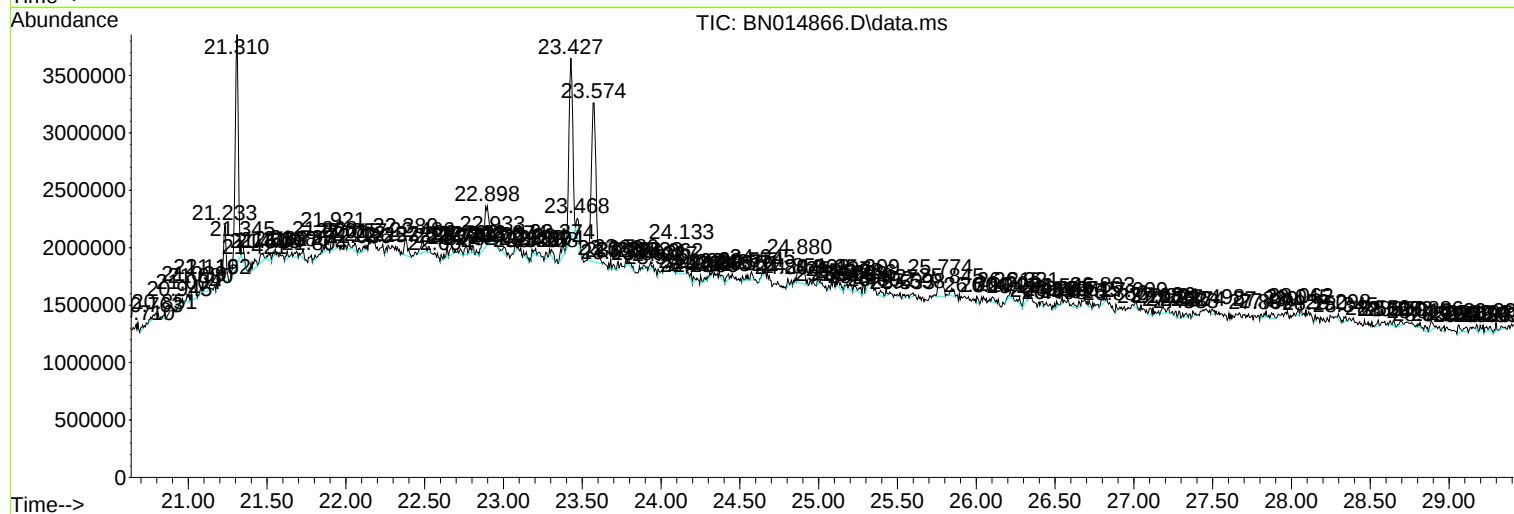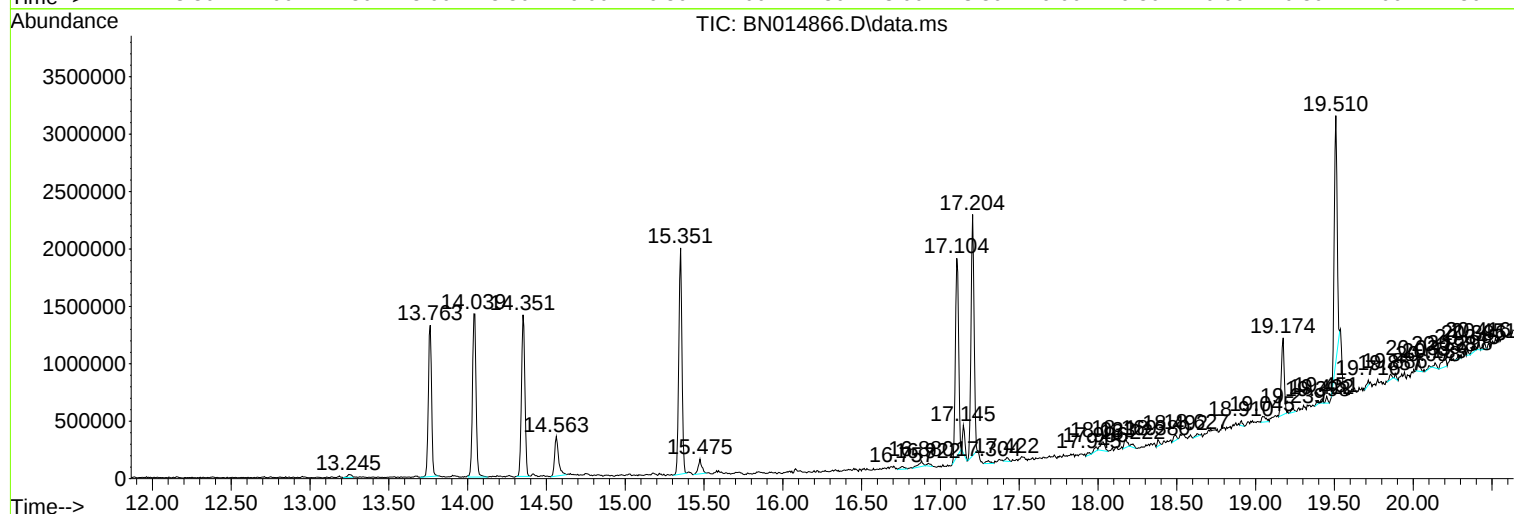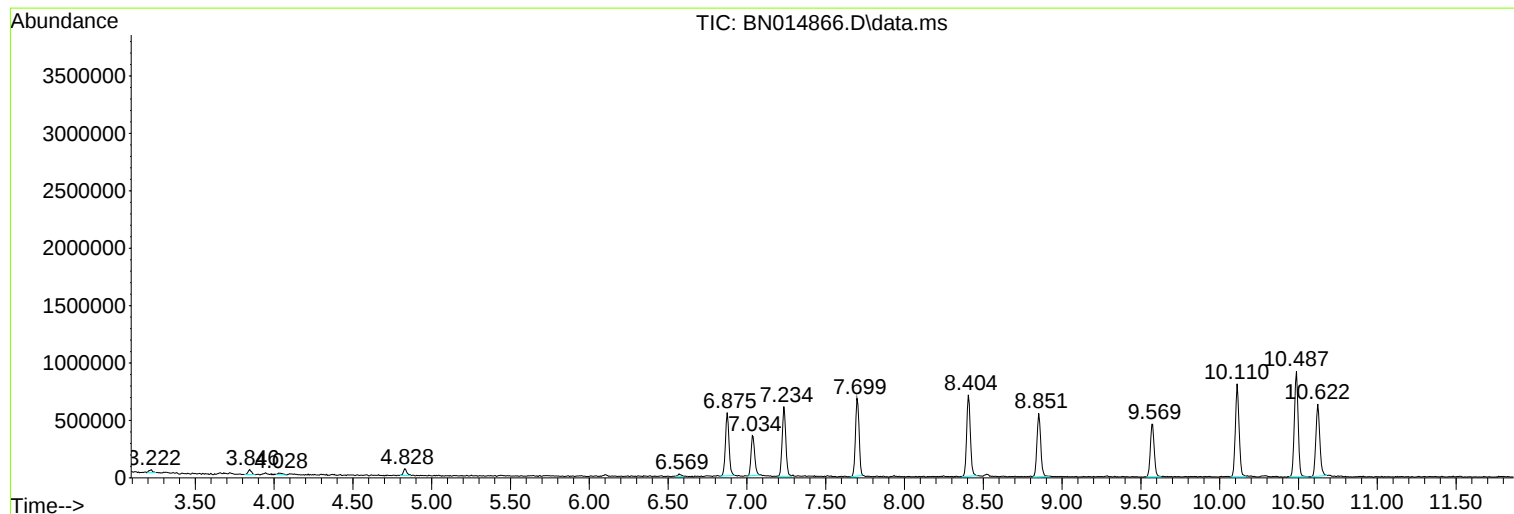

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014866.D
Acq On : 10 Jun 2021 16:32
Operator : CG/JU
Sample : M2618-08
Misc :
ALS Vial : 8 Sample Multiplier: 1










Instrument :
BNA_N
ClientSampleId :
BG5S6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
24.133	4.35 ng/ul	599048	Perylene-d12		23.568	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	Heptacosane		380	C27H56	000593-49-7	91
2	Dotriacontane		451	C32H66	000544-85-4	87
3	Hexatriacontane		507	C36H74	000630-06-8	81
4	Docosane, 1,22-dibromo-		466	C22H44Br2	034540-49-3	68
5	Heptacosane, 1-chloro-		414	C27H55Cl	062016-79-9	68

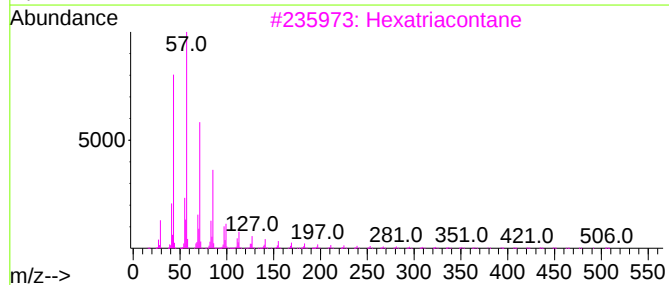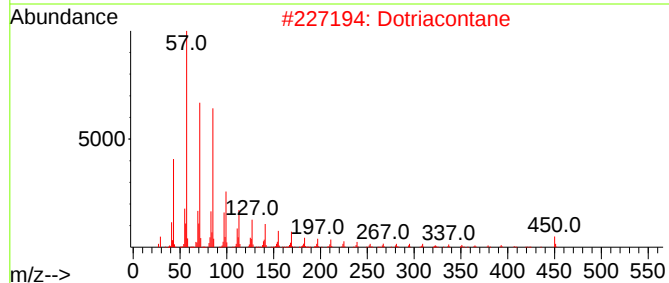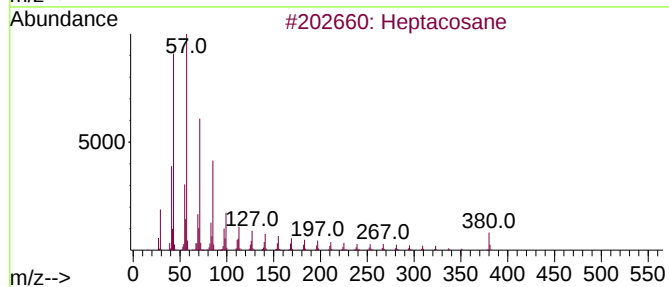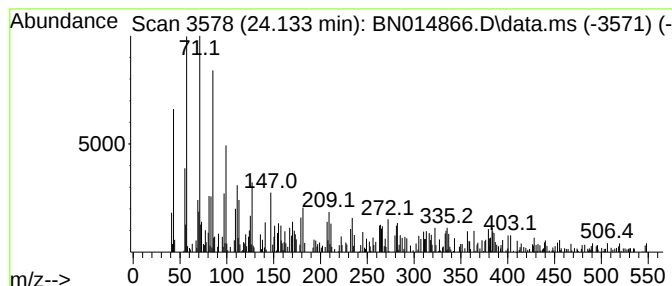

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014866.D
Acq On : 10 Jun 2021 16:32
Operator : CG/JU
Sample : M2618-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG5S6










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
24.880	3.36 ng/ul	463122	Perylene-d12	23.568

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triacontane	422	C30H62	000638-68-6	78
2			Triacontane	422	C30H62	000638-68-6	60
3			Tetradecane, 2,6,10-trimethyl-	240	C17H36	014905-56-7	49
4			Pentadecane	212	C15H32	000629-62-9	47
5			Octa-3,5-diene-2,7-dione, 4,5-di...	170	C8H10O4	1000266-61-0	47

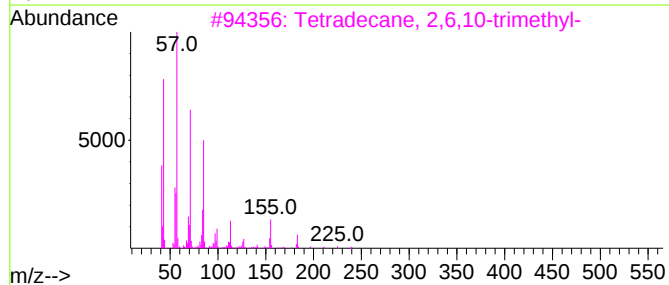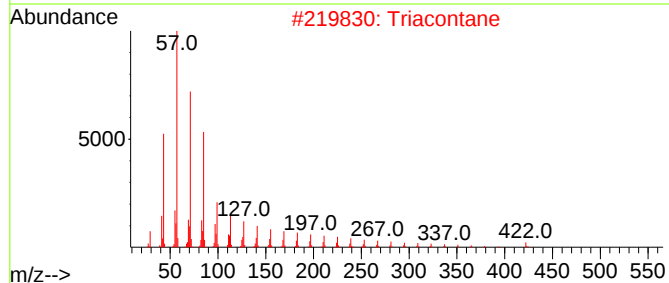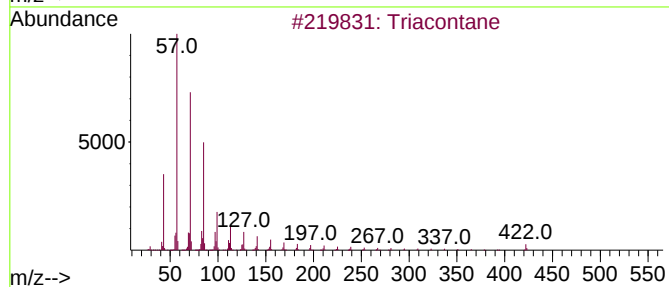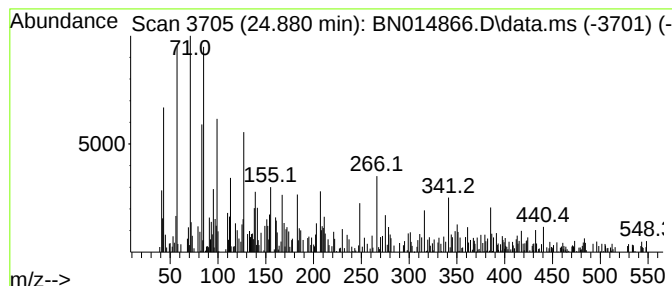

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014866.D
Acq On : 10 Jun 2021 16:32
Operator : CG/JU
Sample : M2618-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
BG5S6










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown-01 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
25.774	2.34 ng/ul	322868	Perylene-d12	23.568

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Thiophene-2-acetamide, N-(4-chlo...	251	C12H10ClNOS	1000339-46-5	35
2			Acetamide, N-(3-chlorophenyl)-2-...	251	C12H10ClNOS	1000306-90-3	25
3			2-Ethyl-5-undecyl-.delta.1--pyrr...	251	C17H33N	114640-31-2	25
4			Benzene, 1-phenyl-4-(2-cyano-2-p...	281	C21H15N	027869-56-3	22
5			Phentolamine	281	C17H19N3O	000050-60-2	22

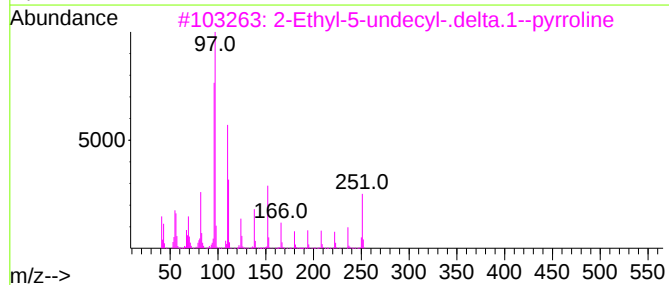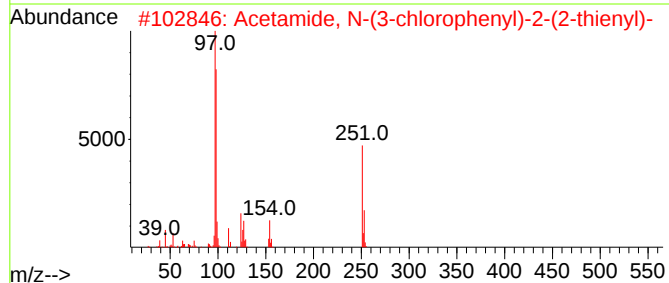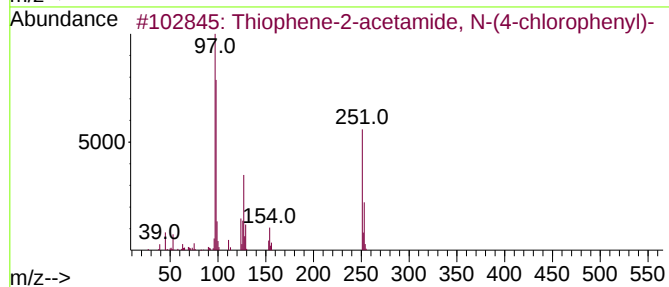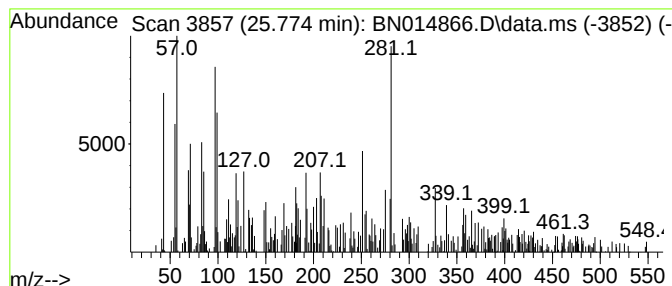

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014866.D
Acq On : 10 Jun 2021 16:32
Operator : CG/JU
Sample : M2618-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG5S6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	24.133	4.3	ng/ul	599048	6	23.568	2755210	20.0
(DEL) Alkane: S...	24.880	3.4	ng/ul	463122	6	23.568	2755210	20.0
unknown-01	25.774	2.3	ng/ul	322868	6	23.568	2755210	20.0