

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014868.D
 Acq On : 10 Jun 2021 19:02
 Operator : CG/JU
 Sample : PB136853BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK853

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014868.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	19	22	24	rBB4	27698	24625	0.53%	0.046%
2	3.617	85	90	106	rBB	288592	529909	11.30%	0.992%
3	6.869	635	643	650	rBB	633104	1051961	22.44%	1.970%
4	7.034	665	671	682	rBB	441323	722760	15.42%	1.354%
5	7.228	697	704	716	rVB	751196	1206371	25.73%	2.259%
6	7.699	776	784	791	rBV	627490	1002919	21.39%	1.878%
7	8.399	895	903	917	rBV	840123	1478522	31.54%	2.769%
8	8.846	973	979	988	rBB	642753	1074294	22.91%	2.012%
9	9.569	1095	1102	1111	rBB	587888	983555	20.98%	1.842%
10	10.104	1187	1193	1200	rBB	895819	1528148	32.59%	2.862%
11	10.481	1250	1257	1265	rBV	801951	1348894	28.77%	2.526%
12	10.616	1273	1280	1289	rBB	806074	1426464	30.42%	2.671%
13	12.075	1524	1528	1533	rBB4	18620	25181	0.54%	0.047%
14	13.757	1805	1814	1822	rBV	1712213	2422904	51.68%	4.538%
15	14.040	1854	1862	1869	rBV	1781835	2675553	57.07%	5.011%
16	14.351	1907	1915	1923	rBV	1294948	1928213	41.13%	3.611%
17	14.557	1943	1950	1965	rBB2	605488	999461	21.32%	1.872%
18	15.345	2078	2084	2095	rBV	2265288	3293508	70.25%	6.168%
19	15.469	2098	2105	2115	rBV	741066	1078302	23.00%	2.019%
20	15.587	2121	2125	2133	rBB9	33623	47998	1.02%	0.090%
21	16.134	2214	2218	2222	rBB5	12755	17638	0.38%	0.033%
22	17.104	2375	2383	2391	rBV	1714319	2442290	52.09%	4.574%
23	17.198	2393	2399	2408	rVB2	2588625	3680103	78.49%	6.892%
24	18.010	2531	2537	2543	rBB8	44503	76103	1.62%	0.143%
25	19.069	2711	2717	2720	rBB8	12542	16101	0.34%	0.030%
26	19.133	2725	2728	2733	rBB	37386	51658	1.10%	0.097%
27	19.298	2753	2756	2759	rBB5	24694	35382	0.75%	0.066%
28	19.392	2768	2772	2774	rBB3	40220	40721	0.87%	0.076%
29	19.504	2784	2791	2799	rBV2	3335643	4688499	100.00%	8.781%
30	19.692	2822	2823	2826	rBB3	22342	17368	0.37%	0.033%
31	19.945	2864	2866	2868	rBB3	17272	15187	0.32%	0.028%
32	20.045	2877	2883	2884	rBB6	18575	36943	0.79%	0.069%
33	20.269	2919	2921	2923	rBB3	19082	17008	0.36%	0.032%
34	20.298	2923	2926	2928	rBB4	21065	26042	0.56%	0.049%
35	20.633	2981	2983	2985	rBB3	18479	16362	0.35%	0.031%
36	20.774	3003	3007	3011	rBB7	22845	40703	0.87%	0.076%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014868.D
 Acq On : 10 Jun 2021 19:02
 Operator : CG/JU
 Sample : PB136853BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK853

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

37	20.904	3026	3029	3030	rBB3	26886	16927	0.36%	0.032%
38	20.916	3030	3031	3034	rBB3	24841	20309	0.43%	0.038%
39	21.027	3047	3050	3052	rBB4	25004	27566	0.59%	0.052%
40	21.074	3055	3058	3059	rBB3	13917	15330	0.33%	0.029%
41	21.086	3059	3060	3062	rBB2	33203	21110	0.45%	0.040%
42	21.192	3074	3078	3079	rBB4	32338	23119	0.49%	0.043%
43	21.227	3079	3084	3085	rBB5	31391	37050	0.79%	0.069%
44	21.298	3091	3096	3107	rBB	2095603	2912799	62.13%	5.455%
45	21.374	3107	3109	3112	rBB4	21571	16311	0.35%	0.031%
46	21.410	3112	3115	3118	rBB5	39918	49126	1.05%	0.092%
47	21.457	3121	3123	3125	rBB3	33930	29570	0.63%	0.055%
48	21.474	3125	3126	3132	rBB6	22563	25845	0.55%	0.048%
49	21.527	3132	3135	3137	rBB4	35451	27138	0.58%	0.051%
50	21.674	3158	3160	3163	rBB4	21671	19161	0.41%	0.036%
51	21.721	3163	3168	3169	rBB5	25955	31829	0.68%	0.060%
52	21.733	3169	3170	3171	rBB	31954	15060	0.32%	0.028%
53	21.792	3175	3180	3182	rBB6	45087	50217	1.07%	0.094%
54	21.833	3186	3187	3189	rBB2	25773	20908	0.45%	0.039%
55	21.869	3189	3193	3194	rBB4	19088	22563	0.48%	0.042%
56	21.904	3194	3199	3203	rBB7	79205	119206	2.54%	0.223%
57	21.933	3203	3204	3207	rBB3	18747	15816	0.34%	0.030%
58	21.963	3207	3209	3210	rBB2	39042	15179	0.32%	0.028%
59	21.986	3210	3213	3217	rBB6	28465	29079	0.62%	0.054%
60	22.104	3230	3233	3235	rBB4	32285	34799	0.74%	0.065%
61	22.145	3237	3240	3241	rBB3	47963	38011	0.81%	0.071%
62	22.180	3243	3246	3247	rBB3	27706	14995	0.32%	0.028%
63	22.210	3249	3251	3252	rBB2	29829	17099	0.36%	0.032%
64	22.227	3252	3254	3255	rBB2	26213	14623	0.31%	0.027%
65	22.239	3255	3256	3257	rBB	43272	18810	0.40%	0.035%
66	22.257	3257	3259	3260	rBB2	14457	17902	0.38%	0.034%
67	22.316	3266	3269	3272	rBB5	52379	59421	1.27%	0.111%
68	22.374	3275	3279	3283	rBB7	122718	176848	3.77%	0.331%
69	22.410	3283	3285	3289	rBB5	16374	20802	0.44%	0.039%
70	22.445	3289	3291	3295	rBB5	36243	41940	0.89%	0.079%
71	22.486	3295	3298	3299	rBB3	22347	17401	0.37%	0.033%
72	22.545	3305	3308	3309	rBB3	40319	25349	0.54%	0.047%
73	22.568	3309	3312	3314	rBB4	26060	27874	0.59%	0.052%
74	22.586	3314	3315	3319	rBB4	34394	30112	0.64%	0.056%
75	22.621	3319	3321	3325	rBB5	28638	34168	0.73%	0.064%
76	22.663	3325	3328	3330	rBB4	19111	25701	0.55%	0.048%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014868.D
 Acq On : 10 Jun 2021 19:02
 Operator : CG/JU
 Sample : PB136853BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK853

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

77	22.680	3330	3331	3333	rBB2	28936	14412	0.31%	0.027%
78	22.751	3341	3343	3345	rBB3	23983	21486	0.46%	0.040%
79	22.810	3349	3353	3358	rBB8	37521	56331	1.20%	0.105%
80	22.886	3361	3366	3371	rBB4	222309	313383	6.68%	0.587%
81	23.016	3384	3388	3389	rBB4	27261	21768	0.46%	0.041%
82	23.098	3399	3402	3408	rBB8	27729	29322	0.63%	0.055%
83	23.186	3415	3417	3419	rBB3	28009	19378	0.41%	0.036%
84	23.210	3419	3421	3423	rBB3	35706	23560	0.50%	0.044%
85	23.239	3423	3426	3427	rBB3	33927	40098	0.86%	0.075%
86	23.263	3427	3430	3433	rBB5	27809	19848	0.42%	0.037%
87	23.298	3433	3436	3437	rBB3	17424	17233	0.37%	0.032%
88	23.363	3446	3447	3448	rBB	24491	17739	0.38%	0.033%
89	23.415	3449	3456	3462	rBB2	2412267	4443561	94.78%	8.322%
90	23.557	3471	3480	3488	rBB2	1594658	3156855	67.33%	5.912%
91	23.668	3496	3499	3502	rBB5	31630	31373	0.67%	0.059%
92	23.715	3504	3507	3510	rBB5	16653	23946	0.51%	0.045%
93	23.798	3518	3521	3523	rBB4	37362	34084	0.73%	0.064%
94	23.815	3523	3524	3530	rBB6	29320	36890	0.79%	0.069%
95	23.868	3530	3533	3534	rBB3	32123	25864	0.55%	0.048%
96	23.886	3534	3536	3537	rBB2	34811	26740	0.57%	0.050%
97	23.915	3539	3541	3544	rBB4	22115	17024	0.36%	0.032%
98	23.963	3546	3549	3551	rBB4	23633	15054	0.32%	0.028%
99	24.039	3560	3562	3563	rBB2	20694	15179	0.32%	0.028%
100	24.051	3563	3564	3567	rBB3	22954	14497	0.31%	0.027%
101	24.110	3567	3574	3581	rBB4	322540	691509	14.75%	1.295%
102	24.163	3581	3583	3586	rBB4	24429	27996	0.60%	0.052%
103	24.321	3607	3610	3611	rBV3	22049	17639	0.38%	0.033%
104	24.339	3611	3613	3615	rBB3	18319	15363	0.33%	0.029%
105	24.421	3624	3627	3631	rBB6	33352	43190	0.92%	0.081%
106	24.492	3635	3639	3642	rBB6	23354	36356	0.78%	0.068%
107	24.533	3642	3646	3647	rBB3	13813	22109	0.47%	0.041%
108	24.580	3652	3654	3658	rBB5	33788	43186	0.92%	0.081%
109	24.651	3662	3666	3667	rBB4	24412	20923	0.45%	0.039%
110	24.668	3667	3669	3671	rBB3	22267	19776	0.42%	0.037%
111	24.704	3674	3675	3677	rBB2	32206	16875	0.36%	0.032%
112	24.745	3680	3682	3687	rBB6	36040	48633	1.04%	0.091%
113	24.780	3687	3688	3690	rBB2	21800	15182	0.32%	0.028%
114	24.804	3690	3692	3695	rBB4	21444	16258	0.35%	0.030%
115	24.874	3695	3704	3710	rBB5	283883	635811	13.56%	1.191%
116	24.968	3718	3720	3722	rBB3	35851	15802	0.34%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014868.D
 Acq On : 10 Jun 2021 19:02
 Operator : CG/JU
 Sample : PB136853BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK853

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

117	25.057	3731	3735	3740	rBB8	27732	58068	1.24%	0.109%
118	25.115	3743	3745	3747	rBB3	23449	16544	0.35%	0.031%
119	25.139	3747	3749	3751	rBB3	20813	16532	0.35%	0.031%
120	25.162	3751	3753	3756	rBB4	21823	19531	0.42%	0.037%
121	25.192	3756	3758	3761	rBB4	18974	19032	0.41%	0.036%
122	25.233	3763	3765	3768	rBB4	34240	26658	0.57%	0.050%
123	25.310	3773	3778	3779	rBB5	14436	27742	0.59%	0.052%
124	25.327	3779	3781	3783	rBB3	18463	17909	0.38%	0.034%
125	25.386	3790	3791	3793	rBB2	50489	27872	0.59%	0.052%
126	25.404	3793	3794	3798	rBB4	40511	27382	0.58%	0.051%
127	25.433	3798	3799	3801	rBB2	41454	26557	0.57%	0.050%
128	25.462	3801	3804	3806	rBB4	30341	25130	0.54%	0.047%
129	25.598	3825	3827	3830	rBB4	21220	16558	0.35%	0.031%
130	25.645	3830	3835	3839	rBB8	23704	35523	0.76%	0.067%
131	25.715	3842	3847	3848	rBB5	15827	25985	0.55%	0.049%
132	25.757	3848	3854	3860	rBB9	172912	412765	8.80%	0.773%
133	25.857	3869	3871	3872	rBB2	16729	14398	0.31%	0.027%
134	25.892	3876	3877	3879	rBB2	24404	15201	0.32%	0.028%
135	25.915	3879	3881	3883	rBB3	29836	21829	0.47%	0.041%
136	26.092	3908	3911	3914	rBB5	18882	17775	0.38%	0.033%
137	26.133	3914	3918	3921	rBB6	28555	29872	0.64%	0.056%
138	26.357	3952	3956	3960	rBB7	41436	53933	1.15%	0.101%
139	26.392	3960	3962	3966	rBB5	42168	38263	0.82%	0.072%
140	26.492	3976	3979	3982	rBB5	14241	17633	0.38%	0.033%
141	26.533	3984	3986	3988	rBB3	23281	14435	0.31%	0.027%
142	26.562	3989	3991	3994	rBB4	29159	23606	0.50%	0.044%
143	26.604	3994	3998	3999	rBB4	22885	38056	0.81%	0.071%
144	26.651	4004	4006	4008	rBB3	32994	16929	0.36%	0.032%
145	26.674	4008	4010	4012	rBB3	24387	15910	0.34%	0.030%
146	26.692	4012	4013	4015	rBB2	29549	15740	0.34%	0.029%
147	26.792	4020	4030	4040	rBB2	161074	530013	11.30%	0.993%
148	26.868	4040	4043	4044	rBB3	46011	25314	0.54%	0.047%
149	26.886	4044	4046	4048	rBB3	17443	20620	0.44%	0.039%
150	26.921	4051	4052	4054	rBB2	34352	16510	0.35%	0.031%
151	26.968	4054	4060	4062	rBB7	24090	49276	1.05%	0.092%
152	26.986	4062	4063	4066	rBB3	21047	17245	0.37%	0.032%
153	27.021	4068	4069	4073	rBB4	33904	27639	0.59%	0.052%
154	27.051	4073	4074	4076	rBB2	30572	14618	0.31%	0.027%
155	27.098	4081	4082	4085	rBB3	30311	16447	0.35%	0.031%
156	27.162	4091	4093	4096	rBB4	33181	31704	0.68%	0.059%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014868.D
 Acq On : 10 Jun 2021 19:02
 Operator : CG/JU
 Sample : PB136853BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK853

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

157	27.192	4096	4098	4099	rBB2	32342	18620	0.40%	0.035%
158	27.221	4102	4103	4105	rBB2	19055	16884	0.36%	0.032%
159	27.256	4107	4109	4112	rBB4	25320	21006	0.45%	0.039%
160	27.327	4118	4121	4122	rBB3	27620	15418	0.33%	0.029%
161	27.345	4122	4124	4126	rBB3	31991	24307	0.52%	0.046%
162	27.404	4130	4134	4135	rBB4	24859	24835	0.53%	0.047%
163	27.427	4135	4138	4141	rBB5	26364	24887	0.53%	0.047%
164	27.451	4141	4142	4144	rBB2	49301	23186	0.49%	0.043%
165	27.504	4147	4151	4152	rBB4	16345	21311	0.45%	0.040%
166	27.562	4160	4161	4166	rBB5	15616	22401	0.48%	0.042%
167	27.709	4184	4186	4187	rBB2	30753	23135	0.49%	0.043%
168	27.721	4187	4188	4191	rBB3	34661	18349	0.39%	0.034%
169	27.762	4193	4195	4198	rBB4	36953	20352	0.43%	0.038%
170	27.898	4215	4218	4220	rBB4	27544	32170	0.69%	0.060%
171	28.009	4233	4237	4239	rBB5	27354	54971	1.17%	0.103%
172	28.027	4239	4240	4246	rBB6	39759	61271	1.31%	0.115%
173	28.068	4246	4247	4250	rBB3	44731	21190	0.45%	0.040%
174	28.098	4250	4252	4253	rBB2	33166	18943	0.40%	0.035%
175	28.121	4255	4256	4258	rBB2	23958	17513	0.37%	0.033%
176	28.162	4260	4263	4264	rBB3	11216	14472	0.31%	0.027%
177	28.198	4266	4269	4271	rBB4	26257	25844	0.55%	0.048%
178	28.227	4271	4274	4275	rBB3	39678	22769	0.49%	0.043%
179	28.380	4298	4300	4301	rBB2	28825	19265	0.41%	0.036%
180	28.403	4301	4304	4307	rBB5	27799	23482	0.50%	0.044%
181	28.456	4311	4313	4315	rBB3	21817	18756	0.40%	0.035%
182	28.503	4320	4321	4324	rBB3	23854	18945	0.40%	0.035%
183	28.539	4326	4327	4330	rBB3	38545	24354	0.52%	0.046%
184	28.574	4330	4333	4334	rBB3	27074	23985	0.51%	0.045%
185	28.645	4340	4345	4346	rBB5	39510	31000	0.66%	0.058%
186	28.709	4354	4356	4361	rBB6	31378	35331	0.75%	0.066%
187	28.745	4361	4362	4364	rBB2	27257	16875	0.36%	0.032%
188	28.809	4367	4373	4374	rBB6	25956	37486	0.80%	0.070%
189	28.856	4379	4381	4384	rBB4	24155	21863	0.47%	0.041%
190	28.909	4386	4390	4392	rBB5	16583	23675	0.50%	0.044%
191	28.945	4394	4396	4398	rBB3	21782	17335	0.37%	0.032%
192	28.974	4398	4401	4403	rBB4	21303	22196	0.47%	0.042%
193	29.009	4403	4407	4408	rBB4	28353	34287	0.73%	0.064%
194	29.056	4412	4415	4419	rBB6	37521	44340	0.95%	0.083%
195	29.127	4424	4427	4432	rBB7	37649	59534	1.27%	0.111%
196	29.162	4432	4433	4436	rBB3	27971	21645	0.46%	0.041%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014868.D
Acq On : 10 Jun 2021 19:02
Operator : CG/JU
Sample : PB136853BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK853

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Title : SVOA CALIBRATION

197	29.186	4436	4437	4441	rBB4	30993	15368	0.33%	0.029%
198	29.215	4441	4442	4446	rBB4	26411	15249	0.33%	0.029%
199	29.298	4454	4456	4458	rBB3	23836	15947	0.34%	0.030%
200	29.345	4461	4464	4469	rBB7	41213	61303	1.31%	0.115%




Sum of corrected areas: 53395765

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014868.D
Acq On : 10 Jun 2021 19:02
Operator : CG/JU
Sample : PB136853BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK853

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

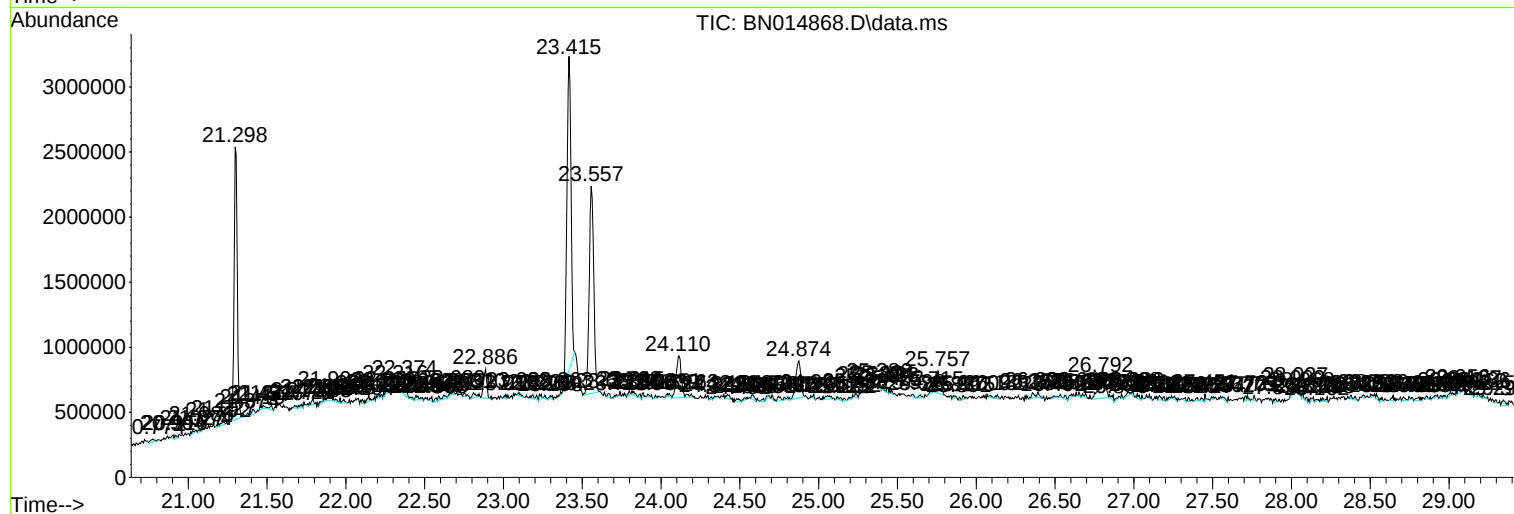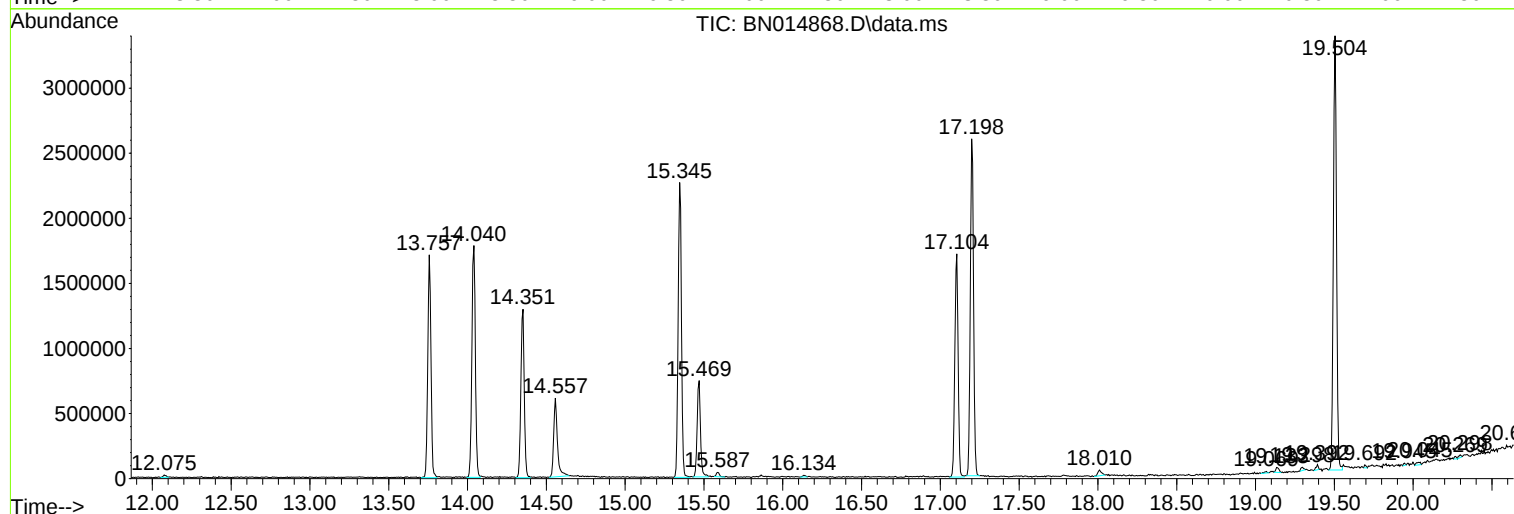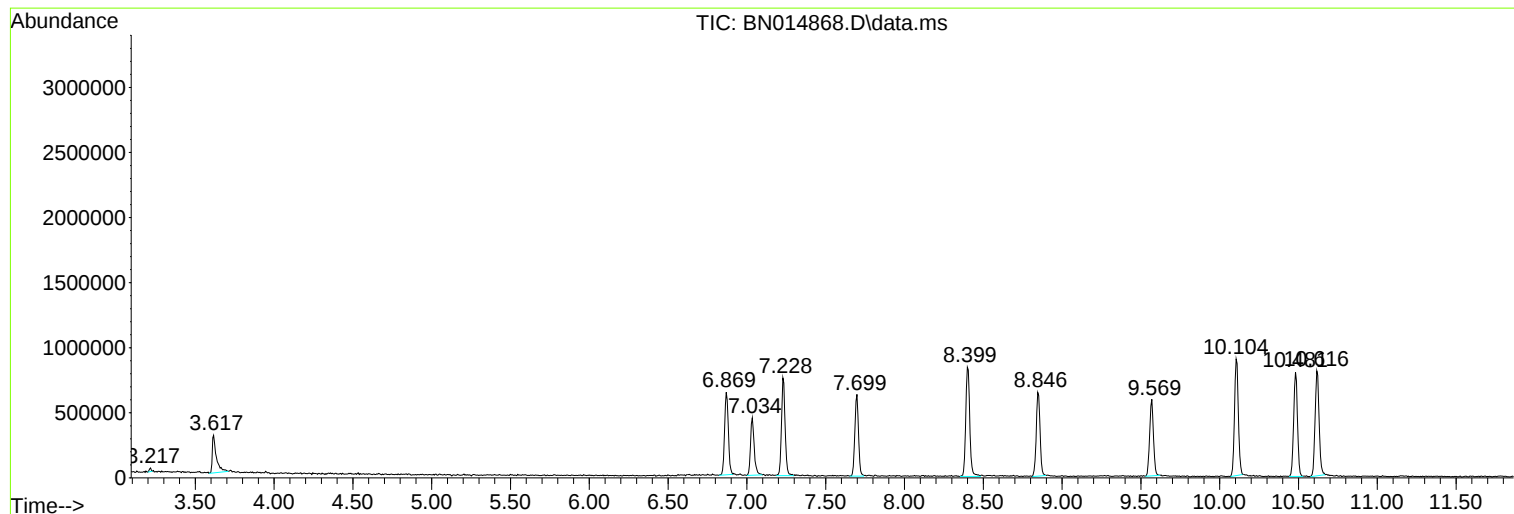

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014868.D
Acq On : 10 Jun 2021 19:02
Operator : CG/JU
Sample : PB136853BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK853










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
24.110	4.38 ng/ul	691509	Perylene-d12	23.563

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Pentacosane	352	C25H52	000629-99-2	91
2		Heneicosane	296	C21H44	000629-94-7	91
3		Hexacosane	366	C26H54	000630-01-3	81
4		Heneicosane	296	C21H44	000629-94-7	81
5		Heptacosane	380	C27H56	000593-49-7	78

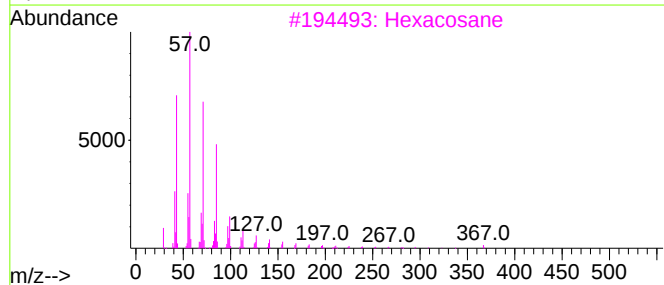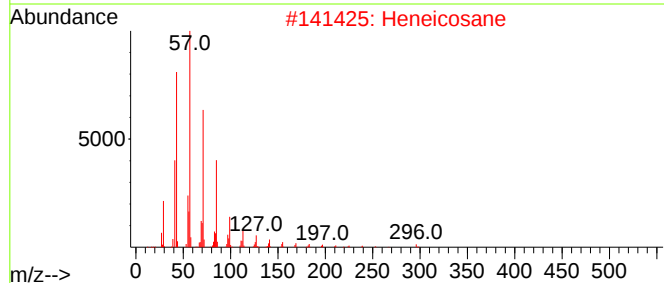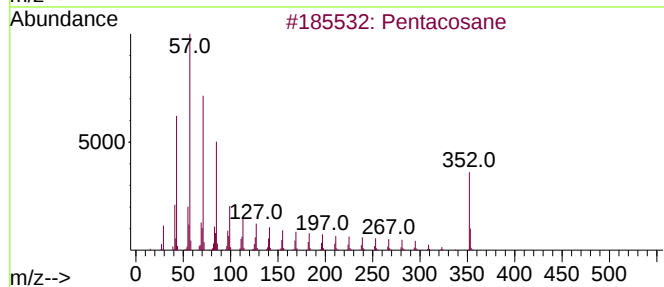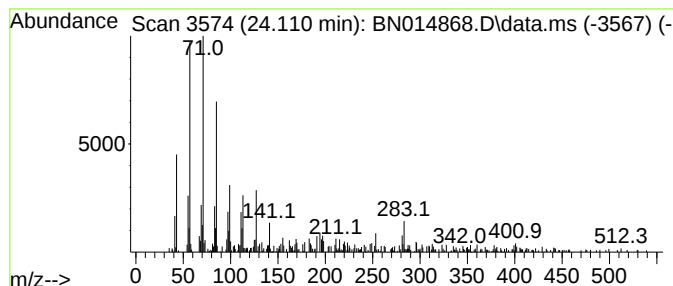

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014868.D
Acq On : 10 Jun 2021 19:02
Operator : CG/JU
Sample : PB136853BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK853










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
24.874	4.03 ng/ul	635811	Perylene-d12	23.563

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Docosane	310	C22H46	000629-97-0	90
2			Octacosane	394	C28H58	000630-02-4	89
3			Pentacosane	352	C25H52	000629-99-2	89
4			Heptacosane	380	C27H56	000593-49-7	68
5			Tetratetracontane	619	C44H90	007098-22-8	64

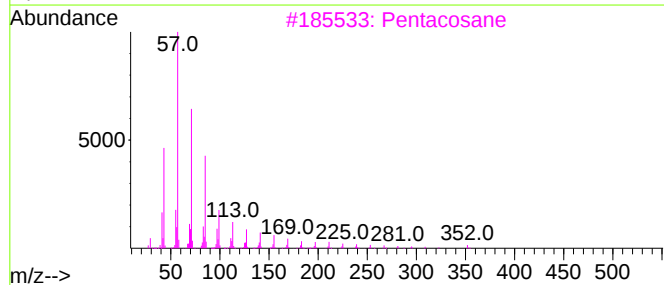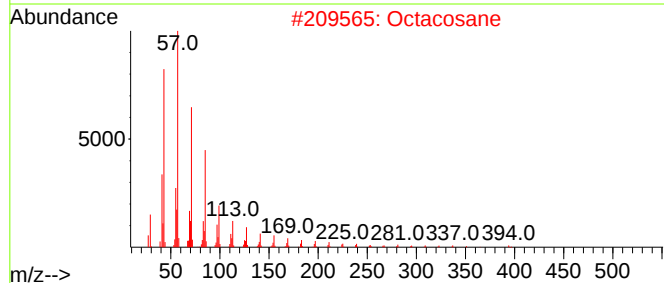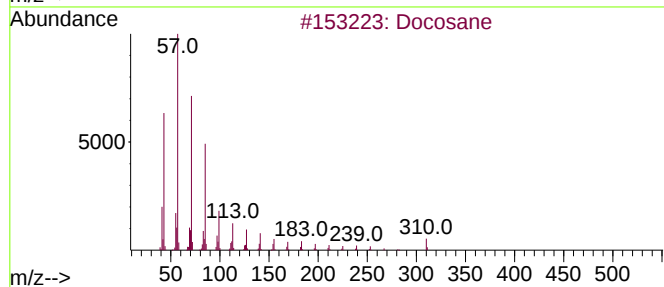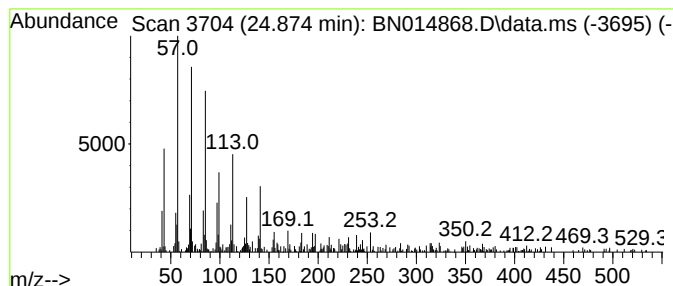

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014868.D
Acq On : 10 Jun 2021 19:02
Operator : CG/JU
Sample : PB136853BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK853










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 (DEL) Alkane: Straight-Chai... Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
25.757	2.62 ng/ul	412765	Perylene-d12	23.563

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tricosane	324	C23H48	000638-67-5	93
2			Hexacosane	366	C26H54	000630-01-3	93
3			Docosane	310	C22H46	000629-97-0	93
4			Tricosane	324	C23H48	000638-67-5	93
5			Docosane	310	C22H46	000629-97-0	90

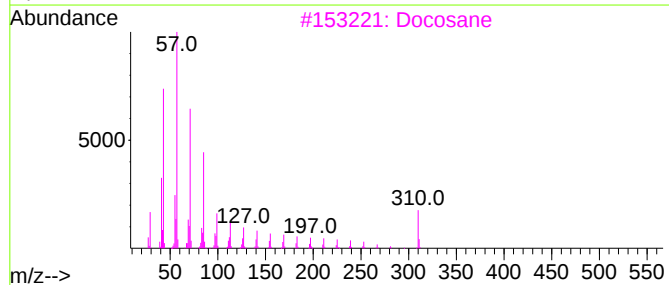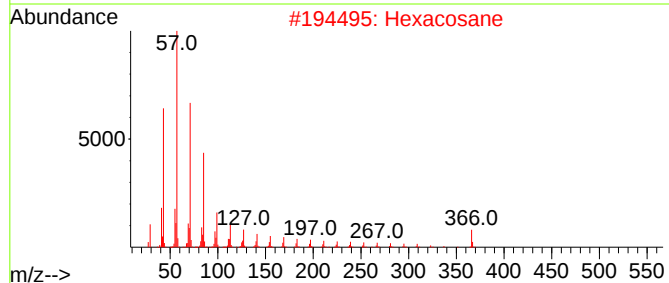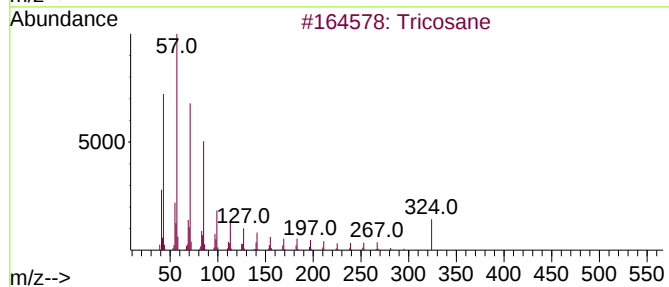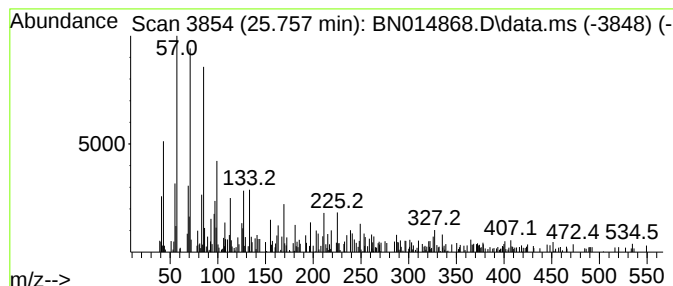

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014868.D
Acq On : 10 Jun 2021 19:02
Operator : CG/JU
Sample : PB136853BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK853










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 (DEL) Alkane: Straight-Chai... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
26.792	3.36 ng/ul	530013	Perylene-d12	23.563

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexadecane	226	C16H34	000544-76-3	90
2			Dotriacontane	451	C32H66	000544-85-4	86
3			Hexacosane	366	C26H54	000630-01-3	81
4			Hexadecane, 1-iodo-	352	C16H33I	000544-77-4	81
5			Pentadecane	212	C15H32	000629-62-9	76

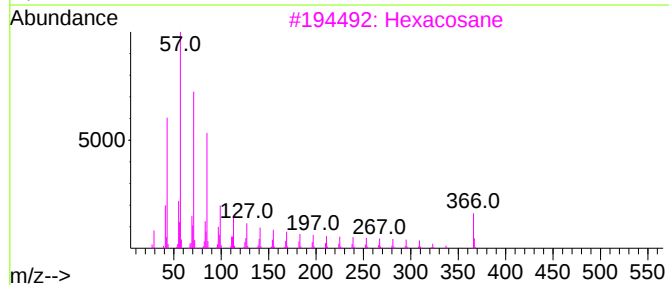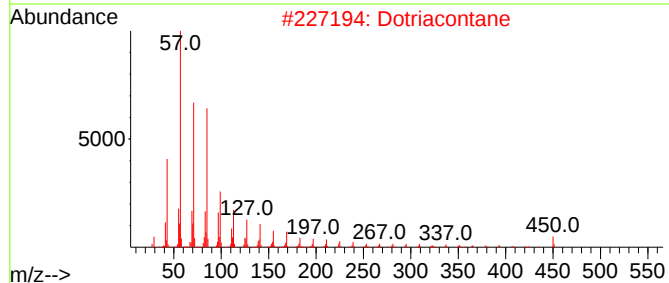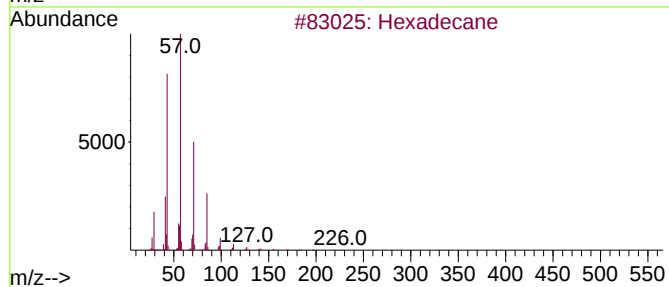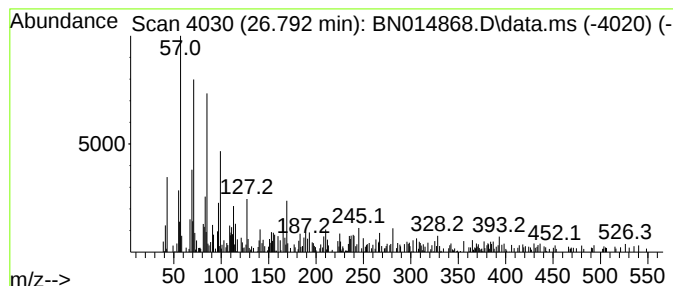

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014868.D
Acq On : 10 Jun 2021 19:02
Operator : CG/JU
Sample : PB136853BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK853

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	24.110	4.4	ng/ul	691509	6	23.563	3156860	20.0
(DEL) Alkane: S...	24.874	4.0	ng/ul	635811	6	23.563	3156860	20.0
(DEL) Alkane: S...	25.757	2.6	ng/ul	412765	6	23.563	3156860	20.0
(DEL) Alkane: S...	26.792	3.4	ng/ul	530013	6	23.563	3156860	20.0