

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014871.D
 Acq On : 10 Jun 2021 20:50
 Operator : CG/JU
 Sample : M2618-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG5R8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014871.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	18	22	25	rBB5	29944	33296	0.86%	0.087%
2	3.846	124	129	134	rBB3	35396	54047	1.40%	0.141%
3	3.934	142	144	151	rBB7	14369	21356	0.55%	0.056%
4	4.828	293	296	302	rBB	37977	52793	1.37%	0.138%
5	6.093	508	511	516	rBB7	11966	18229	0.47%	0.048%
6	6.869	636	643	652	rBB	432801	714464	18.56%	1.869%
7	7.034	666	671	682	rVB	294340	487078	12.65%	1.274%
8	7.228	697	704	712	rVB	513482	803852	20.88%	2.103%
9	7.693	777	783	791	rBV2	322264	499939	12.99%	1.308%
10	8.399	897	903	910	rBB2	568497	902065	23.43%	2.360%
11	8.846	970	979	987	rBB	449962	737780	19.16%	1.930%
12	9.563	1095	1101	1111	rVB2	376935	678492	17.62%	1.775%
13	10.105	1184	1193	1205	rBV	623239	1096565	28.48%	2.869%
14	10.481	1250	1257	1263	rBB	383035	639230	16.60%	1.672%
15	10.616	1271	1280	1295	rBB2	515957	965671	25.08%	2.527%
16	13.757	1807	1814	1825	rBV	1121669	1595804	41.45%	4.175%
17	14.040	1852	1862	1870	rBV	1139616	1804866	46.88%	4.722%
18	14.345	1906	1914	1921	rBV2	657359	951668	24.72%	2.490%
19	14.557	1945	1950	1960	rBB	301101	541719	14.07%	1.417%
20	15.163	2049	2053	2062	rBB8	10083	24984	0.65%	0.065%
21	15.345	2076	2084	2090	rBV	1546035	2250132	58.44%	5.887%
22	15.392	2090	2092	2097	rBB4	15299	21889	0.57%	0.057%
23	15.463	2099	2104	2114	rBV2	406218	604986	15.71%	1.583%
24	15.587	2121	2125	2131	rBB6	17391	31817	0.83%	0.083%
25	15.851	2163	2170	2176	rBB7	23096	43728	1.14%	0.114%
26	16.922	2348	2352	2357	rBB5	15808	23584	0.61%	0.062%
27	17.098	2377	2382	2386	rBB	799128	1094235	28.42%	2.863%
28	17.139	2386	2389	2393	rBB	213248	244615	6.35%	0.640%
29	17.198	2393	2399	2410	rVB2	1807614	2653073	68.91%	6.941%
30	17.298	2413	2416	2421	rBB7	23256	22992	0.60%	0.060%
31	18.028	2533	2540	2545	rBB8	52400	92775	2.41%	0.243%
32	18.104	2548	2553	2556	rBB6	17527	19244	0.50%	0.050%
33	18.175	2559	2565	2569	rBB2	53133	74611	1.94%	0.195%
34	18.486	2614	2618	2621	rBB	34290	44881	1.17%	0.117%
35	18.733	2656	2660	2663	rBB6	19158	19906	0.52%	0.052%
36	18.910	2685	2690	2695	rBB7	27168	43338	1.13%	0.113%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014871.D
 Acq On : 10 Jun 2021 20:50
 Operator : CG/JU
 Sample : M2618-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG5R8

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

37	19.169	2726	2734	2741	rBV	443674	622903	16.18%	1.630%
38	19.304	2750	2757	2761	rBB9	23360	39757	1.03%	0.104%
39	19.386	2765	2771	2777	rBB10	19152	48904	1.27%	0.128%
40	19.504	2785	2791	2802	rBV2	2309633	3850051	100.00%	10.073%

41	19.604	2804	2808	2812	rVB5	27033	41633	1.08%	0.109%
42	19.710	2821	2826	2828	rBB5	20726	26638	0.69%	0.070%
43	19.780	2833	2838	2841	rBB7	19463	35392	0.92%	0.093%
44	19.857	2848	2851	2854	rBB4	23317	22546	0.59%	0.059%
45	20.033	2874	2881	2884	rBB3	49307	68100	1.77%	0.178%

46	20.128	2895	2897	2901	rBB5	39461	45052	1.17%	0.118%
47	20.186	2903	2907	2912	rBB7	47696	72972	1.90%	0.191%
48	20.280	2919	2923	2927	rBB6	16672	27804	0.72%	0.073%
49	20.328	2927	2931	2933	rBB5	36591	38094	0.99%	0.100%
50	20.375	2936	2939	2942	rBB4	26305	34140	0.89%	0.089%

51	20.410	2943	2945	2948	rBB4	20300	21685	0.56%	0.057%
52	20.627	2979	2982	2985	rBB5	24033	28847	0.75%	0.075%
53	20.733	2997	3000	3002	rBB4	22551	19411	0.50%	0.051%
54	20.775	3002	3007	3008	rBB5	19594	29254	0.76%	0.077%
55	20.951	3028	3037	3039	rBB8	45647	81202	2.11%	0.212%

56	20.986	3039	3043	3044	rBB4	17266	22430	0.58%	0.059%
57	21.033	3046	3051	3053	rBB6	53133	77718	2.02%	0.203%
58	21.080	3055	3059	3064	rBB8	42043	76986	2.00%	0.201%
59	21.298	3089	3096	3100	rBB2	1189939	1716271	44.58%	4.490%
60	21.333	3100	3102	3107	rBB2	130319	127040	3.30%	0.332%

61	21.416	3112	3116	3118	rBB5	19028	25863	0.67%	0.068%
62	21.457	3120	3123	3127	rBB6	61917	57525	1.49%	0.151%
63	21.610	3147	3149	3153	rBB5	26814	26904	0.70%	0.070%
64	21.674	3156	3160	3164	rBB7	43398	47534	1.23%	0.124%
65	21.727	3164	3169	3170	rBB5	18998	19398	0.50%	0.051%

66	21.798	3180	3181	3183	rBB2	32288	21748	0.56%	0.057%
67	21.857	3188	3191	3194	rBB5	28600	34846	0.91%	0.091%
68	21.904	3194	3199	3201	rBB6	62356	87960	2.28%	0.230%
69	21.969	3206	3210	3211	rBV4	19121	24387	0.63%	0.064%
70	22.004	3215	3216	3220	rBB4	37735	18808	0.49%	0.049%

71	22.045	3220	3223	3227	rBB6	35026	54348	1.41%	0.142%
72	22.086	3227	3230	3232	rBB4	43928	45150	1.17%	0.118%
73	22.204	3248	3250	3254	rBB5	31047	18893	0.49%	0.049%
74	22.245	3254	3257	3258	rBB3	17451	20439	0.53%	0.053%
75	22.274	3260	3262	3265	rBB4	32451	29760	0.77%	0.078%

76	22.369	3273	3278	3282	rBB8	109026	156497	4.06%	0.409%
----	--------	------	------	------	------	--------	--------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014871.D
 Acq On : 10 Jun 2021 20:50
 Operator : CG/JU
 Sample : M2618-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG5R8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

77	22.457	3289	3293	3296	rBB6	57800	78675	2.04%	0.206%
78	22.498	3296	3300	3301	rBB4	16467	18166	0.47%	0.048%
79	22.574	3311	3313	3317	rBB5	16047	23517	0.61%	0.062%
80	22.627	3317	3322	3323	rBB5	26306	26438	0.69%	0.069%
81	22.763	3344	3345	3348	rBB3	33026	27190	0.71%	0.071%
82	22.880	3359	3365	3370	rBB3	298770	503652	13.08%	1.318%
83	23.057	3392	3395	3398	rBB5	45928	32635	0.85%	0.085%
84	23.092	3398	3401	3403	rBB4	59235	48615	1.26%	0.127%
85	23.174	3411	3415	3416	rBB4	28795	30258	0.79%	0.079%
86	23.204	3416	3420	3423	rBB6	30436	46813	1.22%	0.122%
87	23.357	3441	3446	3449	rBB5	50849	87746	2.28%	0.230%
88	23.416	3449	3456	3461	rBB	1642354	3044567	79.08%	7.966%
89	23.451	3461	3462	3467	rBB3	156610	170950	4.44%	0.447%
90	23.551	3472	3479	3486	rBB2	938299	1758817	45.68%	4.602%
91	23.610	3486	3489	3491	rBB4	24487	29872	0.78%	0.078%
92	23.627	3491	3492	3498	rBB6	32064	33048	0.86%	0.086%
93	23.680	3498	3501	3502	rBB3	38839	20222	0.53%	0.053%
94	23.769	3514	3516	3520	rBB5	15646	18065	0.47%	0.047%
95	23.833	3522	3527	3529	rBB6	37667	44625	1.16%	0.117%
96	23.886	3532	3536	3537	rBV4	25350	18835	0.49%	0.049%
97	23.921	3540	3542	3546	rBB5	23529	27551	0.72%	0.072%
98	24.027	3559	3560	3563	rBB3	20168	17991	0.47%	0.047%
99	24.116	3568	3575	3581	rBB3	316248	650165	16.89%	1.701%
100	24.180	3585	3586	3588	rBB2	37045	18807	0.49%	0.049%
101	24.304	3602	3607	3608	rBB5	17637	32224	0.84%	0.084%
102	24.374	3614	3619	3622	rBB7	27139	38477	1.00%	0.101%
103	24.404	3622	3624	3627	rBB4	18958	20066	0.52%	0.052%
104	24.451	3627	3632	3634	rBB6	29640	45550	1.18%	0.119%
105	24.480	3636	3637	3640	rBB3	42868	20865	0.54%	0.055%
106	24.510	3640	3642	3646	rBB5	37705	29106	0.76%	0.076%
107	24.580	3653	3654	3658	rBB4	25180	23097	0.60%	0.060%
108	24.721	3676	3678	3682	rBB5	33821	26769	0.70%	0.070%
109	24.786	3685	3689	3692	rBB6	27825	34391	0.89%	0.090%
110	24.810	3692	3693	3695	rBV2	41908	23360	0.61%	0.061%
111	24.863	3695	3702	3713	rBB5	312729	758852	19.71%	1.985%
112	24.957	3716	3718	3723	rBB6	24547	25201	0.65%	0.066%
113	24.992	3723	3724	3726	rBB2	37332	18601	0.48%	0.049%
114	25.133	3744	3748	3750	rBB5	31054	31537	0.82%	0.083%
115	25.180	3751	3756	3758	rBB6	28406	31918	0.83%	0.084%
116	25.221	3760	3763	3766	rBB5	18437	26433	0.69%	0.069%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014871.D
 Acq On : 10 Jun 2021 20:50
 Operator : CG/JU
 Sample : M2618-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG5R8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

117	25.263	3766	3770	3772	rBB5	35957	42838	1.11%	0.112%
118	25.315	3777	3779	3780	rBB2	48035	21430	0.56%	0.056%
119	25.351	3783	3785	3786	rBB2	41200	20925	0.54%	0.055%
120	25.380	3788	3790	3793	rBB4	38829	22761	0.59%	0.060%
121	25.510	3809	3812	3815	rBB5	26557	28103	0.73%	0.074%
122	25.586	3822	3825	3827	rBB4	25848	32261	0.84%	0.084%
123	25.751	3845	3853	3861	rBV6	207986	572827	14.88%	1.499%
124	25.815	3861	3864	3865	rBB3	16685	26377	0.69%	0.069%
125	25.827	3865	3866	3871	rBB5	21614	24603	0.64%	0.064%
126	26.062	3904	3906	3909	rBB4	21409	18097	0.47%	0.047%
127	26.104	3911	3913	3916	rBB4	22386	20656	0.54%	0.054%
128	26.168	3921	3924	3925	rBB3	13561	21231	0.55%	0.056%
129	26.180	3925	3926	3931	rBB5	24464	23051	0.60%	0.060%
130	26.227	3933	3934	3937	rVB3	28517	18686	0.49%	0.049%
131	26.315	3945	3949	3951	rBB5	20422	22060	0.57%	0.058%
132	26.345	3951	3954	3956	rBB4	24330	24675	0.64%	0.065%
133	26.392	3960	3962	3965	rBB4	24173	18803	0.49%	0.049%
134	26.515	3980	3983	3984	rBB3	32239	24430	0.63%	0.064%
135	26.533	3984	3986	3988	rBB3	20449	22525	0.59%	0.059%
136	26.580	3991	3994	3995	rBB3	12435	19347	0.50%	0.051%
137	26.686	4011	4012	4016	rBB4	37163	21896	0.57%	0.057%
138	26.798	4022	4031	4036	rBB4	171717	456511	11.86%	1.194%
139	26.998	4063	4065	4067	rBB3	35481	24338	0.63%	0.064%
140	27.204	4098	4100	4104	rBB5	27585	30997	0.81%	0.081%
141	27.298	4112	4116	4118	rBB5	19821	30700	0.80%	0.080%
142	27.339	4120	4123	4127	rBB6	17119	22982	0.60%	0.060%
143	27.380	4127	4130	4131	rBB3	29096	18001	0.47%	0.047%
144	27.668	4176	4179	4180	rBB3	15267	24940	0.65%	0.065%
145	27.704	4180	4185	4186	rBB5	24059	21733	0.56%	0.057%
146	27.727	4186	4189	4191	rBB4	22906	19539	0.51%	0.051%
147	27.804	4200	4202	4205	rBB4	25381	25300	0.66%	0.066%
148	27.833	4205	4207	4208	rBB2	30286	24879	0.65%	0.065%
149	27.939	4223	4225	4227	rBB3	32947	19127	0.50%	0.050%
150	28.027	4230	4240	4244	rBB3	81597	253673	6.59%	0.664%
151	28.092	4248	4251	4254	rBB5	19248	18776	0.49%	0.049%
152	28.145	4259	4260	4262	rBB2	27130	18332	0.48%	0.048%
153	28.239	4273	4276	4280	rBB6	26250	33873	0.88%	0.089%
154	28.368	4295	4298	4304	rBB8	32029	47785	1.24%	0.125%
155	28.421	4304	4307	4310	rBB5	28541	28312	0.74%	0.074%
156	28.498	4319	4320	4324	rBB4	34543	28702	0.75%	0.075%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014871.D
 Acq On : 10 Jun 2021 20:50
 Operator : CG/JU
 Sample : M2618-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG5R8

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

157	28.533	4324	4326	4328	rBB3	29012	18704	0.49%	0.049%
158	28.580	4332	4334	4339	rBB6	25609	32452	0.84%	0.085%
159	28.692	4349	4353	4355	rBB5	12616	20284	0.53%	0.053%
160	28.821	4372	4375	4378	rBB5	28083	26142	0.68%	0.068%
161	28.927	4392	4393	4396	rBB2	26071	19537	0.51%	0.051%
162	28.974	4398	4401	4404	rBB5	30817	33255	0.86%	0.087%
163	29.004	4404	4406	4410	rBB5	23707	26316	0.68%	0.069%
164	29.151	4430	4431	4434	rBB3	33143	19878	0.52%	0.052%
165	29.180	4434	4436	4438	rBB3	28259	26749	0.69%	0.070%
166	29.233	4442	4445	4448	rBB5	39119	39781	1.03%	0.104%
167	29.321	4458	4460	4462	rBB3	27240	24038	0.62%	0.063%




Sum of corrected areas: 38221479

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014871.D
Acq On : 10 Jun 2021 20:50
Operator : CG/JU
Sample : M2618-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG5R8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

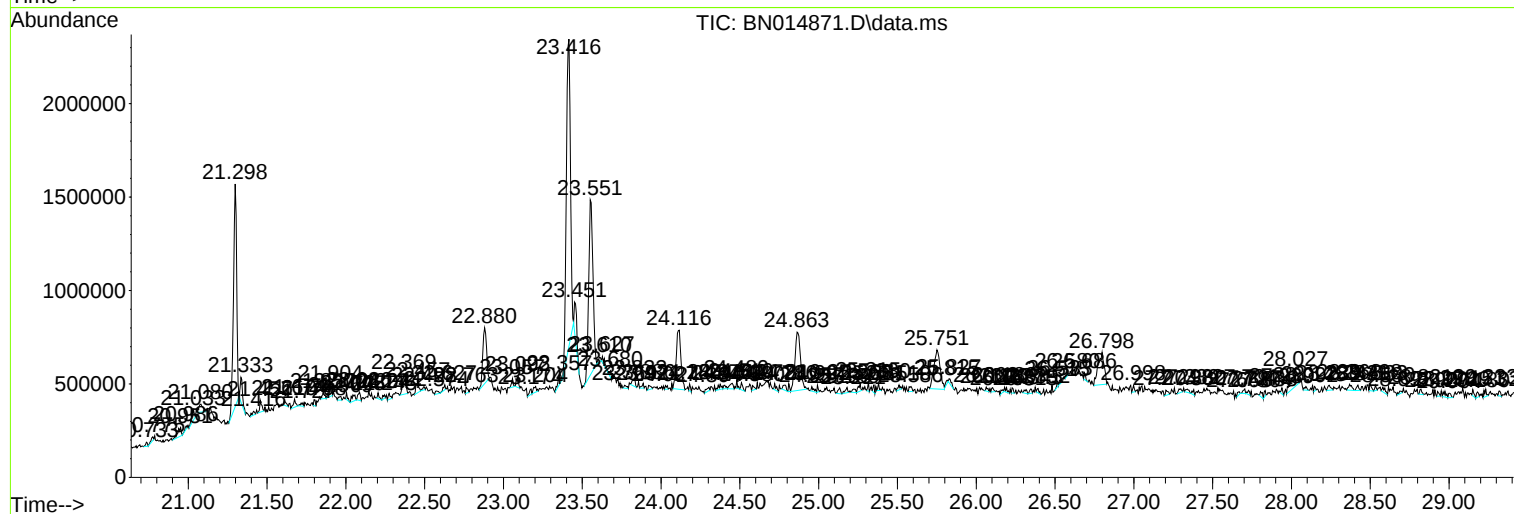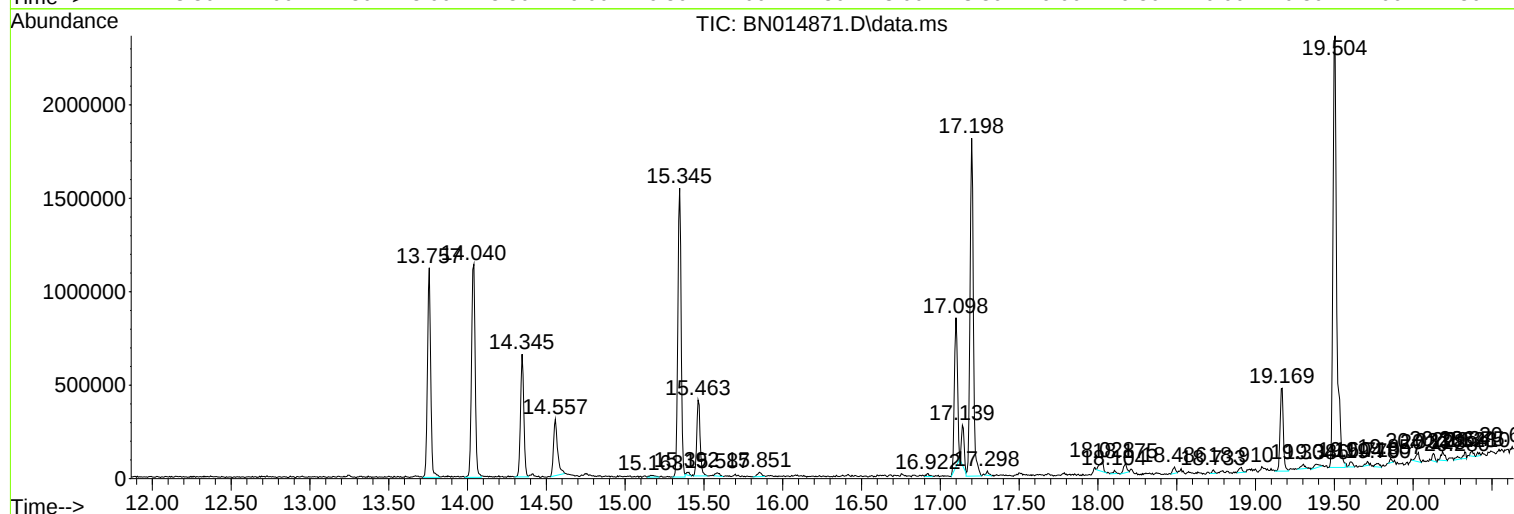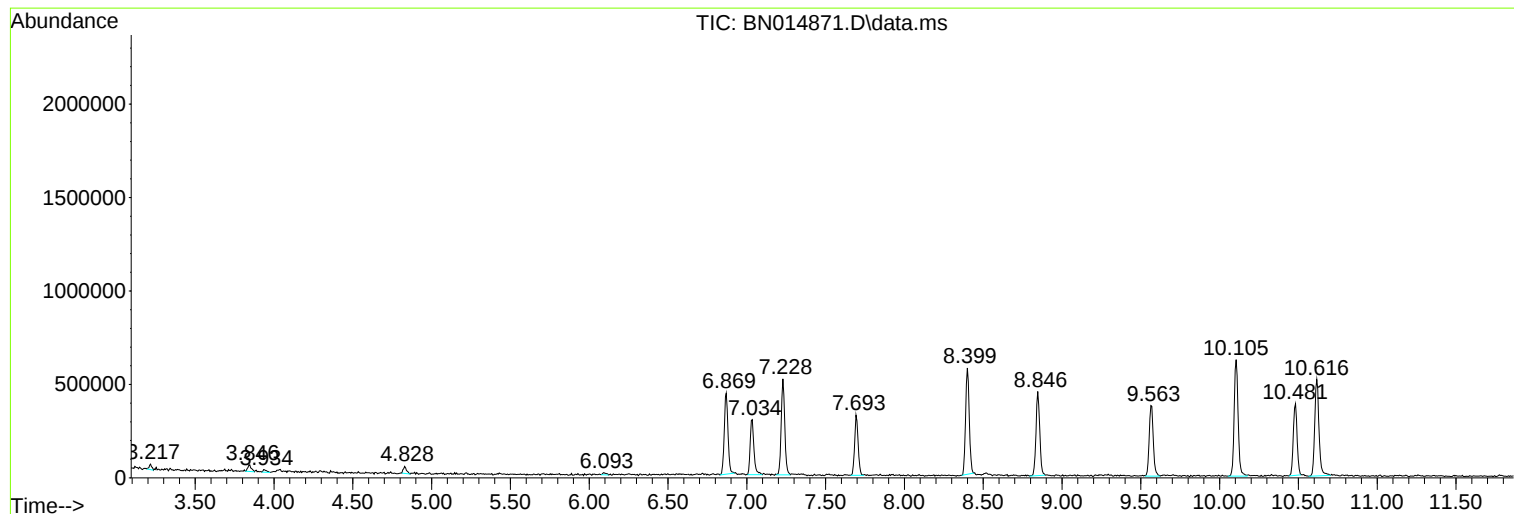

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014871.D
Acq On : 10 Jun 2021 20:50
Operator : CG/JU
Sample : M2618-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG5R8










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 6

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.846	2.16 ng/ul	54047	1,4-Dichlorobenzene-d4	7.699

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2,2-Dimethyl-5-[2-(2-trimethylsi...	318	C15H30O5Si	1000190-51-1	23		
2	N-Ethylformamide	73	C3H7NO	000627-45-2	9		
3	1-Dodecanamine	185	C12H27N	000124-22-1	9		
4	Cyclopentylcarboxylic acid	114	C6H10O2	003400-45-1	9		
5	2,7-Anhydro-1-galacto-heptulofur...	192	C7H12O6	1000126-01-5	9		

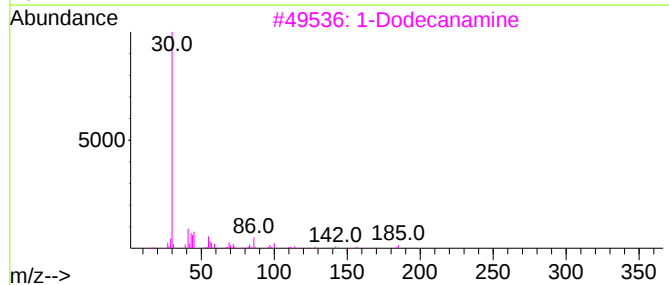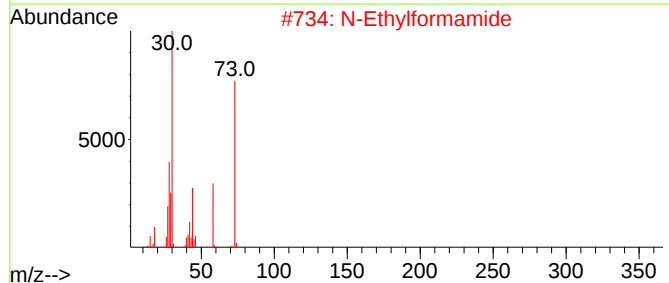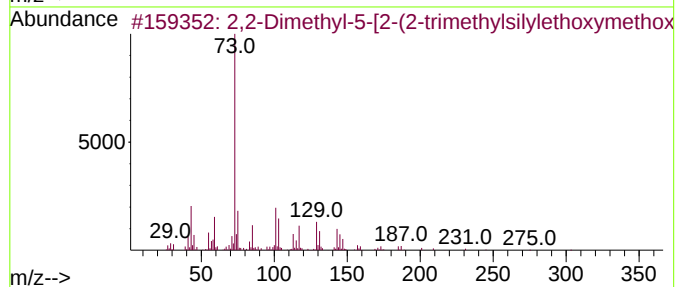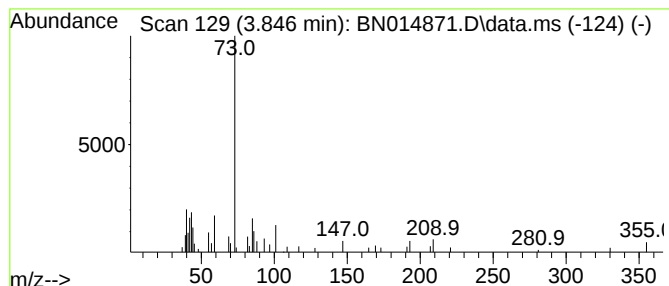

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014871.D
Acq On : 10 Jun 2021 20:50
Operator : CG/JU
Sample : M2618-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG5R8










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown-02 Concentration Rank 7

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.828	2.11 ng/ul	52793	1,4-Dichlorobenzene-d4	7.699

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,3-Dioxolane, 2-(1-methylethyl)-	116	C6H12O2	000822-83-3	9
2			1,3-Dioxolane, 2-(1-methylpropyl)-	130	C7H14O2	014447-25-7	9
3			1,3-Dioxolane, 2-(1-methylethyl)-	116	C6H12O2	000822-83-3	9
4			Pentanoic acid, 2-hydroxy-, ethy...	146	C7H14O3	006938-26-7	9
5			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	9

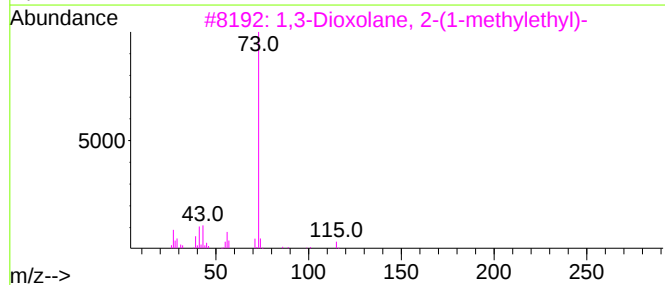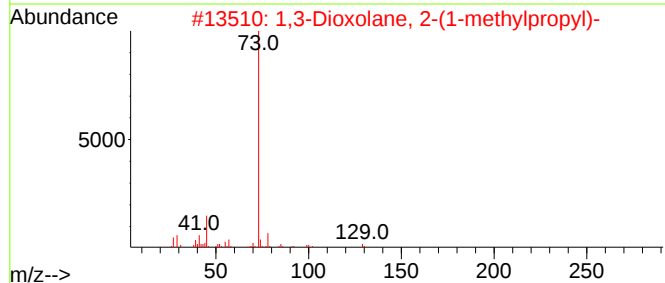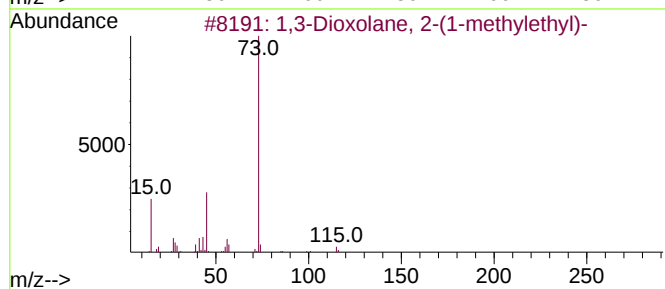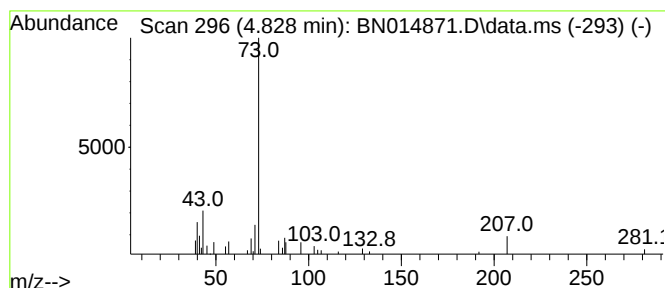

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014871.D
Acq On : 10 Jun 2021 20:50
Operator : CG/JU
Sample : M2618-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG5R8










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
24.116	7.39 ng/ul	650165	Perylene-d12	23.557

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Docosane	310	C22H46	000629-97-0	90
2			Disulfide, di-tert-dodecyl	402	C24H50S2	027458-90-8	53
3			Heptadecane	240	C17H36	000629-78-7	50
4			Octacosane	394	C28H58	000630-02-4	46
5			Hexadecane	226	C16H34	000544-76-3	43

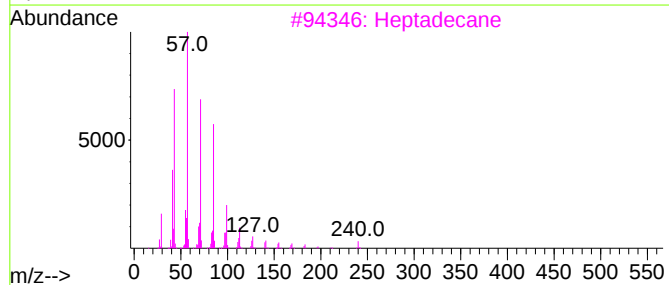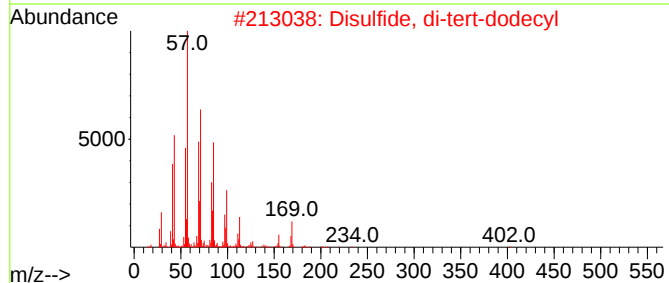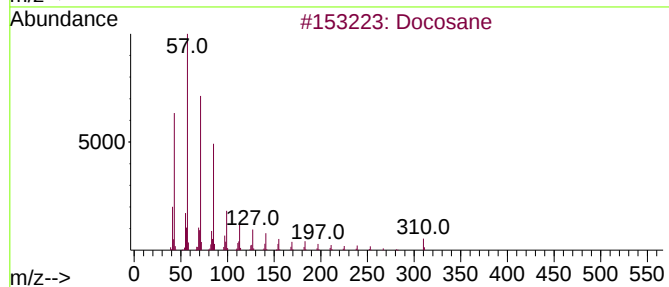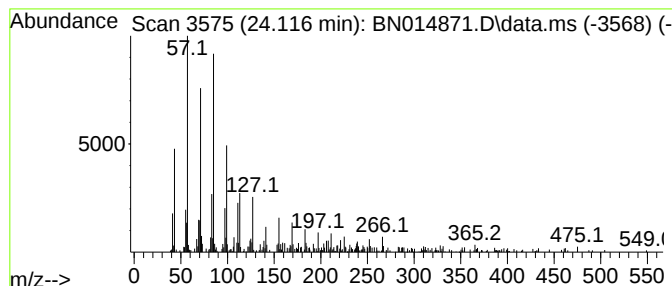

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014871.D
Acq On : 10 Jun 2021 20:50
Operator : CG/JU
Sample : M2618-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
BG5R8










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
24.863	8.63 ng/ul	758852	Perylene-d12	23.557

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triacontane	422	C30H62	000638-68-6	93
2			Octacosane	394	C28H58	000630-02-4	91
3			Hentriacontane	437	C31H64	000630-04-6	91
4			Eicosane, 10-hexyl-10-methyl-	380	C27H56	055282-32-1	90
5			Heptacosane	380	C27H56	000593-49-7	90

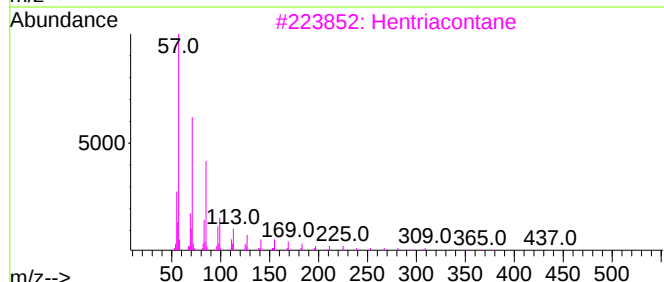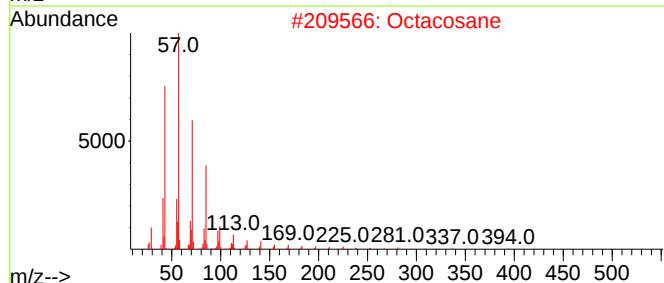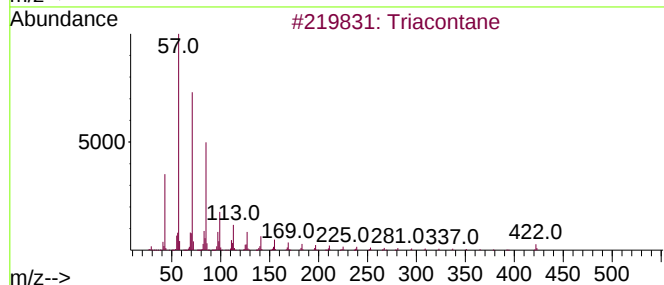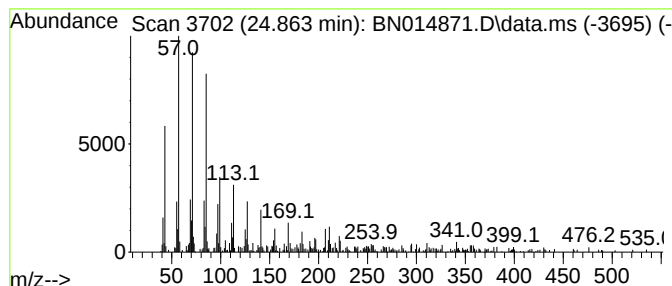

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014871.D
Acq On : 10 Jun 2021 20:50
Operator : CG/JU
Sample : M2618-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG5R8










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 (DEL) Alkane: Straight-Chai... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
25.751	6.51 ng/ul	572827	Perylene-d12	23.557

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetracosane	338	C24H50	000646-31-1	81
2			Hexadecane	226	C16H34	000544-76-3	81
3			Pentatriacontane	493	C35H72	000630-07-9	74
4			Hentriacontane	437	C31H64	000630-04-6	74
5			Tetracosane	338	C24H50	000646-31-1	72

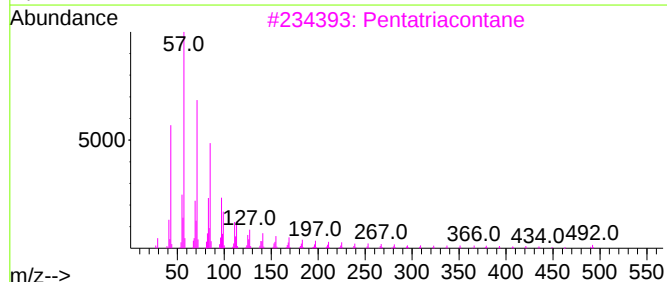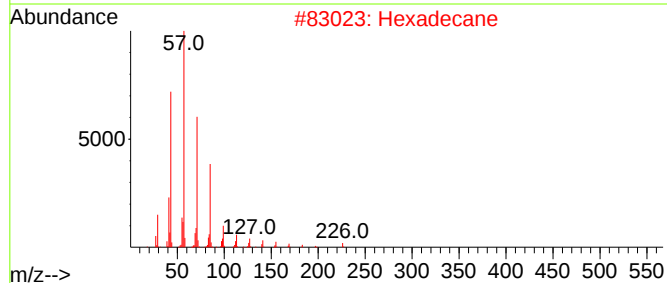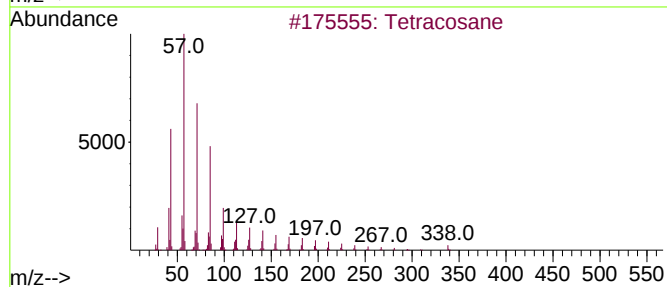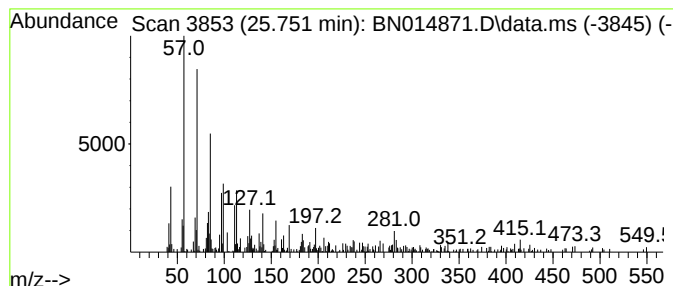

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014871.D
Acq On : 10 Jun 2021 20:50
Operator : CG/JU
Sample : M2618-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG5R8










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 6 Behenyl chloride Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
26.798	5.19 ng/ul	456511	Perylene-d12	23.557

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Behenyl chloride	344	C22H45Cl	042217-03-8	70
2			Docosane	310	C22H46	000629-97-0	62
3			Tetradecane, 2-methyl-	212	C15H32	001560-95-8	58
4			Eicosane	282	C20H42	000112-95-8	58
5			Tetradecane, 2,6,10-trimethyl-	240	C17H36	014905-56-7	49

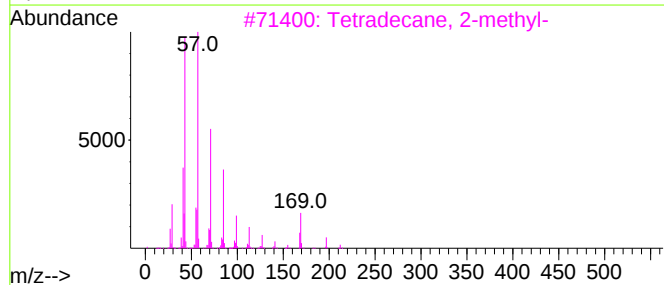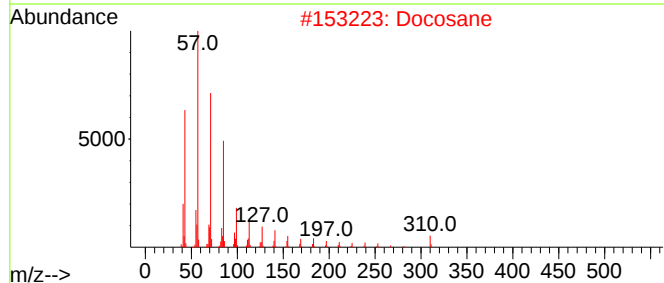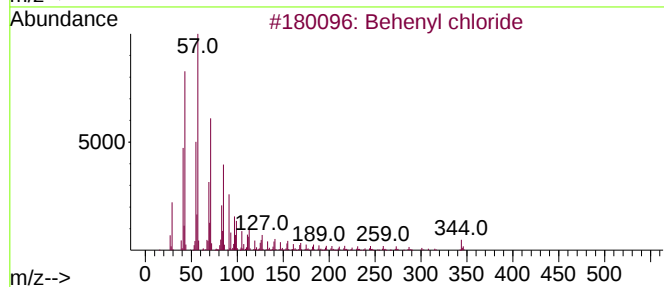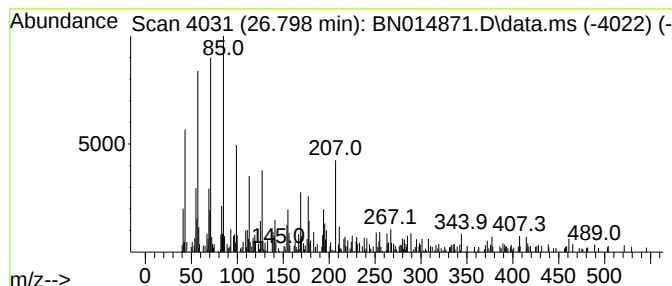

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014871.D
Acq On : 10 Jun 2021 20:50
Operator : CG/JU
Sample : M2618-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG5R8










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 7 unknown-03 Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
28.027	2.88 ng/ul	253673	Perylene-d12	23.557

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Trifluoperazine	407	C21H24F3N3S	000117-89-5	11
2			Eicosane, 10-butyl-10-propyl-	380	C27H56	055282-33-2	10
3			23-Methyl-tetracos-5,9-dienoic a...	431	C29H53NO	1000336-11-5	10
4			17,21-Dimethylheptatriacontane	549	C39H80	067979-79-7	9
5			1-Eicosanol, 2-hexadecyl-	523	C36H74O	017658-63-8	9

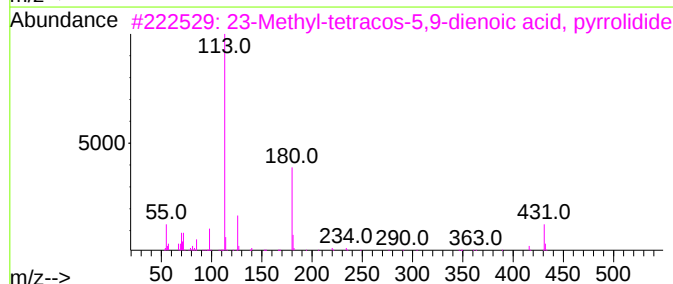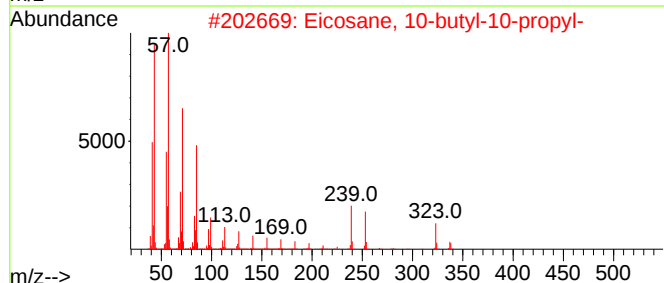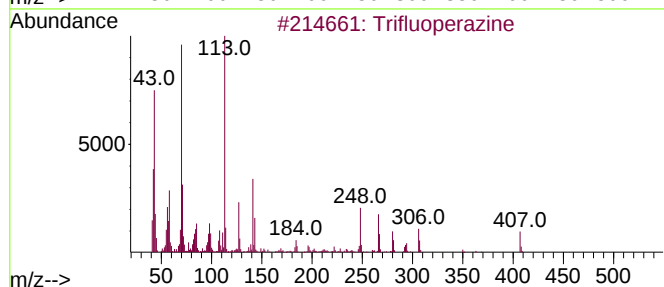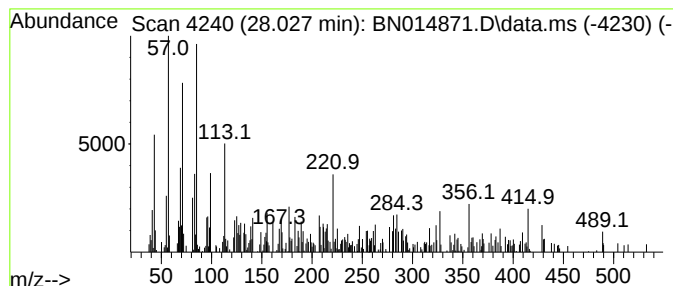

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014871.D
Acq On : 10 Jun 2021 20:50
Operator : CG/JU
Sample : M2618-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG5R8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	3.846	2.2	ng/ul	54047	1	7.699	499939	20.0
unknown-02	4.828	2.1	ng/ul	52793	1	7.699	499939	20.0
(DEL) Alkane: S...	24.116	7.4	ng/ul	650165	6	23.557	1758820	20.0
(DEL) Alkane: S...	24.863	8.6	ng/ul	758852	6	23.557	1758820	20.0
(DEL) Alkane: S...	25.751	6.5	ng/ul	572827	6	23.557	1758820	20.0
Behenyl chloride	26.798	5.2	ng/ul	456511	6	23.557	1758820	20.0
unknown-03	28.027	2.9	ng/ul	253673	6	23.557	1758820	20.0