

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014878.D
 Acq On : 11 Jun 2021 00:59
 Operator : CG/JU
 Sample : M2618-04DL 5X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG5R7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014878.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.834	294	297	303	rBV4	12059	17651	0.49%	0.058%
2	6.875	637	644	650	rBB2	142055	218918	6.03%	0.723%
3	7.034	666	671	679	rBV	88962	152194	4.19%	0.502%
4	7.228	698	704	715	rBB2	163337	269033	7.40%	0.888%
5	7.693	774	783	790	rBB	666202	1085002	29.86%	3.582%
6	8.405	897	904	910	rBB2	170210	280229	7.71%	0.925%
7	8.846	973	979	987	rBB	130196	229916	6.33%	0.759%
8	9.569	1093	1102	1109	rBB3	119606	216295	5.95%	0.714%
9	10.110	1187	1194	1202	rBB2	198375	346773	9.54%	1.145%
10	10.481	1250	1257	1266	rVB	862592	1470137	40.46%	4.853%
11	10.622	1272	1281	1288	rBB2	141312	267420	7.36%	0.883%
12	13.757	1808	1814	1820	rBB	351348	514562	14.16%	1.699%
13	14.034	1854	1861	1867	rBV	373204	562069	15.47%	1.856%
14	14.346	1907	1914	1923	rBV	1432917	2141470	58.94%	7.070%
15	14.569	1945	1952	1963	rBB4	55839	143689	3.95%	0.474%
16	15.345	2076	2084	2091	rBB	512580	757847	20.86%	2.502%
17	15.463	2099	2104	2114	rBB2	69903	112695	3.10%	0.372%
18	16.881	2341	2345	2350	rBB7	9597	16211	0.45%	0.054%
19	17.098	2376	2382	2388	rBB	1804028	2674257	73.61%	8.828%
20	17.198	2393	2399	2408	rVB	606468	850103	23.40%	2.806%
21	18.010	2534	2537	2544	rBB8	19958	41640	1.15%	0.137%
22	18.075	2544	2548	2551	rBB	23641	22118	0.61%	0.073%
23	18.910	2687	2690	2692	rBB4	18297	15864	0.44%	0.052%
24	19.163	2729	2733	2738	rBB	88335	113975	3.14%	0.376%
25	19.392	2768	2772	2773	rBB4	15799	14532	0.40%	0.048%
26	19.498	2784	2790	2801	rBB	840871	1257352	34.61%	4.151%
27	19.616	2806	2810	2812	rBB5	16319	18771	0.52%	0.062%
28	19.704	2822	2825	2828	rBB4	15726	20760	0.57%	0.069%
29	19.739	2828	2831	2834	rBB5	12273	18215	0.50%	0.060%
30	19.945	2864	2866	2870	rBB5	10058	12965	0.36%	0.043%
31	20.033	2877	2881	2883	rBB4	13599	14779	0.41%	0.049%
32	20.263	2917	2920	2922	rBB4	14010	13446	0.37%	0.044%
33	20.322	2925	2930	2933	rBB7	24777	44089	1.21%	0.146%
34	20.363	2933	2937	2939	rBB5	15914	18689	0.51%	0.062%
35	20.428	2947	2948	2952	rVB4	18120	16199	0.45%	0.053%
36	20.498	2954	2960	2963	rBB8	28679	36675	1.01%	0.121%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014878.D
 Acq On : 11 Jun 2021 00:59
 Operator : CG/JU
 Sample : M2618-04DL 5X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG5R7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

37	20.775	3002	3007	3012	rBB	1180253	1275325	35.10%	4.210%
38	20.863	3019	3022	3023	rBB3	13100	15698	0.43%	0.052%
39	20.980	3038	3042	3043	rBB4	23371	20085	0.55%	0.066%
40	20.992	3043	3044	3046	rBB2	27364	17028	0.47%	0.056%
41	21.016	3047	3048	3049	rBB	21098	14283	0.39%	0.047%
42	21.051	3052	3054	3056	rBB3	26462	18699	0.51%	0.062%
43	21.104	3060	3063	3065	rBB4	29175	25638	0.71%	0.085%
44	21.192	3075	3078	3080	rBB	1268909	1338433	36.84%	4.418%
45	21.298	3089	3096	3101	rBB	2581523	3412165	93.92%	11.264%
46	21.386	3109	3111	3113	rBB3	22807	12973	0.36%	0.043%
47	21.416	3113	3116	3117	rBB3	28338	21130	0.58%	0.070%
48	21.451	3119	3122	3125	rBB5	25997	32680	0.90%	0.108%
49	21.533	3132	3136	3140	rBB7	45755	80150	2.21%	0.265%
50	21.598	3143	3147	3149	rBB5	20260	18722	0.52%	0.062%
51	21.622	3149	3151	3153	rBB3	18778	17673	0.49%	0.058%
52	21.869	3185	3193	3194	rBB8	23174	36827	1.01%	0.122%
53	21.898	3194	3198	3203	rBB8	58211	60426	1.66%	0.199%
54	21.933	3203	3204	3207	rBB3	24735	16643	0.46%	0.055%
55	21.998	3212	3215	3217	rBB4	24773	13489	0.37%	0.045%
56	22.039	3217	3222	3228	rBB10	57140	115880	3.19%	0.383%
57	22.092	3228	3231	3233	rBB4	25898	25255	0.70%	0.083%
58	22.175	3243	3245	3247	rBB3	22214	17823	0.49%	0.059%
59	22.275	3260	3262	3266	rBB5	20326	21654	0.60%	0.071%
60	22.316	3266	3269	3270	rBB3	29782	22336	0.61%	0.074%
61	22.369	3270	3278	3282	rBB10	102361	175310	4.83%	0.579%
62	22.410	3282	3285	3288	rBB5	22526	22849	0.63%	0.075%
63	22.451	3288	3292	3293	rBB4	16222	13779	0.38%	0.045%
64	22.486	3296	3298	3299	rBB2	16987	13437	0.37%	0.044%
65	22.545	3305	3308	3309	rBB3	16747	19779	0.54%	0.065%
66	22.569	3309	3312	3314	rBB4	19127	17941	0.49%	0.059%
67	22.592	3314	3316	3318	rBB3	22553	12999	0.36%	0.043%
68	22.622	3318	3321	3322	rBB2	14163	14975	0.41%	0.049%
69	22.710	3334	3336	3338	rBB3	15197	16358	0.45%	0.054%
70	22.880	3359	3365	3371	rBB8	159122	292515	8.05%	0.966%
71	22.927	3371	3373	3378	rBB6	29733	30909	0.85%	0.102%
72	22.986	3381	3383	3385	rBB3	23944	16294	0.45%	0.054%
73	23.033	3388	3391	3395	rBB6	27968	31196	0.86%	0.103%
74	23.063	3395	3396	3399	rBB3	24128	15857	0.44%	0.052%
75	23.122	3404	3406	3407	rBB2	21886	13757	0.38%	0.045%
76	23.145	3407	3410	3413	rBB5	23322	29539	0.81%	0.098%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014878.D
 Acq On : 11 Jun 2021 00:59
 Operator : CG/JU
 Sample : M2618-04DL 5X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG5R7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

77	23.169	3413	3414	3416	rBB2	28300	13815	0.38%	0.046%
78	23.192	3416	3418	3420	rBB3	25461	23242	0.64%	0.077%
79	23.210	3420	3421	3424	rBB3	18091	13131	0.36%	0.043%
80	23.263	3429	3430	3435	rBB5	22960	19181	0.53%	0.063%
81	23.345	3440	3444	3448	rBB7	34781	57912	1.59%	0.191%
82	23.404	3448	3454	3459	rBB	548148	962679	26.50%	3.178%
83	23.451	3459	3462	3467	rBB5	154976	191222	5.26%	0.631%
84	23.557	3469	3480	3487	rBB	1779078	3633205	100.00%	11.994%
85	23.680	3499	3501	3502	rBB2	33355	14565	0.40%	0.048%
86	23.733	3508	3510	3513	rBB4	30817	16852	0.46%	0.056%
87	23.769	3513	3516	3517	rBB3	26753	21966	0.60%	0.073%
88	23.827	3522	3526	3527	rBB4	17900	16195	0.45%	0.053%
89	23.863	3531	3532	3533	rBB	39354	14304	0.39%	0.047%
90	23.904	3537	3539	3540	rBB2	27672	20189	0.56%	0.067%
91	23.916	3540	3541	3544	rBB3	29449	17838	0.49%	0.059%
92	23.951	3544	3547	3550	rBB5	25705	25121	0.69%	0.083%
93	23.998	3553	3555	3556	rBB2	25052	17891	0.49%	0.059%
94	24.051	3562	3564	3565	rBB2	20710	14567	0.40%	0.048%
95	24.104	3565	3573	3579	rBB7	219043	427454	11.77%	1.411%
96	24.180	3584	3586	3587	rBB2	35004	15508	0.43%	0.051%
97	24.298	3604	3606	3608	rBB3	31886	16932	0.47%	0.056%
98	24.321	3608	3610	3611	rBB2	9840	13144	0.36%	0.043%
99	24.392	3620	3622	3623	rBB2	20666	16742	0.46%	0.055%
100	24.439	3628	3630	3632	rBB3	28174	17897	0.49%	0.059%
101	24.486	3635	3638	3640	rBB4	20126	16684	0.46%	0.055%
102	24.521	3640	3644	3647	rBB6	16920	22347	0.62%	0.074%
103	24.574	3652	3653	3656	rBB3	22966	15618	0.43%	0.052%
104	24.639	3659	3664	3665	rBB5	26320	49221	1.35%	0.162%
105	24.710	3673	3676	3679	rBB4	26303	21725	0.60%	0.072%
106	24.792	3687	3690	3691	rBB3	23912	16006	0.44%	0.053%
107	24.869	3694	3703	3707	rBB9	207340	464439	12.78%	1.533%
108	24.951	3714	3717	3719	rBB4	32348	27843	0.77%	0.092%
109	24.974	3719	3721	3724	rBB4	20252	21872	0.60%	0.072%
110	25.039	3729	3732	3736	rBB6	30284	40746	1.12%	0.135%
111	25.080	3736	3739	3742	rBB5	13388	18780	0.52%	0.062%
112	25.127	3745	3747	3749	rBB3	17513	13742	0.38%	0.045%
113	25.145	3749	3750	3752	rBB2	26256	12881	0.35%	0.043%
114	25.263	3768	3770	3771	rBB2	11600	15913	0.44%	0.053%
115	25.316	3777	3779	3781	rBB3	34757	21663	0.60%	0.072%
116	25.357	3785	3786	3789	rBB3	25644	19459	0.54%	0.064%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014878.D
 Acq On : 11 Jun 2021 00:59
 Operator : CG/JU
 Sample : M2618-04DL 5X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG5R7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

117	25.404	3792	3794	3797	rBB4	35646	36357	1.00%	0.120%
118	25.445	3799	3801	3804	rBB4	28431	23591	0.65%	0.078%
119	25.533	3810	3816	3820	rBB9	38321	66946	1.84%	0.221%
120	25.627	3829	3832	3836	rBB6	37168	45010	1.24%	0.149%
121	25.692	3841	3843	3845	rBB3	45439	32097	0.88%	0.106%
122	25.739	3845	3851	3861	rBB3	128169	316406	8.71%	1.045%
123	25.839	3864	3868	3872	rBB7	35633	43288	1.19%	0.143%
124	25.892	3874	3877	3878	rBB3	31739	21197	0.58%	0.070%
125	25.910	3878	3880	3882	rBB3	27149	16768	0.46%	0.055%
126	26.021	3898	3899	3900	rBB	32846	12836	0.35%	0.042%
127	26.074	3906	3908	3913	rBB6	26550	30414	0.84%	0.100%
128	26.116	3913	3915	3918	rBB4	23702	23364	0.64%	0.077%
129	26.163	3920	3923	3925	rBB3	36716	33897	0.93%	0.112%
130	26.186	3925	3927	3928	rBB2	21533	18434	0.51%	0.061%
131	26.221	3931	3933	3936	rBB4	16157	15843	0.44%	0.052%
132	26.286	3941	3944	3946	rBB4	27108	21801	0.60%	0.072%
133	26.315	3948	3949	3951	rBB2	24193	15879	0.44%	0.052%
134	26.386	3959	3961	3963	rBB2	22185	17447	0.48%	0.058%
135	26.427	3966	3968	3970	rBB3	21132	15274	0.42%	0.050%
136	26.457	3970	3973	3975	rBB4	13392	18528	0.51%	0.061%
137	26.580	3992	3994	3997	rBB4	32900	20706	0.57%	0.068%
138	26.627	3999	4002	4005	rBB5	22739	19853	0.55%	0.066%
139	26.651	4005	4006	4009	rBB3	33649	24945	0.69%	0.082%
140	26.686	4009	4012	4013	rBB3	29586	13372	0.37%	0.044%
141	26.715	4013	4017	4019	rBB5	19368	19702	0.54%	0.065%
142	26.780	4023	4028	4037	rBB5	107628	269971	7.43%	0.891%
143	26.868	4040	4043	4045	rBB4	23670	23421	0.64%	0.077%
144	26.892	4045	4047	4048	rBB	32491	13083	0.36%	0.043%
145	26.904	4048	4049	4052	rBB3	17986	17565	0.48%	0.058%
146	26.939	4052	4055	4057	rBB4	43414	40055	1.10%	0.132%
147	26.980	4059	4062	4063	rBB3	17797	13396	0.37%	0.044%
148	26.992	4063	4064	4066	rBB2	29870	15573	0.43%	0.051%
149	27.021	4066	4069	4070	rBB3	27196	21510	0.59%	0.071%
150	27.157	4091	4092	4096	rBB4	24511	19848	0.55%	0.066%
151	27.198	4096	4099	4102	rBB5	27353	40023	1.10%	0.132%
152	27.239	4102	4106	4109	rBB6	18771	26210	0.72%	0.087%
153	27.263	4109	4110	4113	rBB3	35316	24029	0.66%	0.079%
154	27.386	4130	4131	4133	rBB2	33832	17900	0.49%	0.059%
155	27.427	4133	4138	4141	rBB7	42245	59997	1.65%	0.198%
156	27.462	4141	4144	4147	rBB5	19159	22270	0.61%	0.074%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014878.D
 Acq On : 11 Jun 2021 00:59
 Operator : CG/JU
 Sample : M2618-04DL 5X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG5R7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

157	27.486	4147	4148	4151	rBB3	26311	17245	0.47%	0.057%
158	27.510	4151	4152	4157	rBB5	26716	25528	0.70%	0.084%
159	27.551	4157	4159	4160	rBB2	24937	14397	0.40%	0.048%
160	27.610	4165	4169	4171	rBB5	13400	21256	0.59%	0.070%
161	27.662	4177	4178	4181	rBB3	23476	14415	0.40%	0.048%
162	27.686	4181	4182	4185	rBB3	30641	22476	0.62%	0.074%
163	27.727	4187	4189	4192	rBB4	13309	12913	0.36%	0.043%
164	27.780	4196	4198	4201	rBB4	22579	16297	0.45%	0.054%
165	27.851	4208	4210	4213	rBB4	32972	29222	0.80%	0.096%
166	27.874	4213	4214	4216	rBB2	27952	19956	0.55%	0.066%
167	27.986	4228	4233	4234	rBB5	14056	31556	0.87%	0.104%
168	28.004	4234	4236	4237	rBB2	26651	24033	0.66%	0.079%
169	28.015	4237	4238	4240	rBB2	23515	15565	0.43%	0.051%
170	28.039	4240	4242	4246	rBB5	19738	15369	0.42%	0.051%
171	28.115	4253	4255	4257	rBB3	18744	14912	0.41%	0.049%
172	28.133	4257	4258	4263	rBB5	19801	19720	0.54%	0.065%
173	28.168	4263	4264	4269	rBB5	19000	26323	0.72%	0.087%
174	28.233	4274	4275	4277	rBB2	18464	12915	0.36%	0.043%
175	28.351	4292	4295	4296	rBB3	26419	26549	0.73%	0.088%
176	28.386	4298	4301	4303	rBB4	21011	15629	0.43%	0.052%
177	28.427	4306	4308	4312	rBB5	23045	28324	0.78%	0.094%
178	28.474	4312	4316	4317	rBB4	23939	22073	0.61%	0.073%
179	28.504	4320	4321	4323	rBB2	22276	13430	0.37%	0.044%
180	28.645	4342	4345	4347	rBB3	30196	28416	0.78%	0.094%
181	28.686	4347	4352	4354	rBB6	20689	17396	0.48%	0.057%
182	28.733	4356	4360	4362	rBB5	20040	20434	0.56%	0.067%
183	28.762	4362	4365	4370	rBB7	28637	39675	1.09%	0.131%
184	28.809	4370	4373	4374	rVB3	42403	21468	0.59%	0.071%
185	28.827	4374	4376	4379	rBB4	31740	31578	0.87%	0.104%
186	28.874	4379	4384	4387	rBB6	17765	30588	0.84%	0.101%
187	28.962	4398	4399	4401	rBB2	24223	15201	0.42%	0.050%
188	28.992	4401	4404	4407	rBB5	47157	40015	1.10%	0.132%
189	29.015	4407	4408	4410	rBB2	19940	14395	0.40%	0.048%
190	29.033	4410	4411	4414	rBB3	17422	14154	0.39%	0.047%
191	29.068	4414	4417	4418	rBB3	25974	16061	0.44%	0.053%
192	29.080	4418	4419	4422	rBB3	30264	23465	0.65%	0.077%
193	29.104	4422	4423	4426	rBB3	22994	18513	0.51%	0.061%
194	29.151	4430	4431	4434	rBB3	28430	17543	0.48%	0.058%
195	29.192	4434	4438	4439	rBB4	31638	32735	0.90%	0.108%
196	29.251	4445	4448	4452	rBB6	21228	34993	0.96%	0.116%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014878.D
Acq On : 11 Jun 2021 00:59
Operator : CG/JU
Sample : M2618-04DL 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG5R7DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Title : SVOA CALIBRATION

197	29.292	4452	4455	4456	rBB2	38328	24093	0.66%	0.080%
198	29.315	4456	4459	4460	rBB3	26875	16254	0.45%	0.054%
199	29.339	4462	4463	4464	rBB	34035	12749	0.35%	0.042%
200	29.362	4464	4467	4469	rBB4	21623	17397	0.48%	0.057%




Sum of corrected areas: 30291572

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014878.D
Acq On : 11 Jun 2021 00:59
Operator : CG/JU
Sample : M2618-04DL 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG5R7DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

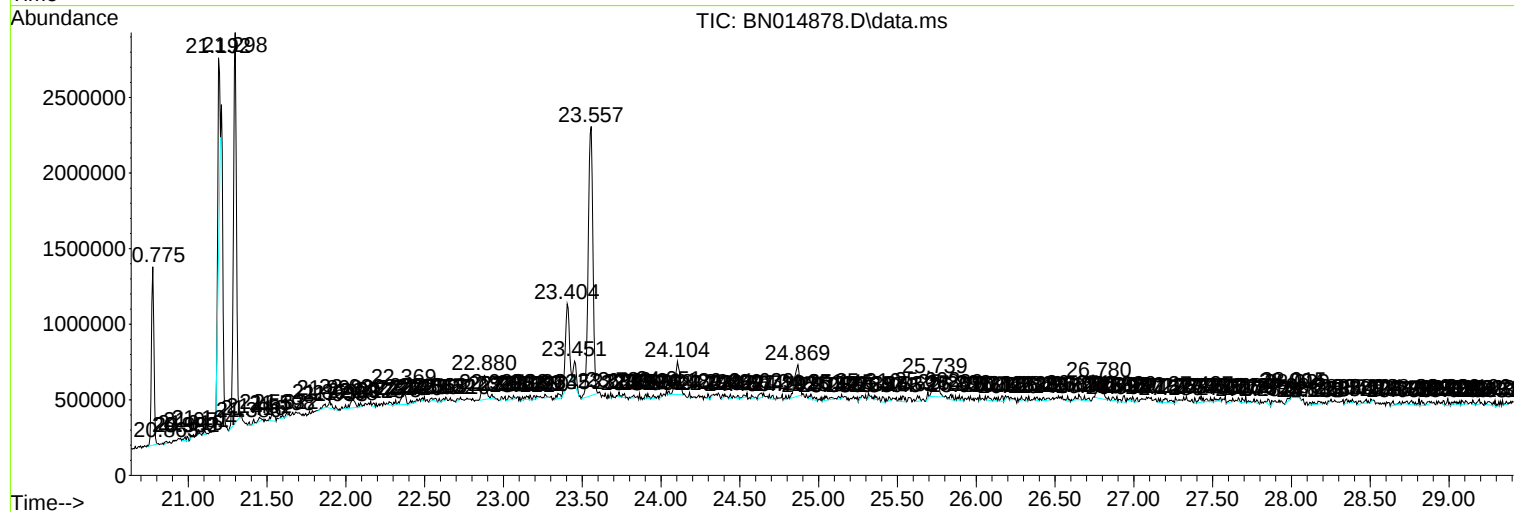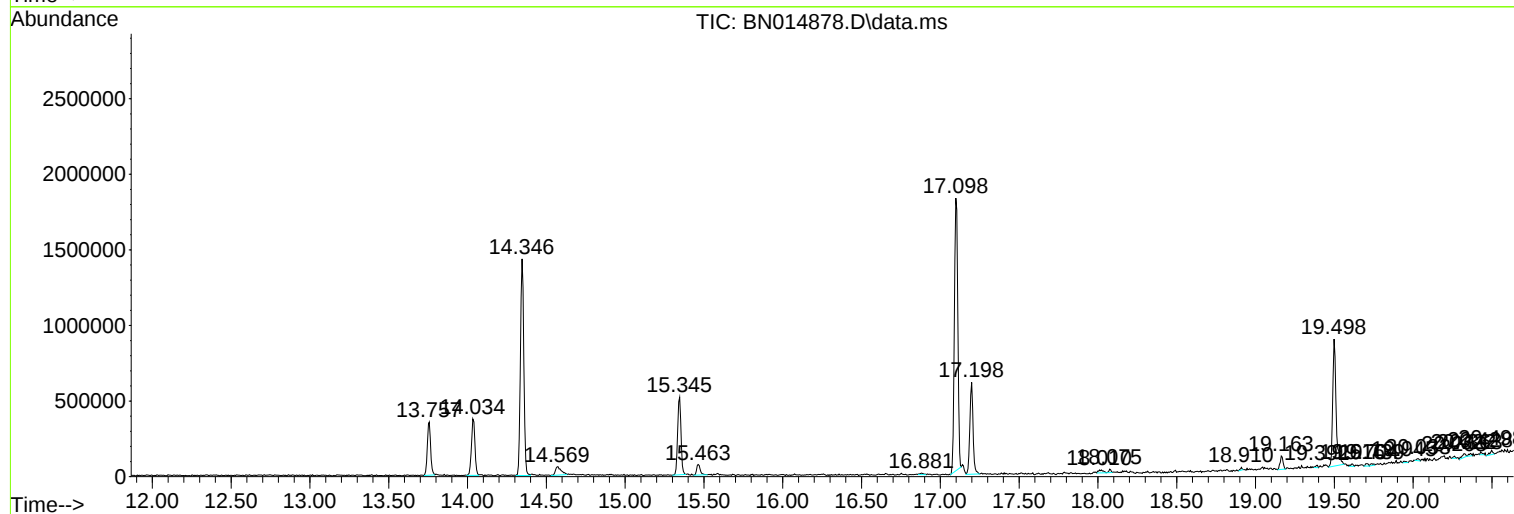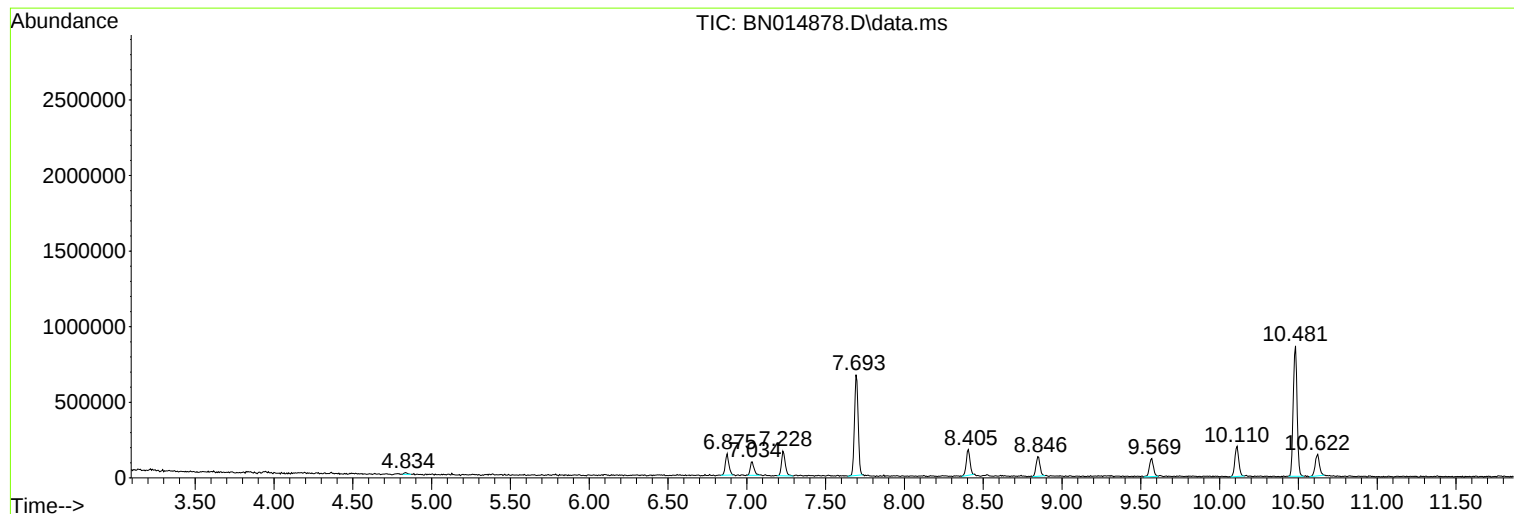

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014878.D
Acq On : 11 Jun 2021 00:59
Operator : CG/JU
Sample : M2618-04DL 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG5R7DL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Phosphoric acid, tris(2-eth... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.775	7.48 ng/ul	1275330	Chrysene-d12	21.298

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Phosphoric acid, tris(2-ethylhex...	434	C24H51O4P	000078-42-2	80
2			Phosphoric acid, tris(2-ethylhex...	434	C24H51O4P	000078-42-2	58
3			Phosphoric acid, trioctyl ester	434	C24H51O4P	001806-54-8	58
4			3,5-Diamino-1,2,4-triazole	99	C2H5N5	001455-77-2	49
5			Phosphoric acid, trioctyl ester	434	C24H51O4P	001806-54-8	40

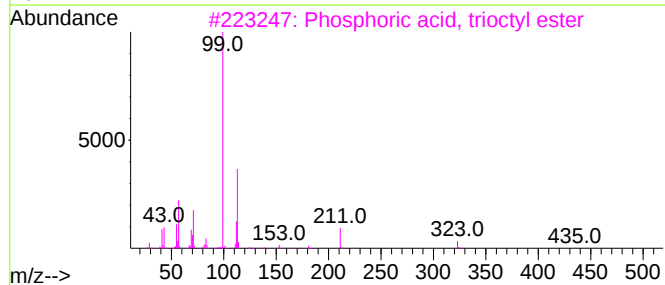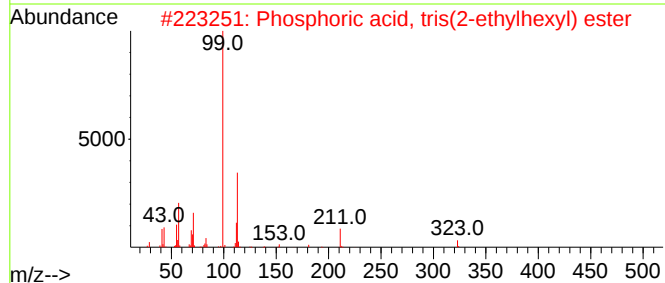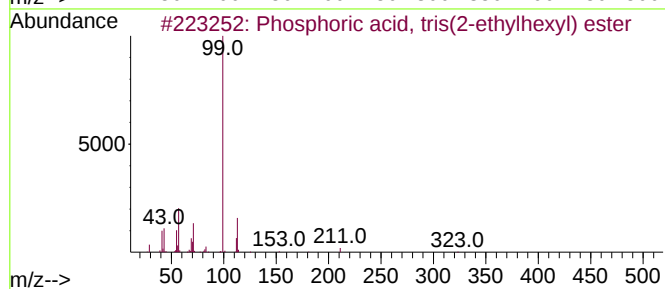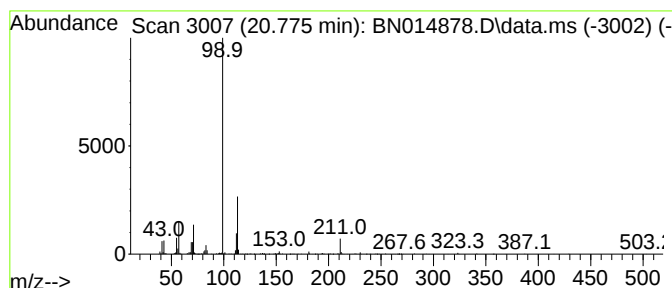

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014878.D
Acq On : 11 Jun 2021 00:59
Operator : CG/JU
Sample : M2618-04DL 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleID :
BG5R7DL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
24.104	2.35 ng/ul	427454	Perylene-d12	23.557

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Docosane	310	C22H46	000629-97-0	93
2		Pentacosane	352	C25H52	000629-99-2	89
3		Hexadecane, 2-methyl-	240	C17H36	001560-92-5	89
4		Octacosane	394	C28H58	000630-02-4	76
5		Heneicosane	296	C21H44	000629-94-7	76

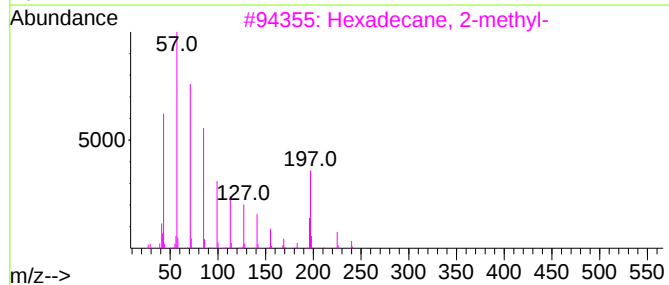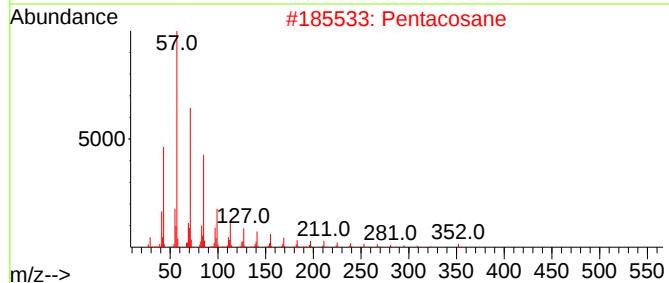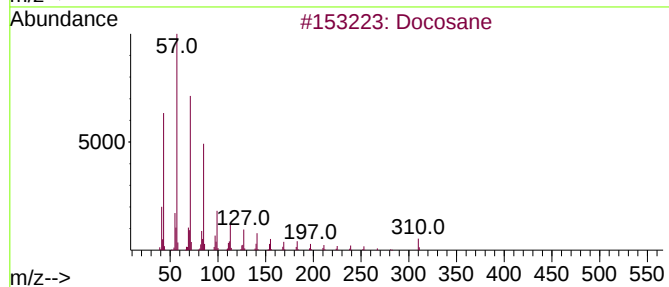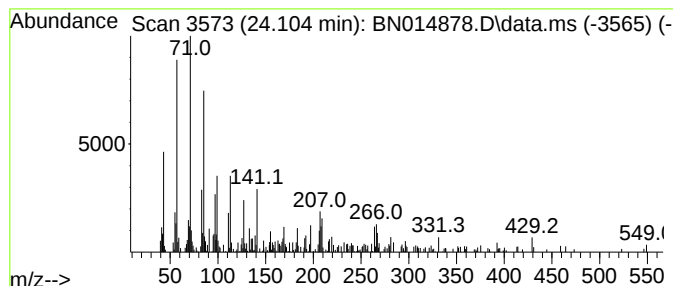

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014878.D
Acq On : 11 Jun 2021 00:59
Operator : CG/JU
Sample : M2618-04DL 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1










Instrument :
BNA_N
ClientSampleId :
BG5R7DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.	
24.869	2.56 ng/ul	464439	Perylene-d12	23.557	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Eicosane	282	C20H42	000112-95-8	78
2	Tetracosane	338	C24H50	000646-31-1	70
3	Eicosane	282	C20H42	000112-95-8	70
4	Behenyl chloride	344	C22H45Cl	042217-03-8	70
5	Nonadecane	268	C19H40	000629-92-5	70

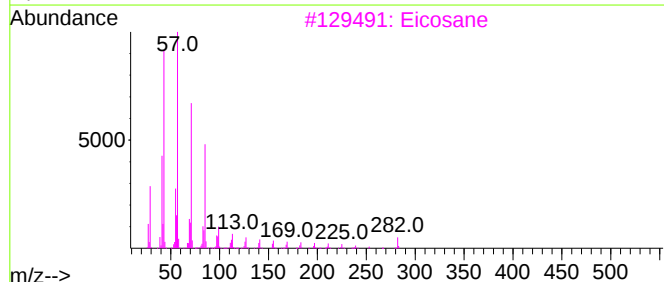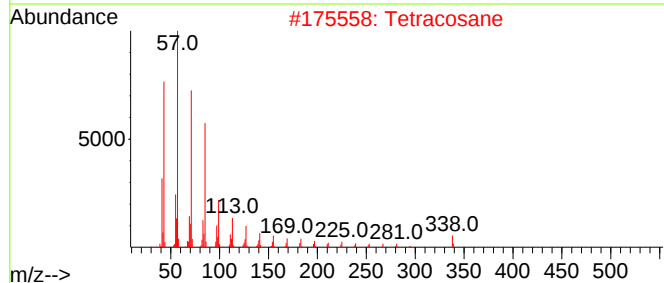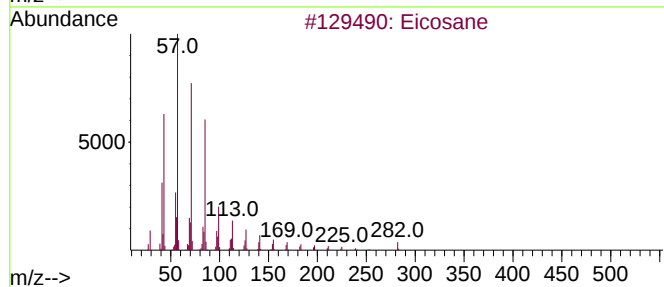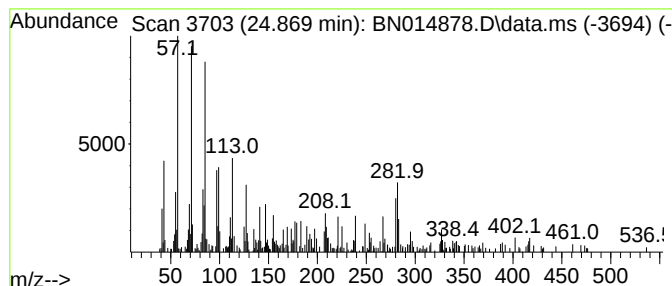

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014878.D
Acq On : 11 Jun 2021 00:59
Operator : CG/JU
Sample : M2618-04DL 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG5R7DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Phosphoric acid...	20.775	7.5	ng/u1	1275330	5	21.298	3412170	20.0
(DEL) Alkane: S...	24.104	2.4	ng/u1	427454	6	23.557	3633210	20.0
(DEL) Alkane: S...	24.869	2.6	ng/u1	464439	6	23.557	3633210	20.0