

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014880.D
 Acq On : 11 Jun 2021 08:54
 Operator : CG/JU
 Sample : PB136853BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK853

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014880.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.211	19	21	27	rVB2	38052	57366	1.01%	0.117%
2	3.328	39	41	44	rBV4	10465	8351	0.15%	0.017%
3	3.464	62	64	65	rBV2	11777	7578	0.13%	0.015%
4	3.617	87	90	105	rBV	219885	405040	7.10%	0.828%
5	3.864	131	132	136	rBV3	7098	7605	0.13%	0.016%
6	3.934	140	144	151	rVV	111204	175350	3.08%	0.359%
7	4.223	191	193	197	rBV4	7323	7352	0.13%	0.015%
8	4.328	209	211	214	rBV4	8685	9538	0.17%	0.020%
9	4.958	317	318	322	rVB3	10836	8277	0.15%	0.017%
10	5.158	351	352	355	rVB3	10957	7125	0.12%	0.015%
11	5.193	355	358	360	rBV3	8234	10163	0.18%	0.021%
12	5.452	401	402	405	rBV3	9528	8241	0.14%	0.017%
13	5.534	413	416	420	rBV5	5201	7709	0.14%	0.016%
14	5.634	432	433	438	rVB5	6443	7231	0.13%	0.015%
15	5.799	458	461	462	rBV3	5622	6688	0.12%	0.014%
16	6.164	521	523	528	rVB3	4514	7692	0.13%	0.016%
17	6.264	536	540	544	rBV6	5818	9593	0.17%	0.020%
18	6.717	614	617	622	rBV7	6710	13257	0.23%	0.027%
19	6.875	638	644	655	rVB	658975	1074646	18.85%	2.197%
20	7.034	665	671	681	rBV	454181	731500	12.83%	1.496%
21	7.234	698	705	711	rBV	723147	1204614	21.13%	2.463%
22	7.381	728	730	735	rBV5	4666	8275	0.15%	0.017%
23	7.693	776	783	791	rBV	606013	992457	17.41%	2.029%
24	8.405	898	904	914	rBV	874389	1409221	24.72%	2.881%
25	8.846	971	979	991	rBV	645076	1102642	19.34%	2.254%
26	9.569	1094	1102	1111	rBV2	601868	996349	17.48%	2.037%
27	10.110	1187	1194	1202	rBV	949517	1611391	28.26%	3.295%
28	10.193	1206	1208	1212	rVB4	6491	7788	0.14%	0.016%
29	10.305	1224	1227	1233	rVB4	6715	8656	0.15%	0.018%
30	10.481	1250	1257	1265	rBV	775372	1324214	23.23%	2.708%
31	10.622	1274	1281	1292	rBV	806907	1450140	25.44%	2.965%
32	10.816	1311	1314	1316	rVB3	7806	9222	0.16%	0.019%
33	12.075	1525	1528	1533	rBV6	14427	22857	0.40%	0.047%
34	12.222	1549	1553	1556	rBV2	4851	7553	0.13%	0.015%
35	12.599	1615	1617	1619	rBV2	9868	6644	0.12%	0.014%
36	13.204	1719	1720	1724	rBV2	5660	6827	0.12%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014880.D
 Acq On : 11 Jun 2021 08:54
 Operator : CG/JU
 Sample : PB136853BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK853

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

37	13.557	1777	1780	1782	rBV3	5916	6897	0.12%	0.014%
38	13.763	1809	1815	1822	rBV	1640516	2403493	42.16%	4.914%
39	14.040	1855	1862	1874	rBV	1835906	2660194	46.66%	5.439%
40	14.351	1908	1915	1922	rBV	1299457	1923216	33.73%	3.932%
41	14.563	1945	1951	1960	rBV	572208	972471	17.06%	1.988%
42	14.740	1979	1981	1984	rVB3	9414	7750	0.14%	0.016%
43	15.345	2078	2084	2092	rBV	2215233	3319540	58.22%	6.787%
44	15.469	2098	2105	2113	rBV	592451	850569	14.92%	1.739%
45	15.587	2119	2125	2131	rVB4	37627	56995	1.00%	0.117%
46	15.910	2177	2180	2181	rBV	5600	6601	0.12%	0.013%
47	16.140	2218	2219	2224	rVB3	14442	14182	0.25%	0.029%
48	16.651	2303	2306	2311	rBV5	8470	11495	0.20%	0.024%
49	16.887	2342	2346	2352	rBV4	9810	15829	0.28%	0.032%
50	17.104	2377	2383	2392	rVB	1752490	2452766	43.02%	5.015%
51	17.204	2392	2400	2411	rBV2	2546020	3781256	66.32%	7.731%
52	17.628	2468	2472	2475	rVB5	6609	9645	0.17%	0.020%
53	17.951	2526	2527	2530	rBV2	5982	7692	0.13%	0.016%
54	18.122	2553	2556	2557	rBV2	7581	7441	0.13%	0.015%
55	18.328	2588	2591	2592	rBV3	11382	9386	0.16%	0.019%
56	18.422	2605	2607	2611	rBV4	5033	7989	0.14%	0.016%
57	18.616	2636	2640	2641	rBV2	5459	7007	0.12%	0.014%
58	18.692	2649	2653	2655	rBV4	9842	12646	0.22%	0.026%
59	18.728	2657	2659	2663	rBV4	6386	8478	0.15%	0.017%
60	18.781	2667	2668	2672	rVB2	10558	8335	0.15%	0.017%
61	18.904	2686	2689	2692	rBV5	10500	16714	0.29%	0.034%
62	19.139	2726	2729	2738	rVB3	35302	53227	0.93%	0.109%
63	19.216	2738	2742	2744	rVB4	16770	17882	0.31%	0.037%
64	19.245	2744	2747	2748	rBV3	10479	12866	0.23%	0.026%
65	19.392	2769	2772	2778	rBV2	34735	52550	0.92%	0.107%
66	19.510	2786	2792	2798	rBV	3404222	4878297	85.56%	9.974%
67	21.304	3092	3097	3107	rBV2	2448427	3305323	57.97%	6.758%
68	23.422	3451	3457	3463	rBV	3007895	5701347	100.00%	11.657%
69	23.569	3475	3482	3491	rVB2	1777592	3569706	62.61%	7.299%




Sum of corrected areas: 48908937

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014880.D
Acq On : 11 Jun 2021 08:54
Operator : CG/JU
Sample : PB136853BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK853

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

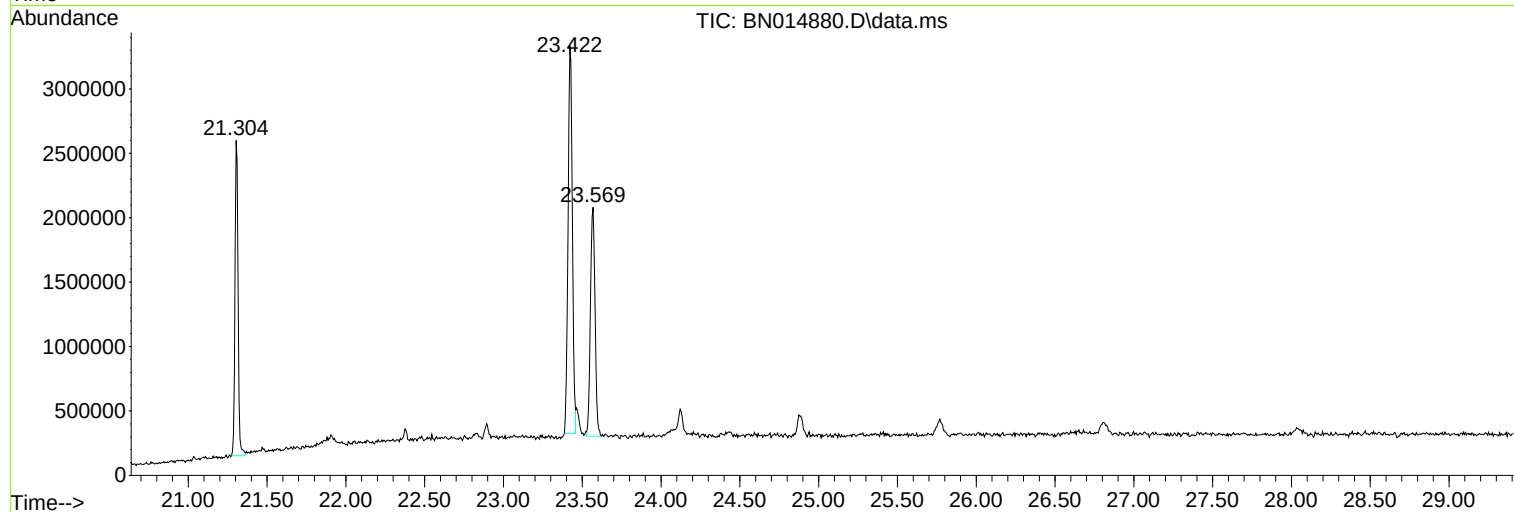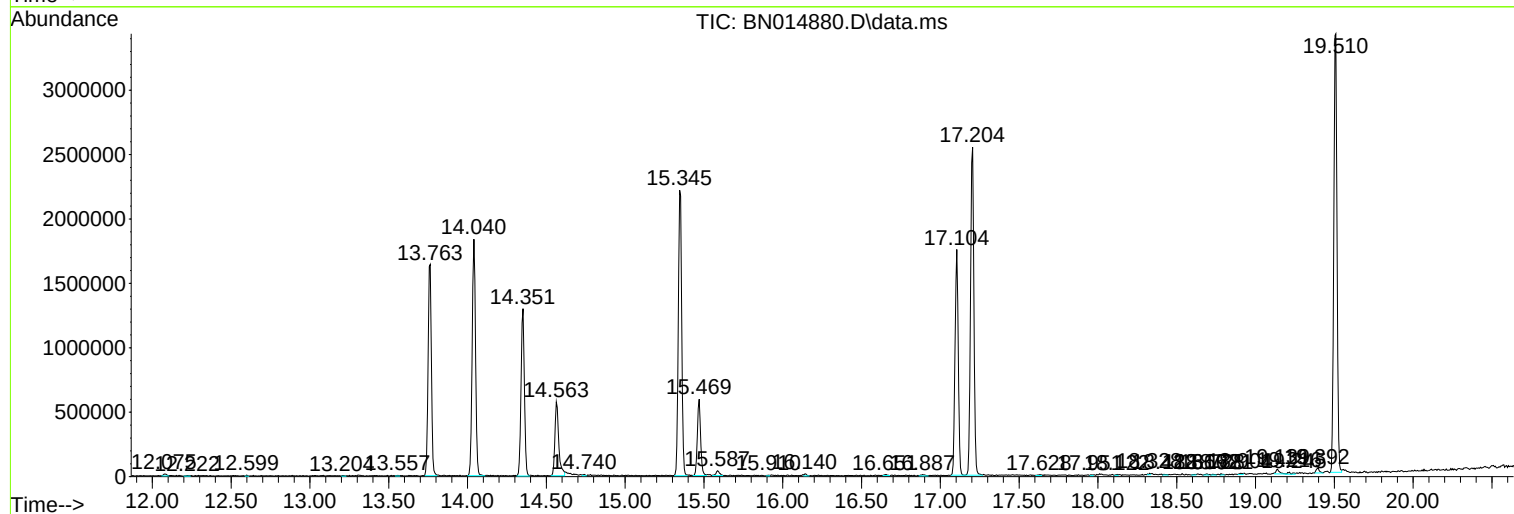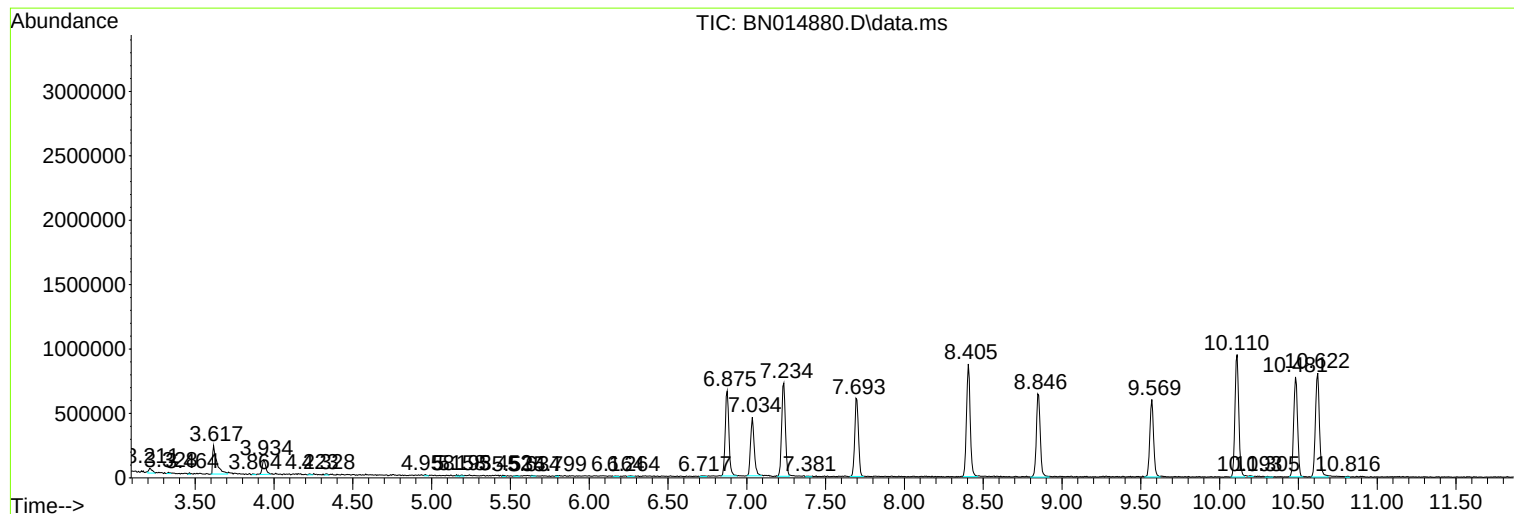

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014880.D
Acq On : 11 Jun 2021 08:54
Operator : CG/JU
Sample : PB136853BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK853

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014880.D
Acq On : 11 Jun 2021 08:54
Operator : CG/JU
Sample : PB136853BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK853

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------