
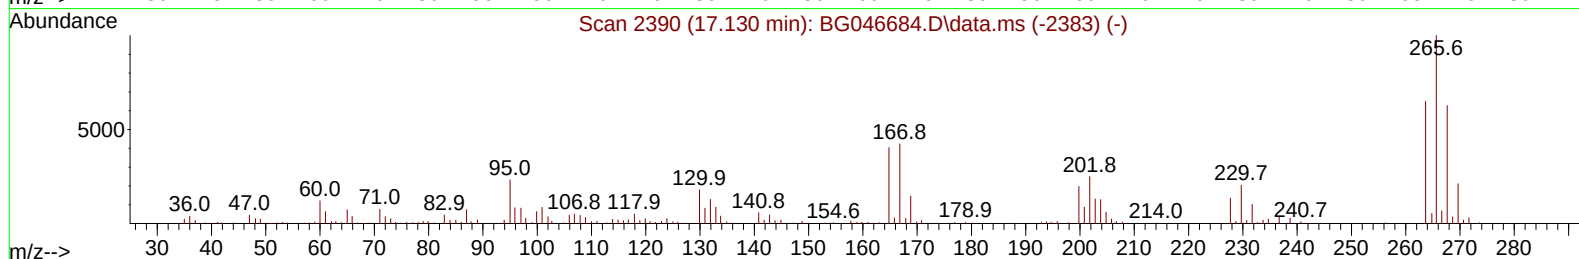
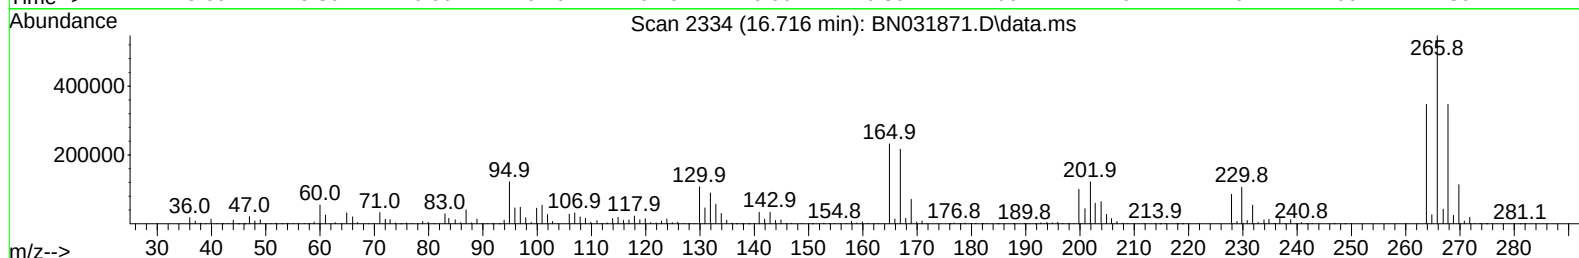


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061024\
Data File : BN031871.D
Acq On : 10 Jun 2024 10:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 12:40:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

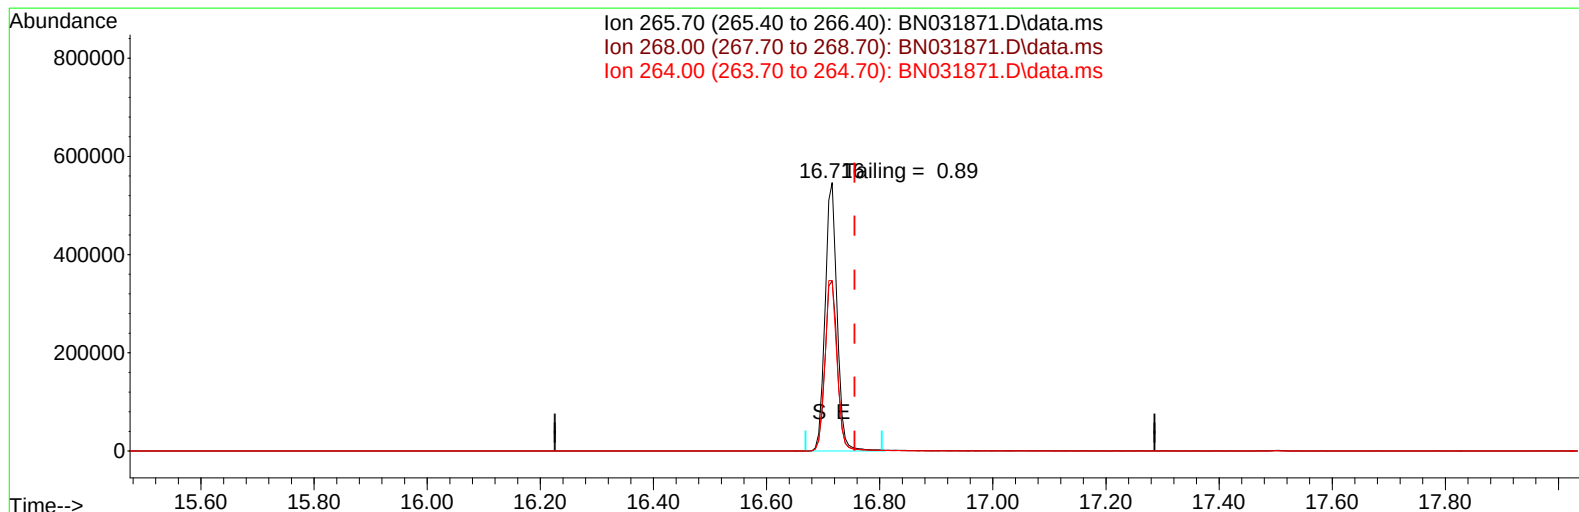

TIC: BN031871.D\data.ms

(70) Pentachlorophenol (C)




16.716min (-0.040) 538434.03 ng

response 802844

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.47
264.00	61.60	63.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061024\
Data File : BN031871.D
Acq On : 10 Jun 2024 10:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 12:40:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

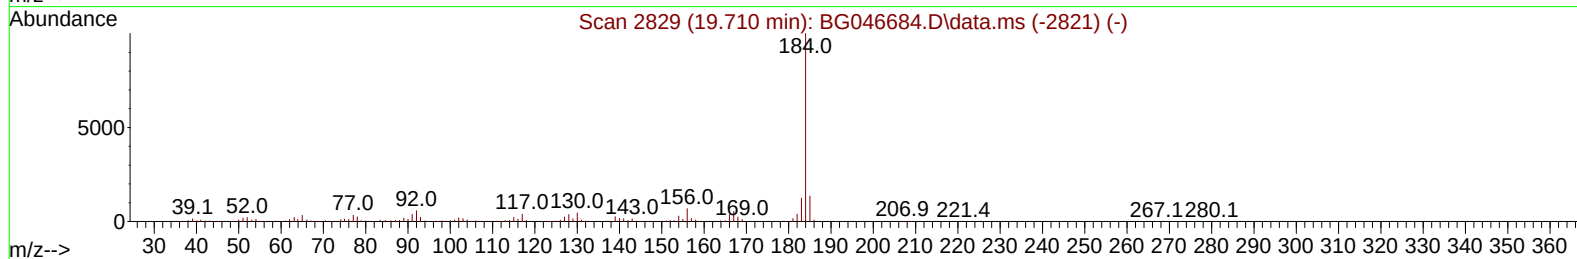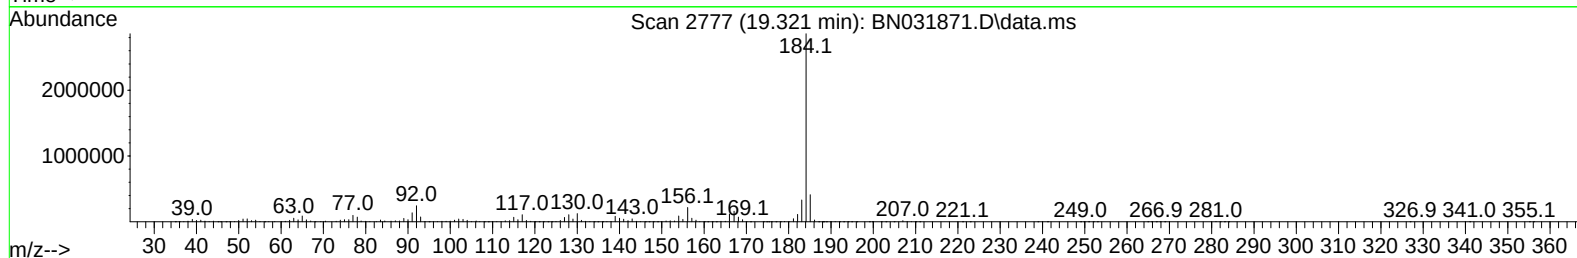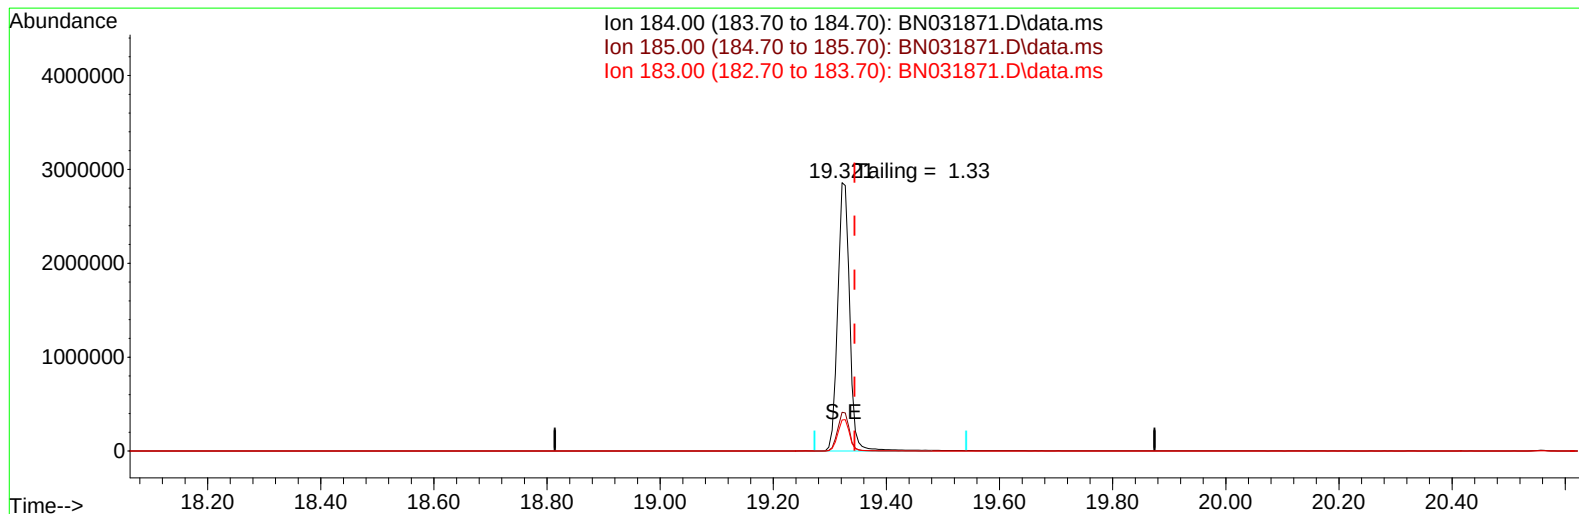

TIC: BN031871.D\data.ms

(77) Benzidine

19.321min (-0.023) 521803.38 ng m

response 4230298

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.42
183.00	13.20	11.59
0.00	0.00	0.00