
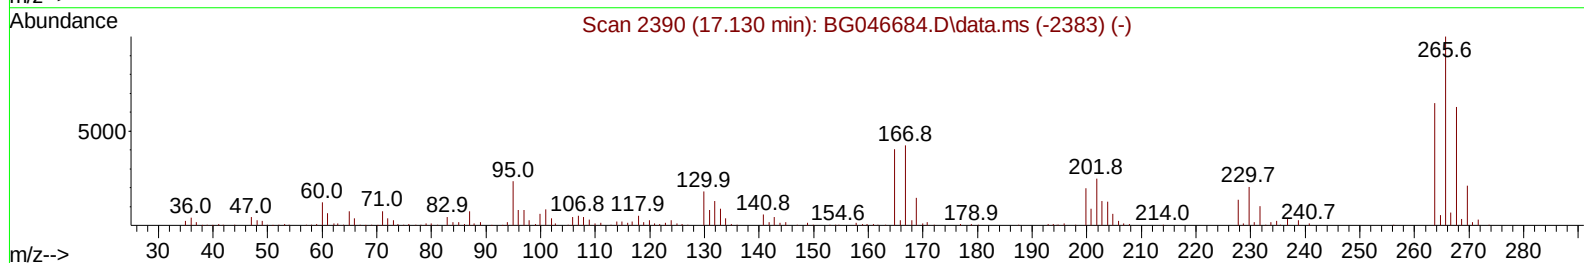
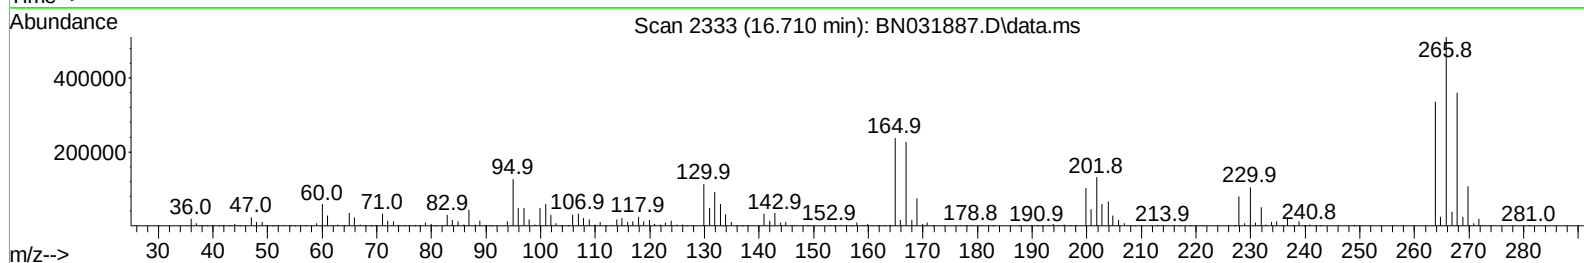


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061024\
Data File : BN031887.D
Acq On : 10 Jun 2024 21:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 01:48:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 11 01:48:18 2024
Response via : Initial Calibration

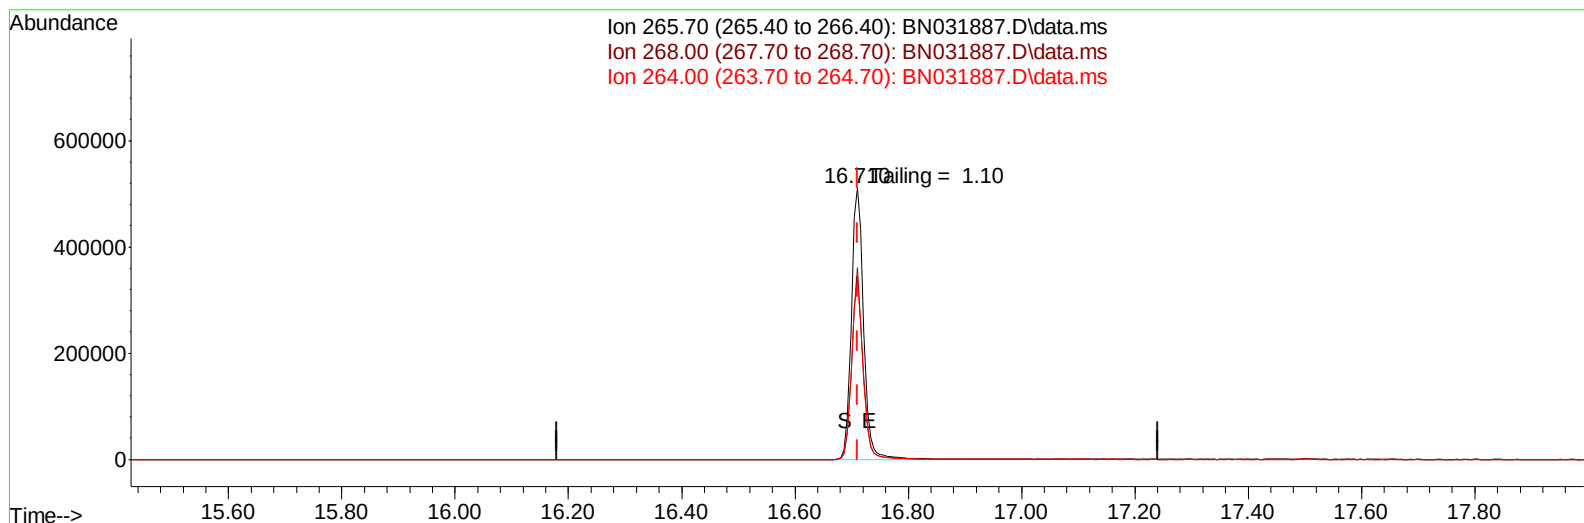




TIC: BN031887.D\data.ms

(70) Pentachlorophenol (C)**16.710min (0.000) 26717.44 ng****response 774737**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	70.66
264.00	61.60	65.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061024\
Data File : BN031887.D
Acq On : 10 Jun 2024 21:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 01:48:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 11 01:48:18 2024
Response via : Initial Calibration

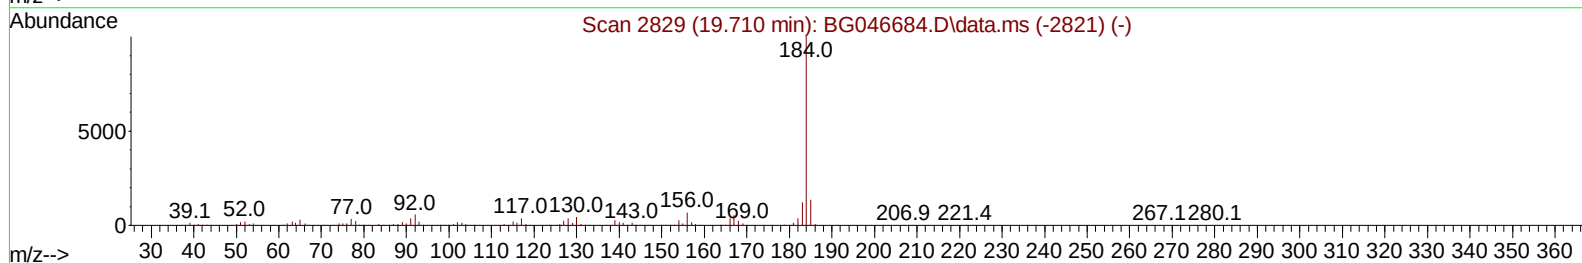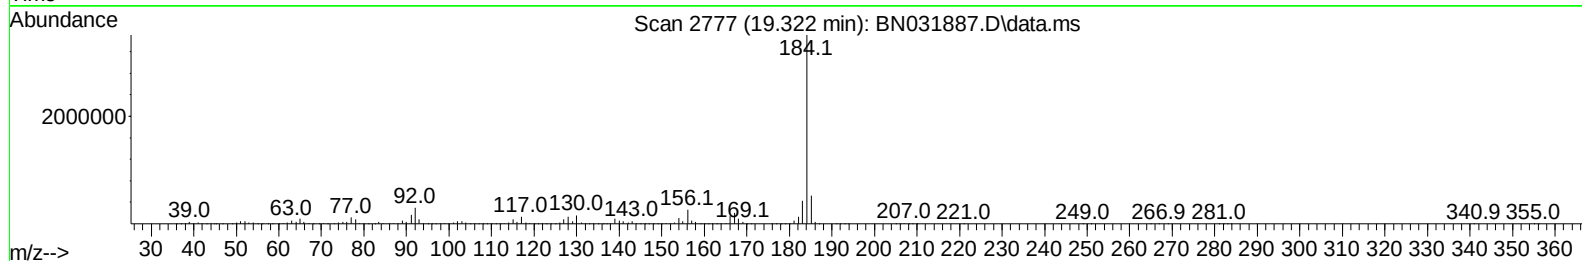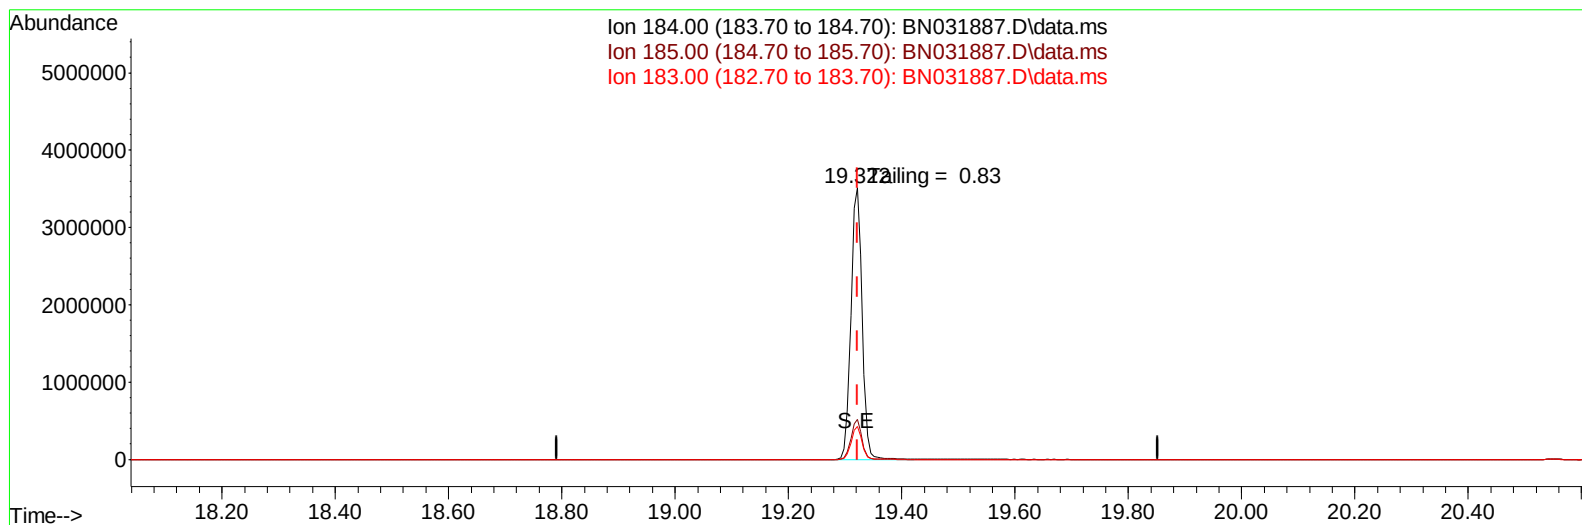

TIC: BN031887.D\data.ms

(77) Benzidine**19.322min (0.000) 0.00 ng****response 4844622**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.84
183.00	13.20	12.05
0.00	0.00	0.00