
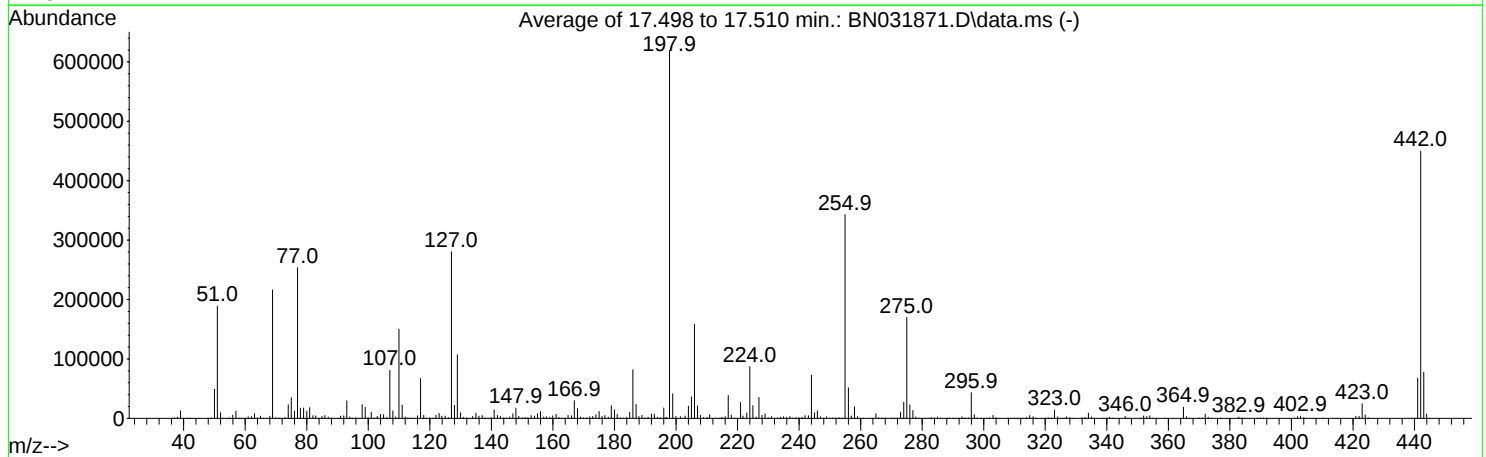


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061024\
Data File : BN031871.D
Acq On : 10 Jun 2024 10:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN061024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 10 15:47:32 2024

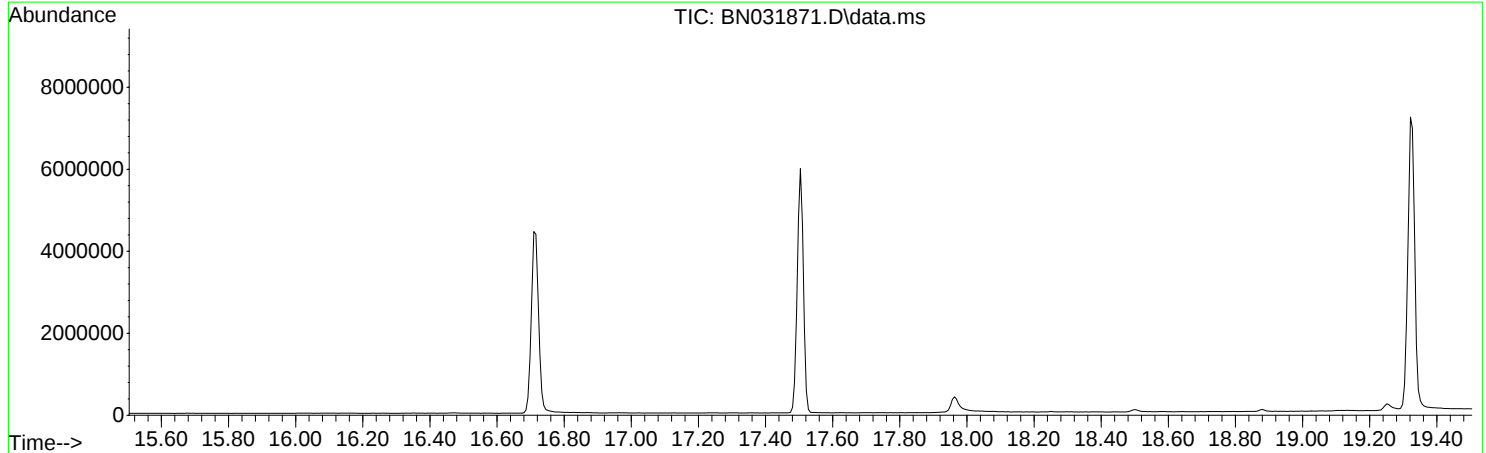




AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	188930	PASS
68	69	0.00	2	1.8	3790	PASS
69	198	0.00	100	34.9	216299	PASS
70	69	0.00	2	0.4	968	PASS
127	198	10	80	45.3	280299	PASS
197	198	0.00	2	0.3	1736	PASS
198	198	100	100	100.0	619157	PASS
199	198	5	9	6.7	41541	PASS
275	198	10	60	27.4	169877	PASS
365	198	1	100	3.0	18807	PASS
441	198	0.01	100	10.9	67709	PASS
442	442	50	100	100.0	449771	PASS
443	442	15	24	17.3	77613	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061024\
Data File : BN031871.D
Acq On : 10 Jun 2024 10:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 10 12:40:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

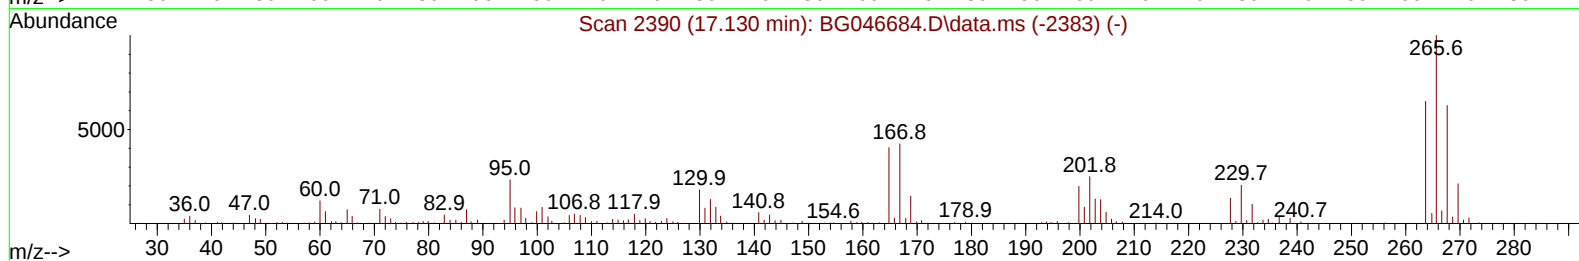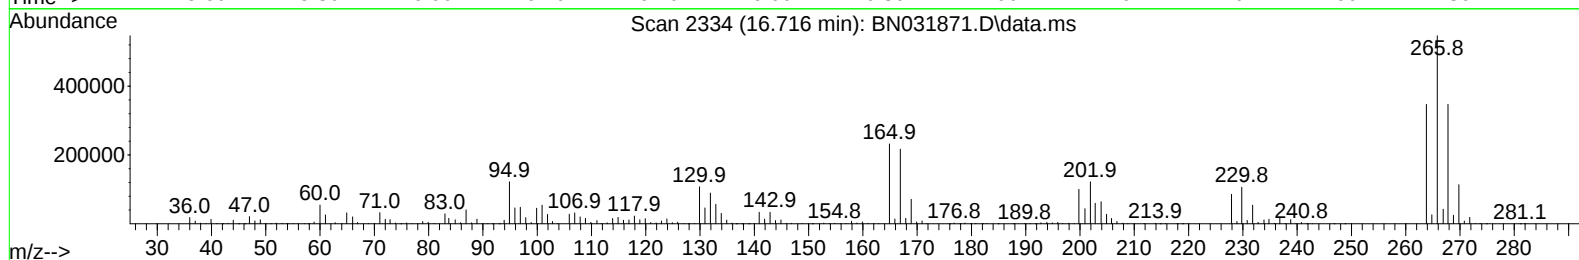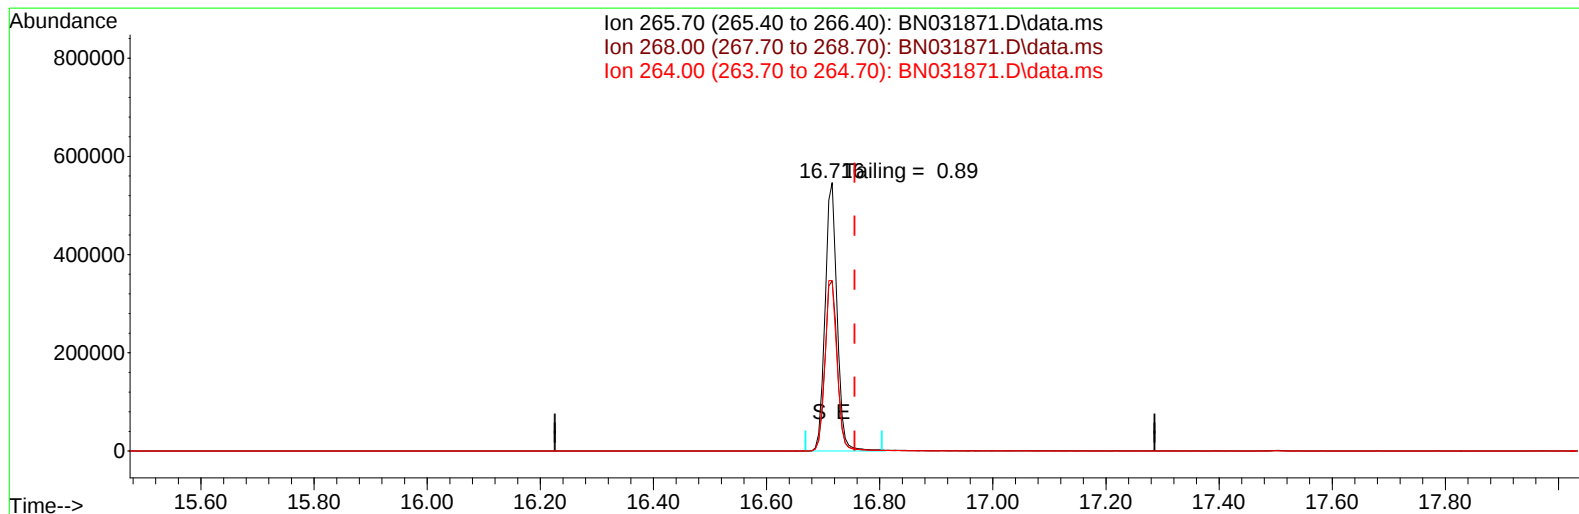

TIC: BN031871.D\data.ms

(70) Pentachlorophenol (C)

16.716min (-0.040) 538434.03 ng




response 802844

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.47
264.00	61.60	63.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061024\
Data File : BN031871.D
Acq On : 10 Jun 2024 10:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 10 12:40:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

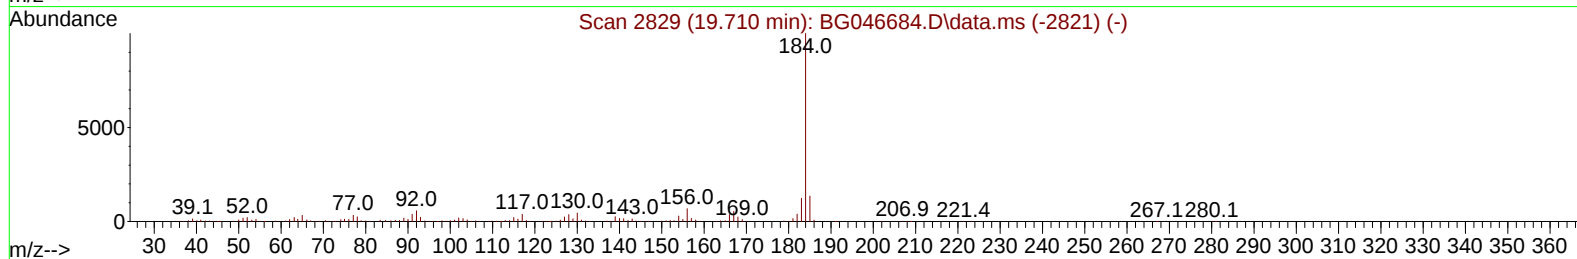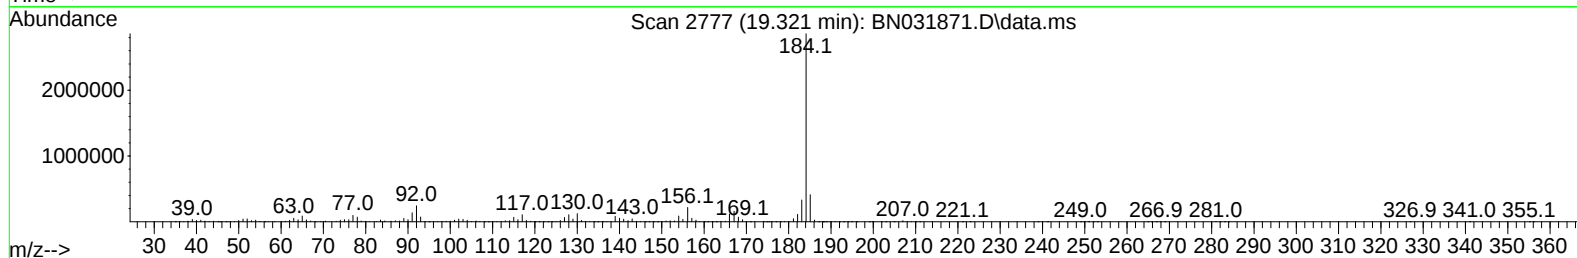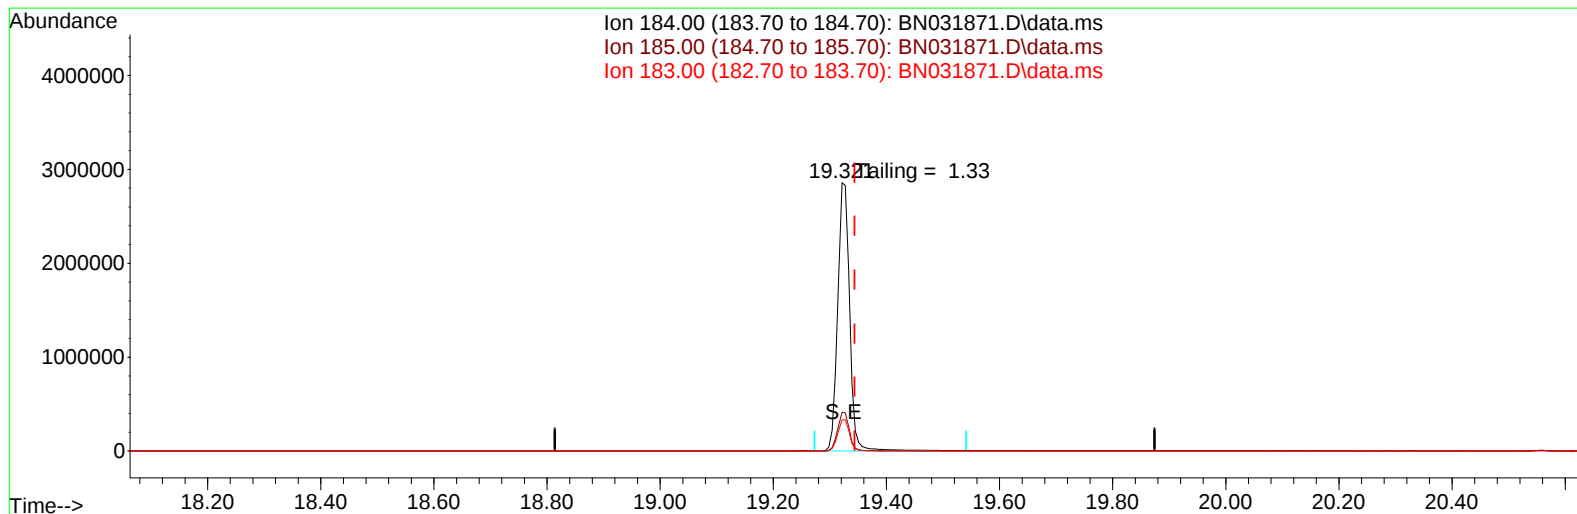

TIC: BN031871.D\data.ms

(77) Benzidine

19.321min (-0.023) 521803.38 ng m

response 4230298

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.42
183.00	13.20	11.59
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/10/2024	BNA_N	<u>BN031871.D</u>
Compound Name	Response	Retention Time
DDT	2239698	20.557
DDD	27117	20.169
DDE	752	19.604
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27869	2267567	1.23

Instrument :
BNA_N
ClientSampleId :
DFTPP