
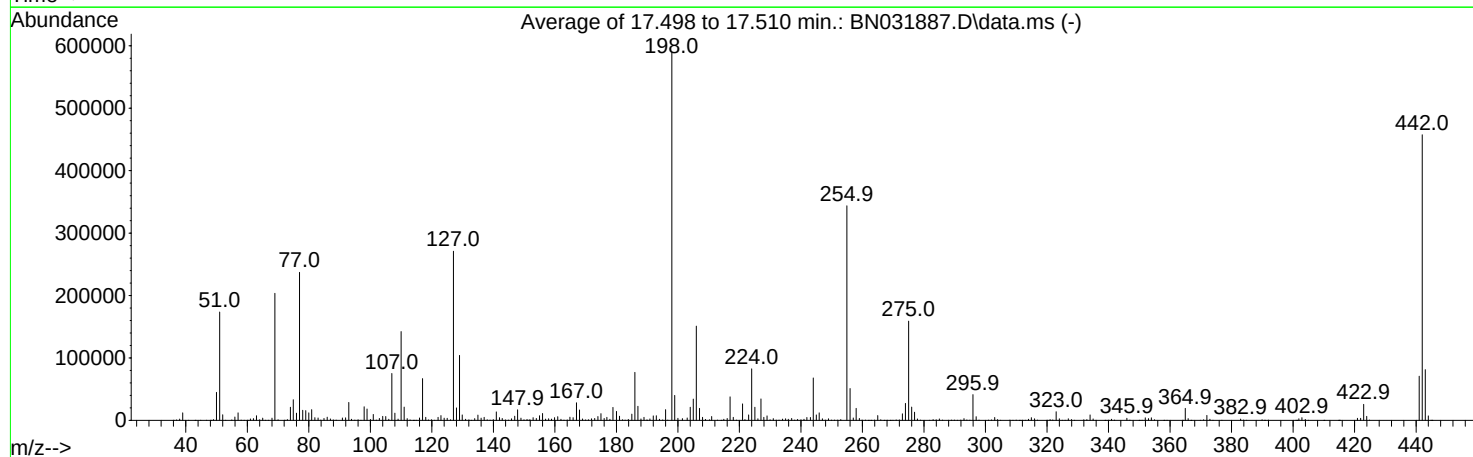


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061024\
Data File : BN031887.D
Acq On : 10 Jun 2024 21:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN061024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 10 15:47:32 2024

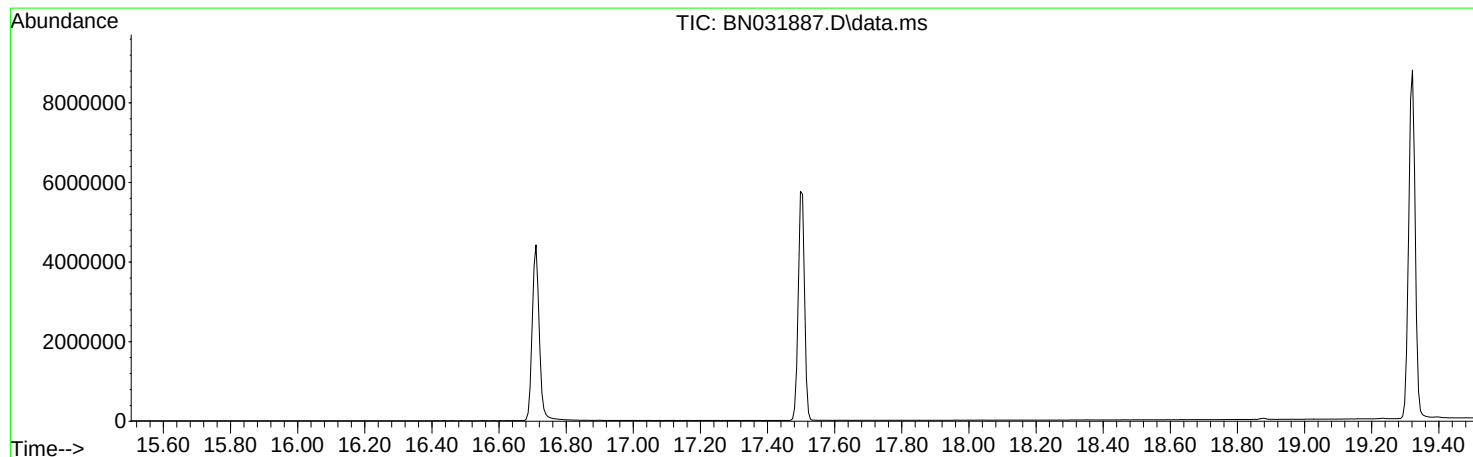




AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.5	173574	PASS
68	69	0.00	2	1.7	3541	PASS
69	198	0.00	100	34.5	203598	PASS
70	69	0.00	2	0.5	1068	PASS
127	198	10	80	46.0	270912	PASS
197	198	0.00	2	0.1	521	PASS
198	198	100	100	100.0	589291	PASS
199	198	5	9	6.8	40125	PASS
275	198	10	60	27.0	158880	PASS
365	198	1	100	3.3	19178	PASS
441	198	0.01	100	12.0	70797	PASS
442	442	50	100	100.0	457643	PASS
443	442	15	24	17.8	81403	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061024\
Data File : BN031887.D
Acq On : 10 Jun 2024 21:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 11 01:48:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 11 01:48:18 2024
Response via : Initial Calibration

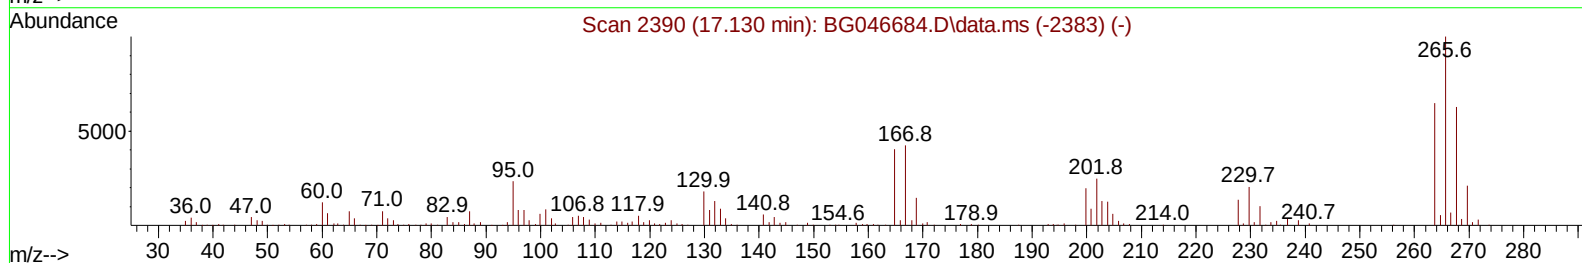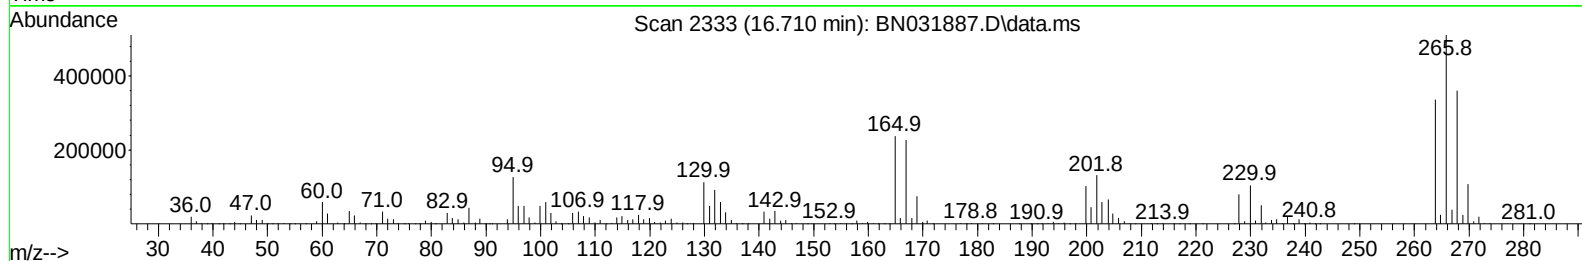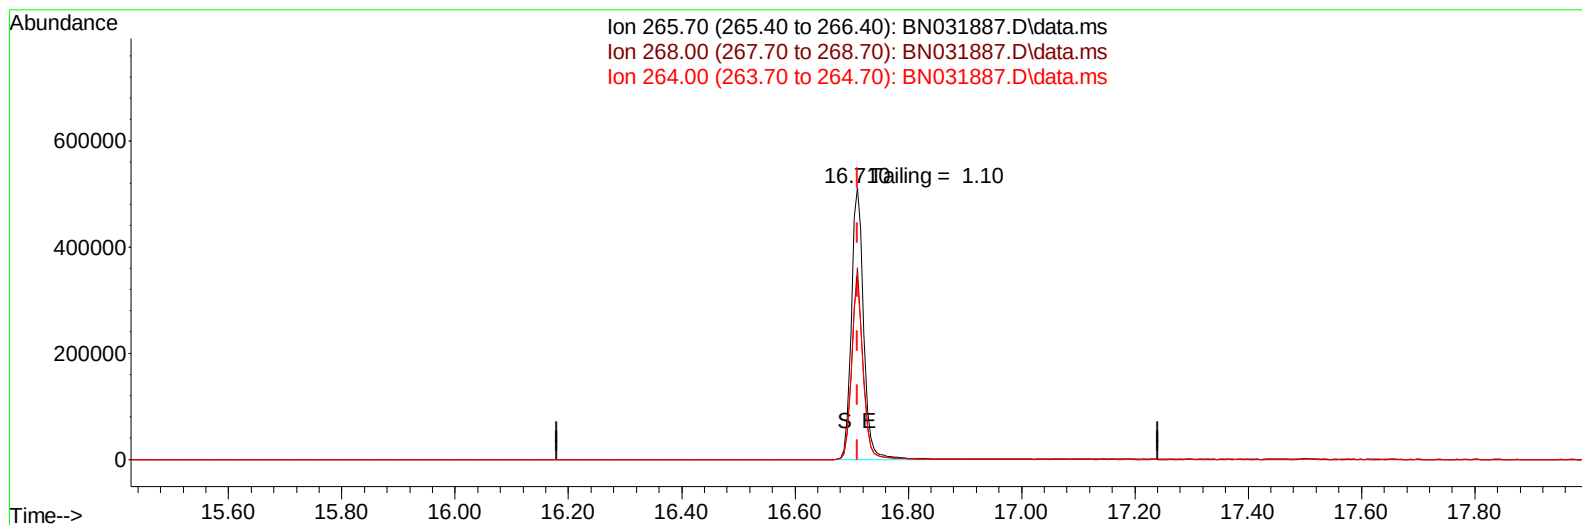

TIC: BN031887.D\data.ms

(70) Pentachlorophenol (C)

16.710min (0.000) 26717.44 ng




response 774737

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	70.66
264.00	61.60	65.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061024\
Data File : BN031887.D
Acq On : 10 Jun 2024 21:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 11 01:48:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 11 01:48:18 2024
Response via : Initial Calibration

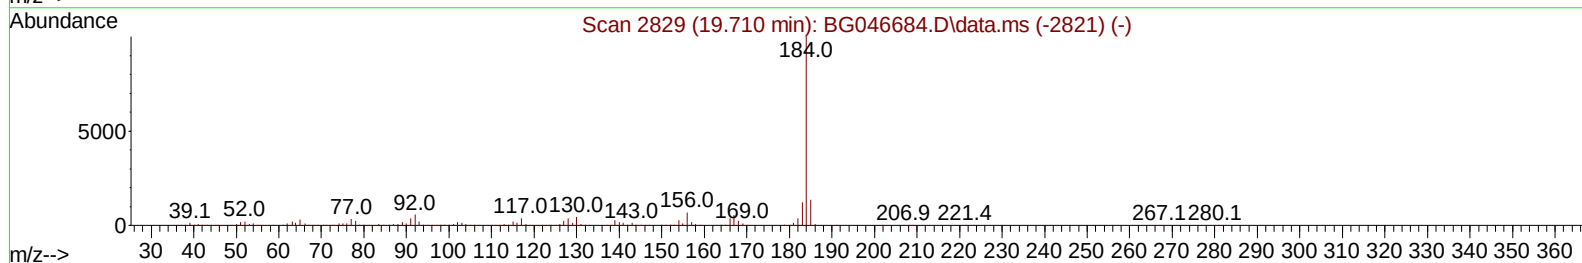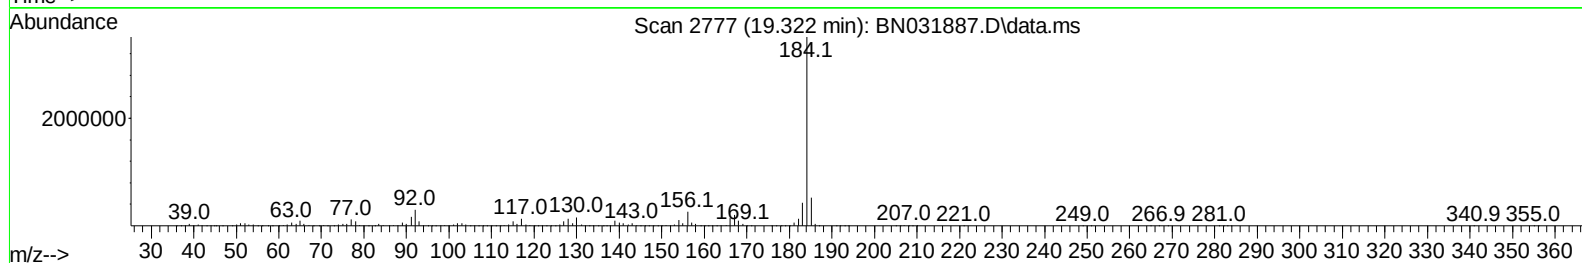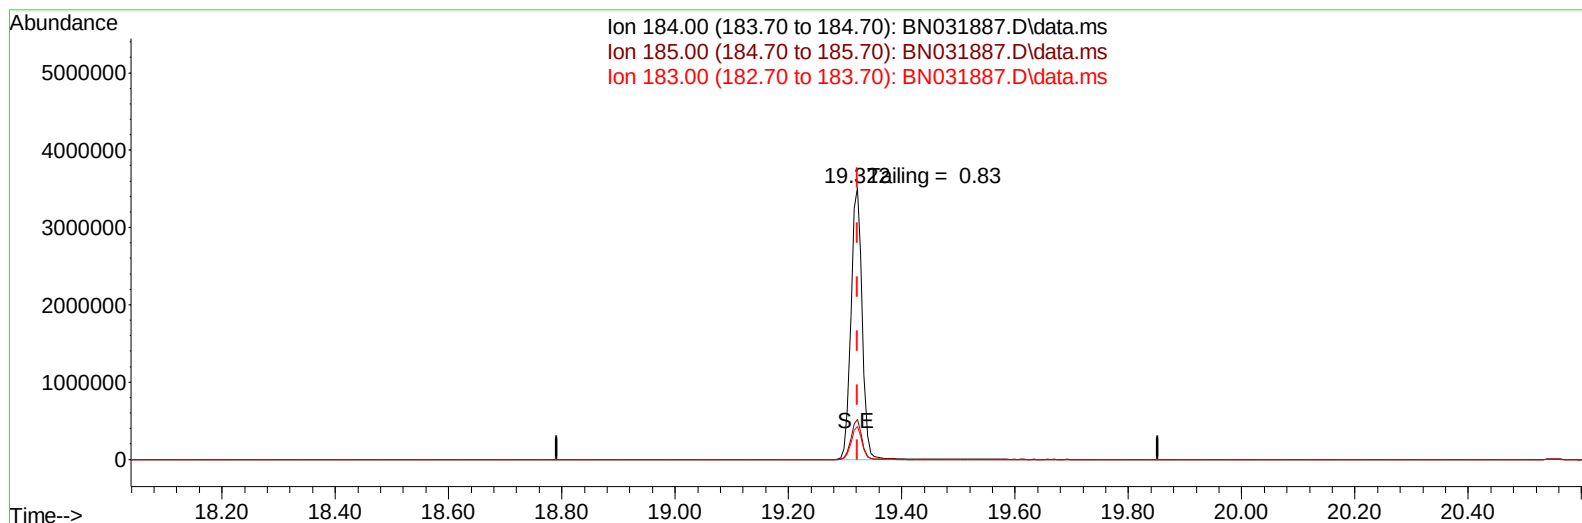

TIC: BN031887.D\data.ms

(77) Benzidine

19.322min (0.000) 0.00 ng

response 4844622

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.84
183.00	13.20	12.05
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/10/2024	BNA_N	<u>BN031887.D</u>
Compound Name	Response	Retention Time
DDT	2221349	20.551
DDD	25364	20.163
DDE	636	19.598
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26000	2247349	1.16

Instrument :
BNA_N
ClientSampleId :
DFTPP