


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061120\
 Data File : BN010833.D
 Acq On : 11 Jun 2020 10:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN061020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 10 15:14:26 2020

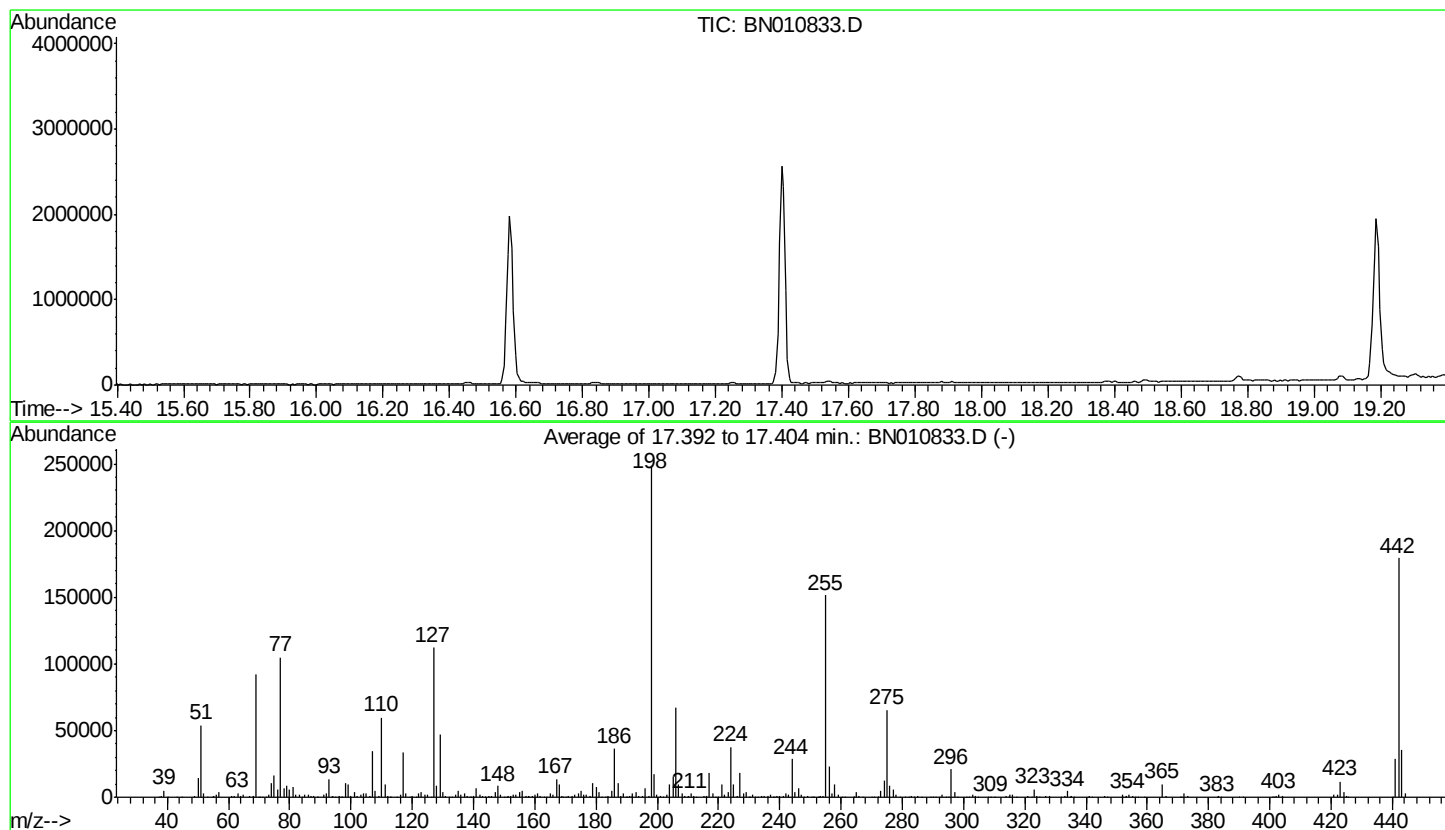

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.7	54085	PASS
68	69	0.00	2	1.0	963	PASS
69	198	0.00	100	37.0	91906	PASS
70	69	0.00	2	0.4	400	PASS
127	198	10	80	45.1	112272	PASS
197	198	0.00	2	0.3	665	PASS
198	198	100	100	100.0	248704	PASS
199	198	5	9	6.8	16916	PASS
275	198	10	60	26.3	65338	PASS
365	198	1	100	4.0	9979	PASS
441	198	0.01	100	11.7	29205	PASS
442	198	50	100	72.1	179325	PASS
443	442	15	24	19.6	35160	PASS