

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020094.D
 Acq On : 10 Jun 2022 11:17
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD020315

Quant Time: Jun 10 22:45:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	161800	20.000	ng/u1	0.00
20) Naphthalene-d8	10.610	136	754636	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.445	164	486886	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.186	188	991963	20.000	ng/u1	0.00
79) Chrysene-d12	21.380	240	894019	20.000	ng/u1	0.00
88) Perylene-d12	23.704	264	834912	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	29281	7.838	ng/uL	0.00
4) Pyridine-d5	3.687	84	197718	19.364	ng/u1	0.00
7) Phenol-d5	6.987	99	262792	19.628	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.152	67	165961	19.840	ng/u1	0.00
11) 2-Chlorophenol-d4	7.352	132	218712	20.105	ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	232306	20.055	ng/u1	0.00
21) Nitrobenzene-d5	8.969	128	113719	19.808	ng/u1	0.00
24) 2-Nitrophenol-d4	9.693	143	124754	20.475	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	217468	20.445	ng/u1	0.00
31) 4-Chloroaniline-d4	10.740	131	338105	19.629	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	687530	19.407	ng/u1	0.00
49) Acenaphthylene-d8	14.140	160	832649	20.267	ng/u1	0.00
54) 4-Nitrophenol-d4	14.640	143	127638	17.980	ng/u1	0.00
60) Fluorene-d10	15.439	176	580193	19.791	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.557	200	97479	16.965	ng/u1	0.00
73) Anthracene-d10	17.286	188	886320	20.473	ng/u1	0.00
81) Pyrene-d10	19.580	212	977325	20.165	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.557	264	802530	19.646	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.317	88	29696	7.530	ng/uL	97
5) Pyridine	3.705	79	209673	19.588	ng/u1	93
6) Benzaldehyde	6.958	77	155679	24.678	ng/u1	94
8) Phenol	7.010	94	286233	20.077	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.240	93	222814	19.968	ng/u1	98
12) 2-Chlorophenol	7.381	128	231859	20.391	ng/u1	97
13) 2-Methylphenol	8.263	108	219866	20.061	ng/u1	97
14) 2,2'-oxybis(1-Chloropr...	8.352	45	349844	19.994	ng/u1	97
16) Acetophenone	8.634	105	361196	20.505	ng/u1	97
17) N-Nitroso-di-n-propyla...	8.622	70	183739	20.418	ng/u1	94
18) 4-Methylphenol	8.587	108	246625	20.388	ng/u1	98
19) Hexachloroethane	8.899	117	89493	19.560	ng/u1	88
22) Nitrobenzene	9.010	77	265884	19.974	ng/u1	98
23) Isophorone	9.534	82	510971	19.441	ng/u1	99
25) 2-Nitrophenol	9.722	139	139097	20.660	ng/u1	97
26) 2,4-Dimethylphenol	9.787	107	278373	19.958	ng/u1	95
27) Bis(2-Chloroethoxy)met...	10.022	93	319035	19.836	ng/u1	97
29) 2,4-Dichlorophenol	10.257	162	224539	20.408	ng/u1	99
30) Naphthalene	10.657	128	781037	19.970	ng/u1	99
32) 4-Chloroaniline	10.763	127	340746	19.778	ng/u1	100
33) Hexachlorobutadiene	10.957	225	125574	19.879	ng/u1	97
34) Caprolactam	11.516	113	50900	11.847	ng/u1	99
35) 4-Chloro-3-methylphenol	11.893	107	265668	20.449	ng/u1	99
36) 2-Methylnaphthalene	12.269	142	527566	19.953	ng/u1	96

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020094.D
 Acq On : 10 Jun 2022 11:17
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1


Instrument :
 BNA_N
 ClientSampleId :
 SSTD020315


Quant Time: Jun 10 22:45:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.493	142	541560	20.071	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.645	216	243676	19.623	ng/ul	99
40) Hexachlorocyclopentadiene	12.628	237	134697	17.832	ng/ul	96
41) 2,4,6-Trichlorophenol	12.881	196	175224	20.464	ng/ul	95
42) 2,4,5-Trichlorophenol	12.951	196	192409	20.290	ng/ul	99
43) 1,1'-Biphenyl	13.281	154	714100	19.807	ng/ul	99
44) 2-Chloronaphthalene	13.322	162	540846	19.775	ng/ul	96
45) 2-Nitroaniline	13.522	65	170067	19.987	ng/ul	95
47) Dimethylphthalate	13.904	163	687946	19.290	ng/ul	99
48) 2,6-Dinitrotoluene	14.022	165	140780	20.190	ng/ul	93
50) Acenaphthylene	14.169	152	895843	19.695	ng/ul	99
51) 3-Nitroaniline	14.345	138	151138	20.503	ng/ul	98
52) Acenaphthene	14.510	153	582989	19.622	ng/ul	99
53) 2,4-Dinitrophenol	14.557	184	40034	8.967	ng/ul	98
55) 4-Nitrophenol	14.657	109	109843	18.127	ng/ul	97
56) Dibenzofuran	14.845	168	827525	19.769	ng/ul	99
57) 2,4-Dinitrotoluene	14.804	165	209237	20.266	ng/ul	95
58) 2,3,4,6-Tetrachlorophenol	15.069	232	143862	19.326	ng/ul	91
59) Diethylphthalate	15.269	149	707751	19.276	ng/ul	98
61) Fluorene	15.492	166	648275	19.903	ng/ul	97
62) 4-Chlorophenyl-phenyle...	15.487	204	295042	19.669	ng/ul	92
63) 4-Nitroaniline	15.504	138	147209	21.371	ng/ul	98
66) 4,6-Dinitro-2-methylph...	15.569	198	95251	16.350	ng/ul#	87
67) N-Nitrosodiphenylamine	15.698	169	577723	20.315	ng/ul	99
68) 4-Bromophenyl-phenylether	16.381	248	177286	20.523	ng/ul#	89
69) Hexachlorobenzene	16.504	284	196439	19.782	ng/ul	93
70) Atrazine	16.651	200	201234	20.281	ng/ul	97
71) Pentachlorophenol	16.839	266	93820	15.170	ng/ul	97
72) Phenanthrene	17.228	178	1035140	19.774	ng/ul	98
74) Anthracene	17.322	178	1044838	19.849	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.245	216	263636	19.847	ng/ul	98
76) Pentachlorobenzene	14.769	250	239449	20.396	ng/ul	94
77) Carbazole	17.586	167	974322	20.346	ng/ul	96
78) Di-n-butylphthalate	18.157	149	1196127	20.143	ng/ul	100
80) Fluoranthene	19.245	202	1180916	20.174	ng/ul	97
82) Pyrene	19.610	202	1208291	20.120	ng/ul	94
83) Butylbenzylphthalate	20.516	149	560606	20.743	ng/ul	95
84) 3,3'-Dichlorobenzidine	21.298	252	354588	20.766	ng/ul#	96
85) Benzo(a)anthracene	21.363	228	1131675	20.046	ng/ul	96
86) Bis(2-ethylhexyl)phtha...	21.304	149	800595	20.995	ng/ul	96
87) Chrysene	21.416	228	1075228	19.468	ng/ul	98
89) Di-n-octyl phthalate	22.204	149	1382496	20.345	ng/ul	100
90) Benzo(b)fluoranthene	23.051	252	985443	18.806	ng/ul	98
91) Benzo(k)fluoranthene	23.051	252	985443	19.755	ng/ul	95
93) Benzo(a)pyrene	23.604	252	1002462	19.764	ng/ul	96
94) Indeno(1,2,3-cd)pyrene	26.098	276	955645	18.312	ng/ul#	93
95) Dibenzo(a,h)anthracene	26.109	278	828581	18.589	ng/ul	98
96) Benzo(g,h,i)perylene	26.833	276	809408	18.366	ng/ul#	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jun 10 22:45:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration









#2
 1,4-Dioxane
 Concen: 7.530 ng/uL
 RT: 3.317 min Scan# 39
 Delta R.T. 0.001 min
 Lab File: BN020094.D
 Acq: 10 Jun 2022 11:17




Instrument :
 BNA_N
 ClientSampleId :
 SST020315


Tgt Ion: 88 Resp: 29696
 Ion Ratio Lower Upper
 88 100
 43 30.7 22.4 33.6
 58 78.1 61.0 91.4



#5
 Pyridine
 Concen: 19.588 ng/uL
 RT: 3.705 min Scan# 105
 Delta R.T. -0.006 min
 Lab File: BN020094.D
 Acq: 10 Jun 2022 11:17

Tgt Ion: 79 Resp: 209673
 Ion Ratio Lower Upper
 79 100
 52 89.4 65.0 97.4
 51 41.0 31.6 47.4









#6
Benzaldehyde
Concen: 24.678 ng/ul
RT: 6.958 min Scan# 658
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion: 77 Resp: 155679
Ion Ratio Lower Upper
77 100
105 98.2 74.7 112.1
106 93.5 70.2 105.4

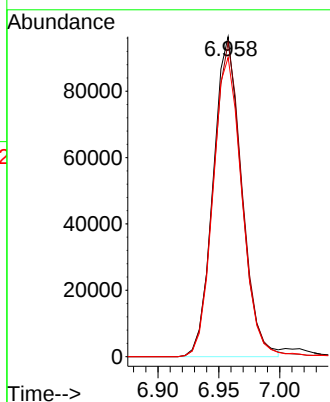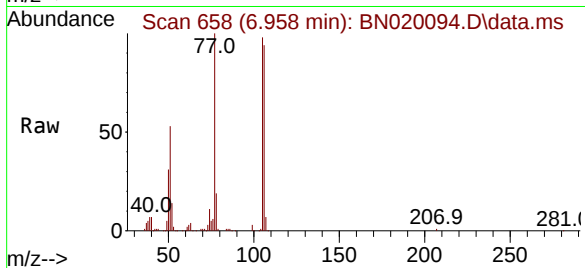

#8
Phenol
Concen: 20.077 ng/ul
RT: 7.010 min Scan# 667
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion: 94 Resp: 286233
Ion Ratio Lower Upper
94 100
65 29.2 23.6 35.4
66 41.2 31.2 46.8

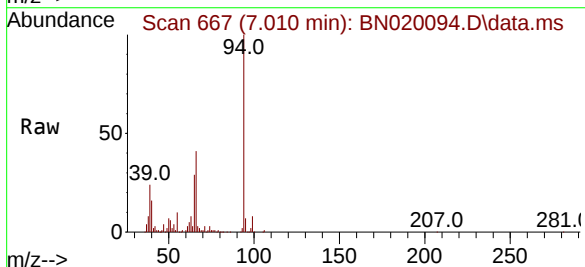



#10

Bis(2-Chloroethyl)ether

Concen: 19.968 ng/ul

RT: 7.240 min Scan# 706

Delta R.T. -0.006 min

Lab File: BN020094.D

Acq: 10 Jun 2022 11:17

Instrument :

BNA_N

ClientSampleId :

SSTD020315





Tgt Ion: 93 Resp: 222814

Ion Ratio Lower Upper

93 100

63 81.1 63.4 95.0

95 32.8 26.2 39.2

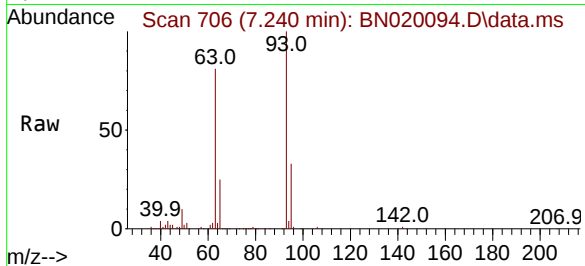

#12

2-Chlorophenol

Concen: 20.391 ng/ul

RT: 7.381 min Scan# 730

Delta R.T. -0.006 min

Lab File: BN020094.D

Acq: 10 Jun 2022 11:17




Tgt Ion:128 Resp: 231859


Ion Ratio Lower Upper

128 100

64 50.0 38.6 57.8

130 33.4 25.0 37.4



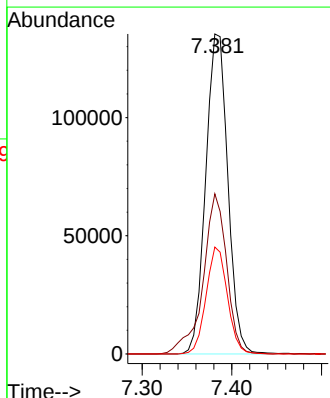
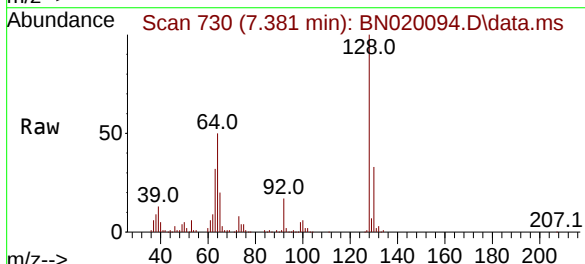




#13
2-Methylphenol
Concen: 20.061 ng/ul
RT: 8.263 min Scan# 880
Delta R.T. 0.000 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion:108 Resp: 219866
Ion Ratio Lower Upper
108 100
107 92.0 71.5 107.3



#14
2,2'-oxybis(1-Chloropropane)
Concen: 19.994 ng/ul
RT: 8.352 min Scan# 895
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion: 45 Resp: 349844
Ion Ratio Lower Upper
45 100
77 12.7 10.9 16.3
79 9.3 8.6 13.0


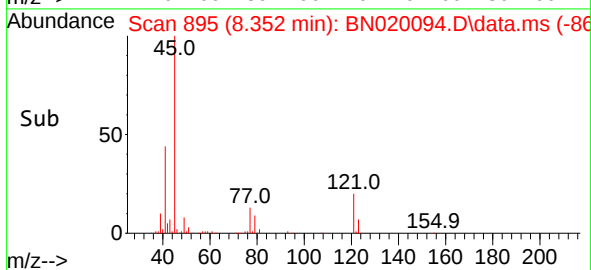






#16
Acetophenone
Concen: 20.505 ng/ul
RT: 8.634 min Scan# 943
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion:105 Resp: 361196
Ion Ratio Lower Upper
105 100
77 76.9 63.5 95.3
51 30.3 23.5 35.3



#17
N-Nitroso-di-n-propylamine
Concen: 20.418 ng/ul
RT: 8.622 min Scan# 941
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion: 70 Resp: 183739
Ion Ratio Lower Upper
70 100
42 64.7 47.8 71.6
101 10.9 7.8 11.6
130 23.1 15.8 23.8


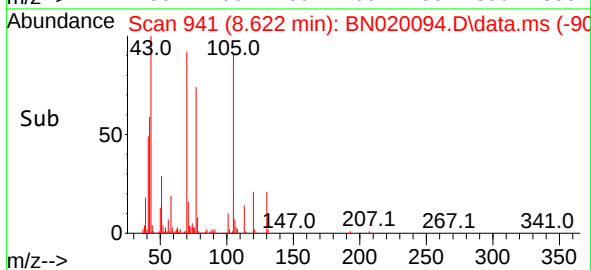






#18
4-Methylphenol
Concen: 20.388 ng/ul
RT: 8.587 min Scan# 911
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion:108 Resp: 246625
Ion Ratio Lower Upper
108 100
107 108.2 88.0 132.0

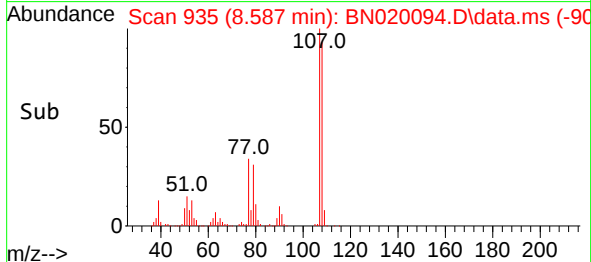

#19
Hexachloroethane
Concen: 19.560 ng/ul
RT: 8.899 min Scan# 988
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion:117 Resp: 89493
Ion Ratio Lower Upper
117 100
201 89.0 83.2 124.8
199 56.6 50.2 75.4




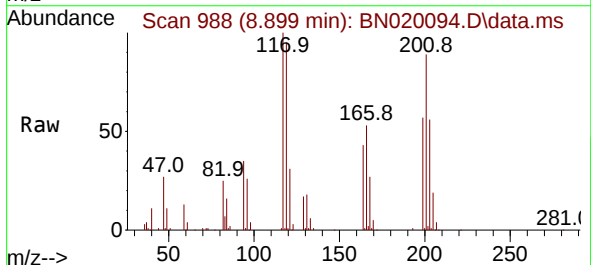




#22
Nitrobenzene
Concen: 19.974 ng/ul
RT: 9.010 min Scan# 1007
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion: 77 Resp: 265884
Ion Ratio Lower Upper
77 100
123 45.0 34.5 51.7
65 14.3 11.1 16.7

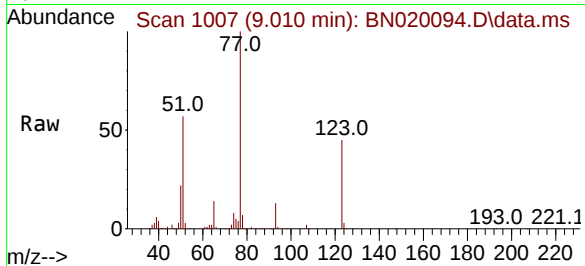

#23
Isophorone
Concen: 19.441 ng/ul
RT: 9.534 min Scan# 1096
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion: 82 Resp: 510971
Ion Ratio Lower Upper
82 100
95 7.6 5.8 8.8
138 17.6 13.8 20.8

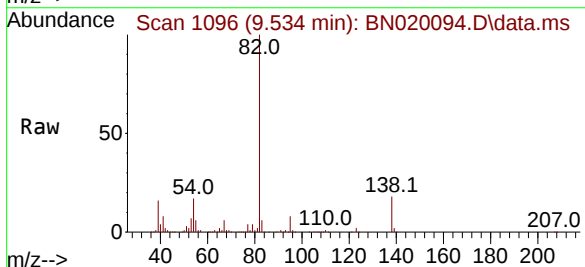

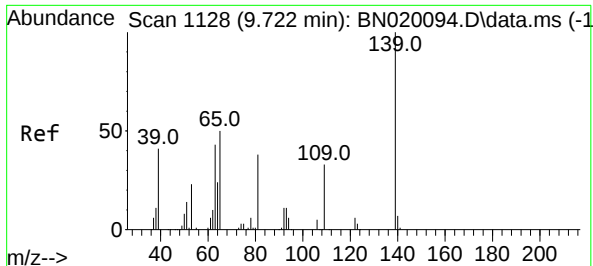

#25

2-Nitrophenol

Concen: 20.660 ng/ul

RT: 9.722 min Scan# 1128

Delta R.T. -0.006 min

Lab File: BN020094.D

Acq: 10 Jun 2022 11:17

Instrument :

BNA_N

ClientSampleId :

SSTD020315





Tgt Ion:139 Resp: 139097

Ion Ratio Lower Upper

139 100

65 51.8 43.7 65.5

109 32.7 25.8 38.6

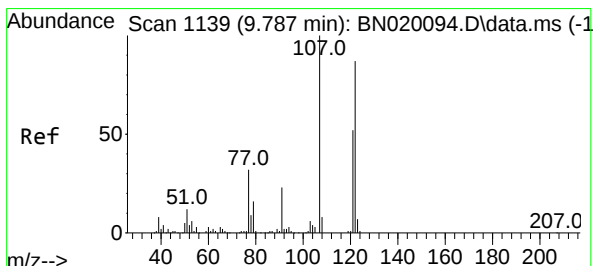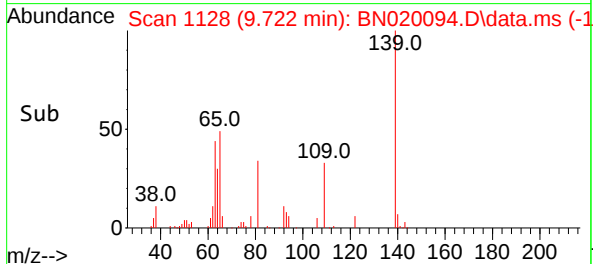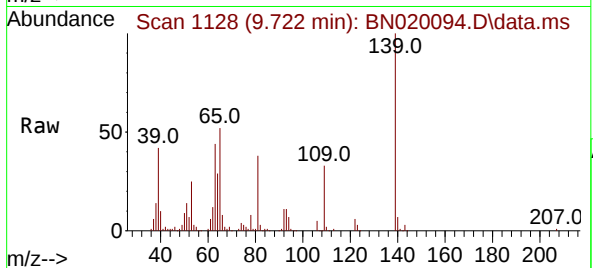

#26

2,4-Dimethylphenol

Concen: 19.958 ng/ul

RT: 9.787 min Scan# 1139

Delta R.T. -0.006 min

Lab File: BN020094.D

Acq: 10 Jun 2022 11:17




Tgt Ion:107 Resp: 278373


Ion Ratio Lower Upper

107 100

121 51.9 38.3 57.5

122 87.5 66.3 99.5


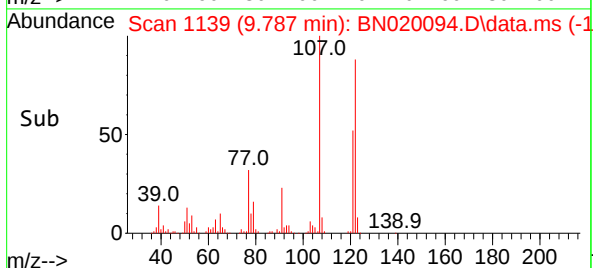

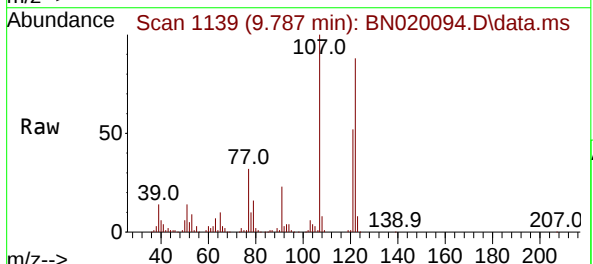




#27
 Bis(2-Chloroethoxy)methane
 Concen: 19.836 ng/ul
 RT: 10.022 min Scan# 1179
 Delta R.T. -0.006 min
 Lab File: BN020094.D
 Acq: 10 Jun 2022 11:17




Instrument :
 BNA_N
 ClientSampleId :
 SSTD020315


Tgt Ion: 93 Resp: 319035
 Ion Ratio Lower Upper
 93 100
 95 32.9 25.4 38.0
 123 11.7 8.3 12.5



#29
 2,4-Dichlorophenol
 Concen: 20.408 ng/ul
 RT: 10.257 min Scan# 1219
 Delta R.T. -0.006 min
 Lab File: BN020094.D
 Acq: 10 Jun 2022 11:17

Tgt Ion: 162 Resp: 224539
 Ion Ratio Lower Upper
 162 100
 164 65.7 52.9 79.3
 98 38.4 29.8 44.8


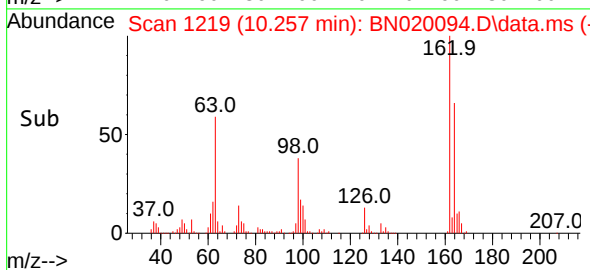






#30
Naphthalene
Concen: 19.970 ng/ul
RT: 10.657 min Scan# 1287
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion:128 Resp: 781037
Ion Ratio Lower Upper
128 100
129 10.6 8.7 13.1
127 13.1 10.6 16.0

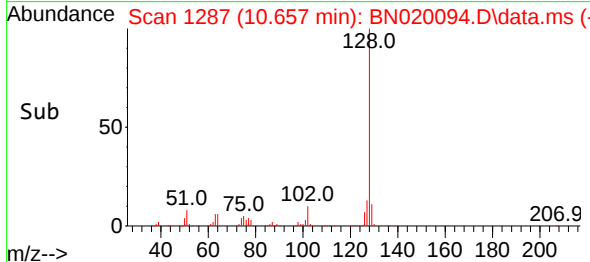

#32
4-Chloroaniline
Concen: 19.778 ng/ul
RT: 10.763 min Scan# 1305
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion:127 Resp: 340746
Ion Ratio Lower Upper
127 100
129 32.4 26.1 39.1




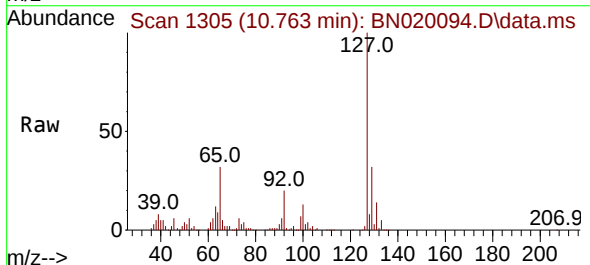




#33
Hexachlorobutadiene
Concen: 19.879 ng/ul
RT: 10.957 min Scan# 1338
Delta R.T. 0.000 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion:225 Resp: 125574
Ion Ratio Lower Upper
225 100
223 60.5 51.8 77.6
227 64.0 50.6 76.0

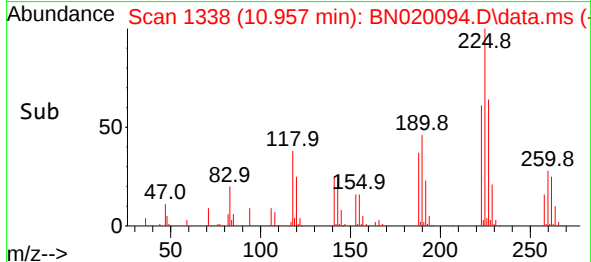

#34
Caprolactam
Concen: 11.847 ng/ul
RT: 11.516 min Scan# 1433
Delta R.T. 0.000 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion:113 Resp: 50900
Ion Ratio Lower Upper
113 100
55 181.2 145.5 218.3
56 130.9 106.5 159.7




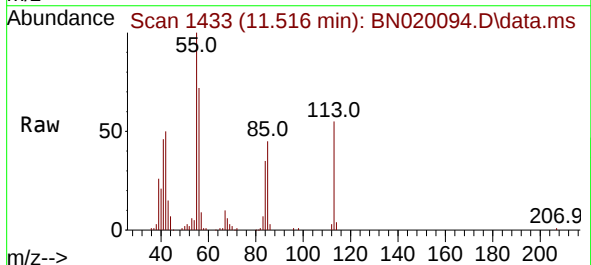




#35
4-Chloro-3-methylphenol
Concen: 20.449 ng/ul
RT: 11.893 min Scan# 1497
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion:107 Resp: 265668
Ion Ratio Lower Upper
107 100
144 25.5 20.6 31.0
142 76.9 62.2 93.4



#36
2-Methylnaphthalene
Concen: 19.953 ng/ul
RT: 12.269 min Scan# 1561
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion:142 Resp: 527566
Ion Ratio Lower Upper
142 100
141 91.5 70.6 105.8


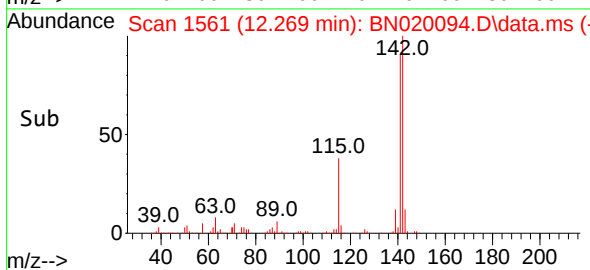






#37
1-Methylnaphthalene
Concen: 20.071 ng/ul
RT: 12.493 min Scan# 1599
Delta R.T. 0.000 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion:142 Resp: 541560
Ion Ratio Lower Upper
142 100
141 88.7 70.9 106.3
116 3.8 3.1 4.7



#39
1,2,4,5-Tetrachlorobenzene
Concen: 19.623 ng/ul
RT: 12.645 min Scan# 1625
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion:216 Resp: 243676
Ion Ratio Lower Upper
216 100
214 79.1 63.4 95.0
179 23.2 17.8 26.8
108 19.6 15.1 22.7


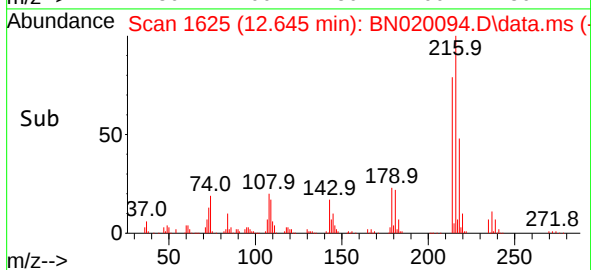






#40
Hexachlorocyclopentadiene
Concen: 17.832 ng/ul
RT: 12.628 min Scan# 1622
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion:237 Resp: 134697
Ion Ratio Lower Upper
237 100
235 63.9 48.8 73.2
272 13.1 9.3 13.9

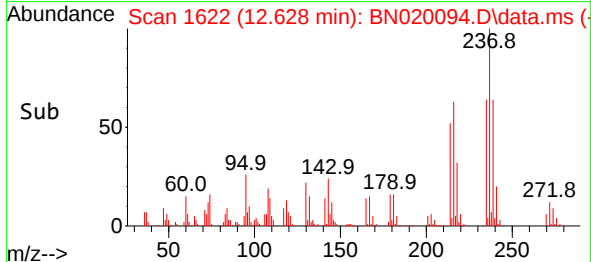

#41
2,4,6-Trichlorophenol
Concen: 20.464 ng/ul
RT: 12.881 min Scan# 1665
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion:196 Resp: 175224
Ion Ratio Lower Upper
196 100
198 92.8 79.8 119.8
200 30.9 25.0 37.6


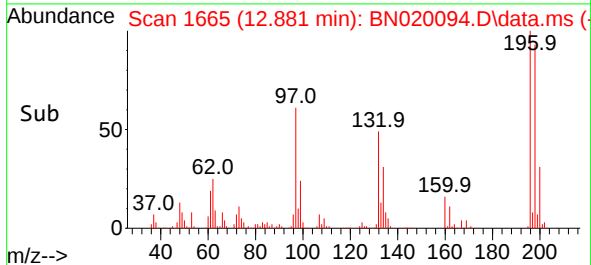






#42
2,4,5-Trichlorophenol
Concen: 20.290 ng/ul
RT: 12.951 min Scan# 1677
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion:196 Resp: 192409
Ion Ratio Lower Upper
196 100
198 95.8 77.6 116.4
200 29.3 24.4 36.6



#43
1,1'-Biphenyl
Concen: 19.807 ng/ul
RT: 13.281 min Scan# 1733
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion:154 Resp: 714100
Ion Ratio Lower Upper
154 100
153 38.4 31.5 47.3
76 13.1 10.5 15.7


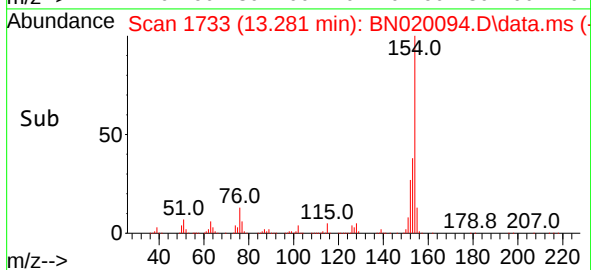






#44
2-Chloronaphthalene
Concen: 19.775 ng/ul
RT: 13.322 min Scan# 1740
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion:162 Resp: 540846
Ion Ratio Lower Upper
162 100
164 33.1 25.8 38.6
127 42.7 31.4 47.2

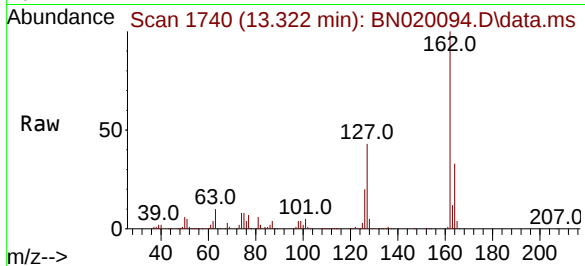

#45
2-Nitroaniline
Concen: 19.987 ng/ul
RT: 13.522 min Scan# 1774
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion: 65 Resp: 170067
Ion Ratio Lower Upper
65 100
92 67.1 54.1 81.1
138 104.7 77.0 115.4


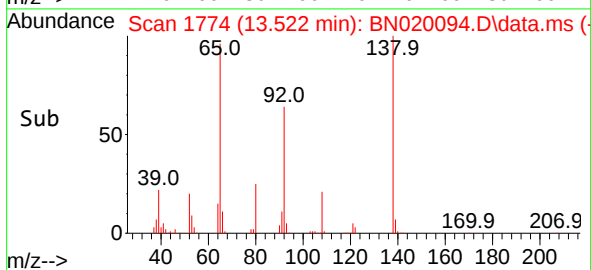

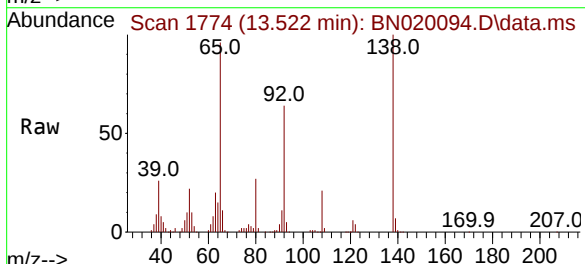




#47
Dimethylphthalate
Concen: 19.290 ng/ul
RT: 13.904 min Scan# 1839
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion:163 Resp: 687946
Ion Ratio Lower Upper
163 100
194 3.8 3.4 5.0
164 9.7 7.7 11.5

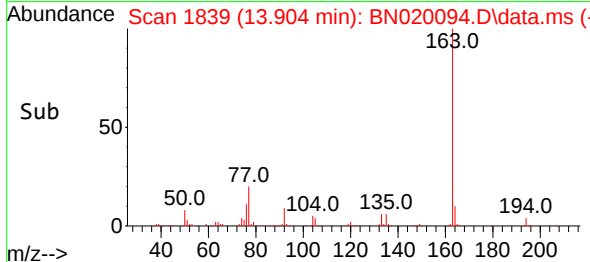

#48
2,6-Dinitrotoluene
Concen: 20.190 ng/ul
RT: 14.022 min Scan# 1859
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion:165 Resp: 140780
Ion Ratio Lower Upper
165 100
89 56.2 50.6 75.8
121 21.4 17.9 26.9

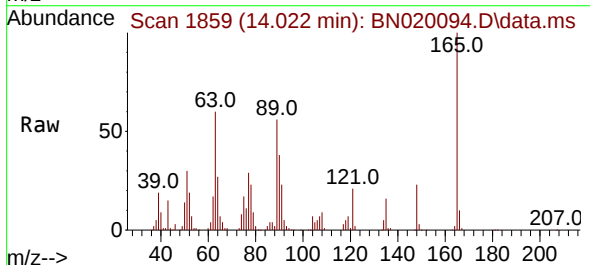




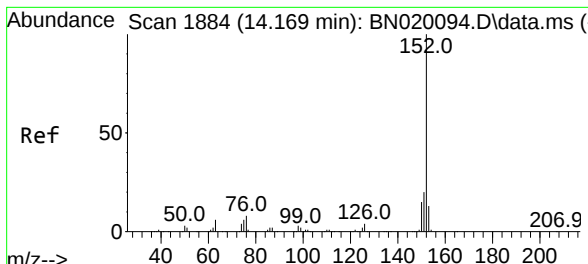


#50
 Acenaphthylene
 Concen: 19.695 ng/ul
 RT: 14.169 min Scan# 1884
 Delta R.T. 0.000 min
 Lab File: BN020094.D
 Acq: 10 Jun 2022 11:17

Instrument :
 BNA_N
 ClientSampleId :
 SSTD020315

Tgt Ion:152 Resp: 895843




Ion	Ratio	Lower	Upper
152	100		
151	20.2	16.0	24.0
153	12.9	10.7	16.1

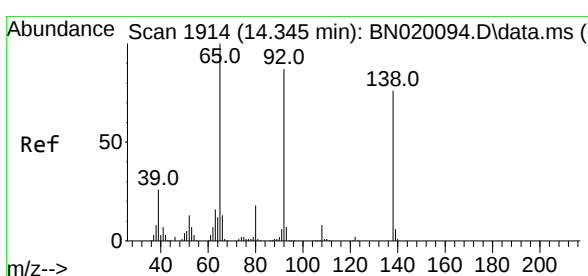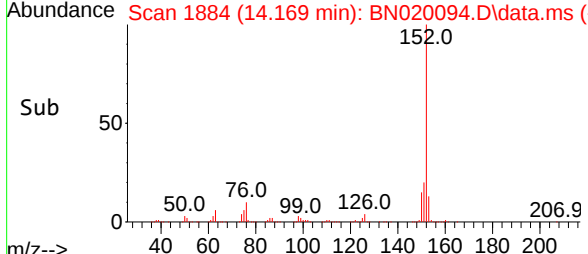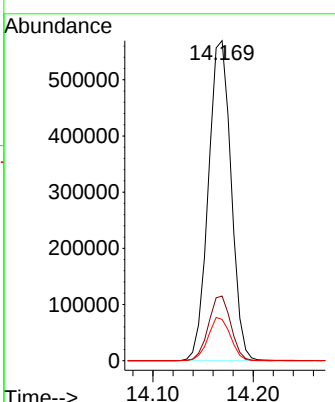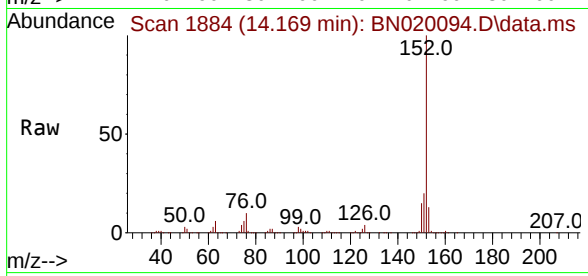


#51
 3-Nitroaniline
 Concen: 20.503 ng/ul
 RT: 14.345 min Scan# 1914
 Delta R.T. -0.006 min
 Lab File: BN020094.D
 Acq: 10 Jun 2022 11:17

Tgt Ion:138 Resp: 151138

Ion	Ratio	Lower	Upper
138	100		
108	10.7	8.6	12.8
92	114.1	92.9	139.3


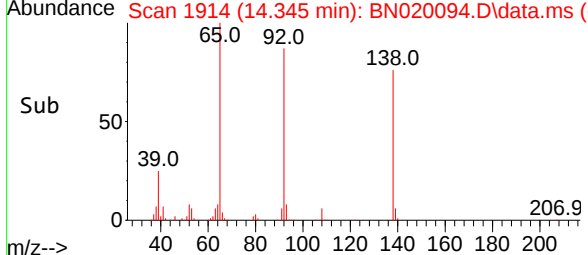
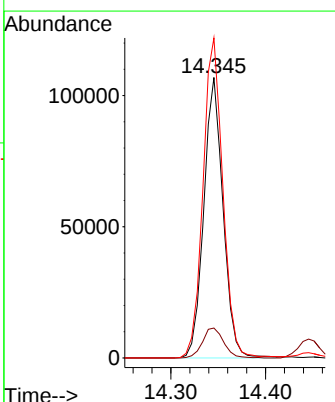
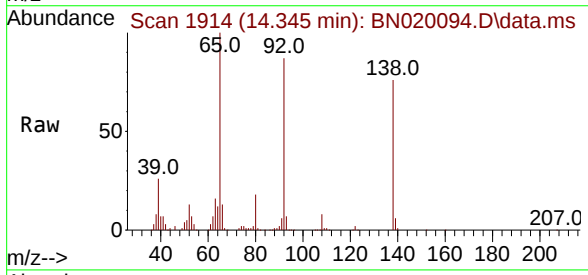




#52
Acenaphthene
Concen: 19.622 ng/ul
RT: 14.510 min Scan# 1942
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion:153 Resp: 582989
Ion Ratio Lower Upper
153 100
152 46.6 38.4 57.6
154 86.5 69.7 104.5



#53
2,4-Dinitrophenol
Concen: 8.967 ng/ul
RT: 14.557 min Scan# 1950
Delta R.T. 0.000 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion:184 Resp: 40034
Ion Ratio Lower Upper
184 100
63 70.0 55.9 83.9
154 62.7 53.1 79.7


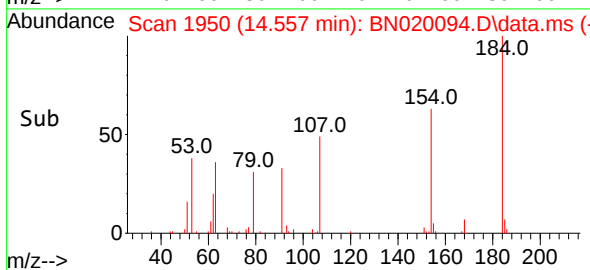






#55
4-Nitrophenol
Concen: 18.127 ng/ul
RT: 14.657 min Scan# 1967
Delta R.T. 0.000 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion:109 Resp: 109843
Ion Ratio Lower Upper
109 100
139 128.8 100.1 150.1
65 127.6 104.6 157.0

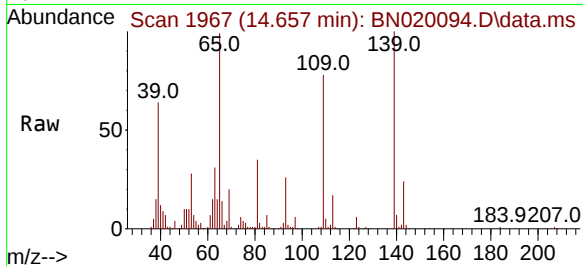

#56
Dibenzofuran
Concen: 19.769 ng/ul
RT: 14.845 min Scan# 1999
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion:168 Resp: 827525
Ion Ratio Lower Upper
168 100
139 38.4 31.1 46.7




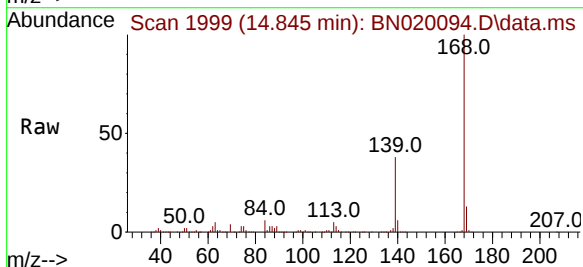




#57
2,4-Dinitrotoluene
Concen: 20.266 ng/ul
RT: 14.804 min Scan# 1992
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion:165 Resp: 209237
Ion Ratio Lower Upper
165 100
63 48.8 36.3 54.5
182 2.8 2.3 3.5



#58
2,3,4,6-Tetrachlorophenol
Concen: 19.326 ng/ul
RT: 15.069 min Scan# 2037
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion:232 Resp: 143862
Ion Ratio Lower Upper
232 100
131 56.6 38.5 57.7
130 2.8 2.2 3.2
166 35.5 25.8 38.8









#59
Diethylphthalate
Concen: 19.276 ng/ul
RT: 15.269 min Scan# 2071
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion:149 Resp: 707751
Ion Ratio Lower Upper
149 100
177 21.2 17.8 26.8
150 12.2 10.5 15.7

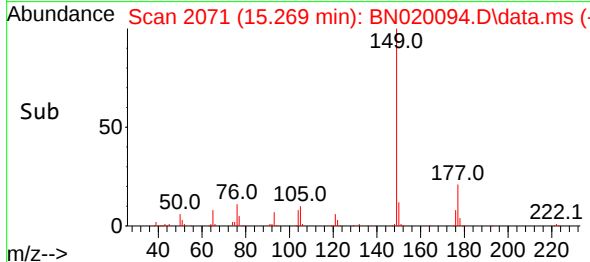

#61
Fluorene
Concen: 19.903 ng/ul
RT: 15.492 min Scan# 2109
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion:166 Resp: 648275
Ion Ratio Lower Upper
166 100
165 100.4 77.7 116.5
167 13.2 11.1 16.7




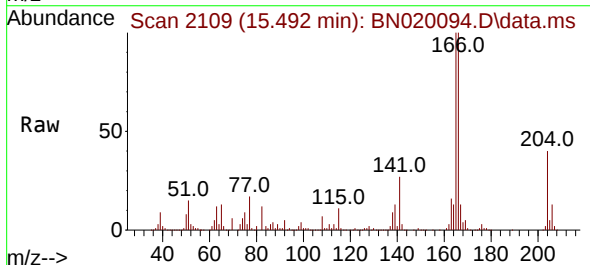




#62
4-Chlorophenyl-phenylether
Concen: 19.669 ng/ul
RT: 15.487 min Scan# 2108
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion:204 Resp: 295042
Ion Ratio Lower Upper
204 100
206 34.6 26.7 40.1
141 71.6 50.2 75.2

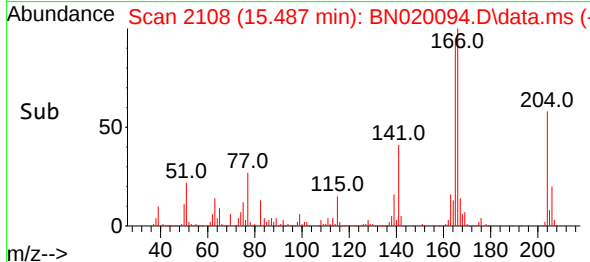

#63
4-Nitroaniline
Concen: 21.371 ng/ul
RT: 15.504 min Scan# 2111
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion:138 Resp: 147209
Ion Ratio Lower Upper
138 100
92 49.9 41.0 61.6
108 83.6 65.3 97.9




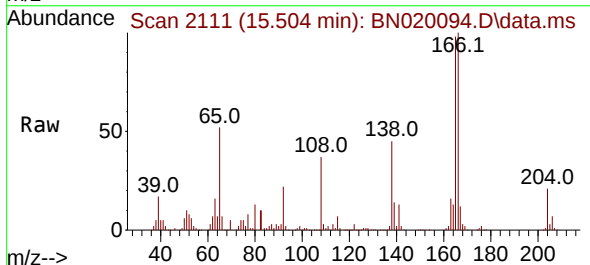




#66
 4,6-Dinitro-2-methylphenol
 Concen: 16.350 ng/ul
 RT: 15.569 min Scan# 2122
 Delta R.T. -0.006 min
 Lab File: BN020094.D
 Acq: 10 Jun 2022 11:17




Instrument :
 BNA_N
 ClientSampleId :
 SSTD020315


Tgt Ion:198 Resp: 95251
 Ion Ratio Lower Upper
 198 100
 182 4.3 3.0 4.4
 77 32.7 20.1 30.1#

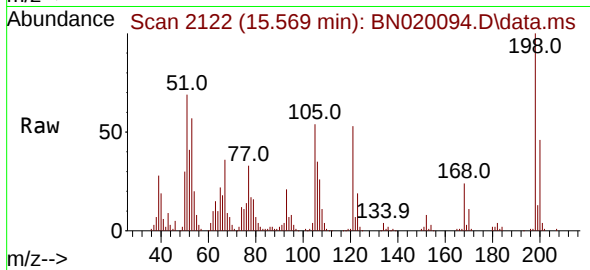

#67
 N-Nitrosodiphenylamine
 Concen: 20.315 ng/ul
 RT: 15.698 min Scan# 2144
 Delta R.T. -0.006 min
 Lab File: BN020094.D
 Acq: 10 Jun 2022 11:17

Tgt Ion:169 Resp: 577723
 Ion Ratio Lower Upper
 169 100
 168 65.2 52.4 78.6
 167 35.7 27.5 41.3


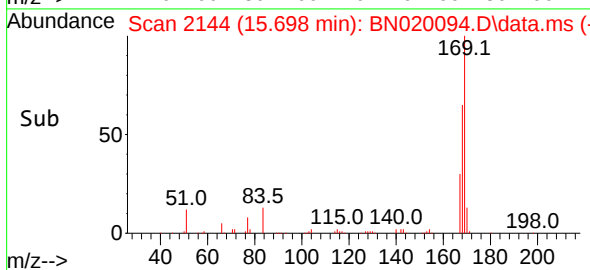






#68
4-Bromophenyl-phenylether
Concen: 20.523 ng/ul
RT: 16.381 min Scan# 2260
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion:248 Resp: 177286
Ion Ratio Lower Upper
248 100
250 100.8 77.8 116.8
141 95.6 62.6 93.8#



#69
Hexachlorobenzene
Concen: 19.782 ng/ul
RT: 16.504 min Scan# 2281
Delta R.T. 0.000 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion:284 Resp: 196439
Ion Ratio Lower Upper
284 100
142 41.1 27.8 41.8
249 30.4 25.7 38.5


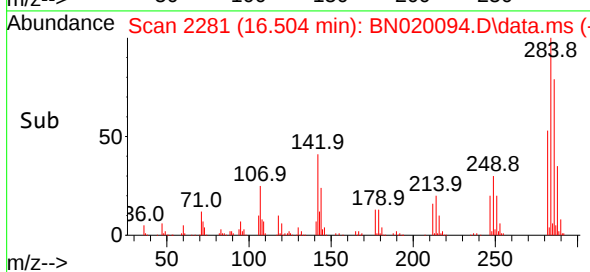






#70
Atrazine
Concen: 20.281 ng/ul
RT: 16.651 min Scan# 21
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion:200 Resp: 201234
Ion Ratio Lower Upper
200 100
173 27.9 20.5 30.7
215 47.0 38.9 58.3



#71
Pentachlorophenol
Concen: 15.170 ng/ul
RT: 16.839 min Scan# 2338
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion:266 Resp: 93820
Ion Ratio Lower Upper
266 100
264 58.0 50.2 75.2
268 61.2 49.3 73.9




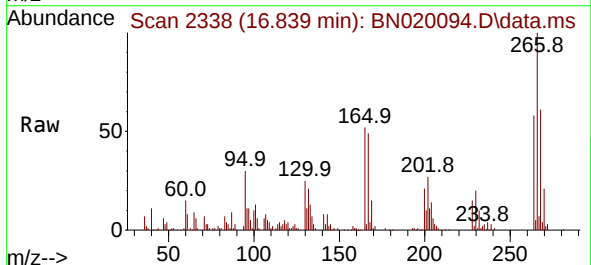




#72
Phenanthrene
Concen: 19.774 ng/ul
RT: 17.228 min Scan# 2404
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion:178 Resp: 1035140
Ion Ratio Lower Upper
178 100
179 15.9 12.2 18.4
176 19.7 15.2 22.8

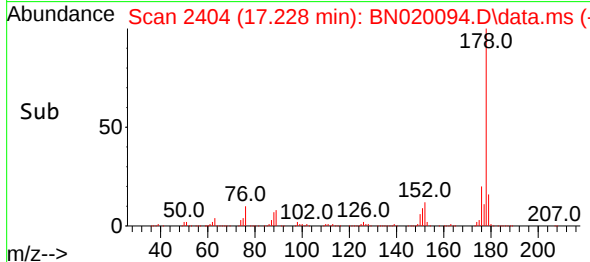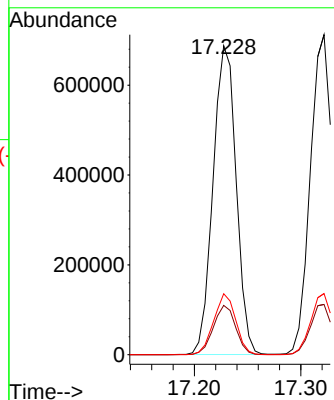

#74
Anthracene
Concen: 19.849 ng/ul
RT: 17.322 min Scan# 2420
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion:178 Resp: 1044838
Ion Ratio Lower Upper
178 100
179 15.7 13.0 19.4
176 19.1 15.5 23.3



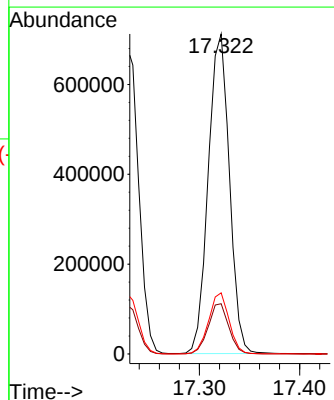
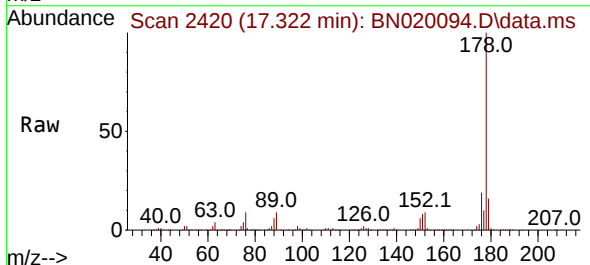




#75
1,2,3,4-Tetrachlorobenzene
Concen: 19.847 ng/uL
RT: 13.245 min Scan# 11
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion:216 Resp: 263636
Ion Ratio Lower Upper
216 100
214 81.3 63.2 94.8
218 46.8 37.9 56.9

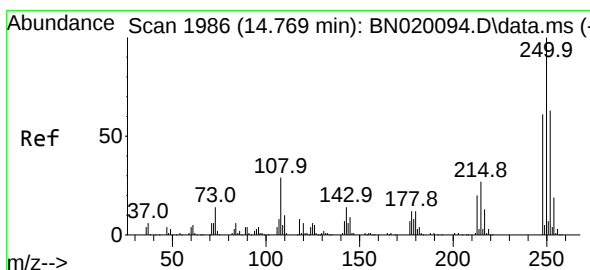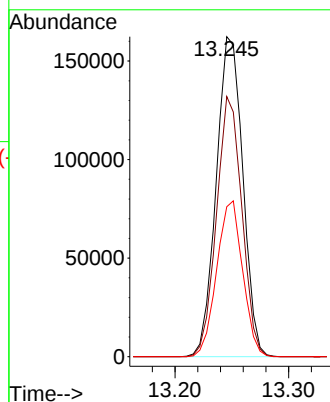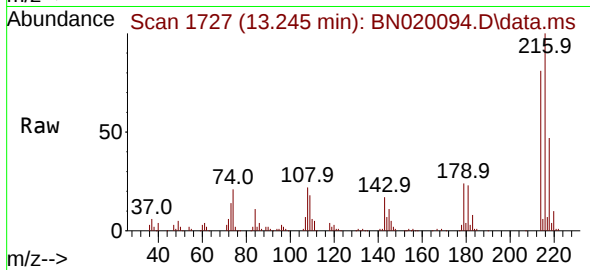

#76
Pentachlorobenzene
Concen: 20.396 ng/uL
RT: 14.769 min Scan# 1986
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion:250 Resp: 239449
Ion Ratio Lower Upper
250 100
248 60.7 53.0 79.4
252 62.8 53.4 80.2









#77
 Carbazole
 Concen: 20.346 ng/ul
 RT: 17.586 min Scan# 2465
 Delta R.T. -0.006 min
 Lab File: BN020094.D
 Acq: 10 Jun 2022 11:17




Instrument :
 BNA_N
 ClientSampleId :
 SSTD020315


Tgt Ion:167 Resp: 974322
 Ion Ratio Lower Upper
 167 100
 166 22.3 16.1 24.1
 139 14.3 10.2 15.2

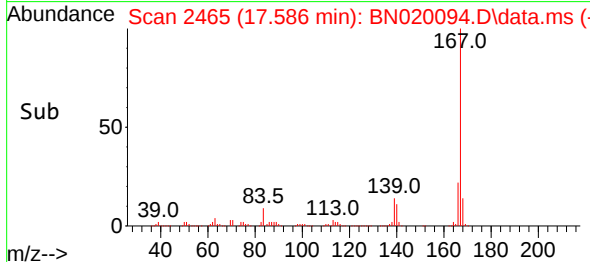

#78
 Di-n-butylphthalate
 Concen: 20.143 ng/ul
 RT: 18.157 min Scan# 2562
 Delta R.T. -0.006 min
 Lab File: BN020094.D
 Acq: 10 Jun 2022 11:17

Tgt Ion:149 Resp: 1196127
 Ion Ratio Lower Upper
 149 100
 150 8.9 7.1 10.7
 104 5.2 4.1 6.1




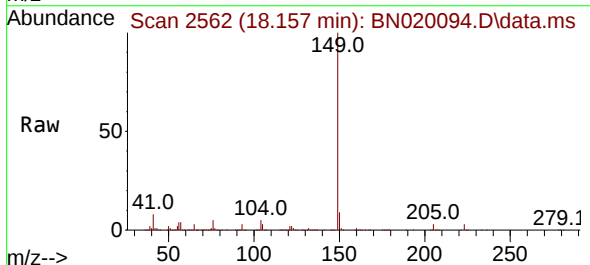


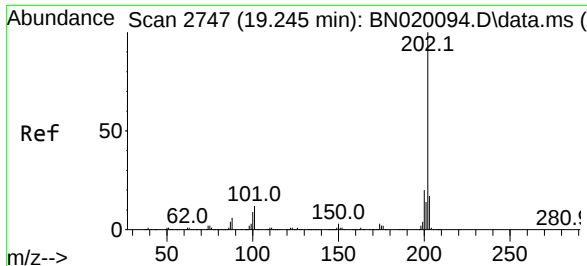

#80
Fluoranthene
Concen: 20.174 ng/ul
RT: 19.245 min Scan# 2747
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion:202 Resp: 1180916
Ion Ratio Lower Upper
202 100
101 12.3 8.9 13.3
100 9.4 6.7 10.1

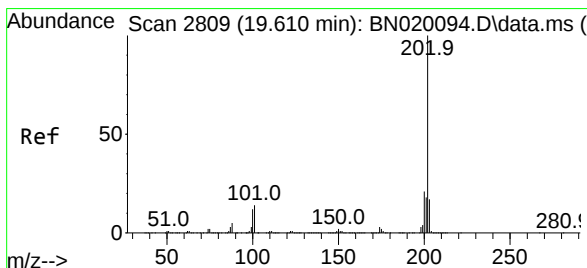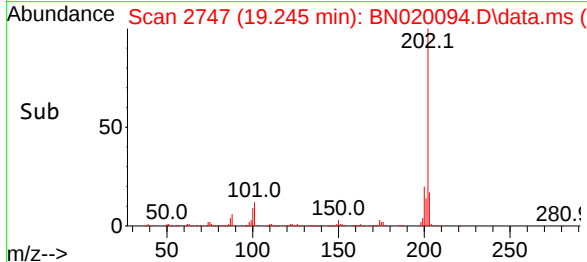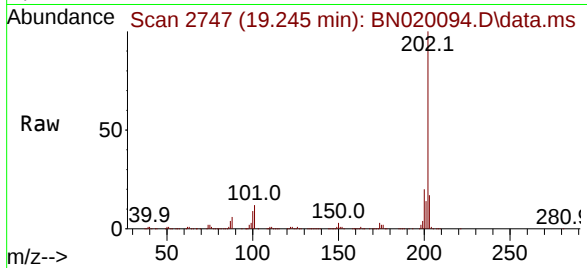

#82
Pyrene
Concen: 20.120 ng/ul
RT: 19.610 min Scan# 2809
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion:202 Resp: 1208291
Ion Ratio Lower Upper
202 100
101 14.5 9.7 14.5
100 11.8 8.0 12.0


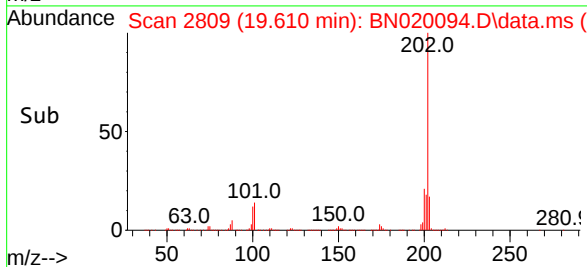

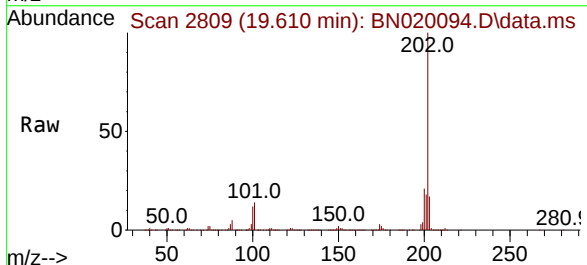




#83
Butylbenzylphthalate
Concen: 20.743 ng/ul
RT: 20.516 min Scan# 2963
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion:149 Resp: 560606
Ion Ratio Lower Upper
149 100
91 70.0 58.8 88.2
206 19.1 18.1 27.1



#84
3,3'-Dichlorobenzidine
Concen: 20.766 ng/ul
RT: 21.298 min Scan# 3096
Delta R.T. 0.000 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion:252 Resp: 354588
Ion Ratio Lower Upper
252 100
254 60.7 50.8 76.2
126 12.7 8.2 12.4#

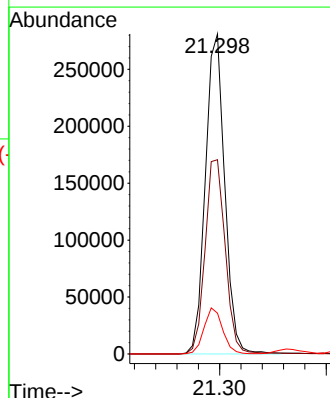



#85

Benzo(a)anthracene

Concen: 20.046 ng/ul

RT: 21.363 min Scan# 3107

Delta R.T. 0.000 min

Lab File: BN020094.D

Acq: 10 Jun 2022 11:17

Instrument :

BNA_N

ClientSampleId :

SSTD020315





Tgt Ion:228 Resp: 1131675

Ion Ratio Lower Upper

228 100

229 19.9 16.3 24.5

226 25.8 23.2 34.8

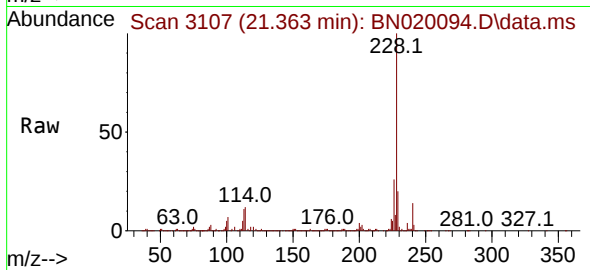

#86

Bis(2-ethylhexyl)phthalate

Concen: 20.995 ng/ul

RT: 21.304 min Scan# 3097

Delta R.T. 0.000 min

Lab File: BN020094.D

Acq: 10 Jun 2022 11:17




Tgt Ion:149 Resp: 800595


Ion Ratio Lower Upper

149 100

167 25.5 22.5 33.7

279 3.7 3.5 5.3


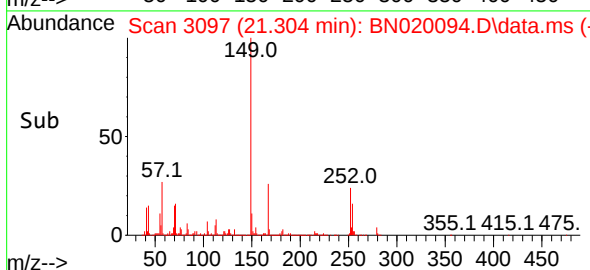






#87
Chrysene
Concen: 19.468 ng/ul
RT: 21.416 min Scan# 3116
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SSTD020315


Tgt Ion:228 Resp: 1075228
Ion Ratio Lower Upper
228 100
226 30.7 24.2 36.2
229 19.0 16.2 24.2

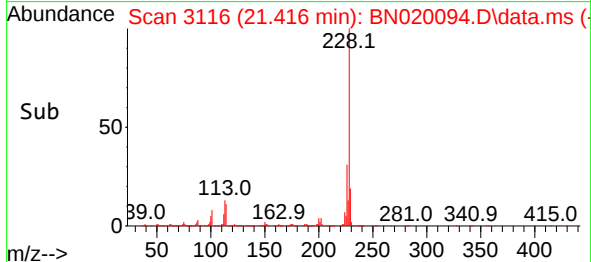

#89
Di-n-octyl phthalate
Concen: 20.345 ng/ul
RT: 22.204 min Scan# 3250
Delta R.T. -0.006 min
Lab File: BN020094.D
Acq: 10 Jun 2022 11:17

Tgt Ion:149 Resp: 1382496

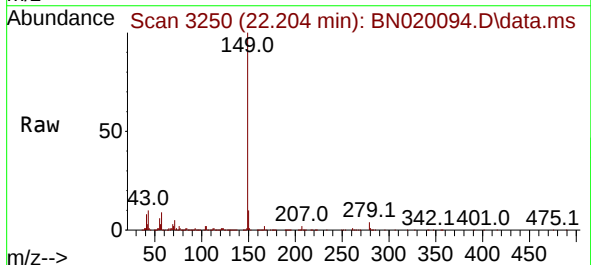



#90

Benzo(b)fluoranthene

Concen: 18.806 ng/ul

RT: 23.051 min Scan# 3394

Delta R.T. 0.047 min

Lab File: BN020094.D

Acq: 10 Jun 2022 11:17

Instrument :

BNA_N

ClientSampleId :

SSTD020315





Tgt Ion:252 Resp: 985443

Ion Ratio Lower Upper

252 100

253 20.2 16.5 24.7

125 11.5 7.8 11.8



#91

Benzo(k)fluoranthene

Concen: 19.755 ng/ul

RT: 23.051 min Scan# 3394

Delta R.T. 0.000 min

Lab File: BN020094.D

Acq: 10 Jun 2022 11:17




Tgt Ion:252 Resp: 985443


Ion Ratio Lower Upper

252 100

253 20.2 18.2 27.4

125 11.5 8.2 12.4





#93

Benzo(a)pyrene

Concen: 19.764 ng/ul

RT: 23.604 min Scan# 3488

Delta R.T. -0.006 min

Lab File: BN020094.D

Acq: 10 Jun 2022 11:17

Instrument :

BNA_N

ClientSampleId :

SSTD020315





Tgt Ion:252 Resp: 1002462

Ion Ratio Lower Upper

252 100

253 21.4 18.7 28.1

125 13.5 9.2 13.8



#94

Indeno(1,2,3-cd)pyrene

Concen: 18.312 ng/ul

RT: 26.098 min Scan# 3912

Delta R.T. 0.000 min

Lab File: BN020094.D

Acq: 10 Jun 2022 11:17




Tgt Ion:276 Resp: 955645


Ion Ratio Lower Upper

276 100

138 30.1 19.5 29.3

277 24.9 21.4 32.0


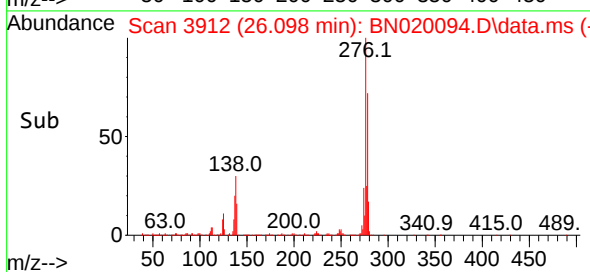






#95
 Dibenzo(a,h)anthracene
 Concen: 18.589 ng/ul
 RT: 26.109 min Scan# 3914
 Delta R.T. -0.012 min
 Lab File: BN020094.D
 Acq: 10 Jun 2022 11:17

Instrument :
 BNA_N
 ClientSampleId :
 SSTD020315

Tgt Ion:278 Resp: 828581
 Ion Ratio Lower Upper
 278 100
 139 18.9 13.8 20.8
 279 22.7 18.3 27.5

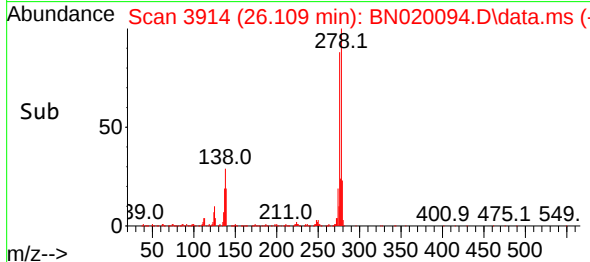

#96
 Benzo(g,h,i)perylene
 Concen: 18.366 ng/ul
 RT: 26.833 min Scan# 4037
 Delta R.T. -0.012 min
 Lab File: BN020094.D
 Acq: 10 Jun 2022 11:17

Tgt Ion:276 Resp: 809408
 Ion Ratio Lower Upper
 276 100
 138 26.7 17.0 25.6#
 277 22.9 17.8 26.6

