

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020095.D
 Acq On : 10 Jun 2022 11:53
 Operator : CG/JU
 Sample : PB145433BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK433

Quant Time: Jun 10 22:45:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	123228	20.000	ng/ul	0.00
20) Naphthalene-d8	10.610	136	576871	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.445	164	386600	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.186	188	799422	20.000	ng/ul	0.00
79) Chrysene-d12	21.380	240	736770	20.000	ng/ul	0.00
88) Perylene-d12	23.710	264	673056	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	18277	6.424	ng/uL	0.00
4) Pyridine-d5	3.687	84	251297	32.316	ng/ul	0.00
7) Phenol-d5	6.987	99	314419	30.835	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.152	67	204563	32.110	ng/ul	0.00
11) 2-Chlorophenol-d4	7.352	132	269572	32.537	ng/ul	0.00
15) 4-Methylphenol-d8	8.522	113	274305	31.094	ng/ul	0.00
21) Nitrobenzene-d5	8.969	128	134666	30.685	ng/ul	0.00
24) 2-Nitrophenol-d4	9.693	143	149720	32.145	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	245749	30.224	ng/ul	0.00
31) 4-Chloroaniline-d4	10.740	131	410108	31.146	ng/ul	0.00
46) Dimethylphthalate-d6	13.857	166	884129	31.430	ng/ul	0.00
49) Acenaphthylene-d8	14.140	160	1004687	30.798	ng/ul	0.00
54) 4-Nitrophenol-d4	14.640	143	144013	25.549	ng/ul	0.00
60) Fluorene-d10	15.434	176	736897	31.657	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.557	200	101381	21.893	ng/ul	0.00
73) Anthracene-d10	17.286	188	1190048	34.110	ng/ul	0.00
81) Pyrene-d10	19.580	212	1364804	34.170	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.563	264	1165310	35.386	ng/ul	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.522	70	7049	1.029 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020095.D
Acq On : 10 Jun 2022 11:53
Operator : CG/JU
Sample : PB145433BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK433


Quant Time: Jun 10 22:45:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration

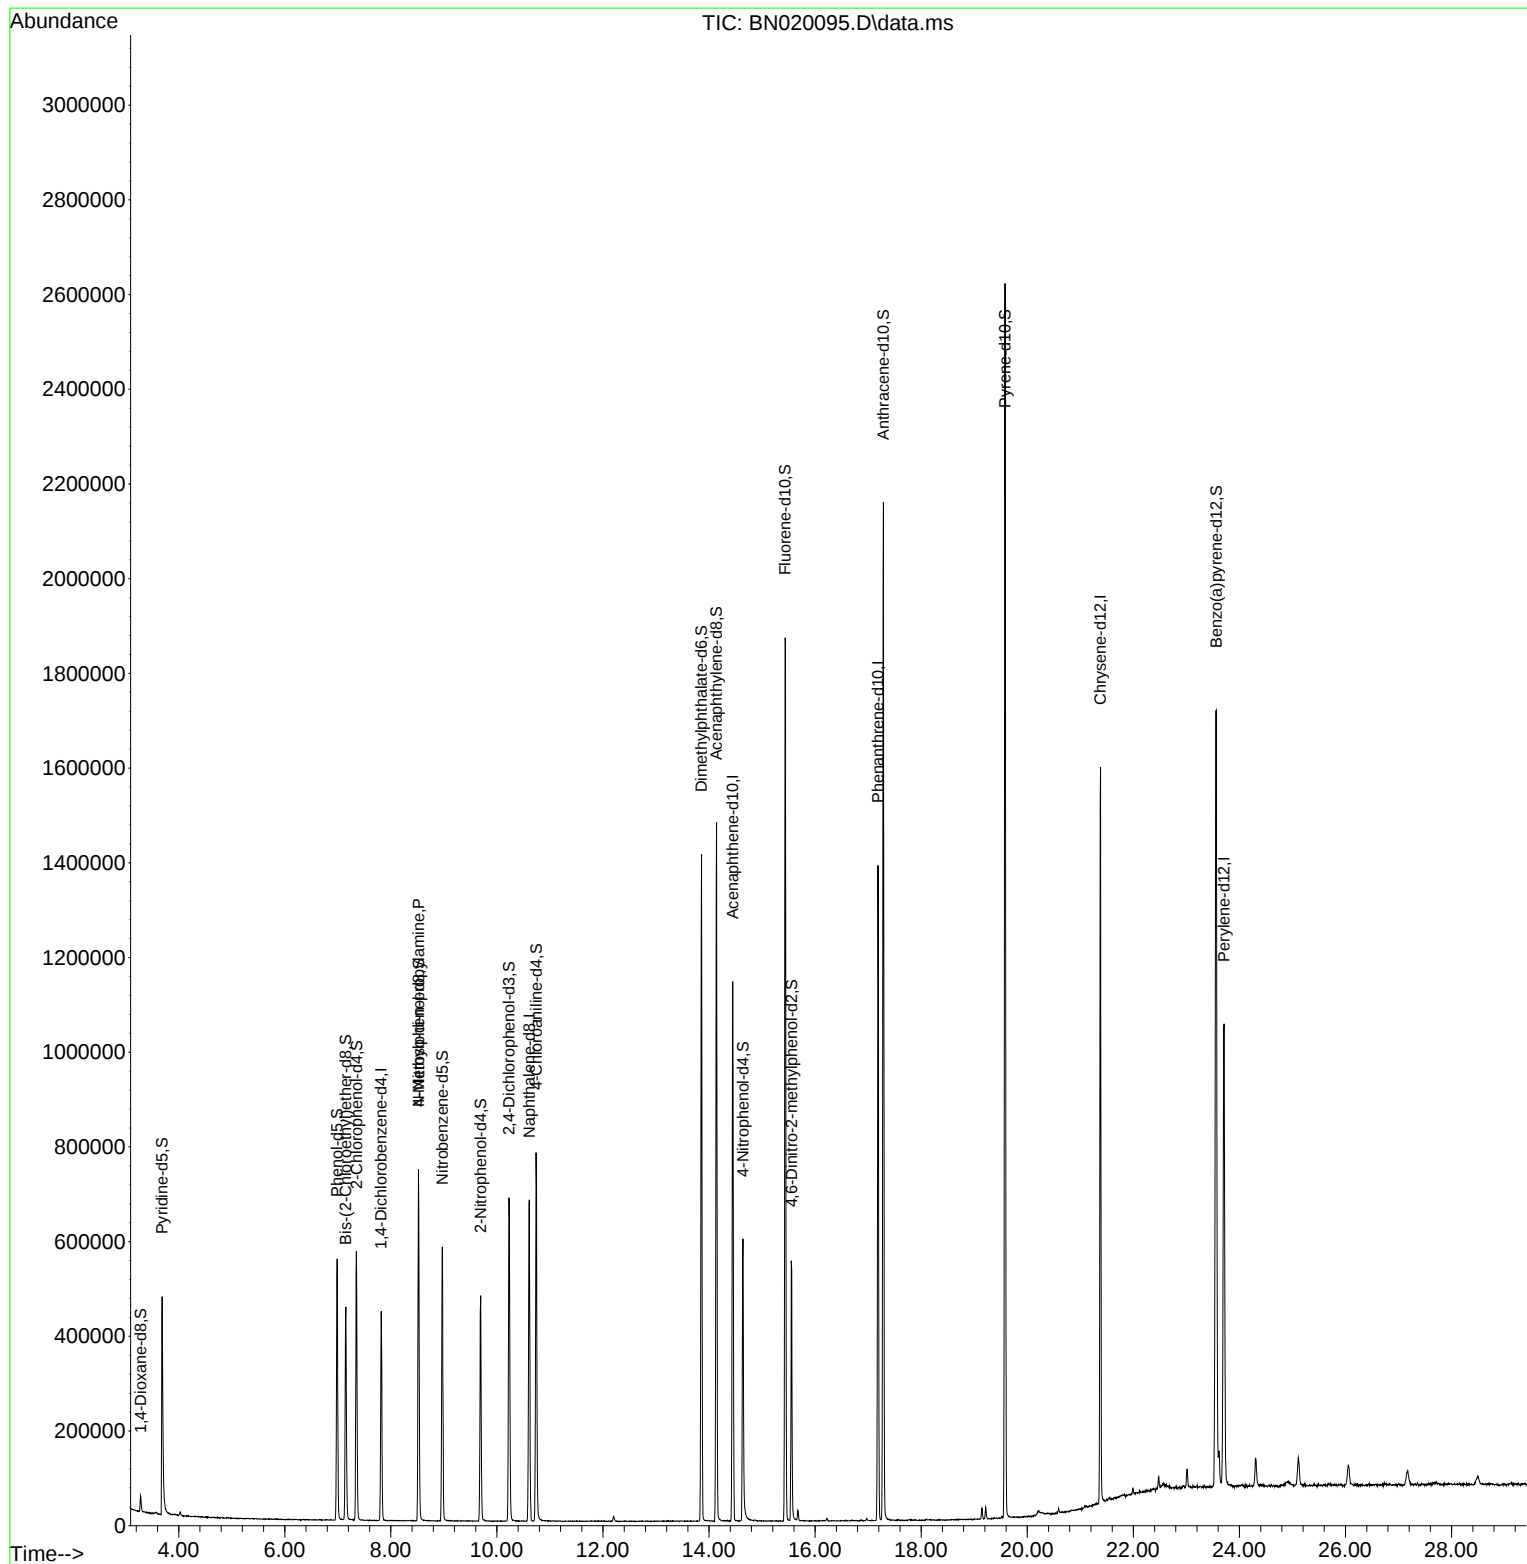

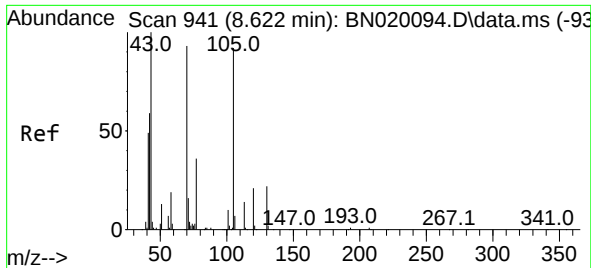

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.029 ng/ul
 RT: 8.522 min Scan# 91
 Delta R.T. -0.106 min
 Lab File: BN020095.D
 Acq: 10 Jun 2022 11:53

Instrument :
 BNA_N
 ClientSampleId :
 SBLK433

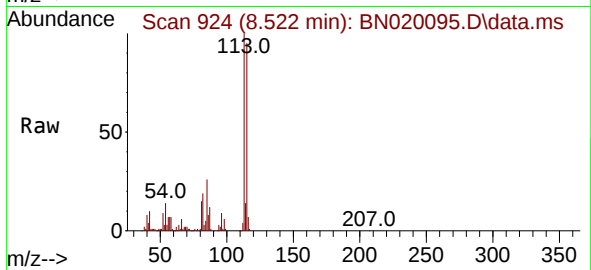

Tgt Ion:	70	Resp:	7049
Ion	Ratio	Lower	Upper
70	100		
42	433.4	47.8	71.6#
101	0.0	7.8	11.6#
130	0.0	15.8	23.8#

