

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020104.D
 Acq On : 10 Jun 2022 17:19
 Operator : CG/JU
 Sample : N3250-22
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYW4

Quant Time: Jun 10 22:46:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	164504	20.000	ng/u1	0.00
20) Naphthalene-d8	10.610	136	764353	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.445	164	497876	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.186	188	1019796	20.000	ng/u1	0.00
79) Chrysene-d12	21.374	240	903448	20.000	ng/u1	0.00
88) Perylene-d12	23.703	264	749033	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	20317	5.349	ng/uL	0.00
4) Pyridine-d5	3.693	84	101653	9.792	ng/u1	0.00
7) Phenol-d5	6.987	99	119078	8.748	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.151	67	326593	38.402	ng/u1	0.00
11) 2-Chlorophenol-d4	7.351	132	341534	30.879	ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	242915	20.626	ng/u1	0.00
21) Nitrobenzene-d5	8.969	128	229730	39.506	ng/u1	0.00
24) 2-Nitrophenol-d4	9.692	143	240627	38.991	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	375401	34.845	ng/u1	0.00
31) 4-Chloroaniline-d4	10.739	131	548913	31.463	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	1454408	40.148	ng/u1	0.00
49) Acenaphthylene-d8	14.139	160	1679306	39.973	ng/u1	0.00
54) 4-Nitrophenol-d4	14.639	143	48679	6.706	ng/u1	0.00
60) Fluorene-d10	15.439	176	1228570	40.983	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.557	200	212629	35.994	ng/u1	0.00
73) Anthracene-d10	17.286	188	1924025	43.230	ng/u1	0.00
81) Pyrene-d10	19.586	212	2153140	43.962	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.556	264	1593578	43.483	ng/u1	0.00
Target Compounds						
48) 2,6-Dinitrotoluene	13.863	165	8543	1.198	ng/u1#	37


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020104.D
Acq On : 10 Jun 2022 17:19
Operator : CG/JU
Sample : N3250-22
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW4


Quant Time: Jun 10 22:46:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration

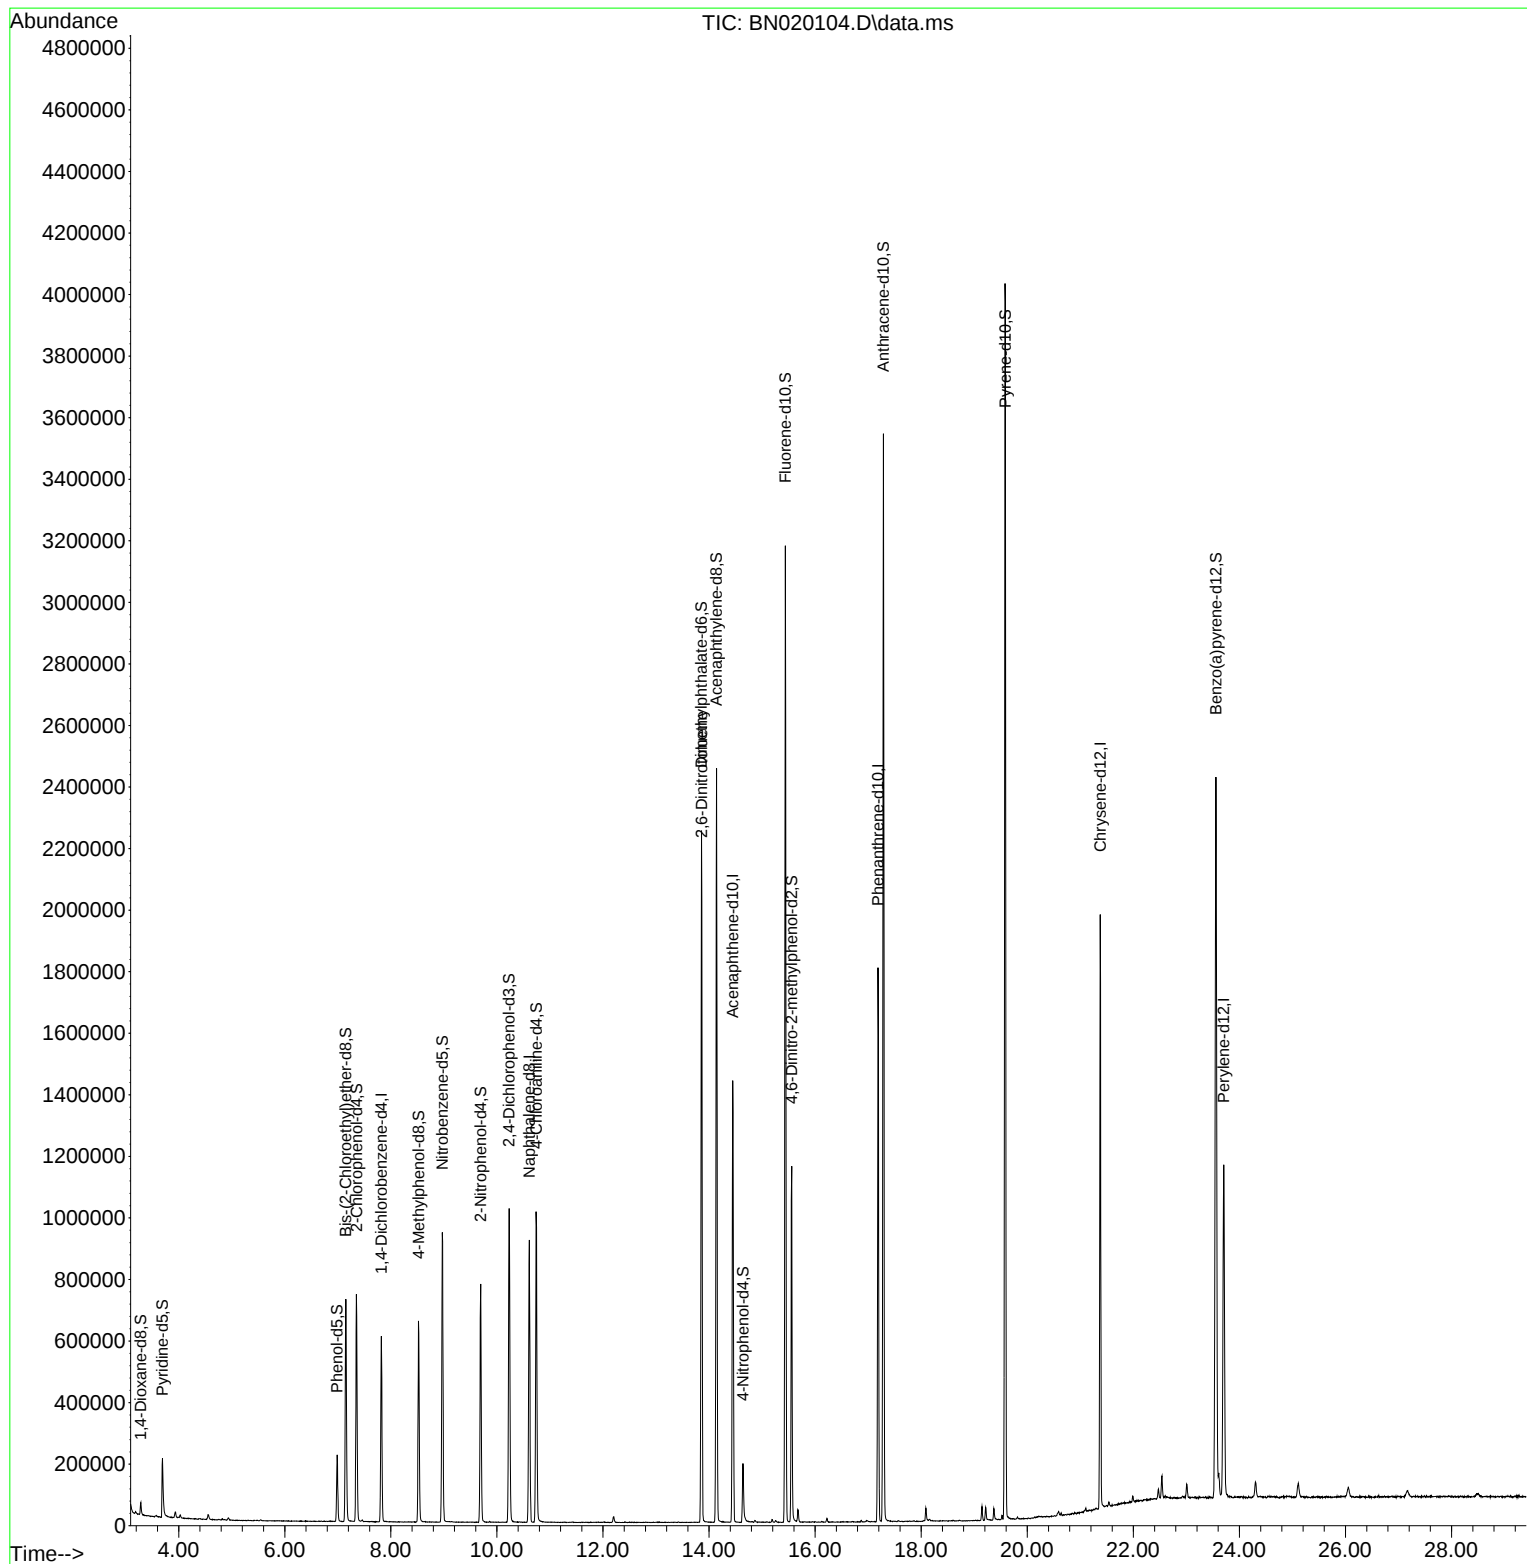

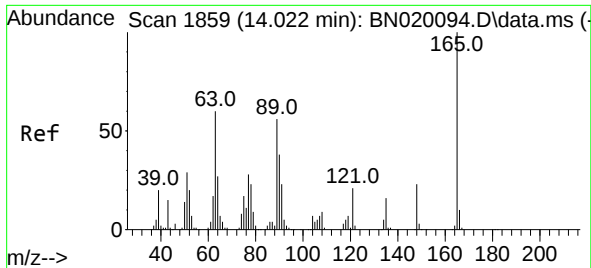

#48
 2,6-Dinitrotoluene
 Concen: 1.198 ng/ul
 RT: 13.863 min Scan# 11
 Delta R.T. -0.165 min
 Lab File: BN020104.D
 Acq: 10 Jun 2022 17:19

Instrument :
 BNA_N
 ClientSampleId :
 EXYW4

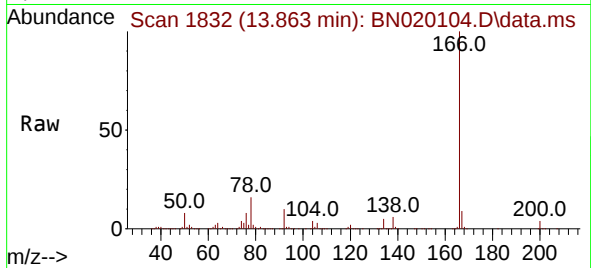

Tgt Ion	Ratio	Lower	Upper
165	100		
89	0.0	50.6	75.8#
121	28.6	17.9	26.9#

