

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020128.D
 Acq On : 11 Jun 2022 08:56
 Operator : CG/JU
 Sample : PB145457BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK457

Quant Time: Jun 13 00:43:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	145371	20.000	ng/u1	0.00
20) Naphthalene-d8	10.604	136	689781	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.445	164	456493	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.180	188	969037	20.000	ng/u1	-0.01
79) Chrysene-d12	21.374	240	851413	20.000	ng/u1	0.00
88) Perylene-d12	23.698	264	748997	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	22210	6.617	ng/uL	0.00
4) Pyridine-d5	3.687	84	314815	34.317	ng/u1	0.00
7) Phenol-d5	6.981	99	401355	33.366	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.146	67	258250	34.362	ng/u1	0.00
11) 2-Chlorophenol-d4	7.346	132	337315	34.512	ng/u1	-0.01
15) 4-Methylphenol-d8	8.522	113	351996	33.822	ng/u1	0.00
21) Nitrobenzene-d5	8.969	128	176063	33.550	ng/u1	0.00
24) 2-Nitrophenol-d4	9.693	143	197365	35.438	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	317387	32.645	ng/u1	0.00
31) 4-Chloroaniline-d4	10.740	131	532450	33.818	ng/u1	0.00
46) Dimethylphthalate-d6	13.851	166	1147491	34.547	ng/u1	-0.01
49) Acenaphthylene-d8	14.134	160	1304653	33.870	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.634	143	195173	29.323	ng/u1	-0.01
60) Fluorene-d10	15.434	176	954947	34.744	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.551	200	154097	27.452	ng/u1	-0.01
73) Anthracene-d10	17.280	188	1512222	35.757	ng/u1	-0.01
81) Pyrene-d10	19.580	212	1695890	36.742	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.551	264	1332931	36.372	ng/u1	-0.01


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.522	70	8606	1.064 ng/u1#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020128.D
Acq On : 11 Jun 2022 08:56
Operator : CG/JU
Sample : PB145457BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK457


Quant Time: Jun 13 00:43:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration

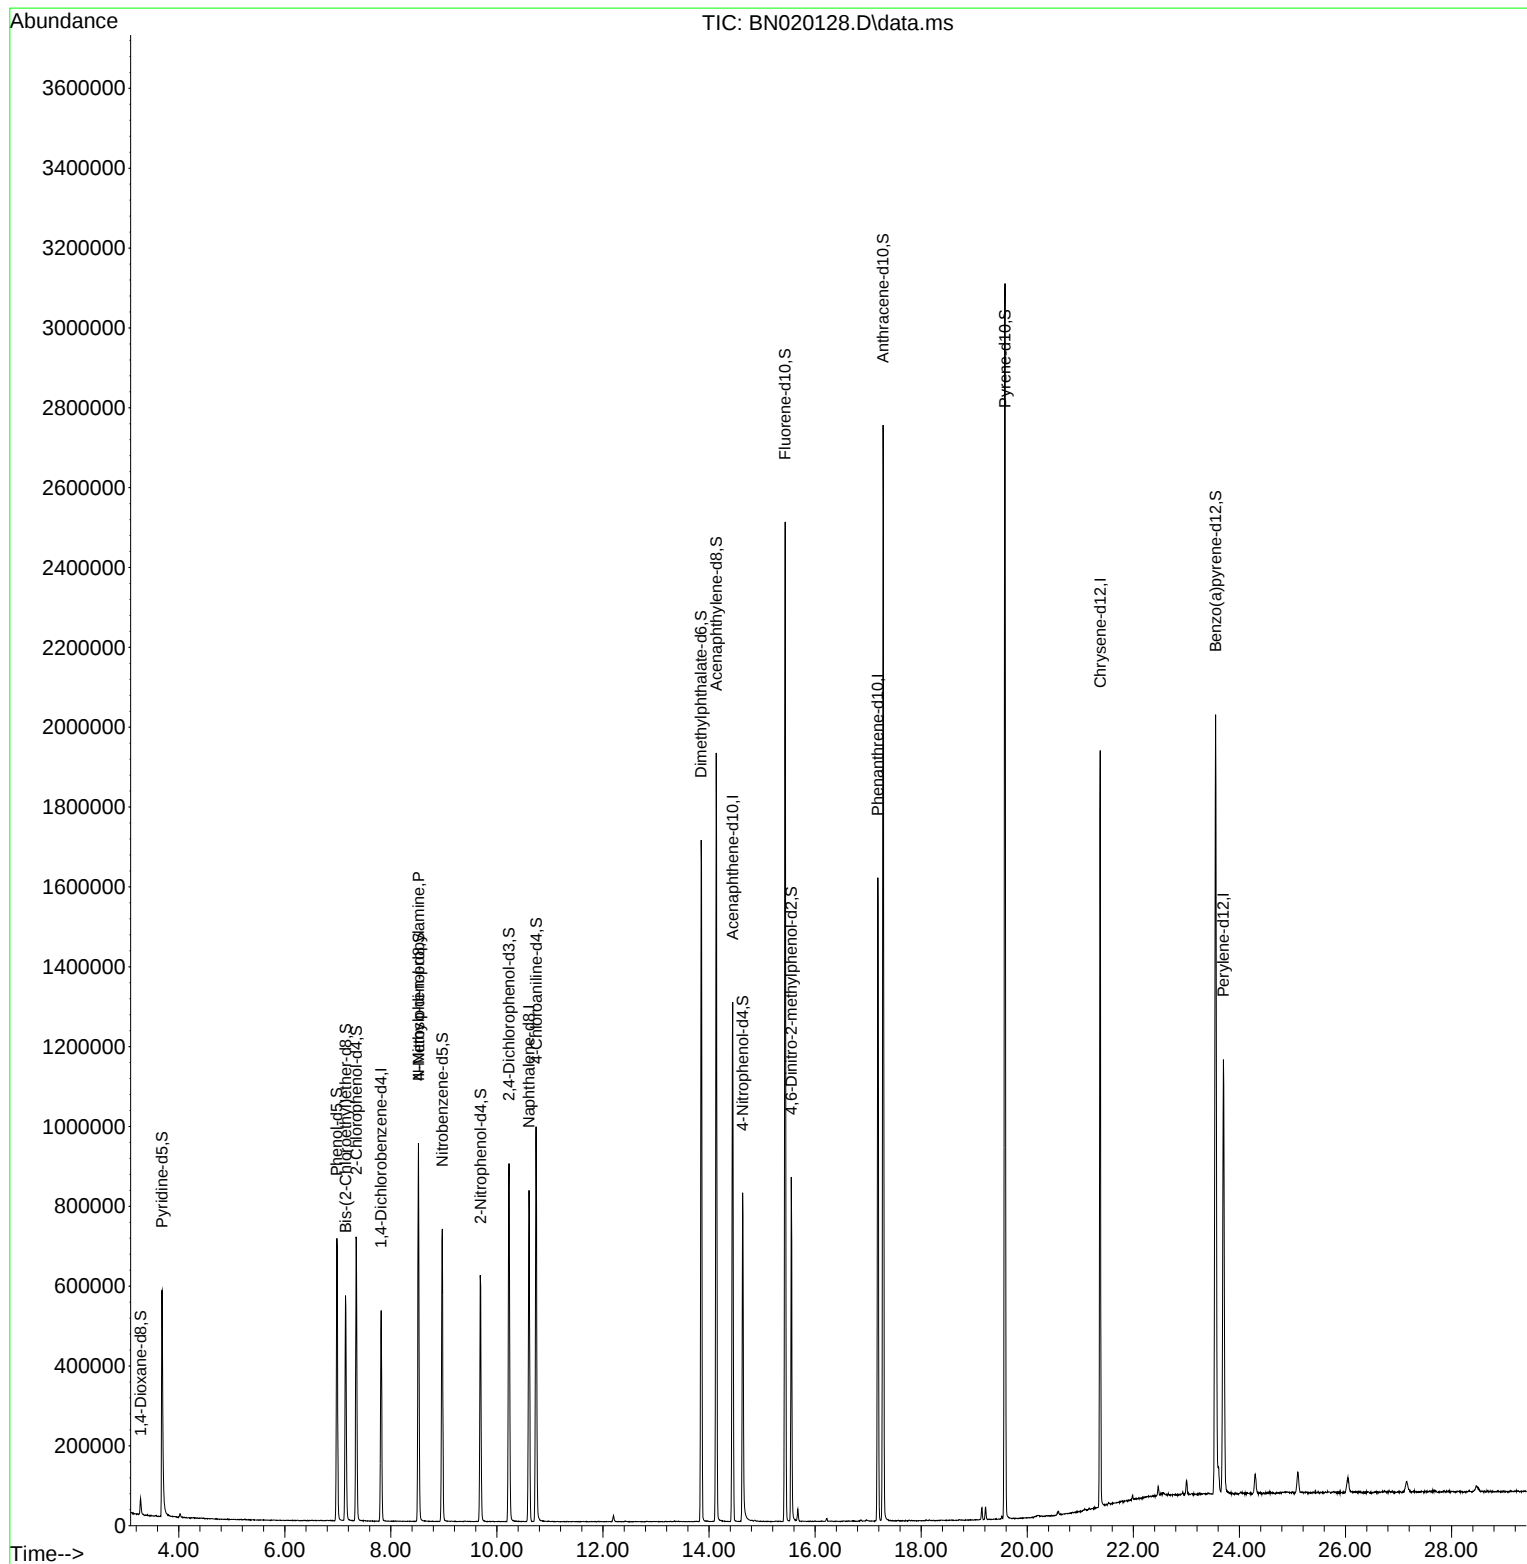

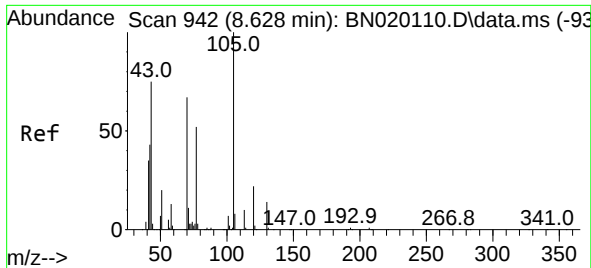

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.064 ng/ul
 RT: 8.522 min Scan# 91
 Delta R.T. -0.106 min
 Lab File: BN020128.D
 Acq: 11 Jun 2022 08:56

Instrument :
 BNA_N
 ClientSampleId :
 SBLK457

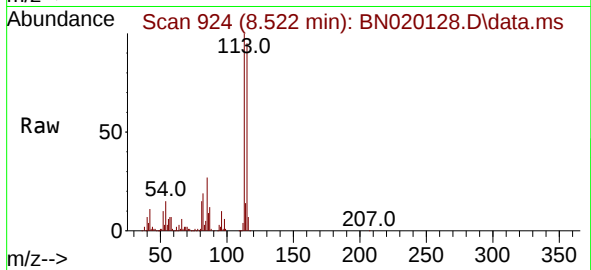

Tgt Ion: 70 Resp: 8606

Ion	Ratio	Lower	Upper
70	100		
42	426.3	47.8	71.6#
101	0.0	7.8	11.6#
130	0.0	15.8	23.8#

