

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020130.D
 Acq On : 11 Jun 2022 10:07
 Operator : CG/JU
 Sample : N3284-01
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYT1

Quant Time: Jun 13 00:43:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	149113	20.000	ng/u1	0.00
20) Naphthalene-d8	10.605	136	710485	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.446	164	470289	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.181	188	988944	20.000	ng/u1	-0.01
79) Chrysene-d12	21.375	240	910609	20.000	ng/u1	0.00
88) Perylene-d12	23.698	264	795500	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	17366	5.044	ng/uL	0.00
4) Pyridine-d5	3.693	84	65585	6.970	ng/u1	0.00
7) Phenol-d5	6.987	99	79464	6.440	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.146	67	241317	31.303	ng/u1	0.00
11) 2-Chlorophenol-d4	7.352	132	246523	24.590	ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	169710	15.898	ng/u1	0.00
21) Nitrobenzene-d5	8.969	128	170511	31.546	ng/u1	0.00
24) 2-Nitrophenol-d4	9.687	143	181668	31.669	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.228	165	281428	28.103	ng/u1	0.00
31) 4-Chloroaniline-d4	10.740	131	409950	25.279	ng/u1	0.00
46) Dimethylphthalate-d6	13.851	166	1120051	32.732	ng/u1	-0.01
49) Acenaphthylene-d8	14.134	160	1256689	31.668	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.634	143	35188	5.132	ng/u1	-0.01
60) Fluorene-d10	15.434	176	972835	34.356	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.551	200	180051	31.430	ng/u1	-0.01
73) Anthracene-d10	17.281	188	1644084	38.093	ng/u1	-0.01
81) Pyrene-d10	19.581	212	1839804	37.269	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.551	264	1491519	38.321	ng/u1	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.317	88	54640	15.034	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020130.D
Acq On : 11 Jun 2022 10:07
Operator : CG/JU
Sample : N3284-01
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYT1


Quant Time: Jun 13 00:43:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration

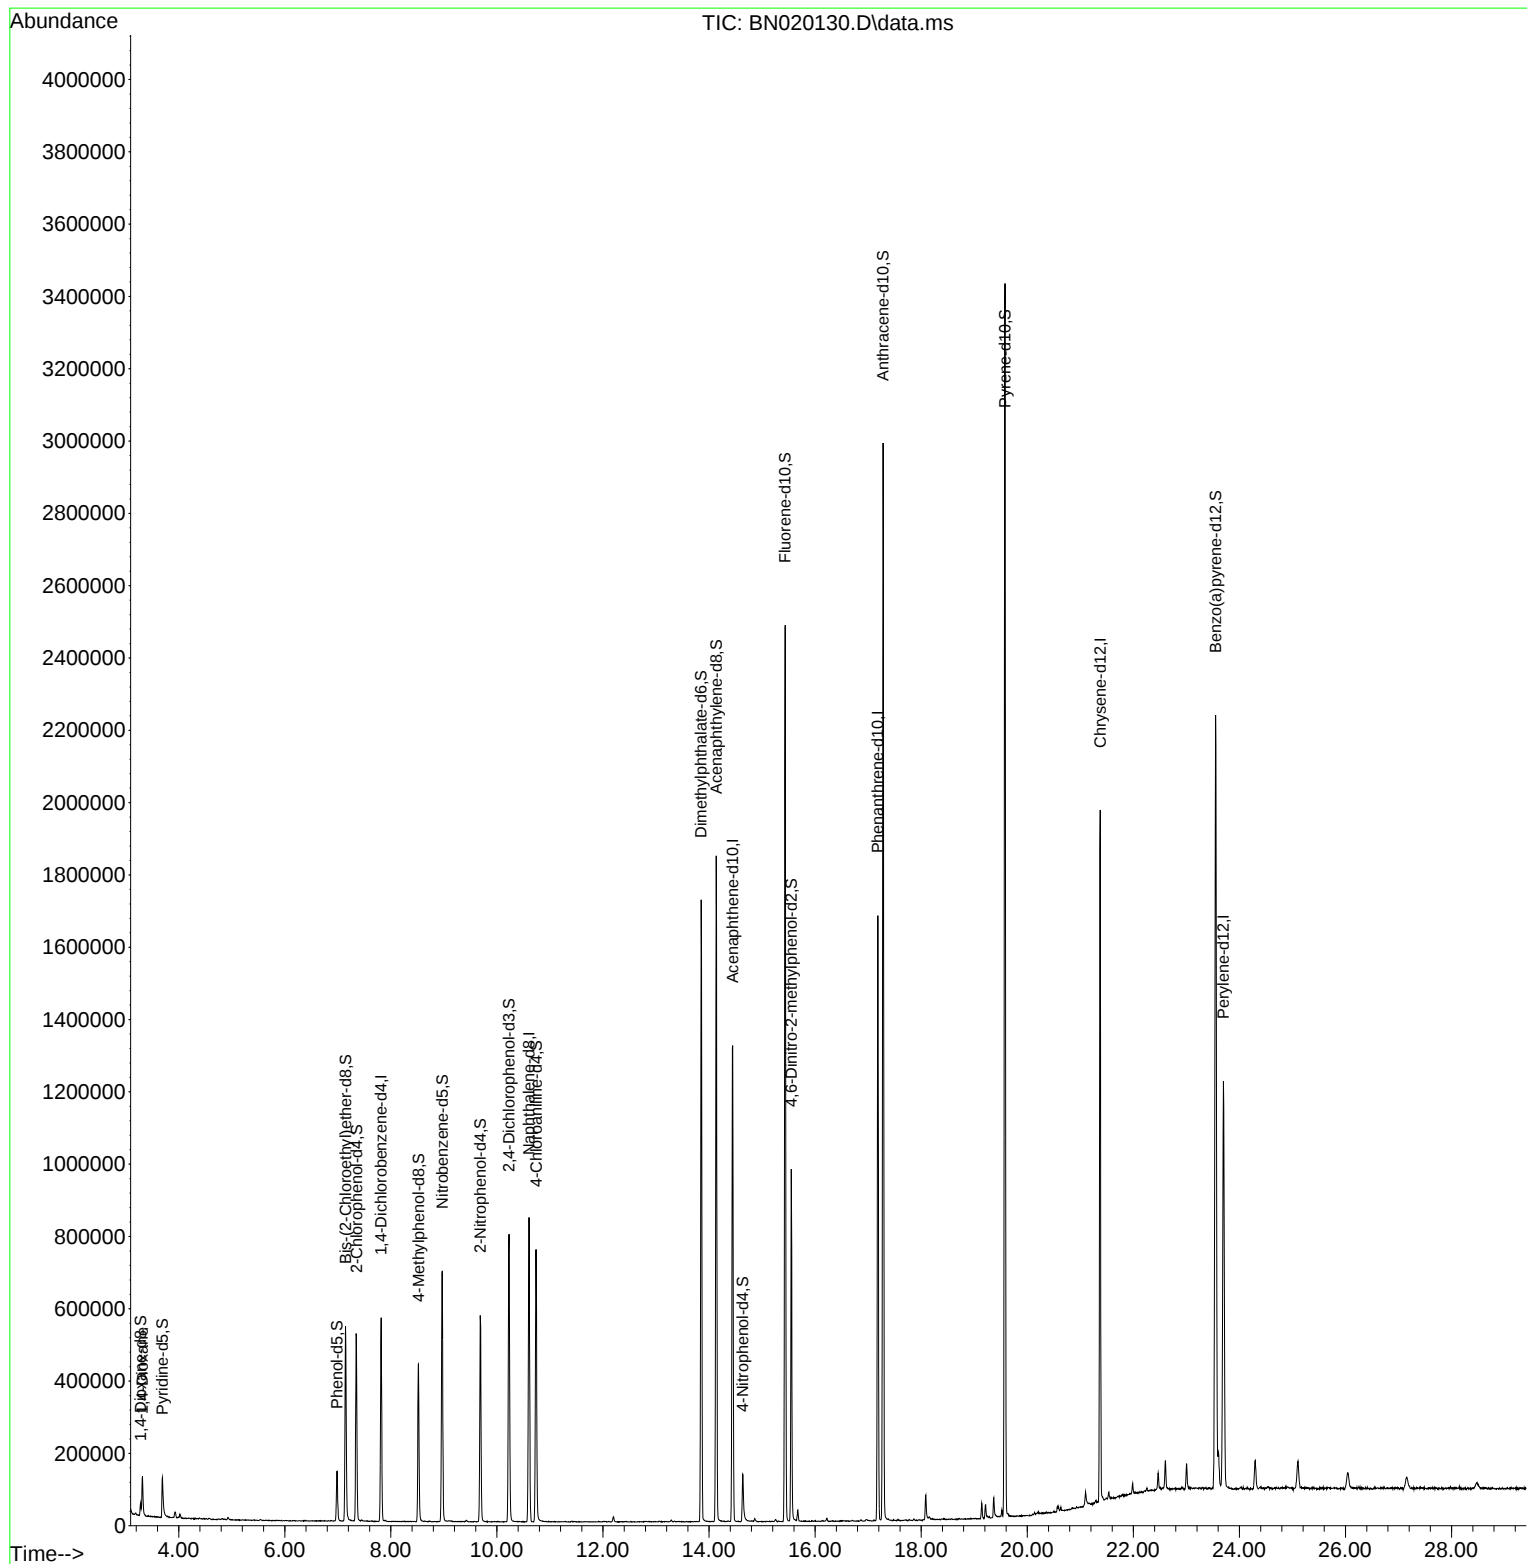

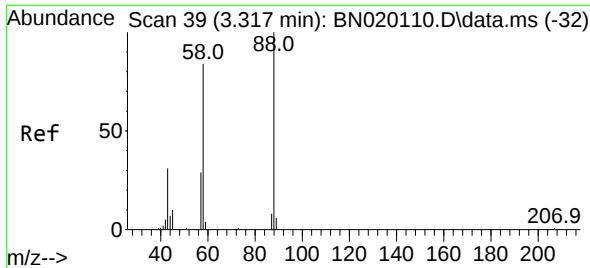

#2
 1,4-Dioxane
 Concen: 15.034 ng/uL
 RT: 3.317 min Scan# 39
 Delta R.T. 0.001 min
 Lab File: BN020130.D
 Acq: 11 Jun 2022 10:07

Instrument :
 BNA_N
 ClientSampleId :
 EXYT1

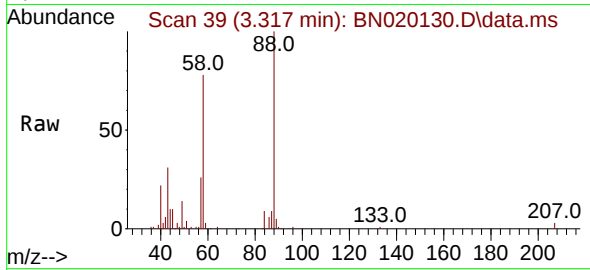

Tgt Ion:	88	Resp:	54640
Ion	Ratio	Lower	Upper
88	100		
43	31.2	22.4	33.6
58	78.0	61.0	91.4

