

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020097.D
 Acq On : 10 Jun 2022 13:05
 Operator : CG/JU
 Sample : N3250-19
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYT7

Quant Time: Jun 10 22:45:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	155582	20.000	ng/u1	0.00
20) Naphthalene-d8	10.610	136	711189	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.445	164	457897	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.186	188	939994	20.000	ng/u1	0.00
79) Chrysene-d12	21.374	240	783932	20.000	ng/u1	0.00
88) Perylene-d12	23.704	264	677250	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	16401	4.566	ng/uL	0.00
4) Pyridine-d5	3.693	84	87091	8.871	ng/u1	0.00
7) Phenol-d5	6.993	99	79475	6.173	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.152	67	243254	30.243	ng/u1	0.00
11) 2-Chlorophenol-d4	7.357	132	246396	23.555	ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	172986	15.531	ng/u1	0.00
21) Nitrobenzene-d5	8.969	128	163525	30.223	ng/u1	0.00
24) 2-Nitrophenol-d4	9.693	143	167868	29.235	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	286006	28.532	ng/u1	0.00
31) 4-Chloroaniline-d4	0.000	131	0d	0.000	ng/u1	
46) Dimethylphthalate-d6	13.857	166	1122957	33.705	ng/u1	0.00
49) Acenaphthylene-d8	14.139	160	1308486	33.865	ng/u1	0.00
54) 4-Nitrophenol-d4	14.639	143	38893	5.826	ng/u1	0.00
60) Fluorene-d10	15.439	176	975266	35.374	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.557	200	112885	20.732	ng/u1	0.00
73) Anthracene-d10	17.286	188	1604835	39.120	ng/u1	0.00
81) Pyrene-d10	19.580	212	1662034	39.108	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.557	264	1338039	40.380	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.322	88	10040	2.648	ng/uL 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020097.D
Acq On : 10 Jun 2022 13:05
Operator : CG/JU
Sample : N3250-19
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYT7


Quant Time: Jun 10 22:45:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration

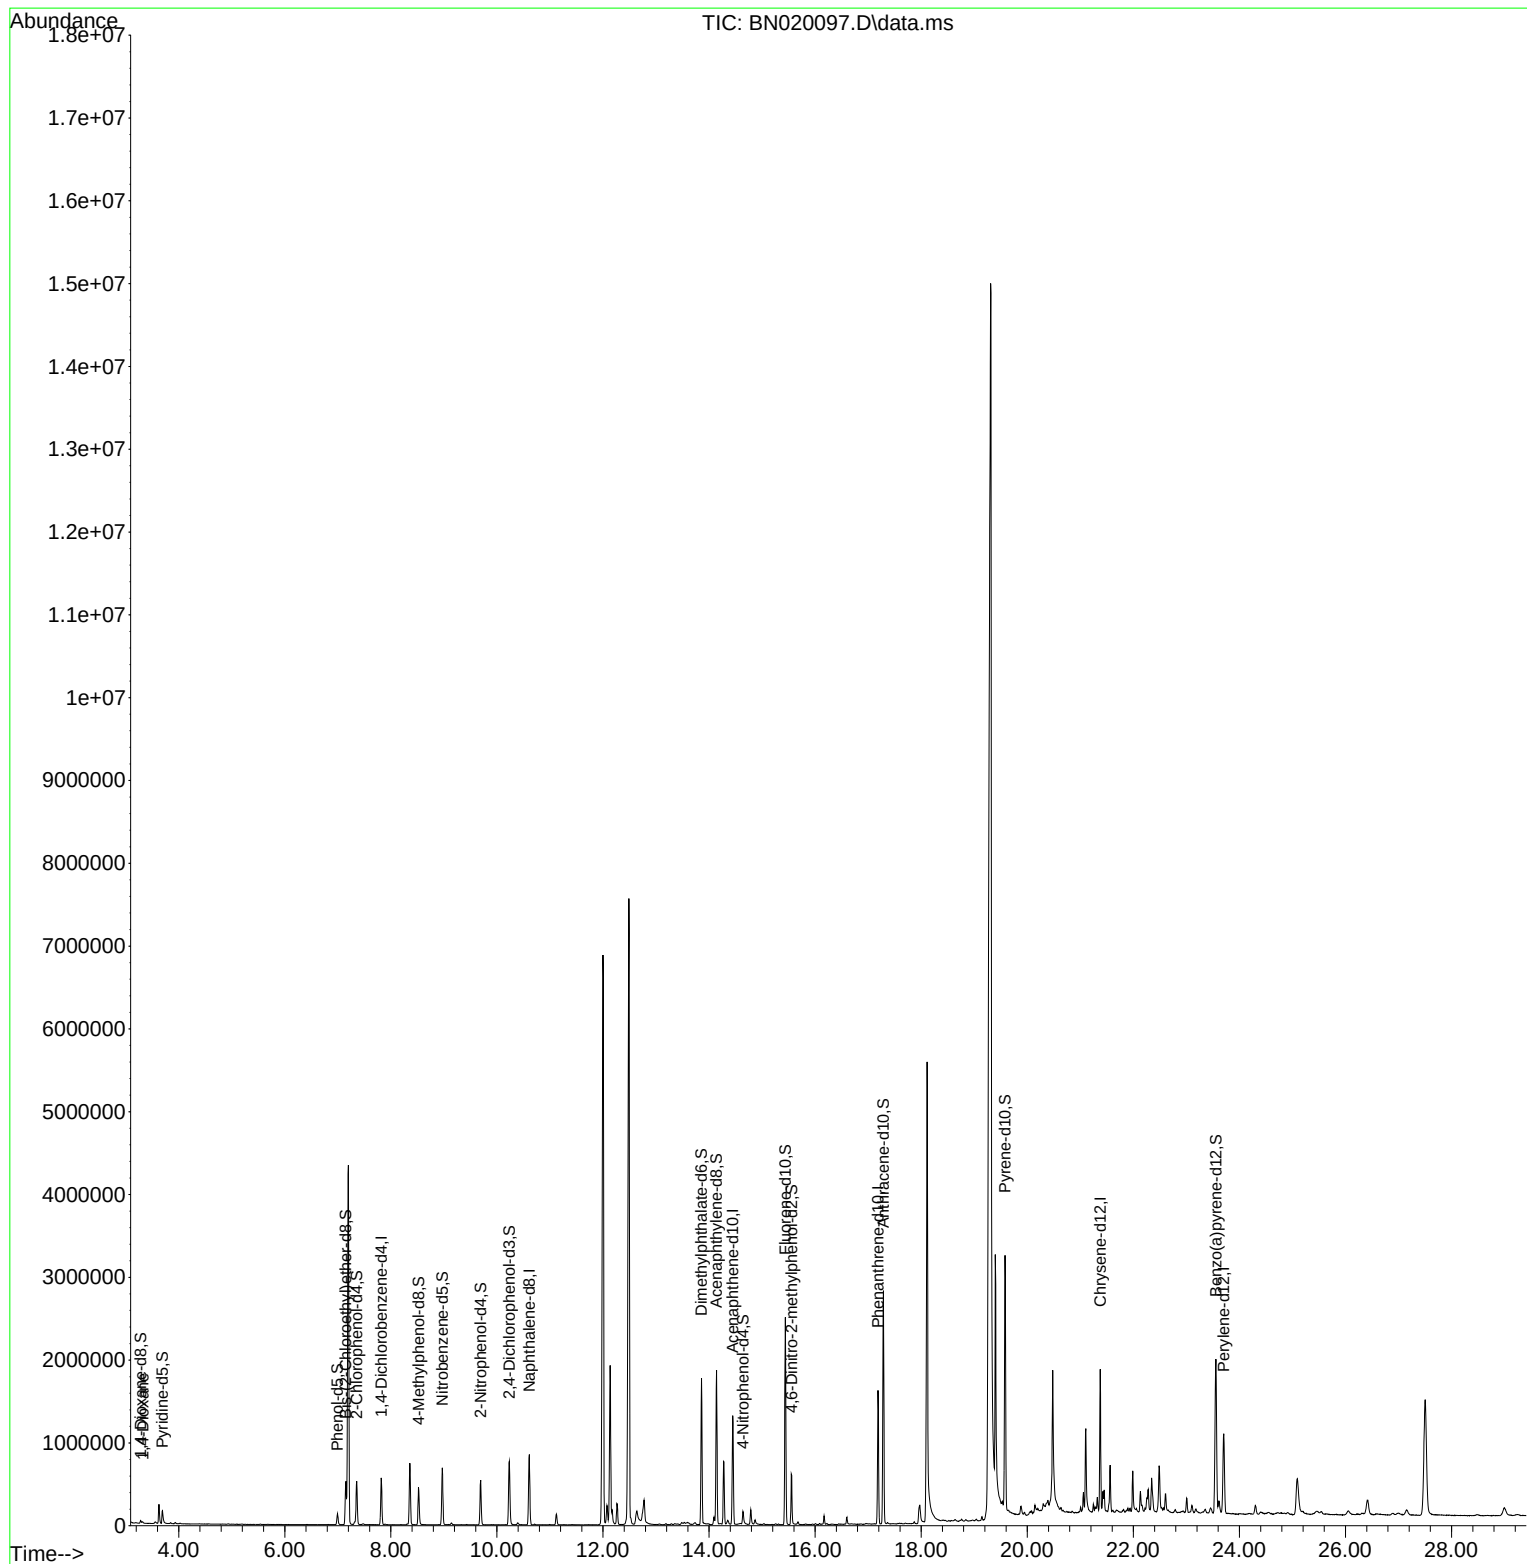

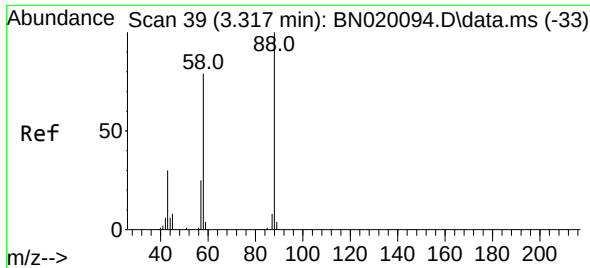

#2
 1,4-Dioxane
 Concen: 2.648 ng/uL
 RT: 3.322 min Scan# 40
 Delta R.T. 0.006 min
 Lab File: BN020097.D
 Acq: 10 Jun 2022 13:05

Instrument :
 BNA_N
 ClientSampleId :
 EXYT7

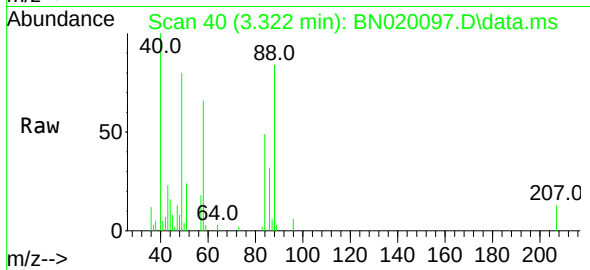

Tgt Ion:	88	Resp:	10040
Ion	Ratio	Lower	Upper
88	100		
43	27.2	22.4	33.6
58	77.8	61.0	91.4

