

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020102.D
 Acq On : 10 Jun 2022 16:06
 Operator : CG/JU
 Sample : N3250-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYW8

Quant Time: Jun 10 22:46:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	148873	20.000	ng/u1	0.00
20) Naphthalene-d8	10.610	136	698597	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.445	164	459162	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.186	188	957683	20.000	ng/u1	0.00
79) Chrysene-d12	21.374	240	868108	20.000	ng/u1	0.00
88) Perylene-d12	23.709	264	798693	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	14817	4.311	ng/uL	0.00
4) Pyridine-d5	3.693	84	62614	6.665	ng/u1	0.00
7) Phenol-d5	6.987	99	70026	5.684	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.151	67	216609	28.144	ng/u1	0.00
11) 2-Chlorophenol-d4	7.351	132	215776	21.558	ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	149464	14.024	ng/u1	0.00
21) Nitrobenzene-d5	8.969	128	146713	27.605	ng/u1	0.00
24) 2-Nitrophenol-d4	9.692	143	157057	27.845	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	248583	25.245	ng/u1	0.00
31) 4-Chloroaniline-d4	10.739	131	342840	21.501	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	964237	28.861	ng/u1	0.00
49) Acenaphthylene-d8	14.139	160	1116220	28.810	ng/u1	0.00
54) 4-Nitrophenol-d4	14.639	143	29999	4.481	ng/u1	0.00
60) Fluorene-d10	15.439	176	833937	30.165	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.557	200	151588	27.326	ng/u1	0.00
73) Anthracene-d10	17.286	188	1462882	35.001	ng/u1	0.00
81) Pyrene-d10	19.580	212	1658436	35.240	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.556	264	1356164	34.704	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.316	88	4213	1.161	ng/uL	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020102.D
Acq On : 10 Jun 2022 16:06
Operator : CG/JU
Sample : N3250-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW8


Quant Time: Jun 10 22:46:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration

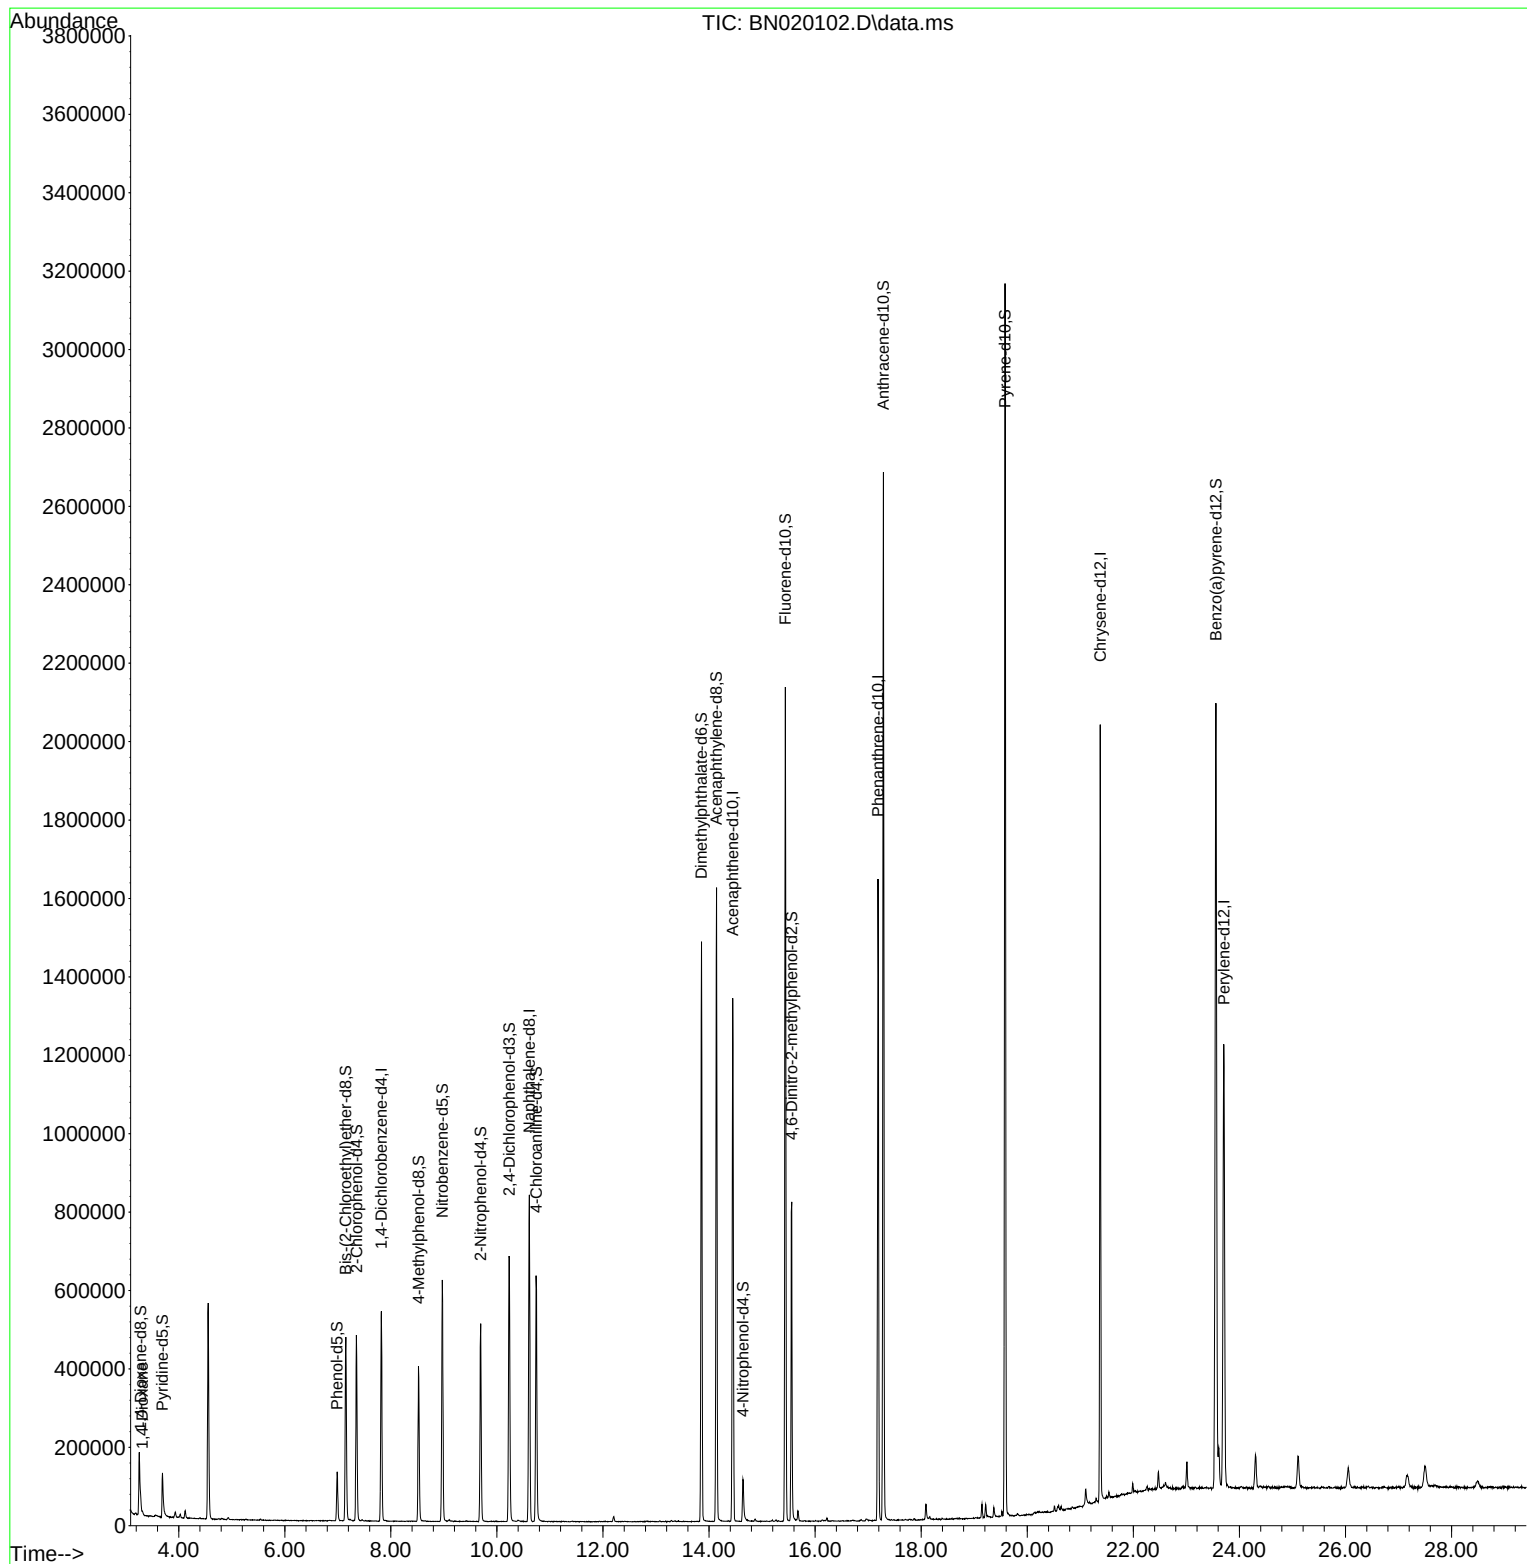

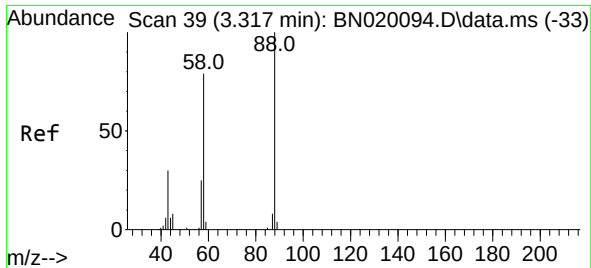

#2
 1,4-Dioxane
 Concen: 1.161 ng/uL
 RT: 3.316 min Scan# 39
 Delta R.T. 0.000 min
 Lab File: BN020102.D
 Acq: 10 Jun 2022 16:06

Instrument :
 BNA_N
 ClientSampleId :
 EXYW8

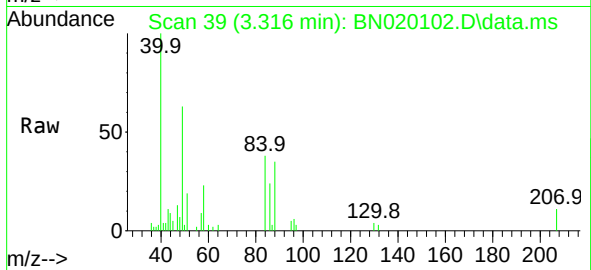

Tgt Ion: 88	Resp:	4213	
Ion	Ratio	Lower	Upper
88	100		
43	31.1	22.4	33.6
58	66.3	61.0	91.4

