

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020113.D
 Acq On : 10 Jun 2022 23:22
 Operator : CG/JU
 Sample : N3250-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYT3

Quant Time: Jun 11 00:14:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	142619	20.000	ng/u1	0.00
20) Naphthalene-d8	10.610	136	674108	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.445	164	445132	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.186	188	932931	20.000	ng/u1	0.00
79) Chrysene-d12	21.374	240	833455	20.000	ng/u1	0.00
88) Perylene-d12	23.698	264	737185	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	17083	5.188	ng/uL	0.00
4) Pyridine-d5	3.687	84	100370	11.152	ng/u1	0.00
7) Phenol-d5	6.987	99	74029	6.273	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.146	67	247066	33.508	ng/u1	0.00
11) 2-Chlorophenol-d4	7.352	132	242510	25.291	ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	162439	15.910	ng/u1	0.00
21) Nitrobenzene-d5	8.969	128	168857	32.925	ng/u1	0.00
24) 2-Nitrophenol-d4	9.693	143	173894	31.950	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	280994	29.574	ng/u1	0.00
31) 4-Chloroaniline-d4	10.740	131	393952	25.603	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	1144824	35.347	ng/u1	0.00
49) Acenaphthylene-d8	14.140	160	1287297	34.272	ng/u1	0.00
54) 4-Nitrophenol-d4	14.640	143	32752	5.046	ng/u1	0.00
60) Fluorene-d10	15.439	176	959112	35.786	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.557	200	175955	32.560	ng/u1	0.00
73) Anthracene-d10	17.286	188	1624048	39.888	ng/u1	0.00
81) Pyrene-d10	19.580	212	1837247	40.662	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.551	264	1504677	41.717	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.317	88	19652	5.653	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020113.D
Acq On : 10 Jun 2022 23:22
Operator : CG/JU
Sample : N3250-17
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYT3


Quant Time: Jun 11 00:14:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration

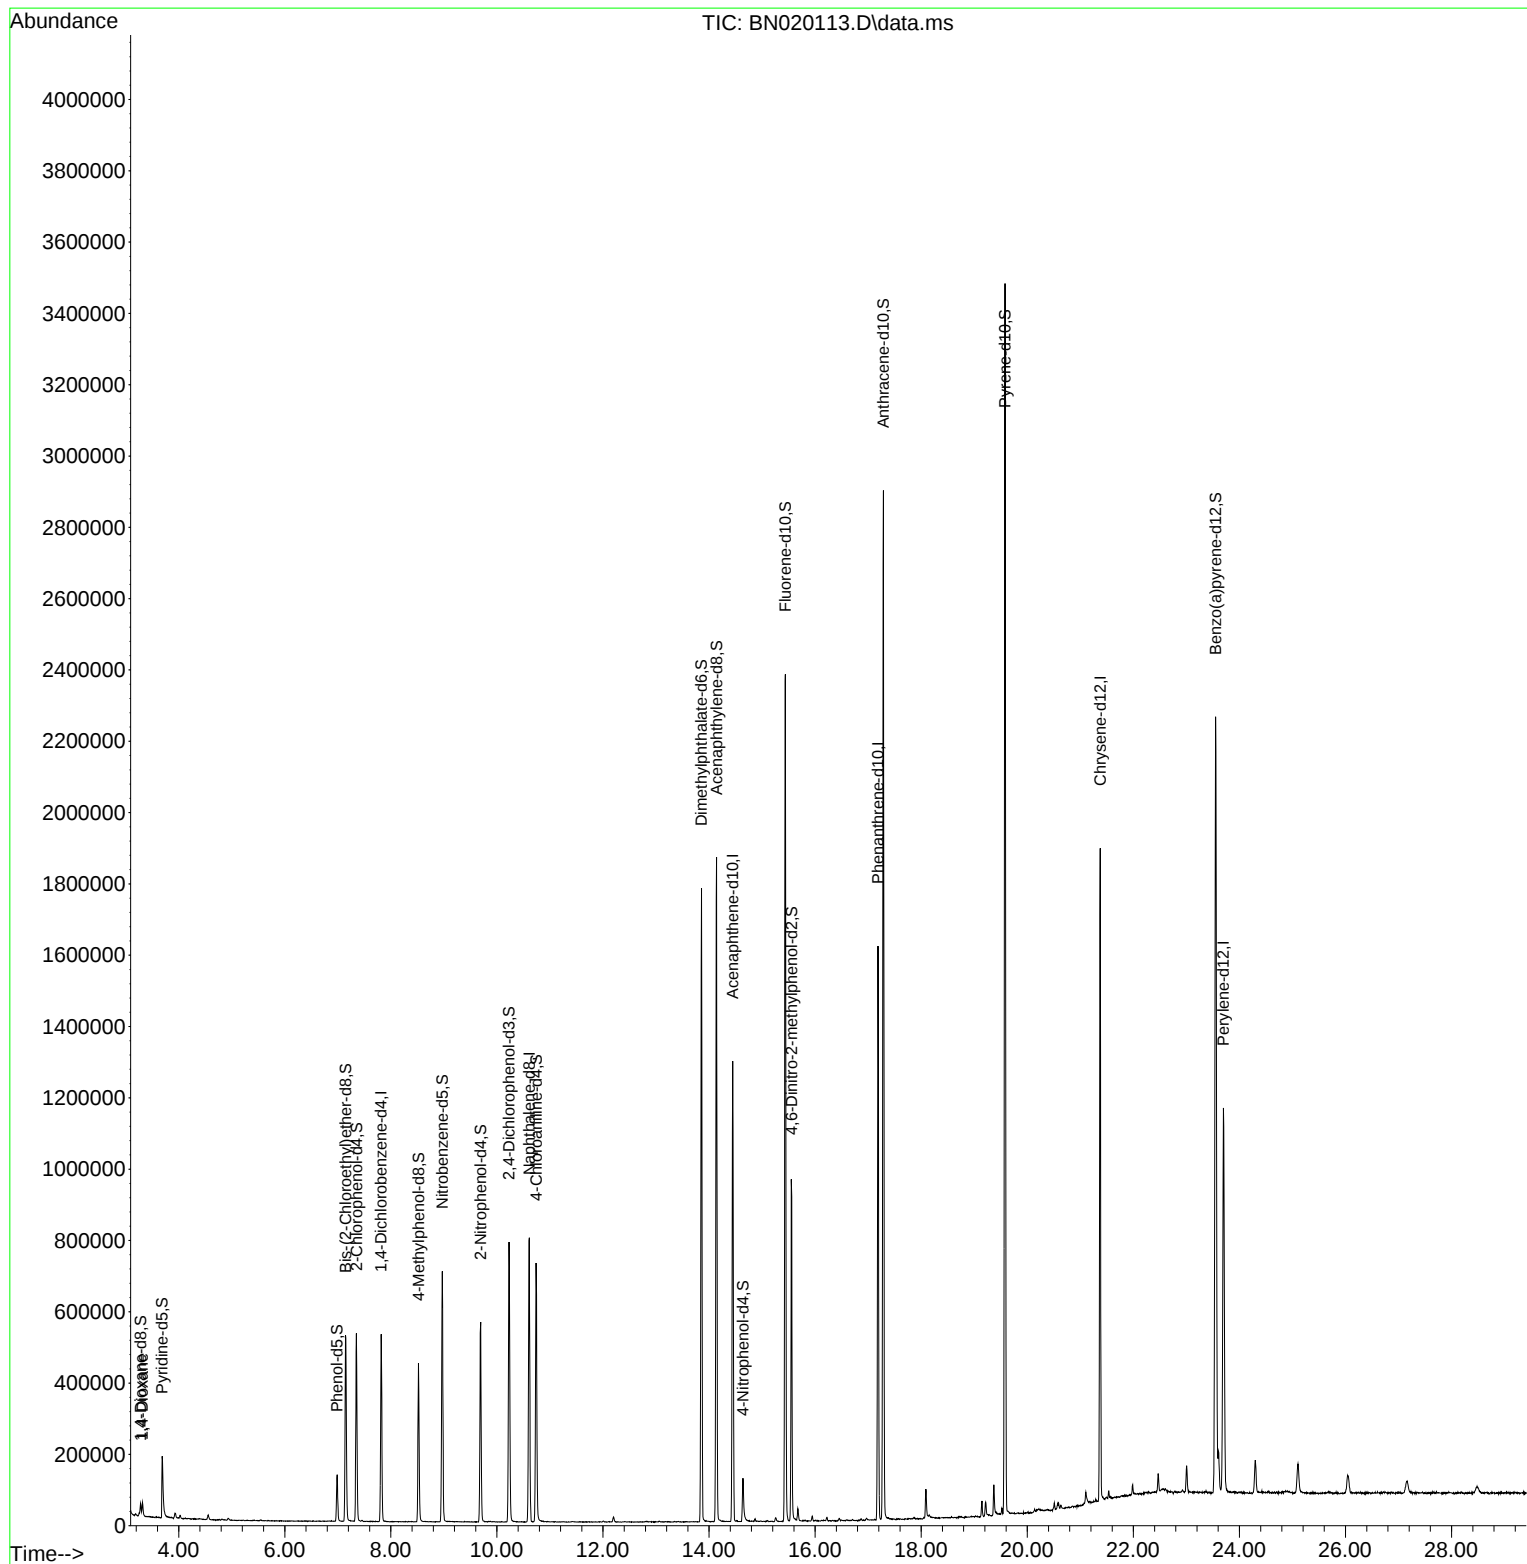

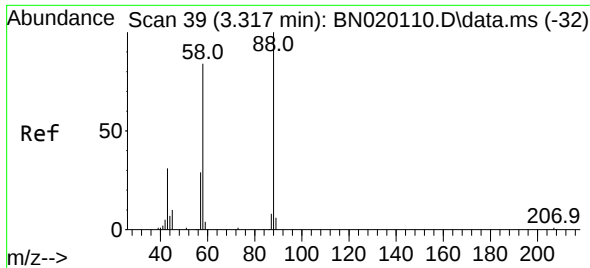

#2
 1,4-Dioxane
 Concen: 5.653 ng/uL
 RT: 3.317 min Scan# 39
 Delta R.T. 0.001 min
 Lab File: BN020113.D
 Acq: 10 Jun 2022 23:22

Instrument :
 BNA_N
 ClientSampleId :
 EXYT3

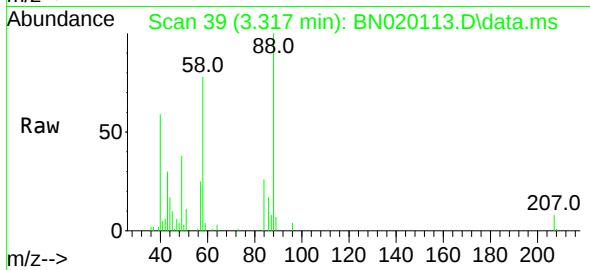

Tgt Ion:	88	Resp:	19652
Ion	Ratio	Lower	Upper
88	100		
43	30.1	22.4	33.6
58	78.2	61.0	91.4

