

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020114.D
 Acq On : 10 Jun 2022 23:58
 Operator : CG/JU
 Sample : N3250-09
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYW7

Quant Time: Jun 11 01:14:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	158907	20.000	ng/u1	0.00
20) Naphthalene-d8	10.610	136	762567	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.445	164	501401	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.186	188	1045032	20.000	ng/u1	0.00
79) Chrysene-d12	21.374	240	936625	20.000	ng/u1	0.00
88) Perylene-d12	23.698	264	821265	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	17777	4.845	ng/uL	0.00
4) Pyridine-d5	3.693	84	74971	7.476	ng/u1	0.00
7) Phenol-d5	6.987	99	83074	6.318	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.146	67	249755	30.401	ng/u1	0.00
11) 2-Chlorophenol-d4	7.352	132	253049	23.685	ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	172789	15.189	ng/u1	0.00
21) Nitrobenzene-d5	8.969	128	171977	29.644	ng/u1	0.00
24) 2-Nitrophenol-d4	9.693	143	181310	29.448	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	284167	26.438	ng/u1	0.00
31) 4-Chloroaniline-d4	10.740	131	401750	23.081	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	1159669	31.787	ng/u1	0.00
49) Acenaphthylene-d8	14.140	160	1301349	30.758	ng/u1	0.00
54) 4-Nitrophenol-d4	14.640	143	39024	5.338	ng/u1	0.00
60) Fluorene-d10	15.434	176	1011531	33.506	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.551	200	195765	32.339	ng/u1	-0.01
73) Anthracene-d10	17.286	188	1748714	38.342	ng/u1	0.00
81) Pyrene-d10	19.580	212	1985963	39.112	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.551	264	1628669	40.532	ng/u1	-0.01


Target Compounds				Qvalue	
2) 1,4-Dioxane	3.317	88	4759	1.229 ng/uL#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020114.D
Acq On : 10 Jun 2022 23:58
Operator : CG/JU
Sample : N3250-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW7


Quant Time: Jun 11 01:14:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration

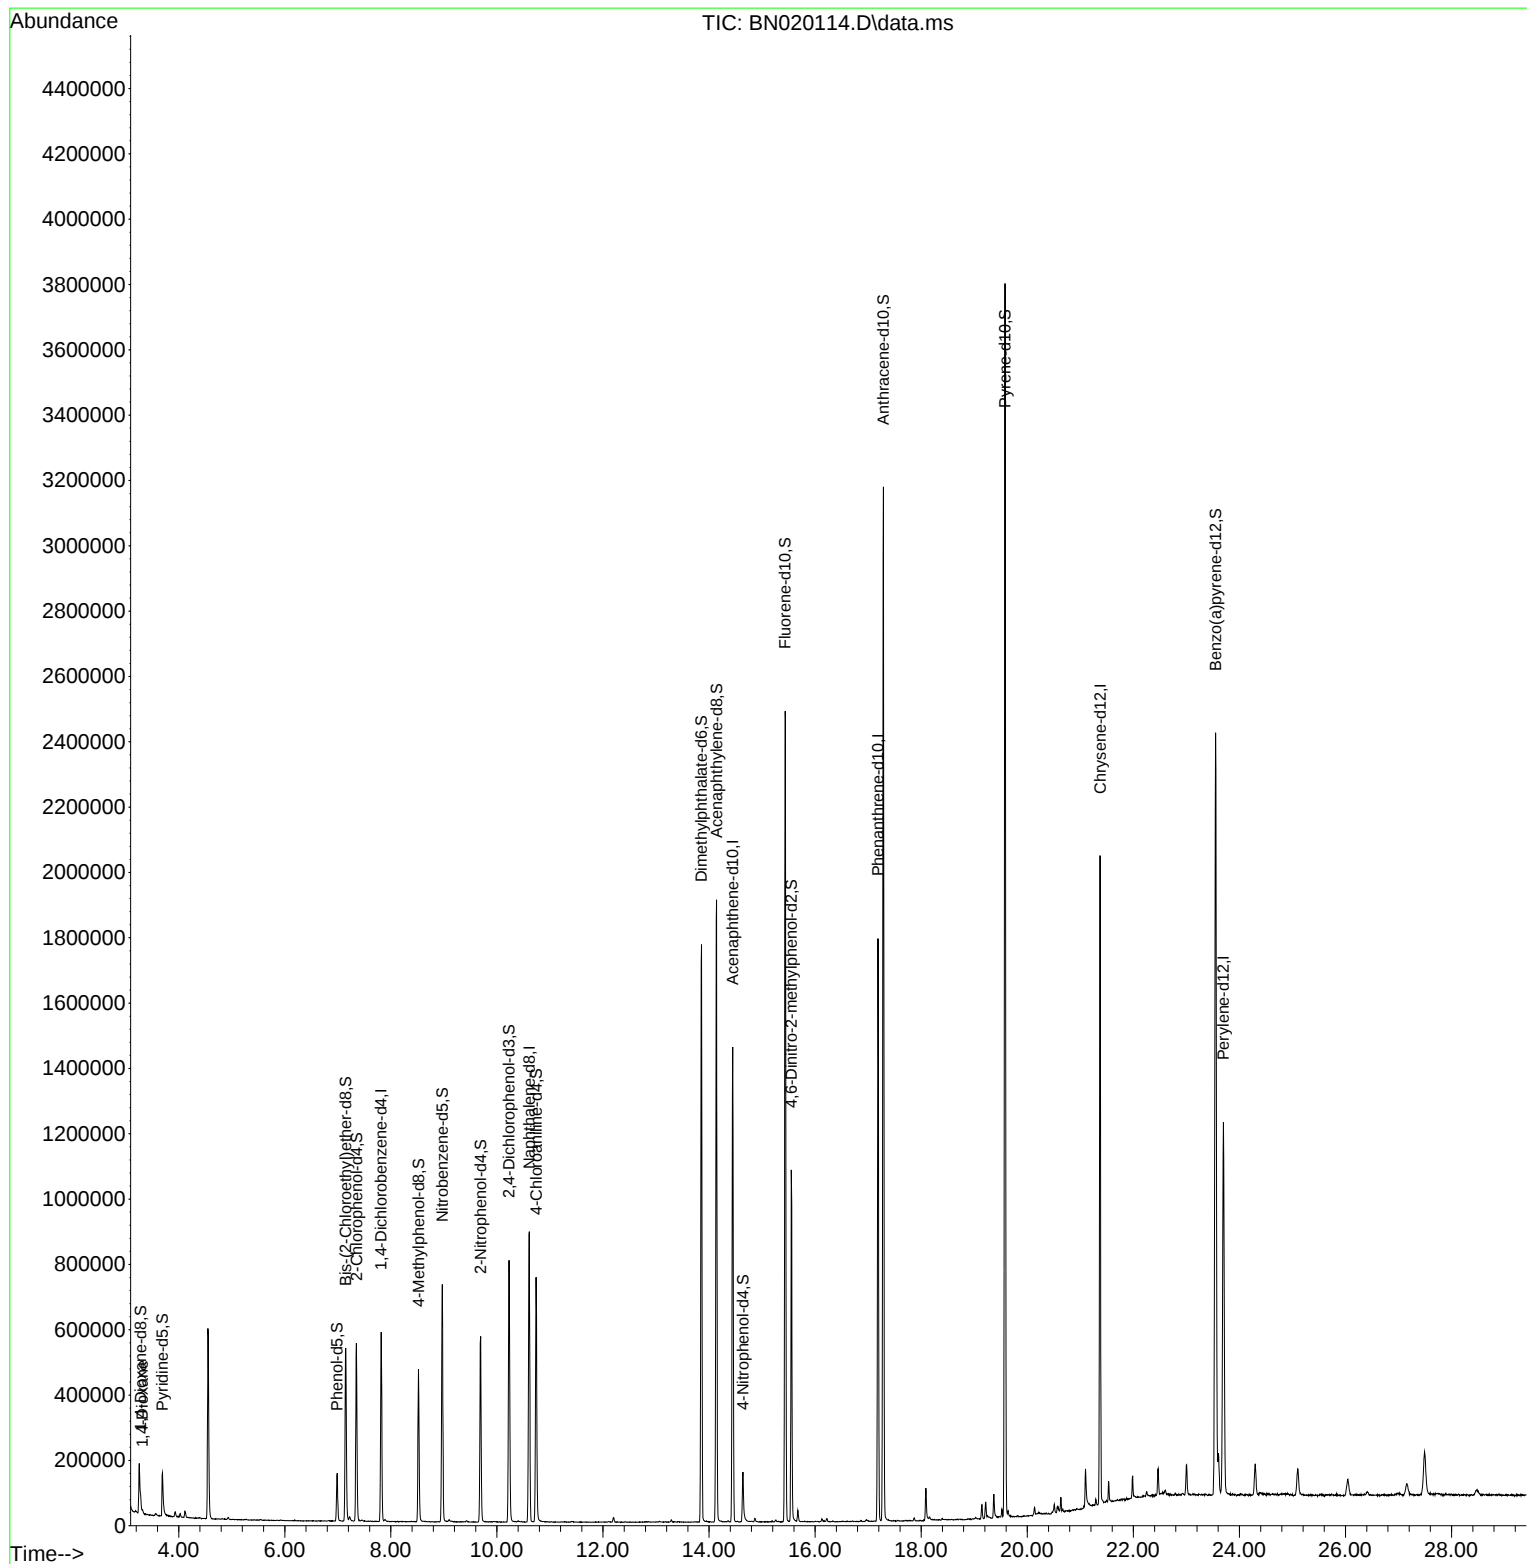

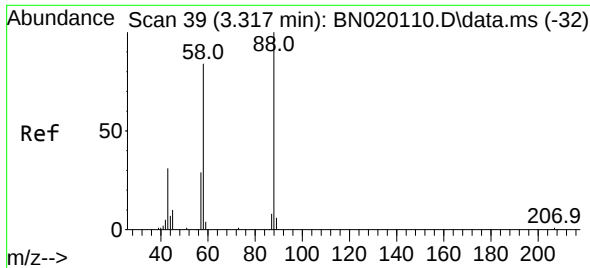

#2
 1,4-Dioxane
 Concen: 1.229 ng/uL
 RT: 3.317 min Scan# 39
 Delta R.T. 0.001 min
 Lab File: BN020114.D
 Acq: 10 Jun 2022 23:58

Instrument :
 BNA_N
 ClientSampleId :
 EXYW7

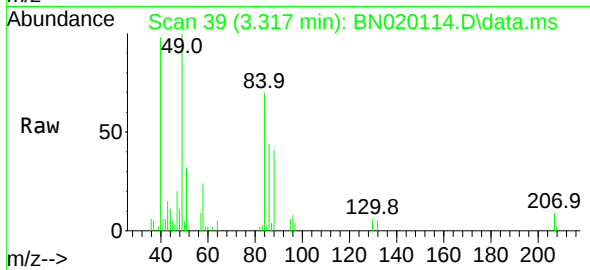

Tgt Ion: 88 Resp: 4759

Ion	Ratio	Lower	Upper
88	100		
43	35.7	22.4	33.6#
58	58.0	61.0	91.4#

