

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020115.D
 Acq On : 11 Jun 2022 00:34
 Operator : CG/JU
 Sample : N3250-16
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYT2

Quant Time: Jun 11 01:14:41 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	81265	20.000	ng/u1	0.00
20) Naphthalene-d8	10.604	136	393332	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.445	164	255446	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.186	188	536197	20.000	ng/u1	0.00
79) Chrysene-d12	21.369	240	507440	20.000	ng/u1	-0.01
88) Perylene-d12	23.698	264	424928	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	16319	8.698	ng/uL	0.00
4) Pyridine-d5	3.687	84	95604	18.643	ng/u1	0.00
7) Phenol-d5	6.987	99	77522	11.528	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.146	67	262316	62.437	ng/u1	0.00
11) 2-Chlorophenol-d4	7.352	132	262413	48.028	ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	173765	29.868	ng/u1	0.00
21) Nitrobenzene-d5	8.969	128	178693	59.716	ng/u1	0.00
24) 2-Nitrophenol-d4	9.693	143	191479	60.294	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	301085	54.308	ng/u1	0.00
31) 4-Chloroaniline-d4	10.740	131	447740	49.871	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	1305620	70.245	ng/u1	0.00
49) Acenaphthylene-d8	14.140	160	1414481	65.623	ng/u1	0.00
54) 4-Nitrophenol-d4	14.640	143	36278	9.740	ng/u1	0.00
60) Fluorene-d10	15.434	176	1065812	69.296	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.551	200	196056	63.122	ng/u1	-0.01
73) Anthracene-d10	17.281	188	1768769	75.585	ng/u1	-0.01
81) Pyrene-d10	19.580	212	1964993	71.430	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.551	264	1601632	77.036	ng/u1	-0.01


Target Compounds					Qvalue
2) 1,4-Dioxane	3.317	88	26089	13.171 ng/uL	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020115.D
Acq On : 11 Jun 2022 00:34
Operator : CG/JU
Sample : N3250-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYT2


Quant Time: Jun 11 01:14:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration

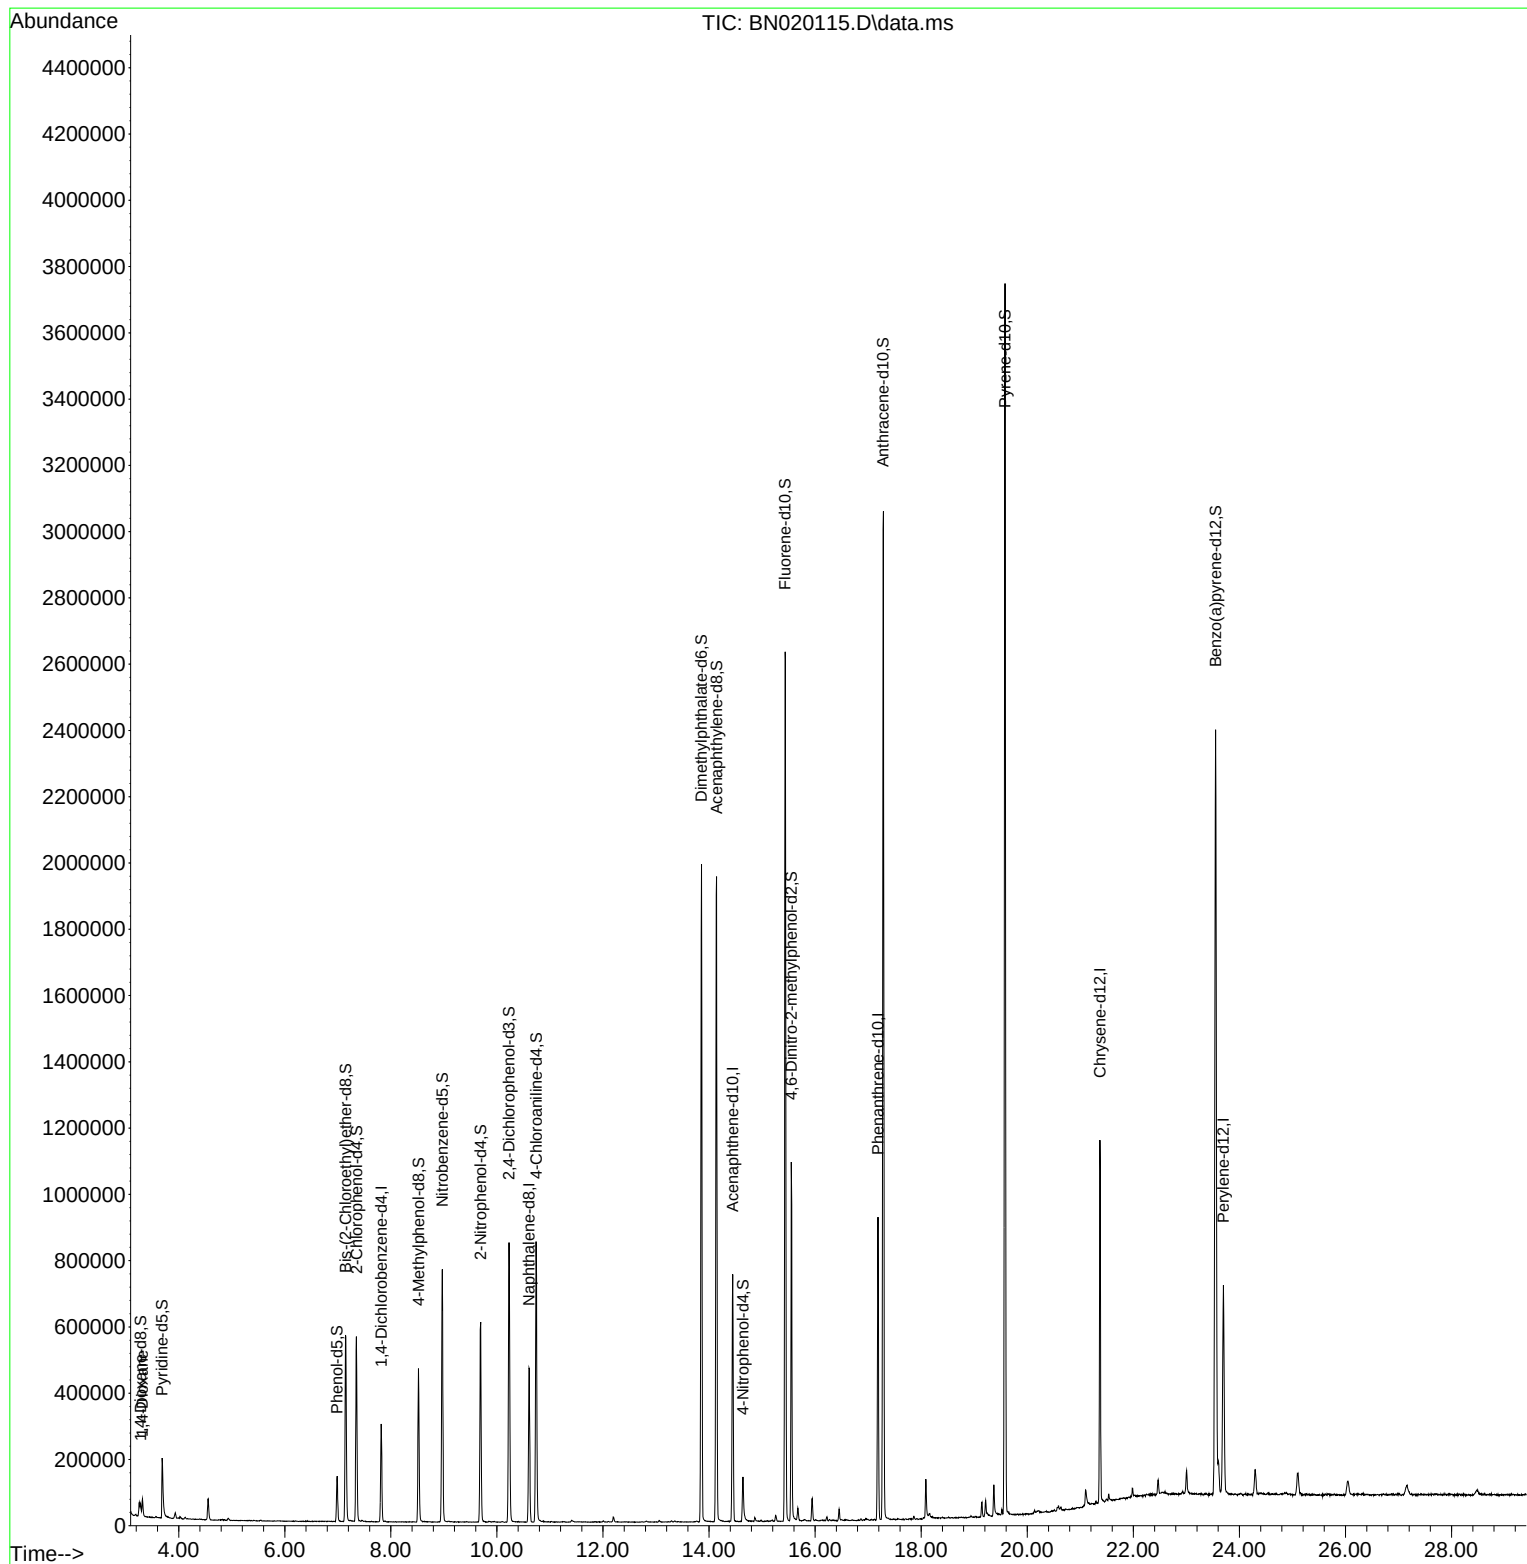

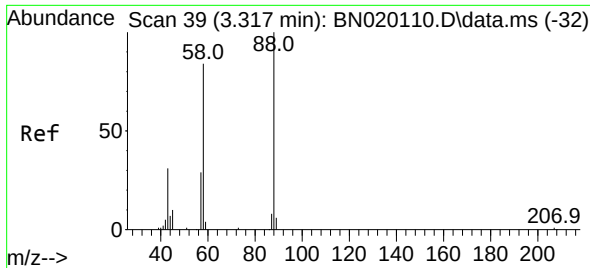

#2
 1,4-Dioxane
 Concen: 13.171 ng/uL
 RT: 3.317 min Scan# 39
 Delta R.T. 0.001 min
 Lab File: BN020115.D
 Acq: 11 Jun 2022 00:34

Instrument :
 BNA_N
 ClientSampleId :
 EXYT2

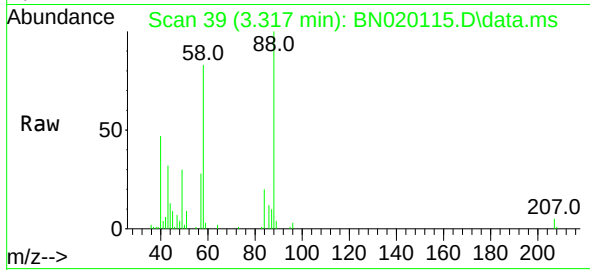

Tgt Ion:	88	Resp:	26089
Ion	Ratio	Lower	Upper
88	100		
43	32.4	22.4	33.6
58	83.3	61.0	91.4

