

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020118.D
 Acq On : 11 Jun 2022 02:22
 Operator : CG/JU
 Sample : N3250-13
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYZ3

Quant Time: Jun 11 03:21:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	154625	20.000	ng/u1	0.00
20) Naphthalene-d8	10.604	136	733216	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.445	164	484574	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.186	188	1012668	20.000	ng/u1	0.00
79) Chrysene-d12	21.368	240	892826	20.000	ng/u1	-0.01
88) Perylene-d12	23.698	264	786263	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	16073	4.502	ng/uL	0.00
4) Pyridine-d5	3.693	84	72521	7.432	ng/u1	0.00
7) Phenol-d5	6.987	99	74102	5.792	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.146	67	243954	30.517	ng/u1	0.00
11) 2-Chlorophenol-d4	7.352	132	246231	23.685	ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	163606	14.780	ng/u1	0.00
21) Nitrobenzene-d5	8.969	128	173561	31.114	ng/u1	0.00
24) 2-Nitrophenol-d4	9.693	143	183501	30.997	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	292181	28.272	ng/u1	0.00
31) 4-Chloroaniline-d4	10.740	131	402939	24.076	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	1140605	32.350	ng/u1	0.00
49) Acenaphthylene-d8	14.139	160	1307341	31.973	ng/u1	0.00
54) 4-Nitrophenol-d4	14.639	143	39111	5.536	ng/u1	0.00
60) Fluorene-d10	15.439	176	970174	33.252	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.551	200	188974	32.215	ng/u1	-0.01
73) Anthracene-d10	17.286	188	1607907	36.382	ng/u1	0.00
81) Pyrene-d10	19.580	212	1853113	38.286	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.551	264	1438415	37.391	ng/u1	-0.01


Target Compounds					Qvalue
2) 1,4-Dioxane	3.316	88	15999	4.245	ng/uL 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020118.D
Acq On : 11 Jun 2022 02:22
Operator : CG/JU
Sample : N3250-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYZ3


Quant Time: Jun 11 03:21:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration

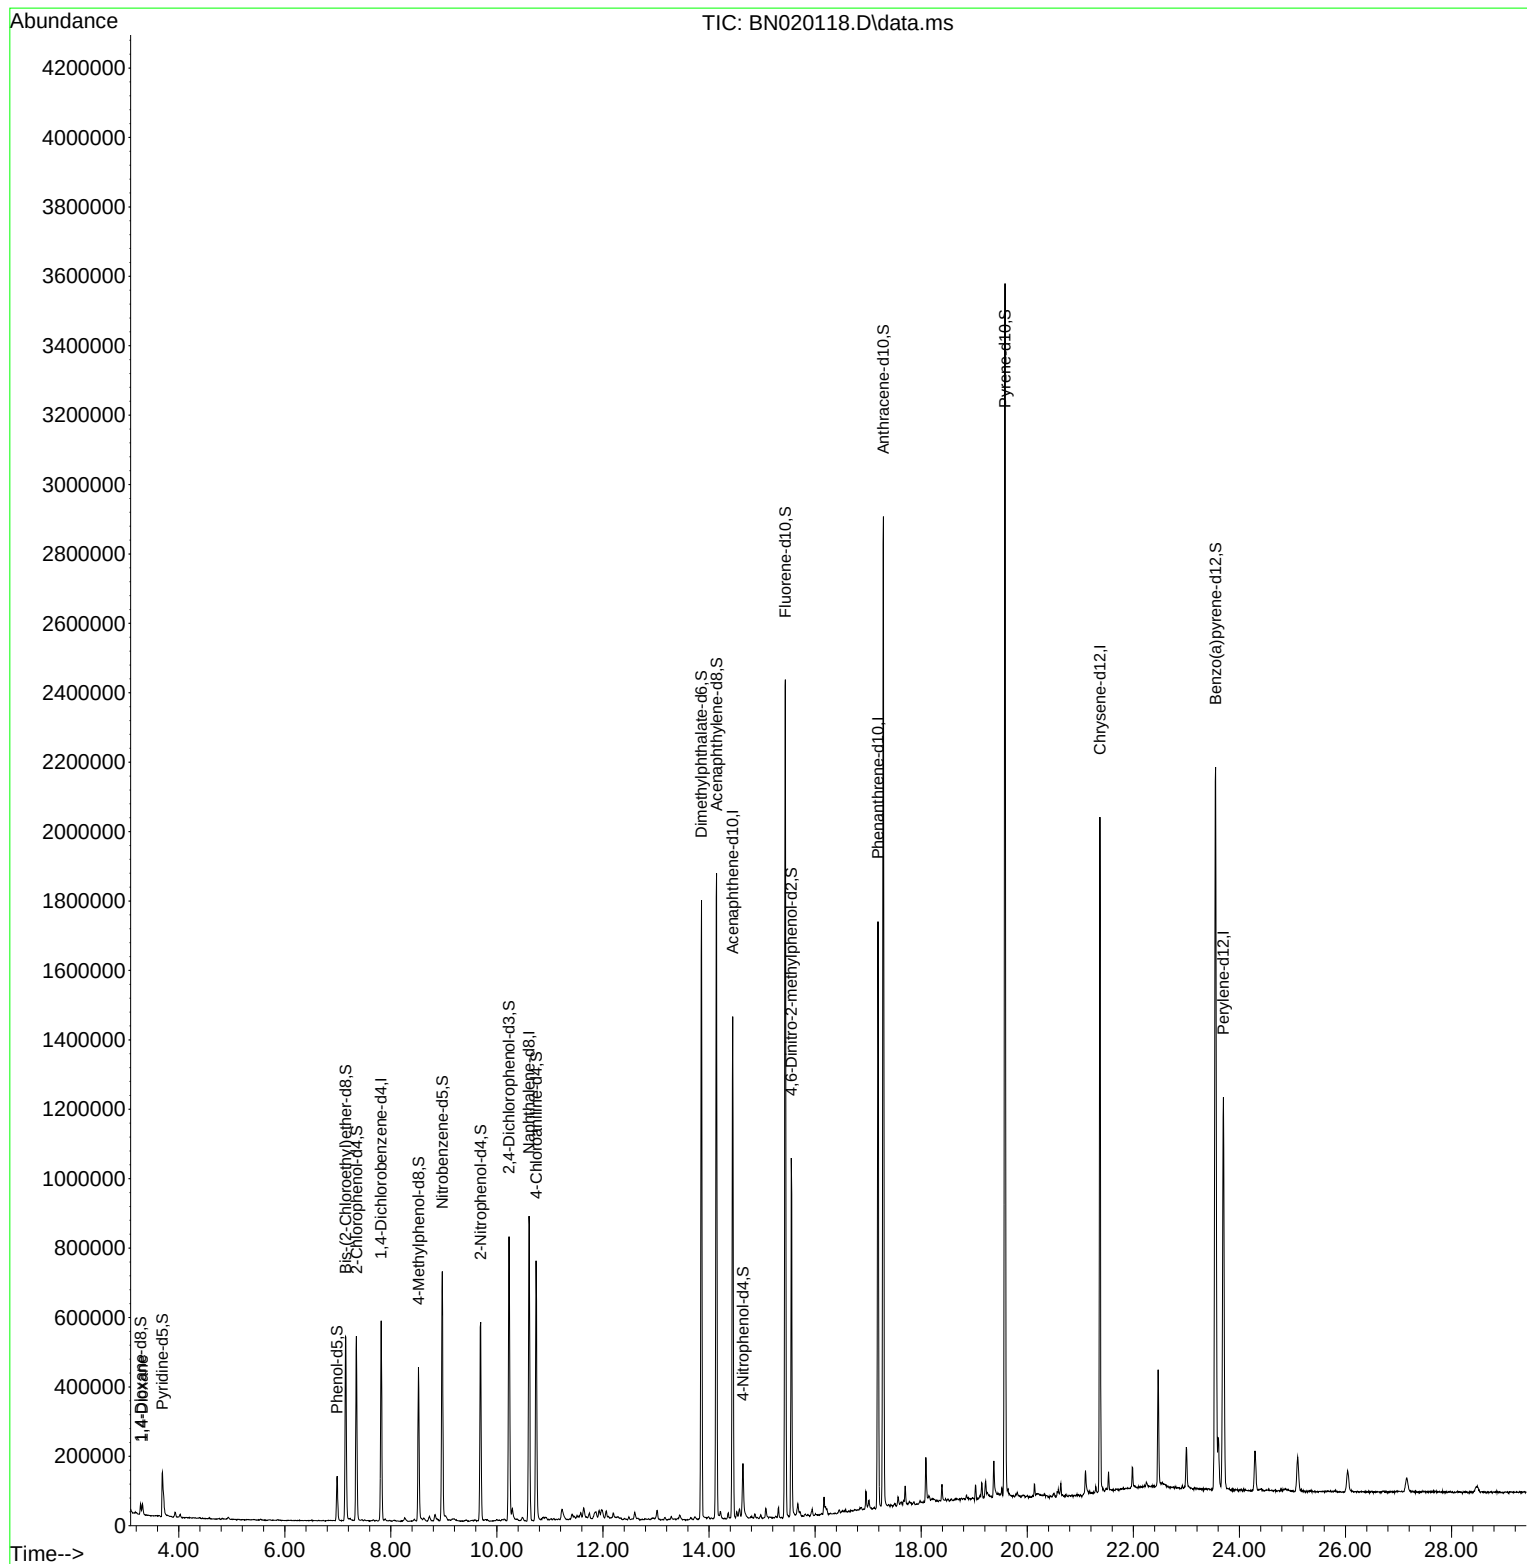

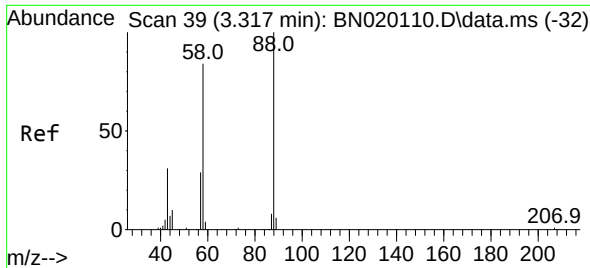

#2
 1,4-Dioxane
 Concen: 4.245 ng/uL
 RT: 3.316 min Scan# 39
 Delta R.T. 0.000 min
 Lab File: BN020118.D
 Acq: 11 Jun 2022 02:22

Instrument :
 BNA_N
 ClientSampleId :
 EXYZ3

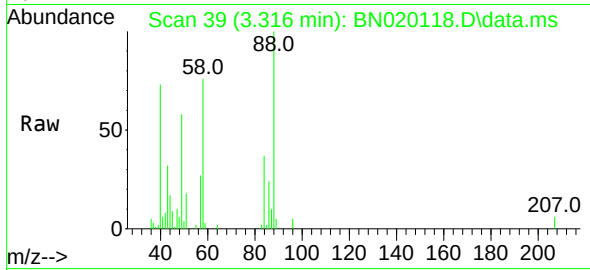

Tgt Ion: 88 Resp: 15999

Ion	Ratio	Lower	Upper
88	100		
43	31.7	22.4	33.6
58	75.7	61.0	91.4

