

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020129.D
 Acq On : 11 Jun 2022 09:32
 Operator : CG/JU
 Sample : N3284-10
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYX5

Quant Time: Jun 13 00:43:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	171168	20.000	ng/u1	0.00
20) Naphthalene-d8	10.604	136	789221	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.445	164	518408	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.186	188	1066491	20.000	ng/u1	0.00
79) Chrysene-d12	21.375	240	920547	20.000	ng/u1	0.00
88) Perylene-d12	23.698	264	791604	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	20838	5.273	ng/uL	0.00
4) Pyridine-d5	3.687	84	139022	12.871	ng/u1	0.00
7) Phenol-d5	6.987	99	109709	7.746	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.146	67	292964	33.106	ng/u1	0.00
11) 2-Chlorophenol-d4	7.352	132	314253	27.307	ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	234625	19.147	ng/u1	0.00
21) Nitrobenzene-d5	8.969	128	208493	34.724	ng/u1	0.00
24) 2-Nitrophenol-d4	9.687	143	226529	35.550	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.228	165	376568	33.852	ng/u1	0.00
31) 4-Chloroaniline-d4	10.740	131	430866	23.918	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	1372374	36.383	ng/u1	0.00
49) Acenaphthylene-d8	14.140	160	1569927	35.889	ng/u1	0.00
54) 4-Nitrophenol-d4	14.640	143	56300	7.448	ng/u1	0.00
60) Fluorene-d10	15.434	176	1145066	36.685	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.551	200	218523	35.373	ng/u1	-0.01
73) Anthracene-d10	17.281	188	1770491	38.039	ng/u1	-0.01
81) Pyrene-d10	19.580	212	1883918	37.750	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.551	264	1457163	37.622	ng/u1	-0.01


Target Compounds					Qvalue
2) 1,4-Dioxane	3.317	88	102914	24.668	ng/uL# 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020129.D
Acq On : 11 Jun 2022 09:32
Operator : CG/JU
Sample : N3284-10
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYX5


Quant Time: Jun 13 00:43:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration

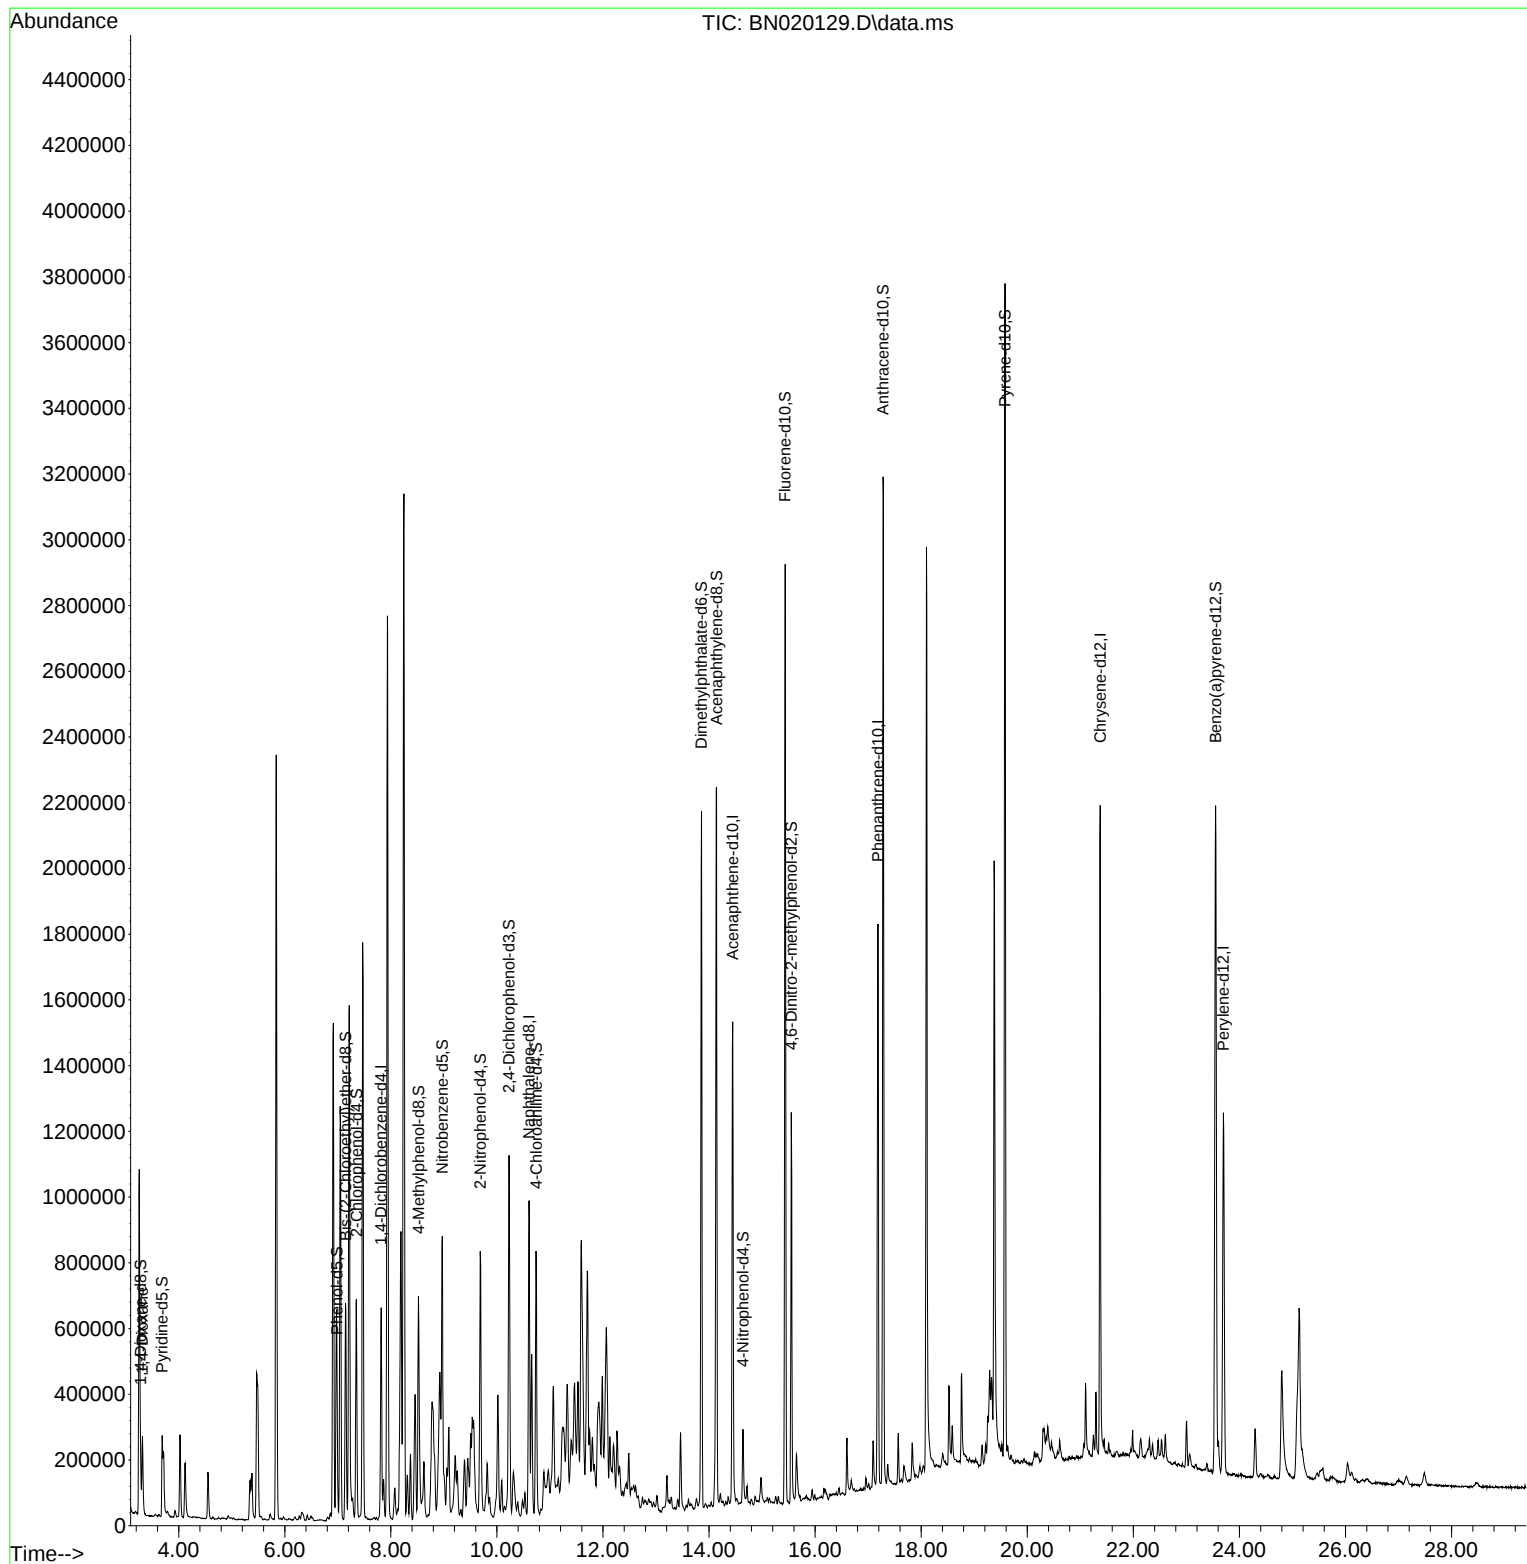

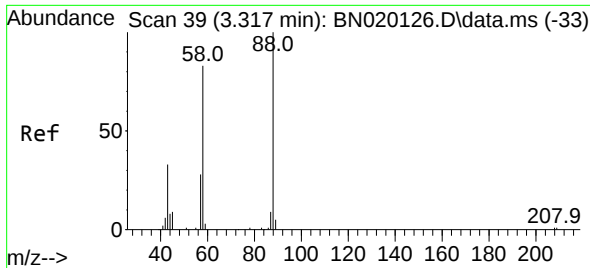

#2
 1,4-Dioxane
 Concen: 24.668 ng/uL
 RT: 3.317 min Scan# 39
 Delta R.T. 0.001 min
 Lab File: BN020129.D
 Acq: 11 Jun 2022 09:32

Instrument :
 BNA_N
 ClientSampleId :
 EXYX5

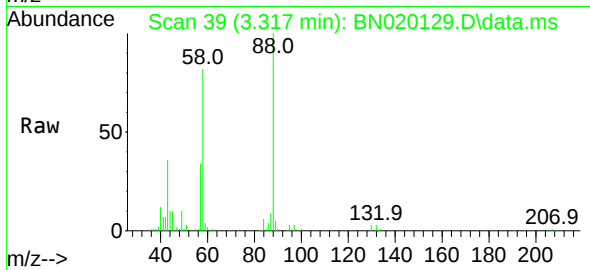

Tgt Ion: 88 Resp: 102914
 Ion Ratio Lower Upper
 88 100
 43 36.0 22.4 33.6#
 58 82.0 61.0 91.4

