

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020134.D
 Acq On : 11 Jun 2022 12:30
 Operator : CG/JU
 Sample : N3284-06
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYX2

Quant Time: Jun 13 00:44:41 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	168192	20.000	ng/u1	0.00
20) Naphthalene-d8	10.605	136	785845	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.440	164	519438	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.181	188	1080528	20.000	ng/u1	-0.01
79) Chrysene-d12	21.369	240	930235	20.000	ng/u1	-0.01
88) Perylene-d12	23.698	264	809466	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	16489	4.246	ng/uL	0.00
4) Pyridine-d5	3.687	84	89470	8.430	ng/u1	0.00
7) Phenol-d5	6.981	99	92687	6.660	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.146	67	258460	29.724	ng/u1	0.00
11) 2-Chlorophenol-d4	7.346	132	272815	24.125	ng/u1	-0.01
15) 4-Methylphenol-d8	8.522	113	189198	15.713	ng/u1	0.00
21) Nitrobenzene-d5	8.969	128	187053	31.287	ng/u1	0.00
24) 2-Nitrophenol-d4	9.687	143	196784	31.015	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.228	165	317487	28.663	ng/u1	0.00
31) 4-Chloroaniline-d4	10.740	131	419728	23.400	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	1285283	34.007	ng/u1	0.00
49) Acenaphthylene-d8	14.134	160	1466907	33.468	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.640	143	47232	6.236	ng/u1	0.00
60) Fluorene-d10	15.434	176	1095252	35.019	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.551	200	205228	32.789	ng/u1	-0.01
73) Anthracene-d10	17.281	188	1779461	37.735	ng/u1	-0.01
81) Pyrene-d10	19.581	212	1930086	38.273	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.551	264	1567127	39.569	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.317	88	31707	7.734	ng/uL	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020134.D
Acq On : 11 Jun 2022 12:30
Operator : CG/JU
Sample : N3284-06
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYX2

Quant Time: Jun 13 00:44:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration

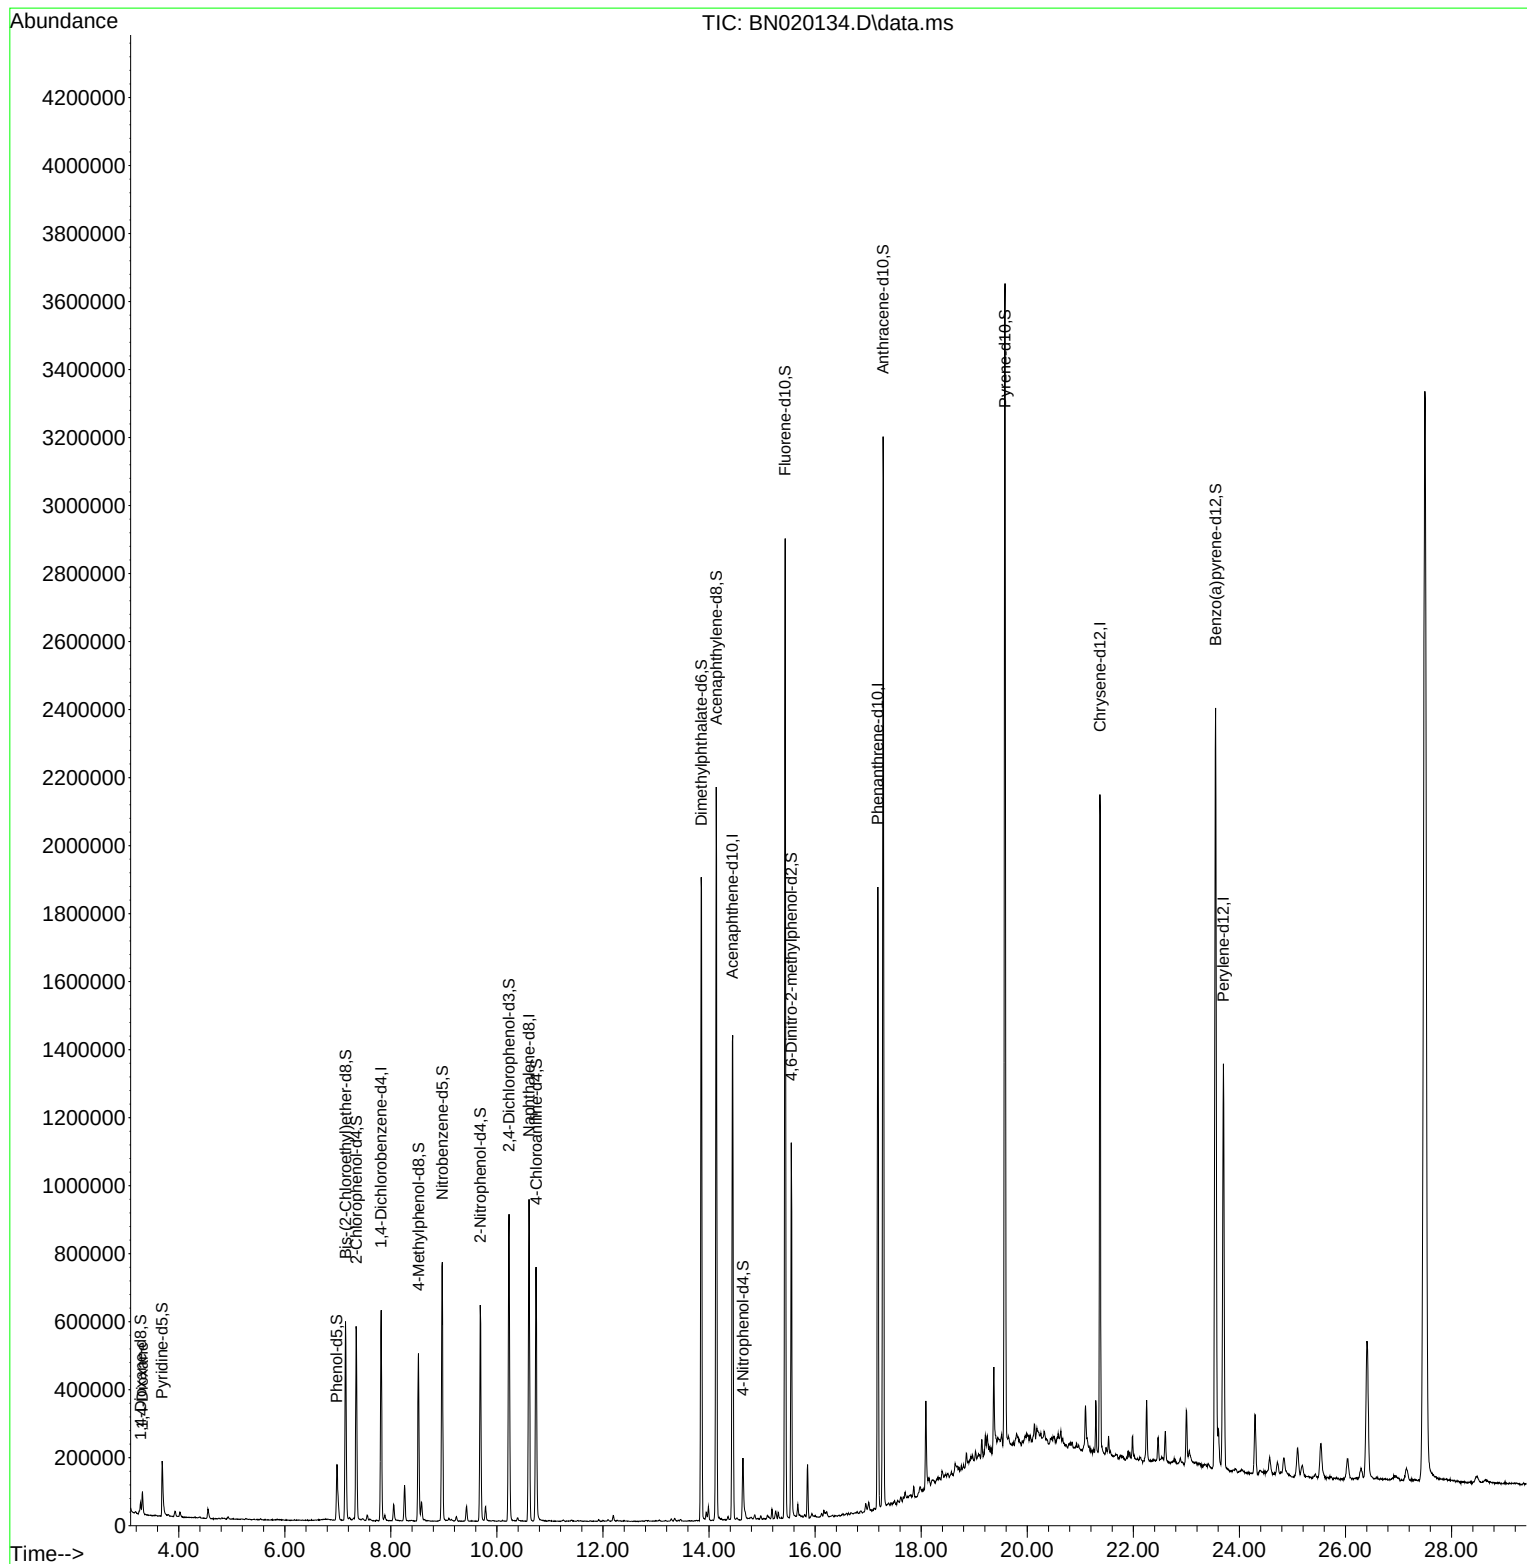

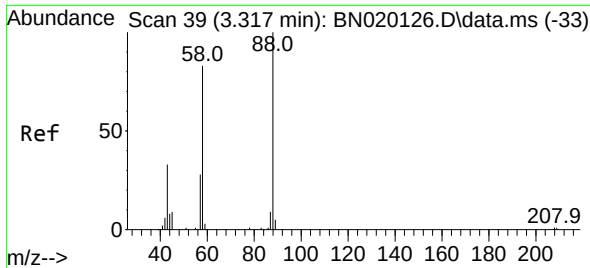

#2

1,4-Dioxane

Concen: 7.734 ng/uL

RT: 3.317 min Scan# 39

Delta R.T. 0.001 min

Lab File: BN020134.D


Acq: 11 Jun 2022 12:30

Instrument :

BNA_N

ClientSampleId :

EXYX2

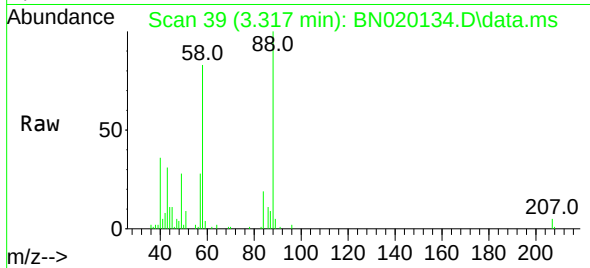

Tgt Ion: 88 Resp: 31707

Ion Ratio Lower Upper

88 100

43 30.7 22.4 33.6

58 82.5 61.0 91.4

