

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020136.D
 Acq On : 11 Jun 2022 13:42
 Operator : CG/JU
 Sample : N3284-08
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYX3

Quant Time: Jun 13 00:44:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	150932	20.000	ng/u1	0.00
20) Naphthalene-d8	10.604	136	721227	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.445	164	480884	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.181	188	1008540	20.000	ng/u1	-0.01
79) Chrysene-d12	21.374	240	897260	20.000	ng/u1	0.00
88) Perylene-d12	23.698	264	764780	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	15956	4.579	ng/uL	0.00
4) Pyridine-d5	3.687	84	99238	10.419	ng/u1	0.00
7) Phenol-d5	6.981	99	82309	6.590	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.146	67	255507	32.745	ng/u1	0.00
11) 2-Chlorophenol-d4	7.346	132	255046	25.133	ng/u1	-0.01
15) 4-Methylphenol-d8	8.522	113	171905	15.909	ng/u1	0.00
21) Nitrobenzene-d5	8.969	128	180458	32.889	ng/u1	0.00
24) 2-Nitrophenol-d4	9.687	143	186636	32.051	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.228	165	293663	28.888	ng/u1	0.00
31) 4-Chloroaniline-d4	10.740	131	429440	26.086	ng/u1	0.00
46) Dimethylphthalate-d6	13.851	166	1159590	33.141	ng/u1	-0.01
49) Acenaphthylene-d8	14.134	160	1337219	32.955	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.640	143	34029	4.853	ng/u1	0.00
60) Fluorene-d10	15.434	176	1026050	35.437	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.551	200	182579	31.252	ng/u1	-0.01
73) Anthracene-d10	17.281	188	1714392	38.950	ng/u1	-0.01
81) Pyrene-d10	19.580	212	1891945	38.895	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.551	264	1514461	40.473	ng/u1	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.317	88	25216	6.854	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020136.D
Acq On : 11 Jun 2022 13:42
Operator : CG/JU
Sample : N3284-08
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYX3


Quant Time: Jun 13 00:44:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration

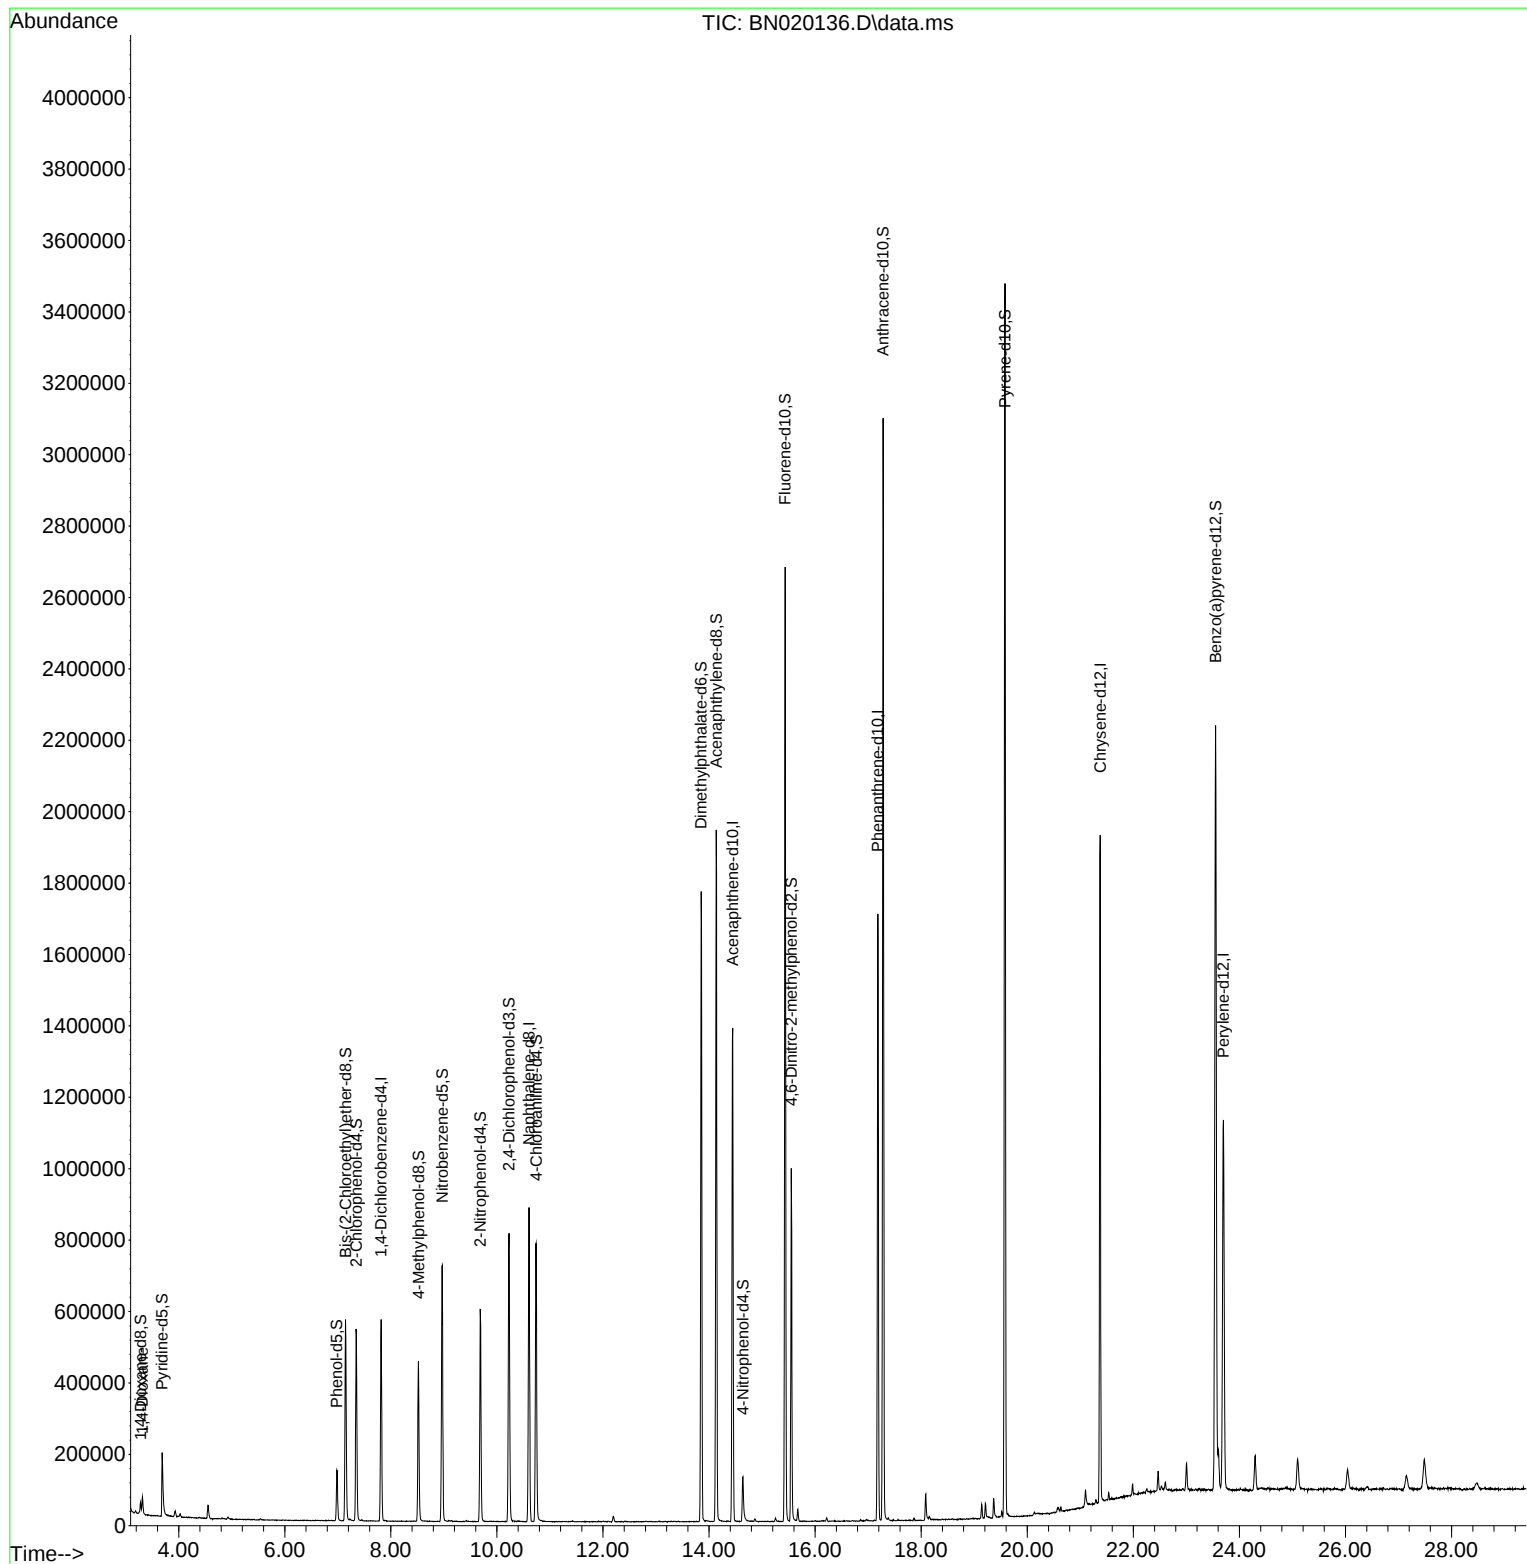

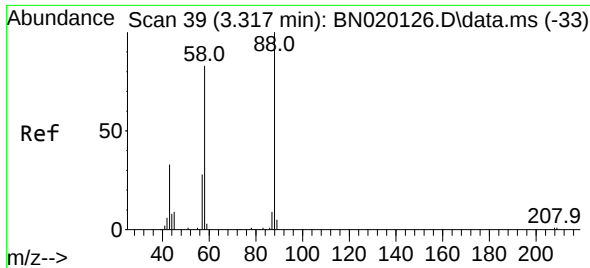

#2
 1,4-Dioxane
 Concen: 6.854 ng/uL
 RT: 3.317 min Scan# 39
 Delta R.T. 0.001 min
 Lab File: BN020136.D
 Acq: 11 Jun 2022 13:42

Instrument :
 BNA_N
 ClientSampleId :
 EXYX3

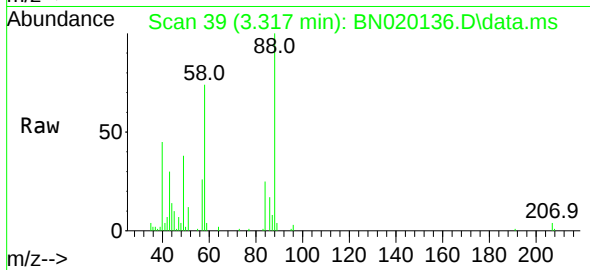

Tgt Ion:	88	Resp:	25216
Ion	Ratio	Lower	Upper
88	100		
43	29.7	22.4	33.6
58	73.7	61.0	91.4

