

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020095.D
 Acq On : 10 Jun 2022 11:53
 Operator : CG/JU
 Sample : PB145433BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK433

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020095.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	39	rVB	33826	48145	1.31%	0.126%
2	3.687	98	102	119	rBV	460910	750965	20.44%	1.969%
3	4.028	157	160	167	rVB	8793	12831	0.35%	0.034%
4	6.987	655	663	675	rBV	552025	912067	24.83%	2.391%
5	7.152	684	691	700	rBV	448909	729104	19.85%	1.911%
6	7.352	718	725	737	rBV	567823	950173	25.87%	2.491%
7	7.816	797	804	813	rBV	441660	748097	20.37%	1.961%
8	8.522	917	924	940	rBV	742278	1214833	33.07%	3.185%
9	8.969	993	1000	1013	rBV	579520	958659	26.10%	2.513%
10	9.693	1116	1123	1135	rBV	476529	802382	21.84%	2.103%
11	10.228	1204	1214	1225	rBV	683289	1184938	32.26%	3.106%
12	10.610	1269	1279	1293	rBV	678963	1202842	32.75%	3.153%
13	10.740	1293	1301	1317	rBV	778257	1340473	36.49%	3.514%
14	12.199	1543	1549	1557	rBV3	10398	20089	0.55%	0.053%
15	13.857	1824	1831	1843	rBV	1407783	1928794	52.51%	5.056%
16	14.140	1872	1879	1889	rBV	1475926	2224523	60.56%	5.831%
17	14.445	1924	1931	1939	rBV	1139556	1690776	46.03%	4.432%
18	14.640	1957	1964	1982	rBV	595513	938483	25.55%	2.460%
19	15.434	2093	2099	2113	rBV	1865894	2818224	76.72%	7.388%
20	15.551	2113	2119	2135	rVV	549602	797116	21.70%	2.090%
21	15.675	2136	2140	2146	rVB	21907	32638	0.89%	0.086%
22	16.222	2228	2233	2237	rVB5	6011	9973	0.27%	0.026%
23	16.869	2337	2343	2348	rBV5	3072	4795	0.13%	0.013%
24	16.975	2355	2361	2365	rBV4	4672	6641	0.18%	0.017%
25	17.186	2390	2397	2407	rBV	1383603	2005848	54.61%	5.258%
26	17.286	2407	2414	2428	rVV	2150304	3184133	86.69%	8.347%
27	19.145	2723	2730	2735	rBV3	23648	36175	0.98%	0.095%
28	19.216	2737	2742	2749	rVB2	24437	34216	0.93%	0.090%
29	19.580	2798	2804	2817	rBV	2606967	3673221	100.00%	9.629%
30	20.192	2902	2908	2909	rBV4	8701	12255	0.33%	0.032%
31	20.216	2909	2912	2915	rVV5	5406	9014	0.25%	0.024%
32	20.592	2969	2976	2980	rBV6	11960	19650	0.53%	0.052%
33	21.380	3104	3110	3122	rBV	1556059	2144881	58.39%	5.623%
34	22.480	3294	3297	3301	rVB2	23237	28291	0.77%	0.074%
35	23.010	3384	3387	3392	rVB	35310	53357	1.45%	0.140%
36	23.563	3472	3481	3487	rBV	1637897	3351246	91.23%	8.785%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020095.D
Acq On : 10 Jun 2022 11:53
Operator : CG/JU
Sample : PB145433BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK433

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Title : SVOA CALIBRATION

37	23.710	3498	3506	3517	rVB2	970857	1924212	52.38%	5.044%
38	24.304	3603	3607	3617	rVB2	56961	119786	3.26%	0.314%
39	25.110	3738	3744	3752	rVB3	56557	131322	3.58%	0.344%
40	26.051	3900	3904	3911	rVB3	38435	92418	2.52%	0.242%




Sum of corrected areas: 38147586

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020095.D
Acq On : 10 Jun 2022 11:53
Operator : CG/JU
Sample : PB145433BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK433

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

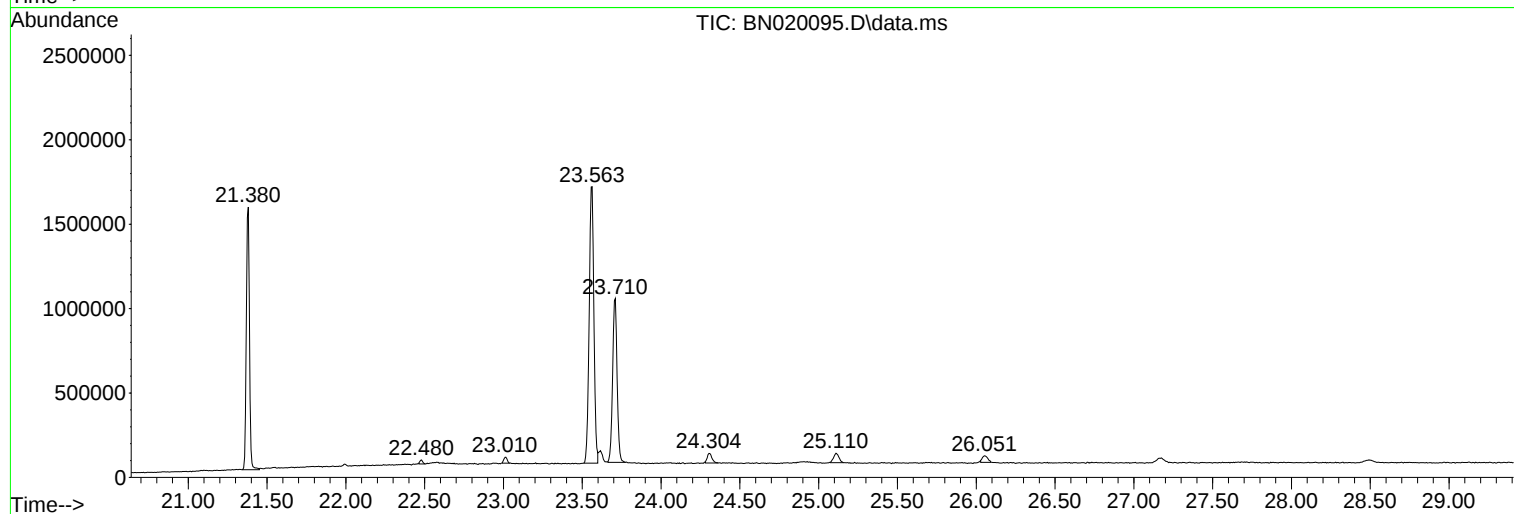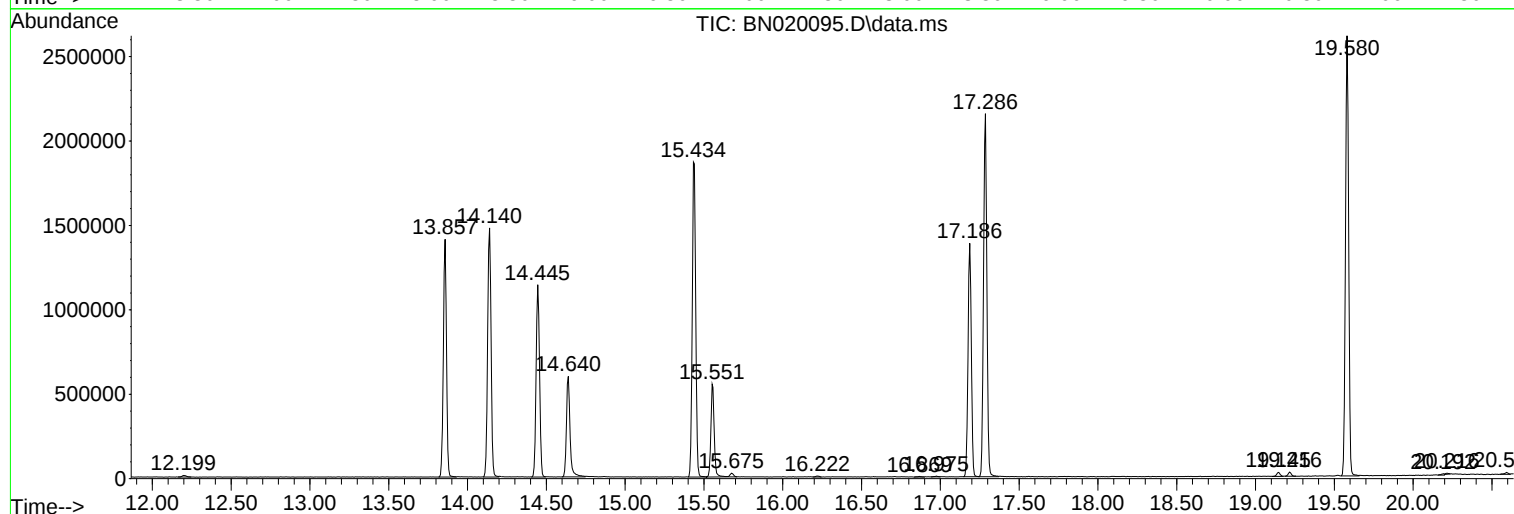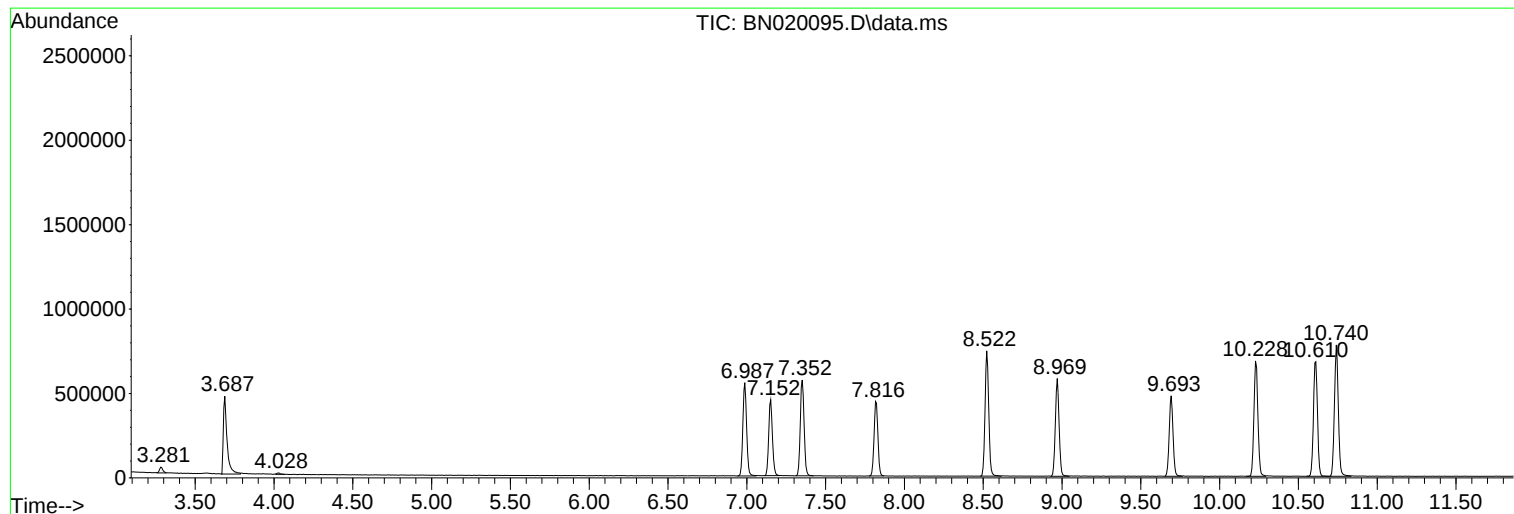

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020095.D
Acq On : 10 Jun 2022 11:53
Operator : CG/JU
Sample : PB145433BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK433

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020095.D
Acq On : 10 Jun 2022 11:53
Operator : CG/JU
Sample : PB145433BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK433

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc