

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020096.D
 Acq On : 10 Jun 2022 12:29
 Operator : CG/JU
 Sample : PB145445BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK445

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020096.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	41	rVB	38180	57178	1.44%	0.137%
2	3.687	98	102	127	rBV	526896	862469	21.75%	2.061%
3	4.028	157	160	169	rVB3	9329	14584	0.37%	0.035%
4	6.987	657	663	677	rBV	640252	1035048	26.10%	2.473%
5	7.152	684	691	703	rBV	512497	831901	20.98%	1.988%
6	7.352	717	725	741	rVB	650218	1076900	27.16%	2.573%
7	7.816	798	804	813	rBV	492250	806620	20.34%	1.928%
8	8.522	917	924	937	rBV	840517	1370063	34.55%	3.274%
9	8.969	993	1000	1014	rBV	643842	1081064	27.27%	2.583%
10	9.693	1115	1123	1132	rBV	531371	900420	22.71%	2.152%
11	10.228	1207	1214	1225	rBV	777159	1346498	33.96%	3.218%
12	10.610	1271	1279	1288	rBV	740493	1306765	32.96%	3.123%
13	10.740	1293	1301	1317	rBV	863598	1553566	39.18%	3.712%
14	12.198	1543	1549	1559	rVB2	12417	23556	0.59%	0.056%
15	13.357	1741	1746	1750	rVB4	3528	5459	0.14%	0.013%
16	13.857	1824	1831	1843	rBV	1552403	2167574	54.67%	5.180%
17	14.139	1871	1879	1893	rBV	1687777	2542233	64.12%	6.075%
18	14.445	1923	1931	1940	rBV	1228069	1825991	46.05%	4.363%
19	14.639	1958	1964	1979	rBV	691050	1054846	26.60%	2.521%
20	15.439	2092	2100	2109	rBV	2156078	3186501	80.37%	7.614%
21	15.551	2114	2119	2135	rVV	607262	888392	22.41%	2.123%
22	15.675	2135	2140	2146	rVB3	26536	40227	1.01%	0.096%
23	16.222	2225	2233	2238	rVB3	7083	12858	0.32%	0.031%
24	16.975	2357	2361	2365	rVB5	2841	5178	0.13%	0.012%
25	17.186	2390	2397	2406	rBV	1501269	2180888	55.00%	5.211%
26	17.286	2406	2414	2428	rVV2	2365453	3503765	88.37%	8.373%
27	18.092	2547	2551	2556	rBV6	2998	5274	0.13%	0.013%
28	18.163	2556	2563	2566	rBV6	2619	4535	0.11%	0.011%
29	18.727	2653	2659	2663	rBV3	2284	4222	0.11%	0.010%
30	19.145	2725	2730	2735	rBV2	29500	40111	1.01%	0.096%
31	19.216	2738	2742	2749	rVV	27329	36136	0.91%	0.086%
32	19.522	2790	2794	2798	rBV5	5163	8362	0.21%	0.020%
33	19.580	2798	2804	2816	rVV	2867561	3964993	100.00%	9.475%
34	20.592	2974	2976	2980	rVB3	8920	9995	0.25%	0.024%
35	21.374	3103	3109	3120	rBV	1795971	2323079	58.59%	5.551%
36	23.010	3383	3387	3391	rVB2	22294	35535	0.90%	0.085%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020096.D
Acq On : 10 Jun 2022 12:29
Operator : CG/JU
Sample : PB145445BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK445

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Title : SVOA CALIBRATION

37	23.557	3471	3480	3488	rBV	1751765	3557221	89.72%	8.500%
38	23.704	3497	3505	3517	rVB2	999415	2093450	52.80%	5.003%
39	24.304	3603	3607	3620	rVB3	37618	84360	2.13%	0.202%




Sum of corrected areas: 41847817

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020096.D
Acq On : 10 Jun 2022 12:29
Operator : CG/JU
Sample : PB145445BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK445

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

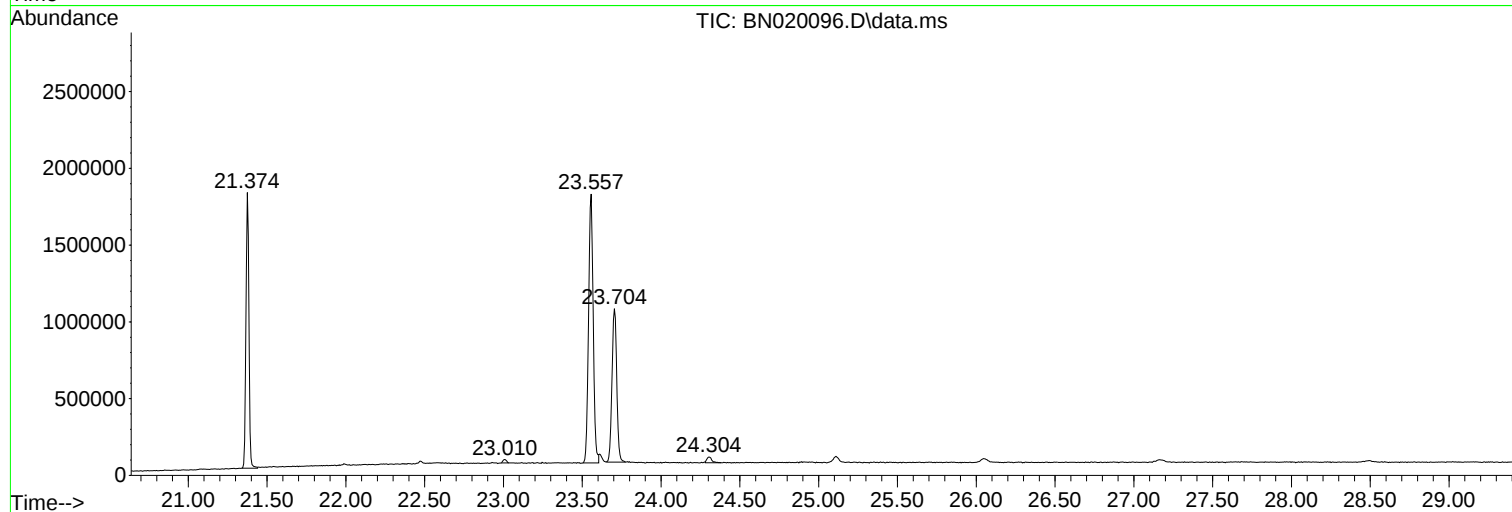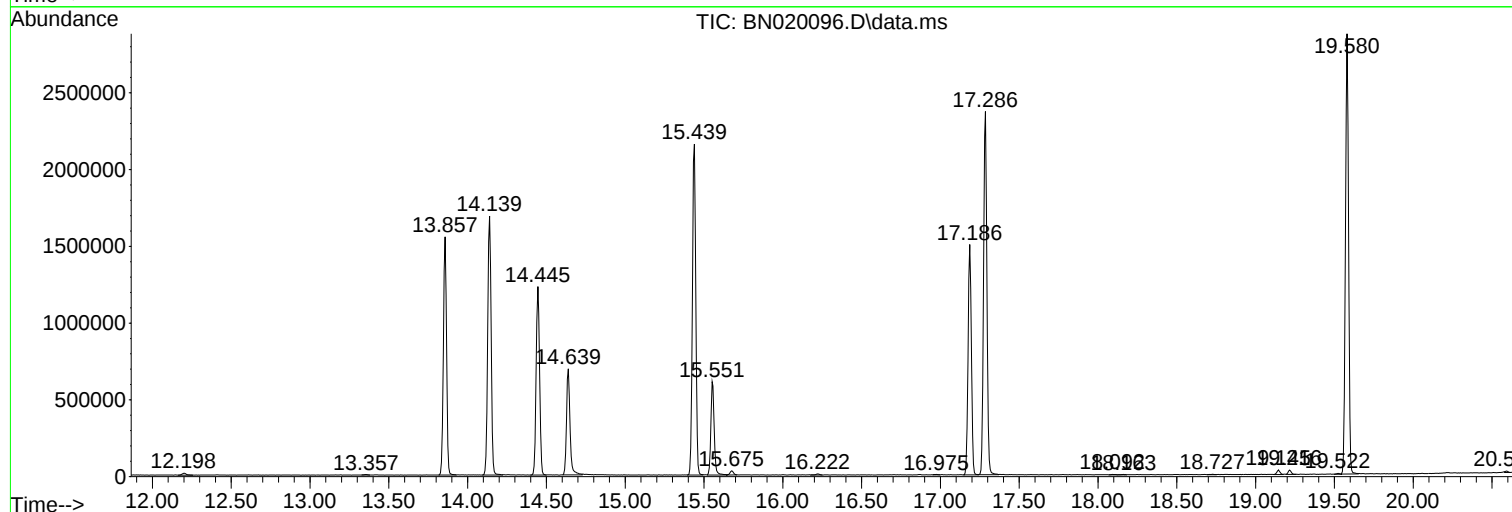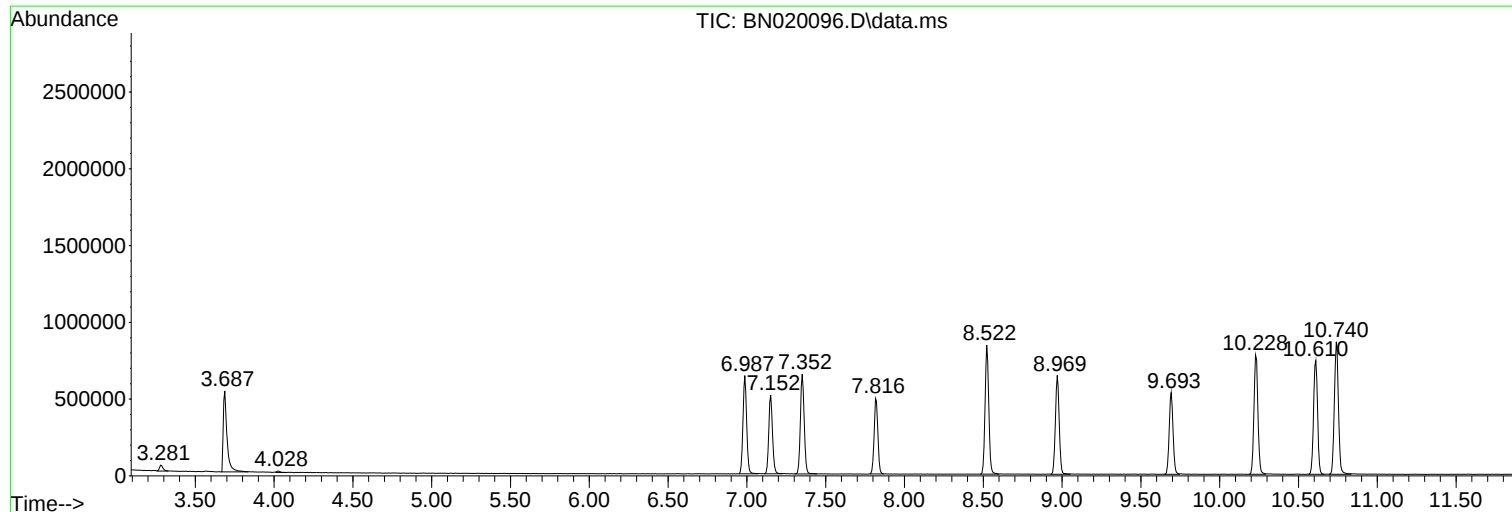

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020096.D
Acq On : 10 Jun 2022 12:29
Operator : CG/JU
Sample : PB145445BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK445

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020096.D
Acq On : 10 Jun 2022 12:29
Operator : CG/JU
Sample : PB145445BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK445

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------