

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020097.D
 Acq On : 10 Jun 2022 13:05
 Operator : CG/JU
 Sample : N3250-19
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYT7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020097.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.628	87	92	99	rVV	230548	306495	0.61%	0.182%
2	3.693	99	103	117	rVB	154778	257572	0.52%	0.153%
3	6.993	655	664	673	rBV	132597	235543	0.47%	0.140%
4	7.152	684	691	693	rBV	521797	783611	1.57%	0.465%
5	7.199	693	699	711	rVV	4341264	7010223	14.04%	4.163%
6	7.357	715	726	737	rVB	523923	929246	1.86%	0.552%
7	7.816	797	804	813	rBV	565430	937386	1.88%	0.557%
8	8.357	890	896	908	rVB	742488	1171625	2.35%	0.696%
9	8.522	916	924	936	rBV	452127	767238	1.54%	0.456%
10	8.969	992	1000	1010	rBV	688536	1131068	2.27%	0.672%
11	9.693	1116	1123	1134	rBV	540382	915611	1.83%	0.544%
12	10.234	1207	1215	1227	rBV	767690	1375806	2.76%	0.817%
13	10.610	1271	1279	1288	rBV	849554	1486993	2.98%	0.883%
14	11.122	1358	1366	1373	rBV	130900	221837	0.44%	0.132%
15	11.998	1503	1515	1523	rBV	6881076	12728834	25.50%	7.558%
16	12.075	1523	1528	1532	rVV2	232892	404365	0.81%	0.240%
17	12.134	1532	1538	1543	rVV	1921902	3186141	6.38%	1.892%
18	12.175	1543	1545	1553	rVV2	178397	239036	0.48%	0.142%
19	12.263	1553	1560	1568	rVB	253376	418385	0.84%	0.248%
20	12.487	1581	1598	1603	rBV	7559225	14233320	28.51%	8.451%
21	12.640	1614	1624	1636	rBV2	160884	569626	1.14%	0.338%
22	12.775	1637	1647	1666	rVB2	291015	860949	1.72%	0.511%
23	13.739	1803	1811	1819	rVB6	22117	52903	0.11%	0.031%
24	13.857	1824	1831	1837	rBV	1766977	2485100	4.98%	1.476%
25	14.092	1864	1871	1873	rBV	89632	125224	0.25%	0.074%
26	14.139	1873	1879	1887	rVB	1858453	2868445	5.75%	1.703%
27	14.275	1896	1902	1909	rBV	757622	1146797	2.30%	0.681%
28	14.351	1909	1915	1925	rVV4	46660	98407	0.20%	0.058%
29	14.445	1925	1931	1942	rVB	1313064	1983165	3.97%	1.178%
30	14.639	1959	1964	1979	rVB	155383	275170	0.55%	0.163%
31	14.786	1984	1989	1997	rVV	175827	265217	0.53%	0.157%
32	14.869	1998	2003	2017	rVB2	53909	106197	0.21%	0.063%
33	15.439	2092	2100	2110	rBV	2505141	3772487	7.56%	2.240%
34	15.551	2113	2119	2132	rBV	612214	887904	1.78%	0.527%
35	15.675	2135	2140	2146	rVB	32485	53021	0.11%	0.031%
36	16.169	2219	2224	2229	rVV	102743	125706	0.25%	0.075%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020097.D
 Acq On : 10 Jun 2022 13:05
 Operator : CG/JU
 Sample : N3250-19
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYT7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	16.598	2292	2297	2304	rBV	83369	117244	0.23%	0.070%
38	17.186	2388	2397	2406	rBV	1614568	2369334	4.75%	1.407%
39	17.286	2407	2414	2423	rVV2	2817670	4271534	8.56%	2.536%
40	17.969	2523	2530	2541	rBV3	222636	603613	1.21%	0.358%
41	18.110	2546	2554	2597	rVV	5557771	10279004	20.59%	6.103%
42	19.145	2726	2730	2734	rBV2	44858	61285	0.12%	0.036%
43	19.310	2738	2758	2770	rBV	14928119	49922481	100.00%	29.643%
44	19.398	2770	2773	2791	rVB	3025719	4897166	9.81%	2.908%
45	19.580	2799	2804	2812	rVB	3081190	4487778	8.99%	2.665%
46	19.880	2850	2855	2863	rVB3	97828	191364	0.38%	0.114%
47	20.145	2896	2900	2907	rBV5	89709	189547	0.38%	0.113%
48	20.304	2924	2927	2933	rBV5	55462	111342	0.22%	0.066%
49	20.480	2950	2957	2980	rVB	1681610	3445601	6.90%	2.046%
50	21.057	3051	3055	3059	rVV	231722	327652	0.66%	0.195%
51	21.104	3059	3063	3078	rVB	1003928	1539243	3.08%	0.914%
52	21.245	3084	3087	3090	rBV	96129	113210	0.23%	0.067%
53	21.280	3091	3093	3096	rVV	60253	82884	0.17%	0.049%
54	21.321	3097	3100	3104	rVV	174920	218379	0.44%	0.130%
55	21.374	3104	3109	3114	rVV2	1717299	2269559	4.55%	1.348%
56	21.427	3114	3118	3120	rVV	239802	315476	0.63%	0.187%
57	21.451	3120	3122	3127	rVB	256198	259099	0.52%	0.154%
58	21.563	3134	3141	3146	rVB	561996	769789	1.54%	0.457%
59	21.986	3209	3213	3223	rBV	488295	736985	1.48%	0.438%
60	22.133	3234	3238	3242	rBV	241855	356545	0.71%	0.212%
61	22.257	3255	3259	3260	rBV	135808	169807	0.34%	0.101%
62	22.280	3260	3263	3269	rVV	249522	339590	0.68%	0.202%
63	22.345	3269	3274	3285	rVB	407881	784417	1.57%	0.466%
64	22.486	3292	3298	3304	rBV	532597	920701	1.84%	0.547%
65	22.604	3314	3318	3326	rVB	199017	295220	0.59%	0.175%
66	23.004	3382	3386	3392	rVB	173876	261983	0.52%	0.156%
67	23.104	3399	3403	3410	rVB2	89524	154805	0.31%	0.092%
68	23.557	3472	3480	3486	rBV2	1856047	3819624	7.65%	2.268%
69	23.615	3486	3490	3497	rVV2	147818	310427	0.62%	0.184%
70	23.704	3498	3505	3514	rVB2	963083	1955507	3.92%	1.161%
71	24.298	3602	3606	3617	rVB	105404	221521	0.44%	0.132%
72	25.092	3732	3741	3756	rBV4	426580	1443902	2.89%	0.857%
73	26.409	3958	3965	3979	rVB2	173284	569323	1.14%	0.338%
74	27.503	4139	4151	4170	rVB	1379821	4813605	9.64%	2.858%

Sum of corrected areas: 168413199




Instrument :
BNA_N
ClientSampleId :
EXYT7

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020097.D
Acq On : 10 Jun 2022 13:05
Operator : CG/JU
Sample : N3250-19
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYT7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

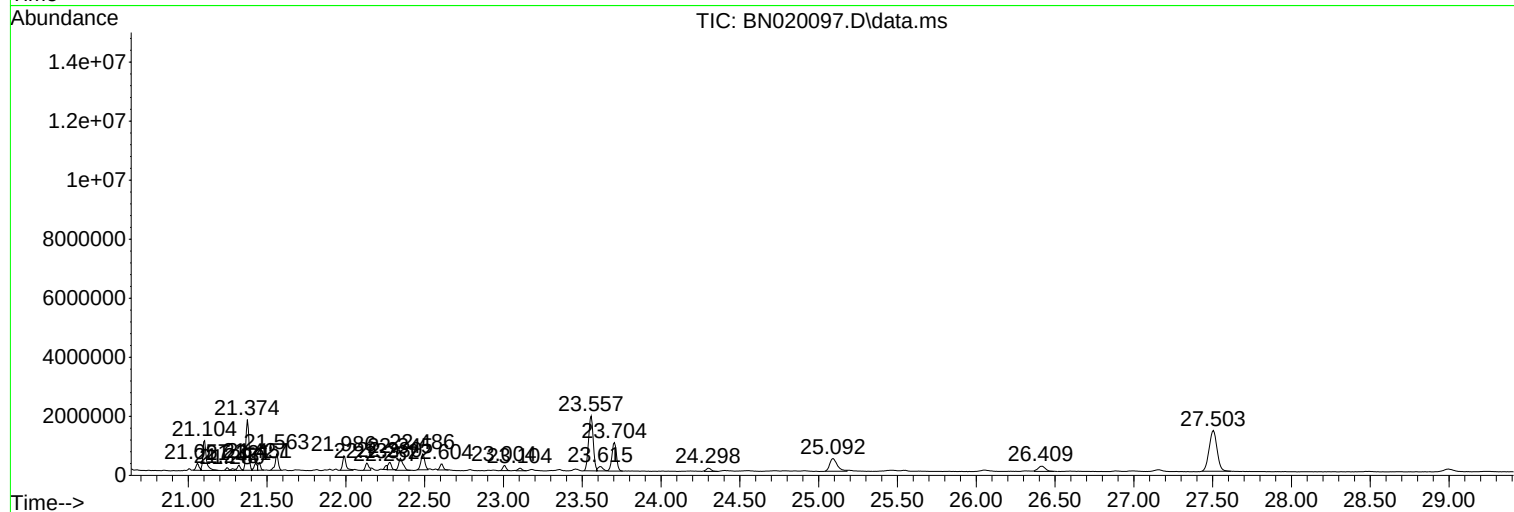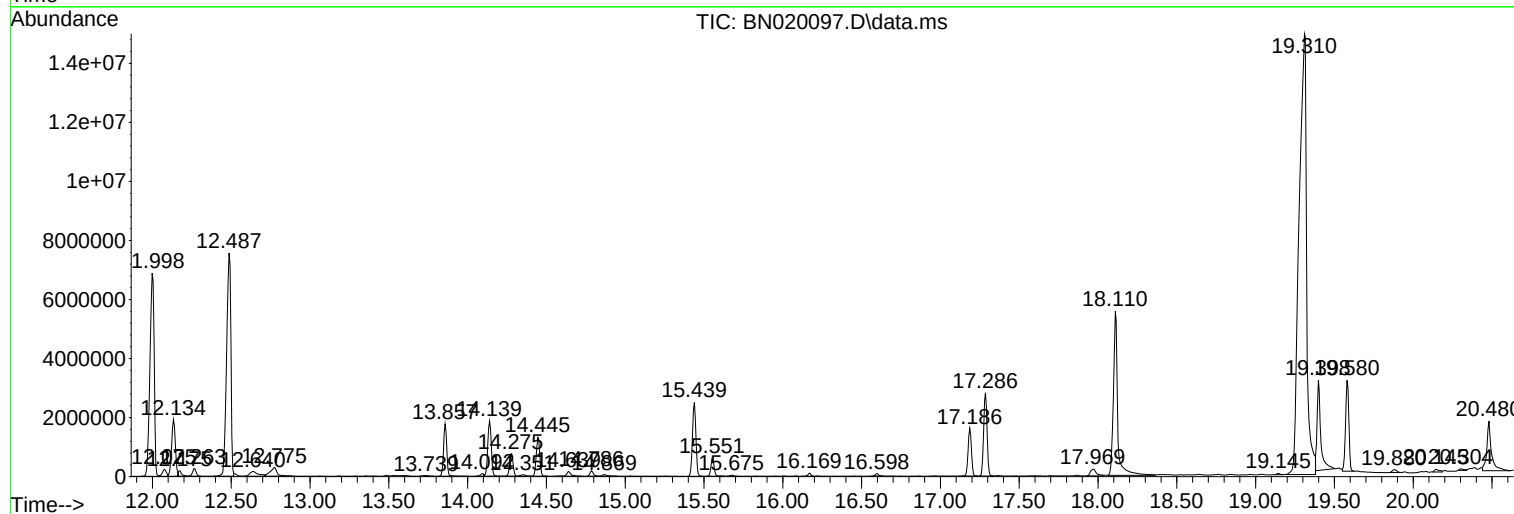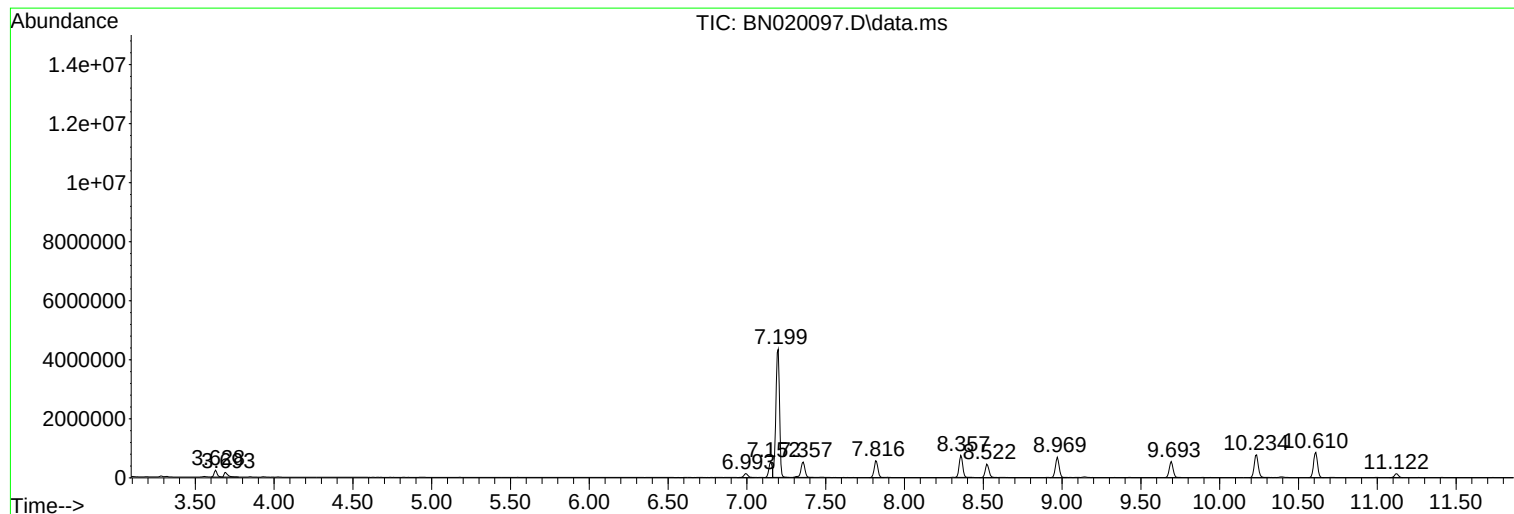

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020097.D
Acq On : 10 Jun 2022 13:05
Operator : CG/JU
Sample : N3250-19
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYT7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020097.D
Acq On : 10 Jun 2022 13:05
Operator : CG/JU
Sample : N3250-19
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYT7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc