

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020098.D
 Acq On : 10 Jun 2022 13:41
 Operator : CG/JU
 Sample : N3250-21
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYW3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020098.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	15	17	21	rVB4	7508	9159	0.18%	0.020%
2	3.281	29	33	44	rVB	31959	50445	1.00%	0.110%
3	3.693	99	103	117	rBV	158338	277307	5.52%	0.604%
4	3.934	139	144	150	rBV2	14562	26148	0.52%	0.057%
5	4.028	156	160	164	rVB2	10957	13051	0.26%	0.028%
6	4.558	246	250	256	rBV7	4579	9988	0.20%	0.022%
7	4.934	309	314	320	rVB3	7396	11915	0.24%	0.026%
8	6.987	657	663	673	rBV	159366	261610	5.21%	0.570%
9	7.152	683	691	703	rBV	602181	981602	19.54%	2.138%
10	7.352	718	725	734	rBV	586793	955791	19.02%	2.082%
11	7.457	739	743	748	rVB4	3125	5265	0.10%	0.011%
12	7.822	798	805	815	rBV	488237	823673	16.39%	1.794%
13	8.522	917	924	936	rBV	506525	827898	16.48%	1.803%
14	8.969	993	1000	1016	rBV	792687	1326377	26.40%	2.889%
15	9.693	1116	1123	1136	rBV	617900	1051820	20.93%	2.291%
16	10.228	1207	1214	1227	rBV	813735	1456898	29.00%	3.173%
17	10.398	1238	1243	1247	rBV5	2769	5028	0.10%	0.011%
18	10.610	1270	1279	1287	rBV	780304	1333832	26.55%	2.905%
19	10.740	1293	1301	1315	rBV	912949	1577887	31.40%	3.436%
20	12.198	1544	1549	1556	rBV	17998	29776	0.59%	0.065%
21	13.057	1691	1695	1701	rVB4	3350	6182	0.12%	0.013%
22	13.857	1823	1831	1843	rBV	1873176	2630309	52.35%	5.728%
23	14.139	1871	1879	1897	rBV	2023348	3107068	61.84%	6.767%
24	14.445	1924	1931	1941	rBV	1258474	1858603	36.99%	4.048%
25	14.639	1958	1964	1980	rBV2	136876	252547	5.03%	0.550%
26	14.869	2000	2003	2009	rVB4	6023	8371	0.17%	0.018%
27	15.186	2053	2057	2062	rBV3	7053	12245	0.24%	0.027%
28	15.257	2065	2069	2074	rVV3	5905	8994	0.18%	0.020%
29	15.439	2093	2100	2107	rBV	2683155	3918291	77.99%	8.533%
30	15.557	2113	2120	2131	rBV	868310	1251623	24.91%	2.726%
31	15.681	2136	2141	2146	rVB2	32752	48057	0.96%	0.105%
32	16.133	2212	2218	2222	rBV7	2961	5769	0.11%	0.013%
33	16.222	2226	2233	2237	rVB3	9324	13957	0.28%	0.030%
34	16.869	2340	2343	2349	rVB4	5103	5957	0.12%	0.013%
35	16.975	2356	2361	2365	rBV6	4129	8361	0.17%	0.018%
36	17.186	2390	2397	2407	rBV	1547275	2222233	44.23%	4.840%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020098.D
 Acq On : 10 Jun 2022 13:41
 Operator : CG/JU
 Sample : N3250-21
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYW3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	17.286	2407	2414	2422	rBV2	3036496	4446238	88.49%	9.683%
38	17.569	2458	2462	2467	rBV4	3216	5605	0.11%	0.012%
39	17.839	2504	2508	2511	rBV2	6934	10498	0.21%	0.023%
40	18.086	2546	2550	2557	rBV5	24802	37026	0.74%	0.081%
41	18.157	2557	2562	2567	rVV2	4954	8466	0.17%	0.018%
42	18.992	2698	2704	2709	rBV5	17374	25048	0.50%	0.055%
43	19.145	2725	2730	2735	rVB	39974	55167	1.10%	0.120%
44	19.216	2736	2742	2746	rBV	39808	54224	1.08%	0.118%
45	19.251	2746	2748	2752	rVV4	9460	12665	0.25%	0.028%
46	19.286	2752	2754	2759	rVB6	5797	5286	0.11%	0.012%
47	19.369	2764	2768	2771	rBV4	19714	25522	0.51%	0.056%
48	19.522	2791	2794	2797	rBV3	11045	12899	0.26%	0.028%
49	19.580	2797	2804	2813	rBV	3544978	5024388	100.00%	10.942%
50	20.574	2969	2973	2974	rBV4	10437	12160	0.24%	0.026%
51	20.592	2974	2976	2980	rVB3	13191	13593	0.27%	0.030%
52	21.098	3060	3062	3066	rBV3	8289	10757	0.21%	0.023%
53	21.374	3103	3109	3116	rBV2	1777810	2370926	47.19%	5.163%
54	22.474	3293	3296	3301	rVB	30196	41090	0.82%	0.089%
55	22.539	3302	3307	3313	rVV	167656	248036	4.94%	0.540%
56	23.010	3383	3387	3392	rVB	45227	71101	1.42%	0.155%
57	23.557	3471	3480	3487	rBV2	2213412	4644895	92.45%	10.116%
58	23.704	3497	3505	3516	rVB2	1024017	2159563	42.98%	4.703%
59	24.304	3602	3607	3614	rVB	57590	116308	2.31%	0.253%
60	25.104	3740	3743	3751	rVB	54943	112827	2.25%	0.246%




Sum of corrected areas: 45918325

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020098.D
Acq On : 10 Jun 2022 13:41
Operator : CG/JU
Sample : N3250-21
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

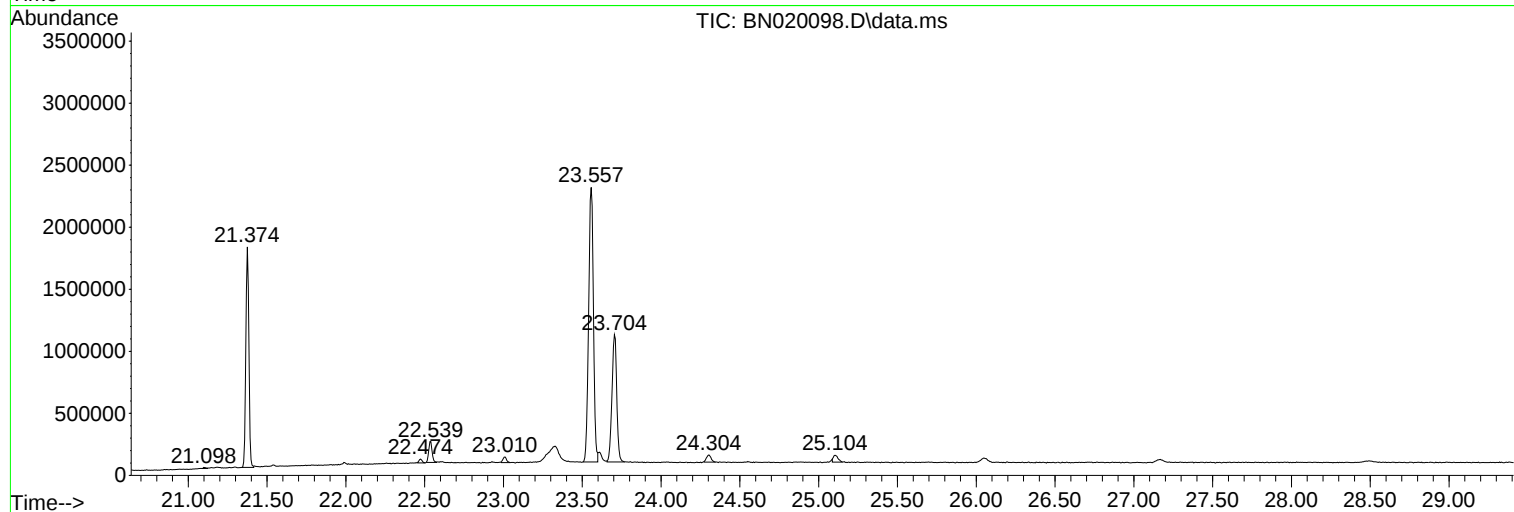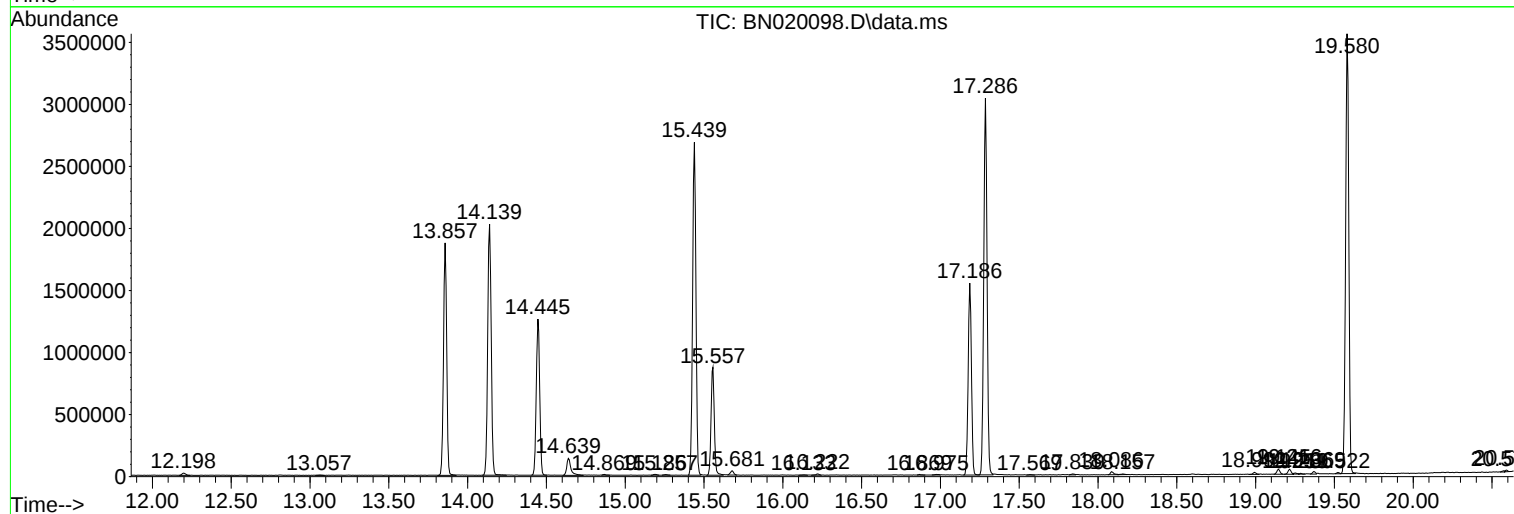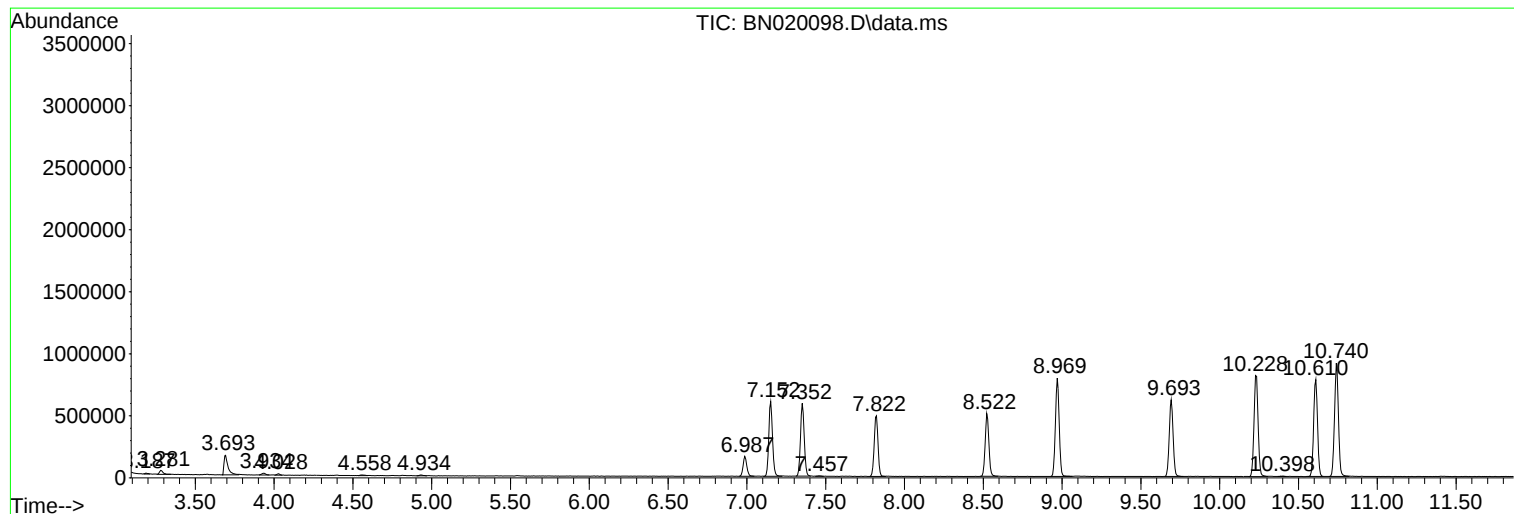

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020098.D
Acq On : 10 Jun 2022 13:41
Operator : CG/JU
Sample : N3250-21
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexanedioic acid, bis[2-(2-... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
22.539	2.09 ng/ul	248036	Chrysene-d12	21.374

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexanedioic acid, bis[2-(2-butox...	434	C22H42O8	000141-17-3	87
2			1-Decanamine	157	C10H23N	002016-57-1	22
3			Butane, 1,1'-[oxybis(2,1-ethaned...	218	C12H26O3	000112-73-2	16
4			Butane, 1,1'-[oxybis(2,1-ethaned...	218	C12H26O3	000112-73-2	16
5			Propane, 1,1'-[ethylidenebis(oxy...	174	C10H22O2	005669-09-0	14

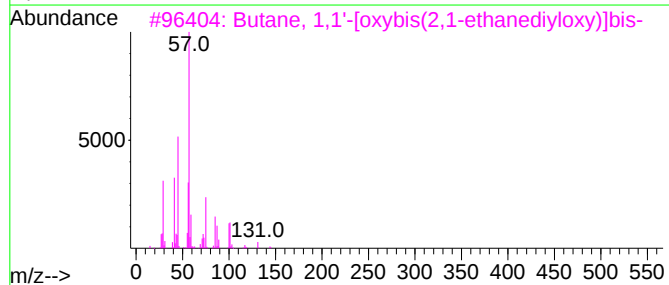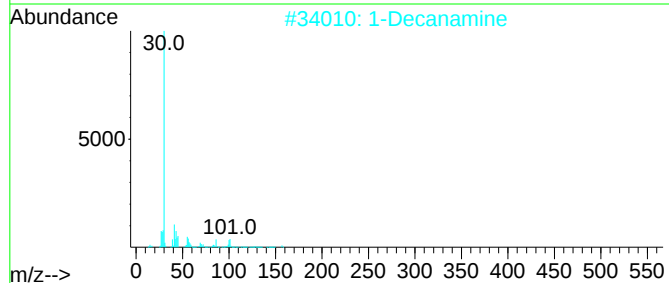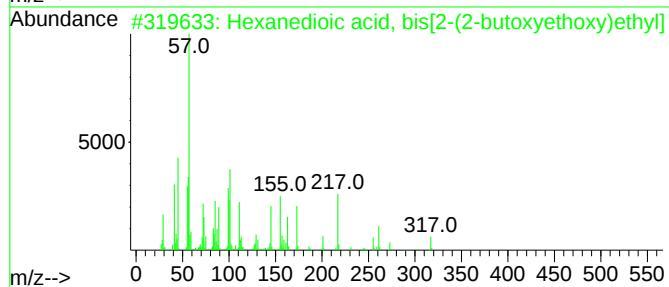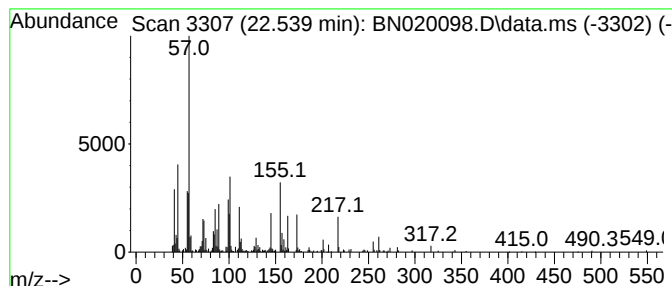

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020098.D
Acq On : 10 Jun 2022 13:41
Operator : CG/JU
Sample : N3250-21
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexanedioic aci...	22.539	2.1	ng/ul	248036	5	21.374	2370930	20.0