

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020101.D
 Acq On : 10 Jun 2022 15:30
 Operator : CG/JU
 Sample : N3250-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020101.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	31	rBV	25911	36169	0.77%	0.086%
2	3.281	31	33	38	rVB	28694	35516	0.76%	0.084%
3	3.687	99	102	122	rBV2	160211	324993	6.95%	0.770%
4	3.934	139	144	149	rVB2	14059	25316	0.54%	0.060%
5	4.028	156	160	168	rVB3	9510	16628	0.36%	0.039%
6	4.558	244	250	259	rVB	59260	102850	2.20%	0.244%
7	4.934	310	314	322	rBV5	7528	13365	0.29%	0.032%
8	6.987	656	663	672	rBV	133997	220760	4.72%	0.523%
9	7.152	683	691	704	rBV	517754	854311	18.27%	2.024%
10	7.352	718	725	735	rBV	511691	845745	18.09%	2.004%
11	7.458	741	743	748	rVB4	3566	4748	0.10%	0.011%
12	7.816	797	804	814	rBV	460544	776804	16.61%	1.841%
13	8.522	917	924	937	rBV	438988	722882	15.46%	1.713%
14	8.969	992	1000	1015	rBV	682094	1148097	24.56%	2.720%
15	9.693	1116	1123	1133	rBV	562473	940601	20.12%	2.229%
16	10.228	1207	1214	1227	rBV	753052	1333372	28.52%	3.159%
17	10.610	1271	1279	1286	rBV	712502	1249863	26.73%	2.961%
18	10.740	1293	1301	1316	rBV	793066	1407624	30.11%	3.335%
19	12.198	1543	1549	1558	rVB3	15242	27143	0.58%	0.064%
20	13.857	1824	1831	1846	rBV	1736234	2488016	53.21%	5.895%
21	14.140	1872	1879	1892	rBV	1873006	2773041	59.31%	6.570%
22	14.445	1924	1931	1940	rBV	1147376	1734130	37.09%	4.109%
23	14.639	1959	1964	1976	rBV	117538	218358	4.67%	0.517%
24	14.869	1999	2003	2008	rVB5	3629	5201	0.11%	0.012%
25	15.187	2053	2057	2062	rVB2	7017	10293	0.22%	0.024%
26	15.263	2064	2070	2074	rVB4	2681	5769	0.12%	0.014%
27	15.439	2092	2100	2110	rBV	2392861	3641417	77.88%	8.628%
28	15.557	2113	2120	2132	rVV	868791	1241269	26.55%	2.941%
29	15.675	2136	2140	2147	rVB	32465	47618	1.02%	0.113%
30	16.222	2229	2233	2238	rBV5	9409	14509	0.31%	0.034%
31	16.863	2339	2342	2346	rBV2	4378	4697	0.10%	0.011%
32	16.969	2356	2360	2363	rBV4	4231	6522	0.14%	0.015%
33	17.186	2390	2397	2407	rBV	1414856	2097449	44.86%	4.970%
34	17.286	2407	2414	2429	rBV2	2776240	4120825	88.14%	9.764%
35	18.086	2542	2550	2557	rBV6	21988	40012	0.86%	0.095%
36	18.157	2558	2562	2565	rVV4	3539	5783	0.12%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020101.D
 Acq On : 10 Jun 2022 15:30
 Operator : CG/JU
 Sample : N3250-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYX0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	18.598	2635	2637	2640	rVB4	5114	4919	0.11%	0.012%
38	19.145	2725	2730	2737	rBV3	38744	56420	1.21%	0.134%
39	19.216	2737	2742	2748	rBV	39436	60211	1.29%	0.143%
40	19.369	2764	2768	2775	rBV6	18026	29747	0.64%	0.070%
41	19.522	2791	2794	2797	rBV4	13789	13152	0.28%	0.031%
42	19.580	2797	2804	2817	rBV	3305879	4675493	100.00%	11.078%
43	20.574	2970	2973	2974	rBV3	9835	11665	0.25%	0.028%
44	21.374	3103	3109	3119	rBV	1713536	2211314	47.30%	5.239%
45	22.474	3293	3296	3301	rVB	42156	52231	1.12%	0.124%
46	22.533	3304	3306	3312	rVB4	24371	31961	0.68%	0.076%
47	23.010	3383	3387	3393	rVB2	61072	96336	2.06%	0.228%
48	23.557	3472	3480	3487	rBV2	2056495	4123157	88.19%	9.769%
49	23.704	3497	3505	3518	rVB2	961420	1957879	41.88%	4.639%
50	24.304	3601	3607	3613	rVB2	85486	163804	3.50%	0.388%
51	25.104	3738	3743	3752	rVB	72545	175328	3.75%	0.415%




Sum of corrected areas: 42205313

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020101.D
Acq On : 10 Jun 2022 15:30
Operator : CG/JU
Sample : N3250-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYX0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

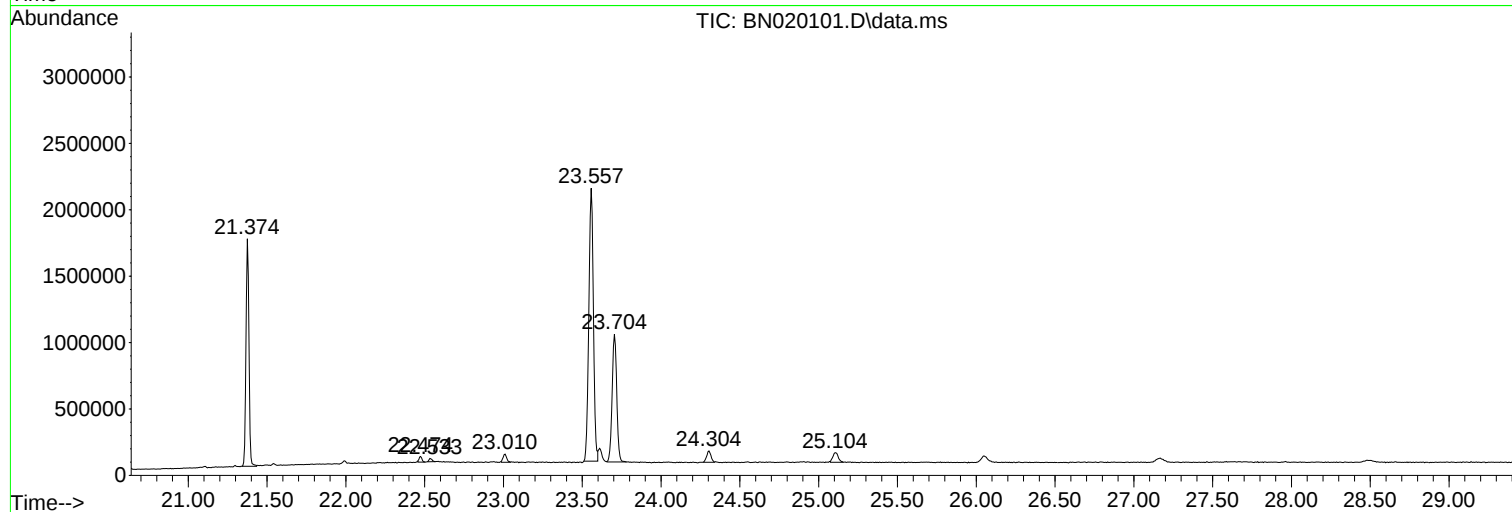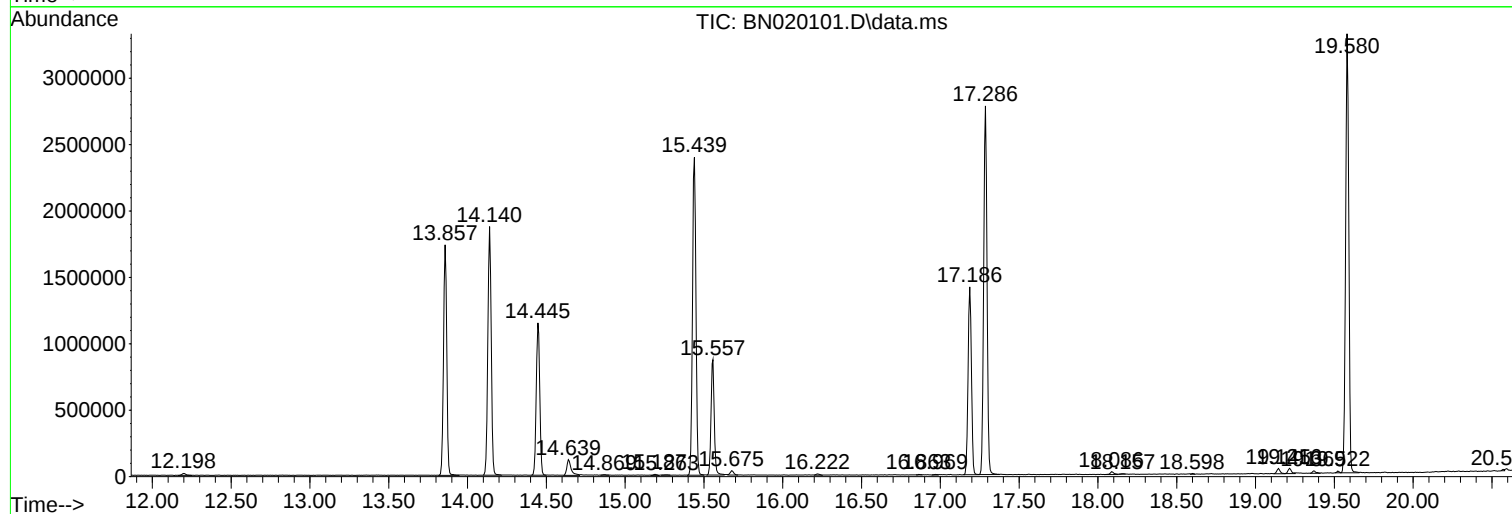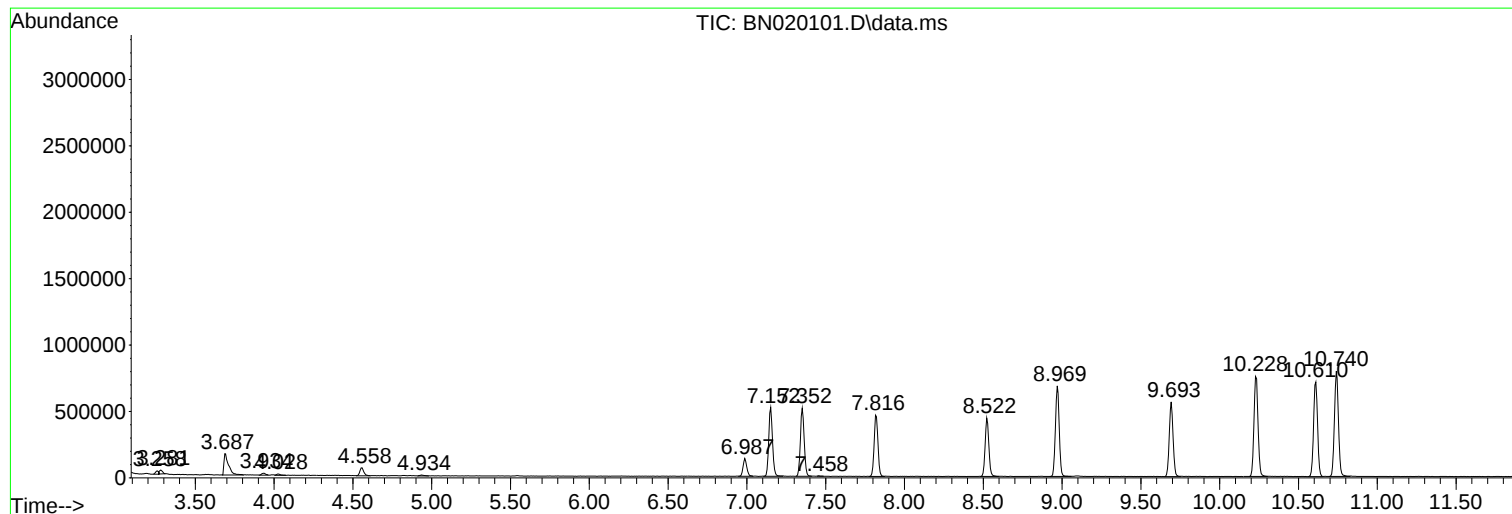

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020101.D
Acq On : 10 Jun 2022 15:30
Operator : CG/JU
Sample : N3250-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYX0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020101.D
Acq On : 10 Jun 2022 15:30
Operator : CG/JU
Sample : N3250-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYX0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc