

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020102.D
 Acq On : 10 Jun 2022 16:06
 Operator : CG/JU
 Sample : N3250-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020102.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.257	24	29	37	rBV2	158609	282055	6.33%	0.667%
2	3.693	100	103	118	rBV	112985	197324	4.43%	0.467%
3	3.934	139	144	150	rBV2	14465	25018	0.56%	0.059%
4	4.028	156	160	164	rVB2	8677	10756	0.24%	0.025%
5	4.122	172	176	183	rVB2	19315	29483	0.66%	0.070%
6	4.557	242	250	263	rVB	551922	910575	20.43%	2.153%
7	4.934	309	314	320	rBV4	5972	10743	0.24%	0.025%
8	6.987	657	663	672	rBV	124711	205011	4.60%	0.485%
9	7.151	684	691	702	rBV	468407	779337	17.48%	1.843%
10	7.234	702	705	713	rVB3	3989	8334	0.19%	0.020%
11	7.351	718	725	735	rVV	473994	775865	17.40%	1.835%
12	7.457	739	743	749	rVB6	3355	5440	0.12%	0.013%
13	7.822	798	805	815	rBV	535565	902382	20.24%	2.134%
14	8.522	916	924	934	rBV	396154	662827	14.87%	1.567%
15	8.969	991	1000	1013	rBV	616124	1041179	23.36%	2.462%
16	9.098	1015	1022	1028	rVV7	4375	8820	0.20%	0.021%
17	9.692	1115	1123	1134	rBV	505709	849310	19.05%	2.008%
18	10.228	1207	1214	1228	rBV	676739	1201978	26.96%	2.842%
19	10.398	1237	1243	1252	rVB5	4015	9800	0.22%	0.023%
20	10.610	1271	1279	1288	rBV	833516	1452414	32.58%	3.434%
21	10.739	1294	1301	1317	rBV	626760	1127577	25.29%	2.666%
22	12.204	1544	1550	1554	rBV3	12930	20950	0.47%	0.050%
23	13.292	1729	1735	1738	rBV4	3302	5501	0.12%	0.013%
24	13.857	1825	1831	1843	rBV	1478765	2118740	47.53%	5.010%
25	14.139	1871	1879	1888	rBV	1616728	2463222	55.26%	5.825%
26	14.445	1924	1931	1940	rBV	1334551	2017629	45.26%	4.771%
27	14.639	1958	1964	1977	rBV	107559	201169	4.51%	0.476%
28	14.869	1999	2003	2006	rBV3	5785	7358	0.17%	0.017%
29	15.263	2065	2070	2074	rVB5	4308	6409	0.14%	0.015%
30	15.439	2093	2100	2107	rBV	2127941	3197560	71.73%	7.561%
31	15.557	2113	2120	2132	rBV	813231	1154828	25.91%	2.731%
32	15.674	2136	2140	2146	rVB	26435	39812	0.89%	0.094%
33	16.133	2214	2218	2222	rBV5	3333	6347	0.14%	0.015%
34	16.222	2228	2233	2236	rVB4	8048	10518	0.24%	0.025%
35	16.869	2338	2343	2349	rVB3	3922	6285	0.14%	0.015%
36	16.963	2355	2359	2360	rBV2	5001	6277	0.14%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020102.D
 Acq On : 10 Jun 2022 16:06
 Operator : CG/JU
 Sample : N3250-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYW8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	17.186	2390	2397	2407	rBV	1636035	2420179	54.29%	5.723%
38	17.286	2407	2414	2429	rVV2	2672940	3934013	88.25%	9.302%
39	17.868	2509	2513	2516	rBV5	4554	6832	0.15%	0.016%
40	18.086	2546	2550	2557	rBV	39319	61268	1.37%	0.145%
41	18.163	2560	2563	2568	rVB	6701	8736	0.20%	0.021%
42	19.027	2704	2710	2714	rBV7	3143	6869	0.15%	0.016%
43	19.145	2725	2730	2734	rBV2	35203	46974	1.05%	0.111%
44	19.215	2737	2742	2746	rBV	34452	50148	1.12%	0.119%
45	19.368	2764	2768	2774	rBV3	24975	37064	0.83%	0.088%
46	19.521	2791	2794	2797	rBV3	12615	12285	0.28%	0.029%
47	19.580	2798	2804	2812	rBV2	3142719	4457718	100.00%	10.541%
48	20.510	2960	2962	2966	rVB	13383	14055	0.32%	0.033%
49	20.574	2970	2973	2974	rBV3	8906	9753	0.22%	0.023%
50	20.639	2981	2984	2986	rBV3	8846	8358	0.19%	0.020%
51	21.104	3059	3063	3071	rBV	36037	57632	1.29%	0.136%
52	21.374	3104	3109	3122	rBV	1977084	2546000	57.11%	6.020%
53	21.539	3135	3137	3142	rVB5	15260	16925	0.38%	0.040%
54	21.986	3211	3213	3216	rBV3	20423	21155	0.47%	0.050%
55	22.474	3292	3296	3302	rVB	41566	56803	1.27%	0.134%
56	23.009	3383	3387	3394	rVB	64916	95179	2.14%	0.225%
57	23.556	3472	3480	3487	rBV2	1996443	4004151	89.83%	9.468%
58	23.703	3497	3505	3515	rVB	1126169	2310564	51.83%	5.464%
59	24.303	3602	3607	3617	rVB2	84093	174658	3.92%	0.413%
60	25.103	3738	3743	3752	rVB2	77772	173798	3.90%	0.411%




Sum of corrected areas: 42289950

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020102.D
Acq On : 10 Jun 2022 16:06
Operator : CG/JU
Sample : N3250-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

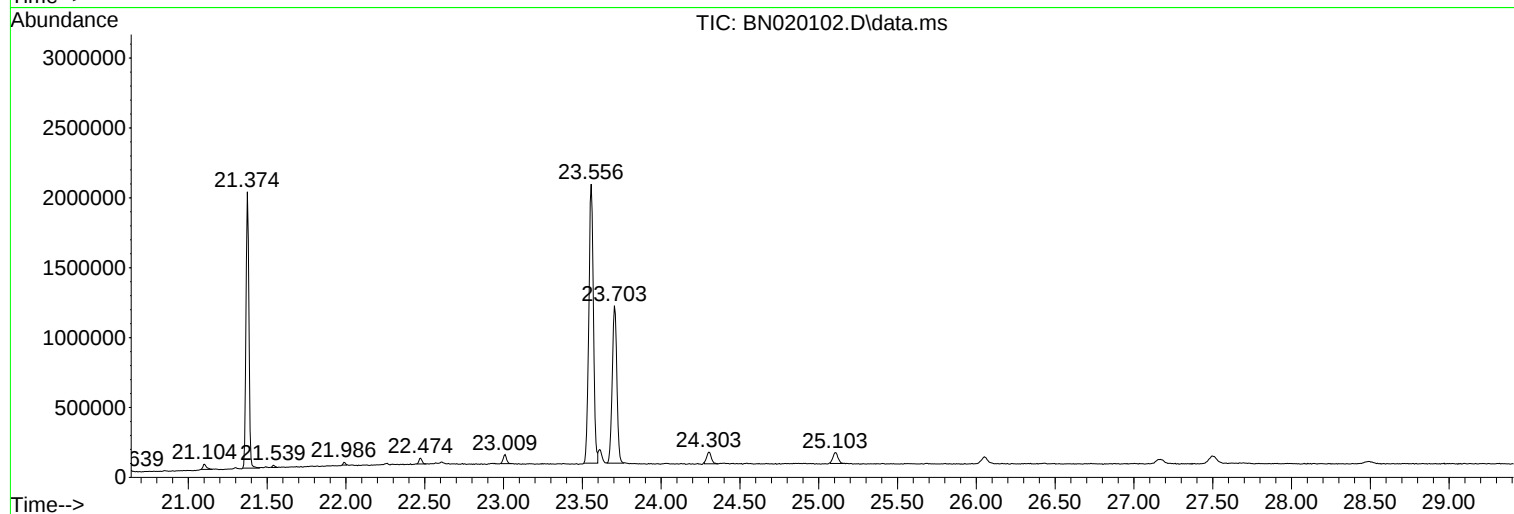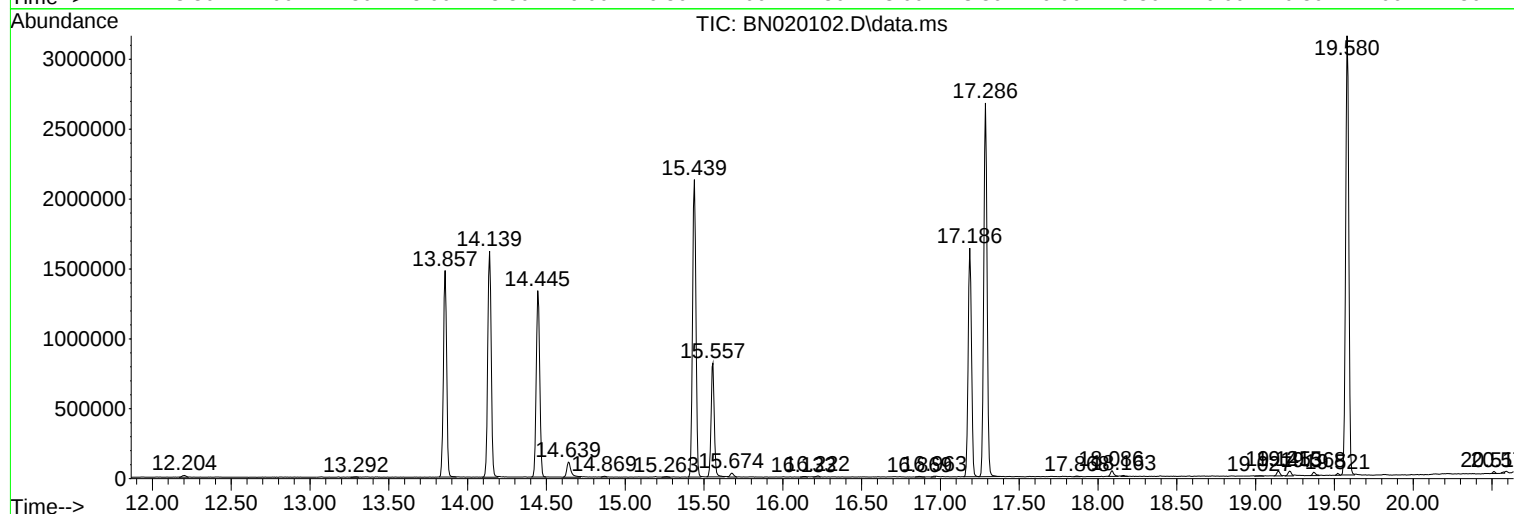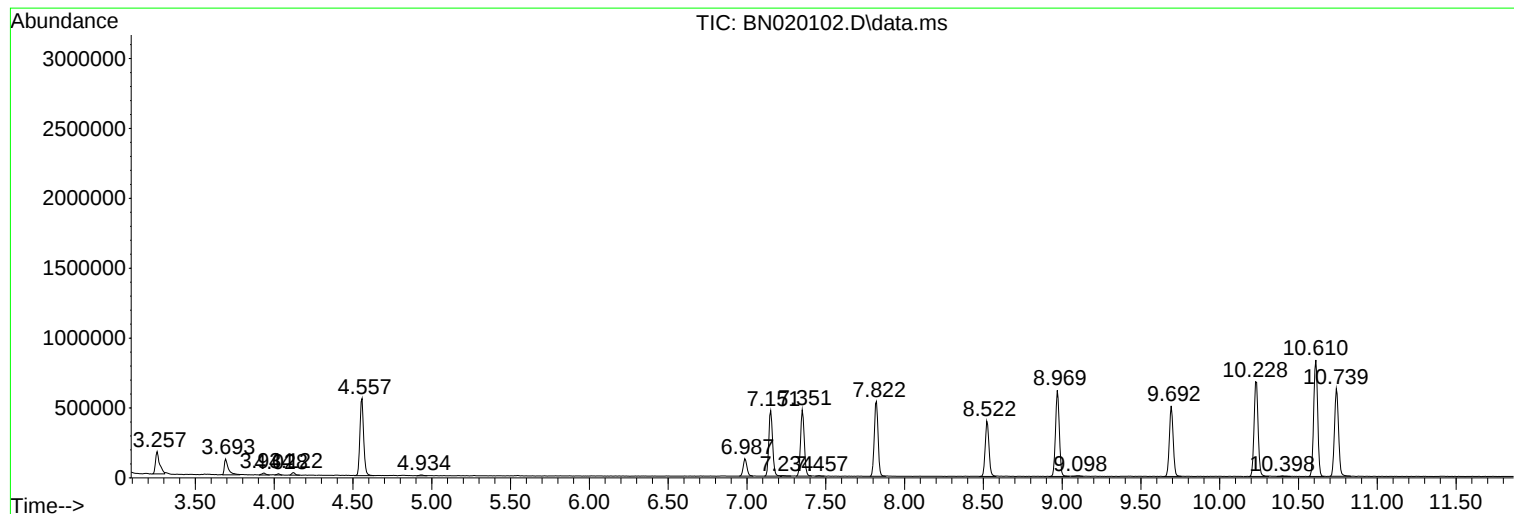

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020102.D
Acq On : 10 Jun 2022 16:06
Operator : CG/JU
Sample : N3250-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW8










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.557	20.18 ng/ul	910575	1,4-Dichlorobenzene-d4	7.822

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	16

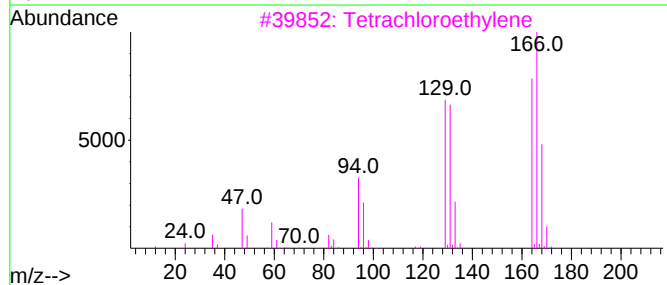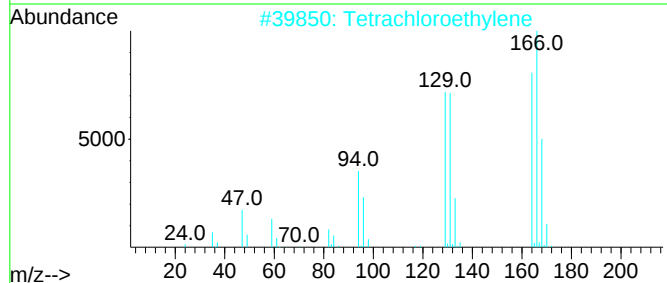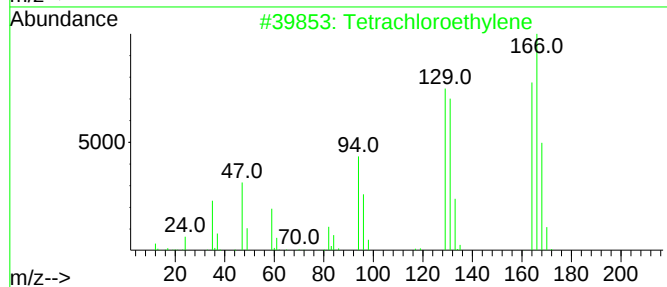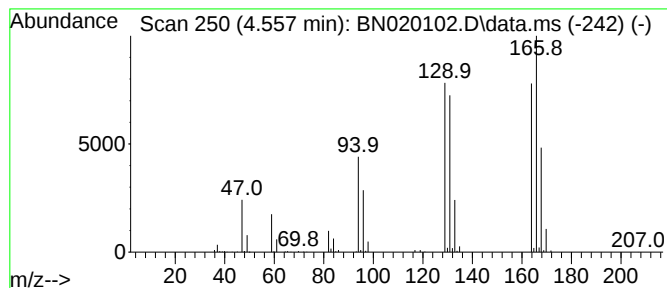

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020102.D
Acq On : 10 Jun 2022 16:06
Operator : CG/JU
Sample : N3250-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.557	20.2	ng/u1	910575	1	7.822	902382	20.0