

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020103.D
 Acq On : 10 Jun 2022 16:43
 Operator : CG/JU
 Sample : N3250-15
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYT0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020103.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	38	rBV	25667	35188	0.75%	0.081%
2	3.693	99	103	116	rBV	119717	210865	4.49%	0.487%
3	3.934	139	144	149	rVB	14251	24447	0.52%	0.056%
4	4.022	156	159	165	rVB2	8088	12153	0.26%	0.028%
5	4.934	310	314	318	rVV3	4826	7283	0.15%	0.017%
6	5.475	401	406	412	rVB4	5063	9440	0.20%	0.022%
7	6.987	658	663	675	rVB	128150	209872	4.46%	0.484%
8	7.152	684	691	700	rBV	533148	875856	18.63%	2.021%
9	7.228	701	704	709	rVB2	4138	6543	0.14%	0.015%
10	7.352	718	725	735	rBV	522049	864892	18.40%	1.996%
11	7.822	797	805	814	rBV	496540	837770	17.82%	1.933%
12	8.522	917	924	939	rBV	414959	693150	14.74%	1.599%
13	8.969	993	1000	1013	rBV	698680	1178011	25.06%	2.718%
14	9.098	1017	1022	1027	rBV5	4603	6991	0.15%	0.016%
15	9.428	1070	1078	1086	rBV3	18329	38359	0.82%	0.089%
16	9.693	1114	1123	1133	rBV	581237	961015	20.44%	2.218%
17	10.228	1207	1214	1226	rBV	772942	1338482	28.47%	3.089%
18	10.610	1270	1279	1293	rBV	766436	1364449	29.02%	3.149%
19	10.740	1293	1301	1316	rBV	688554	1206915	25.67%	2.785%
20	12.198	1544	1549	1556	rBV2	13936	22906	0.49%	0.053%
21	13.292	1731	1735	1739	rBV3	8573	12808	0.27%	0.030%
22	13.357	1739	1746	1752	rVB7	4263	6763	0.14%	0.016%
23	13.857	1824	1831	1842	rBV	1686286	2397492	50.99%	5.532%
24	14.139	1871	1879	1893	rBV	1847488	2787008	59.28%	6.431%
25	14.445	1924	1931	1938	rBV	1233196	1891304	40.23%	4.364%
26	14.639	1958	1964	1981	rBV	112978	206247	4.39%	0.476%
27	14.869	1999	2003	2008	rVB4	4801	6578	0.14%	0.015%
28	15.104	2037	2043	2050	rBV6	9468	16897	0.36%	0.039%
29	15.186	2053	2057	2062	rVV2	10615	15281	0.33%	0.035%
30	15.257	2062	2069	2076	rVV2	17632	30110	0.64%	0.069%
31	15.439	2093	2100	2113	rBV	2406587	3550713	75.52%	8.194%
32	15.557	2113	2120	2127	rBV	895627	1243515	26.45%	2.870%
33	15.675	2136	2140	2146	rVB2	32157	49425	1.05%	0.114%
34	15.804	2159	2162	2165	rBV4	4878	5758	0.12%	0.013%
35	15.945	2181	2186	2190	rVV3	15917	22198	0.47%	0.051%
36	16.222	2226	2233	2237	rBV5	9544	14883	0.32%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020103.D
 Acq On : 10 Jun 2022 16:43
 Operator : CG/JU
 Sample : N3250-15
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYT0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	16.451	2266	2272	2276	rBV3	6358	11401	0.24%	0.026%
38	16.498	2277	2280	2286	rVB4	4900	6440	0.14%	0.015%
39	16.698	2312	2314	2319	rVB5	3383	4857	0.10%	0.011%
40	16.875	2339	2344	2346	rBV3	5010	5705	0.12%	0.013%
41	16.951	2353	2357	2363	rBV4	12827	22683	0.48%	0.052%
42	17.186	2390	2397	2404	rBV	1553080	2259071	48.05%	5.213%
43	17.286	2407	2414	2427	rVV	2768068	4144584	88.15%	9.564%
44	17.386	2430	2431	2436	rVB4	5445	5594	0.12%	0.013%
45	17.751	2488	2493	2495	rBV3	5263	6980	0.15%	0.016%
46	17.863	2507	2512	2519	rVB6	14050	22675	0.48%	0.052%
47	18.051	2540	2544	2546	rBV2	9507	10527	0.22%	0.024%
48	18.086	2546	2550	2558	rVV	74283	114892	2.44%	0.265%
49	18.157	2559	2562	2570	rVB3	13403	21721	0.46%	0.050%
50	18.839	2674	2678	2683	rBV4	7897	12162	0.26%	0.028%
51	18.898	2685	2688	2692	rBV4	3526	6456	0.14%	0.015%
52	19.145	2725	2730	2737	rBV3	38465	52158	1.11%	0.120%
53	19.216	2737	2742	2747	rBV	36830	57511	1.22%	0.133%
54	19.369	2764	2768	2777	rBV2	55819	81244	1.73%	0.187%
55	19.527	2790	2795	2797	rBV6	14411	17735	0.38%	0.041%
56	19.580	2797	2804	2812	rVV	3296982	4701499	100.00%	10.849%
57	19.639	2812	2814	2817	rVB4	6881	5843	0.12%	0.013%
58	20.510	2959	2962	2967	rVB3	12199	14345	0.31%	0.033%
59	20.592	2974	2976	2979	rVB2	12463	11397	0.24%	0.026%
60	21.098	3057	3062	3072	rBV2	73449	153233	3.26%	0.354%
61	21.298	3092	3096	3100	rBV	80129	93110	1.98%	0.215%
62	21.374	3103	3109	3122	rBV	1896716	2426887	51.62%	5.600%
63	21.539	3134	3137	3142	rBV3	21150	27204	0.58%	0.063%
64	21.992	3211	3214	3218	rBV2	21699	24625	0.52%	0.057%
65	22.474	3293	3296	3300	rVB	37834	51192	1.09%	0.118%
66	23.010	3382	3387	3395	rVB	60212	101396	2.16%	0.234%
67	23.557	3472	3480	3487	rBV2	2109775	4257791	90.56%	9.825%
68	23.704	3498	3505	3522	rVB2	1059012	2175973	46.28%	5.021%
69	24.304	3602	3607	3616	rVB3	69306	142139	3.02%	0.328%
70	25.109	3739	3744	3751	rVB3	55408	122904	2.61%	0.284%




Sum of corrected areas: 43335501

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020103.D
Acq On : 10 Jun 2022 16:43
Operator : CG/JU
Sample : N3250-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYT0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

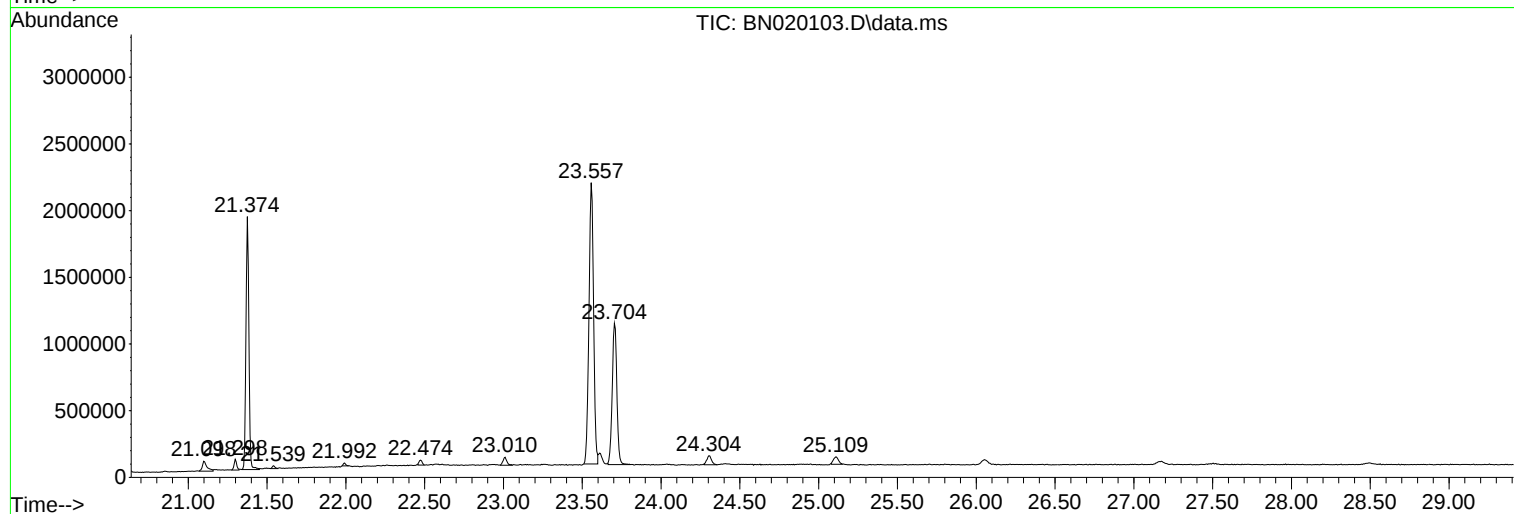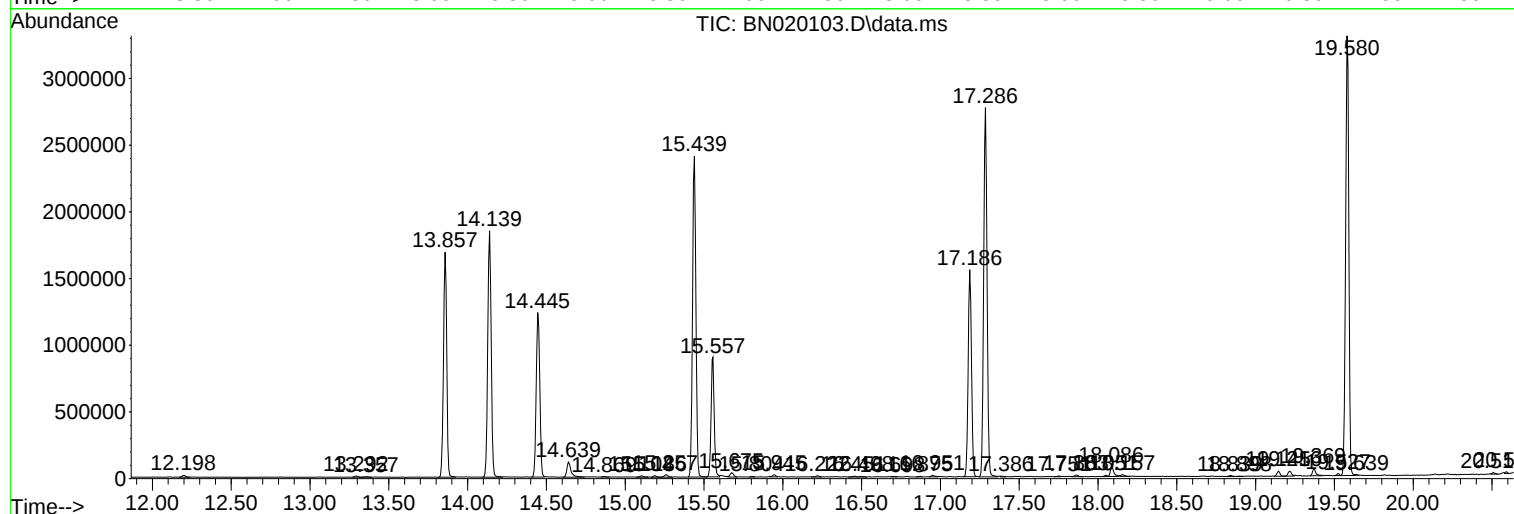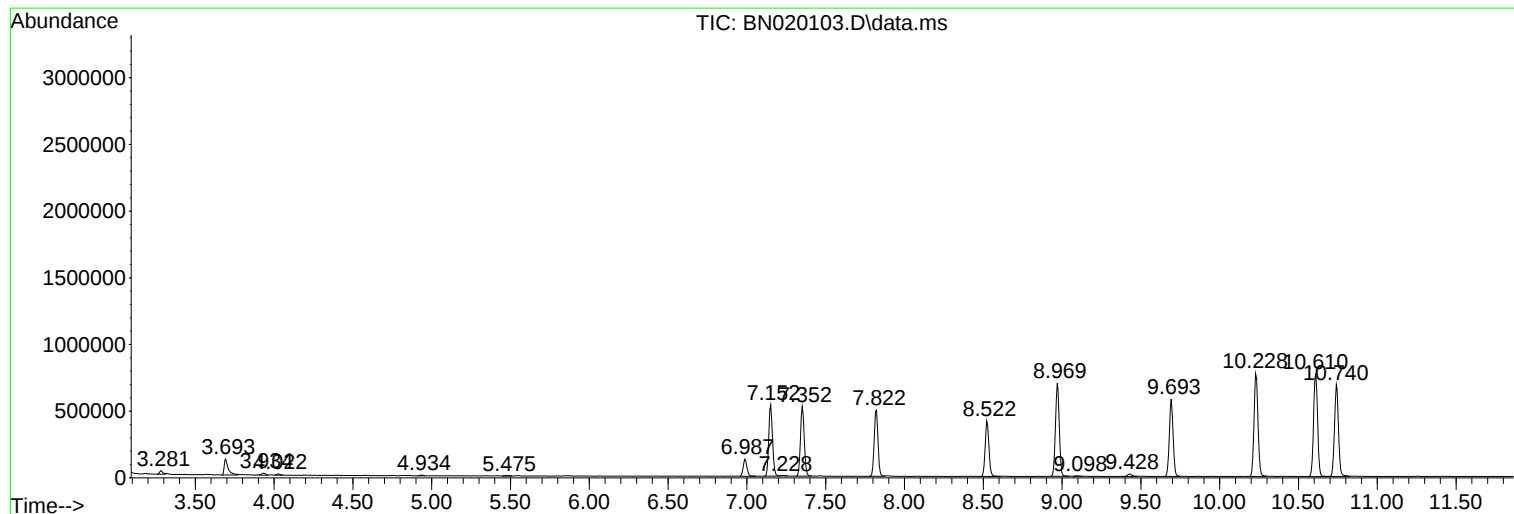

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020103.D
Acq On : 10 Jun 2022 16:43
Operator : CG/JU
Sample : N3250-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYT0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020103.D
Acq On : 10 Jun 2022 16:43
Operator : CG/JU
Sample : N3250-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYT0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc