

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020104.D
 Acq On : 10 Jun 2022 17:19
 Operator : CG/JU
 Sample : N3250-22
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020104.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	40	rVB	40587	55967	0.97%	0.105%
2	3.693	100	103	116	rBV	191401	312538	5.40%	0.589%
3	3.934	139	144	151	rVB2	18705	32118	0.55%	0.061%
4	4.028	157	160	166	rVB2	10928	15093	0.26%	0.028%
5	4.557	245	250	262	rVB6	17047	37504	0.65%	0.071%
6	4.940	310	315	318	rBV3	7211	11573	0.20%	0.022%
7	5.546	414	418	423	rBV3	3490	6124	0.11%	0.012%
8	6.987	657	663	676	rVB	217125	349982	6.04%	0.659%
9	7.151	684	691	704	rBV	721868	1181319	20.40%	2.225%
10	7.351	718	725	738	rBV	738426	1223043	21.12%	2.304%
11	7.463	740	744	748	rVB4	5824	8475	0.15%	0.016%
12	7.822	798	805	814	rBV	603149	999709	17.27%	1.883%
13	8.522	915	924	937	rBV	654535	1079015	18.64%	2.033%
14	8.969	993	1000	1014	rBV	941024	1591057	27.48%	2.997%
15	9.692	1116	1123	1136	rBV	775174	1301004	22.47%	2.451%
16	10.234	1207	1215	1225	rBV	1018531	1809608	31.25%	3.409%
17	10.610	1271	1279	1289	rBV	917443	1590024	27.46%	2.995%
18	10.739	1294	1301	1315	rBV	1009715	1778139	30.71%	3.350%
19	12.204	1542	1550	1558	rVB2	18751	33716	0.58%	0.064%
20	13.857	1824	1831	1843	rBV	2247497	3193552	55.16%	6.016%
21	14.139	1871	1879	1896	rBV	2449298	3729231	64.41%	7.025%
22	14.445	1922	1931	1940	rBV	1435124	2191104	37.84%	4.128%
23	14.639	1958	1964	1984	rBV	190927	328899	5.68%	0.620%
24	14.863	1998	2002	2010	rVB8	6714	12034	0.21%	0.023%
25	15.186	2051	2057	2064	rBV2	9705	14760	0.25%	0.028%
26	15.257	2064	2069	2075	rVB3	5844	9553	0.16%	0.018%
27	15.439	2093	2100	2109	rBV	3172986	4660660	80.50%	8.780%
28	15.557	2113	2120	2135	rVV	1156938	1638427	28.30%	3.087%
29	15.674	2135	2140	2147	rVB3	41402	65672	1.13%	0.124%
30	16.221	2228	2233	2238	rBV3	12253	17331	0.30%	0.033%
31	16.868	2340	2343	2346	rBV5	6229	7486	0.13%	0.014%
32	16.980	2360	2362	2368	rVB5	4149	6378	0.11%	0.012%
33	17.186	2390	2397	2407	rBV	1800242	2571966	44.42%	4.845%
34	17.286	2407	2414	2428	rBV2	3533819	5206328	89.92%	9.808%
35	18.086	2546	2550	2556	rVV	43151	61415	1.06%	0.116%
36	18.157	2559	2562	2565	rVB4	5061	7858	0.14%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020104.D
 Acq On : 10 Jun 2022 17:19
 Operator : CG/JU
 Sample : N3250-22
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	19.145	2725	2730	2735	rVB	45608	61023	1.05%	0.115%
38	19.215	2737	2742	2747	rBV	42421	61231	1.06%	0.115%
39	19.368	2764	2768	2773	rBV	37778	51214	0.88%	0.096%
40	19.521	2790	2794	2798	rBV4	14036	17427	0.30%	0.033%
41	19.580	2798	2804	2813	rBV	4014633	5789869	100.00%	10.907%
42	19.815	2840	2844	2849	rBV3	6946	9672	0.17%	0.018%
43	20.592	2970	2976	2981	rBV4	12623	25671	0.44%	0.048%
44	20.639	2981	2984	2987	rVB5	8755	8870	0.15%	0.017%
45	21.374	3103	3109	3122	rBV2	1931695	2617969	45.22%	4.932%
46	21.986	3211	3213	3220	rVB4	19432	26923	0.47%	0.051%
47	22.474	3293	3296	3302	rVB3	29653	38716	0.67%	0.073%
48	22.539	3302	3307	3312	rBV	72200	108610	1.88%	0.205%
49	23.003	3383	3386	3393	rVB	43978	67944	1.17%	0.128%
50	23.556	3471	3480	3487	rBV	2341081	4723509	81.58%	8.898%
51	23.703	3497	3505	3516	rVB2	1072648	2140457	36.97%	4.032%
52	24.303	3603	3607	3615	rVB2	49698	97791	1.69%	0.184%
53	25.109	3739	3744	3752	rVB3	44443	97057	1.68%	0.183%




Sum of corrected areas: 53082615

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020104.D
Acq On : 10 Jun 2022 17:19
Operator : CG/JU
Sample : N3250-22
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

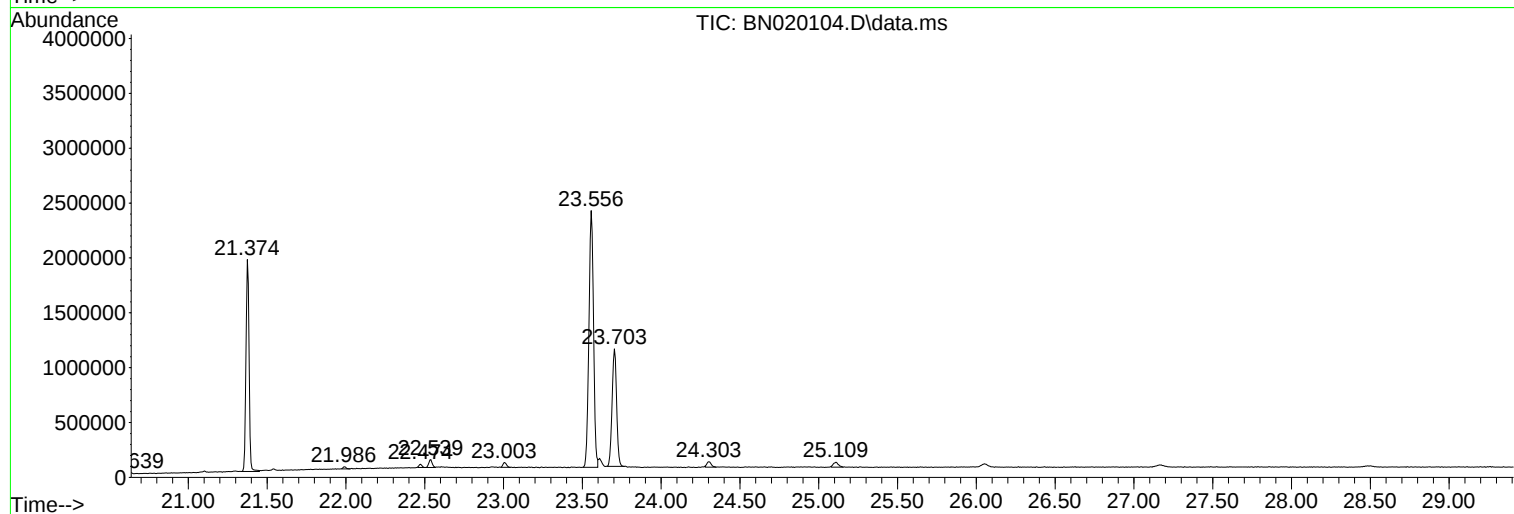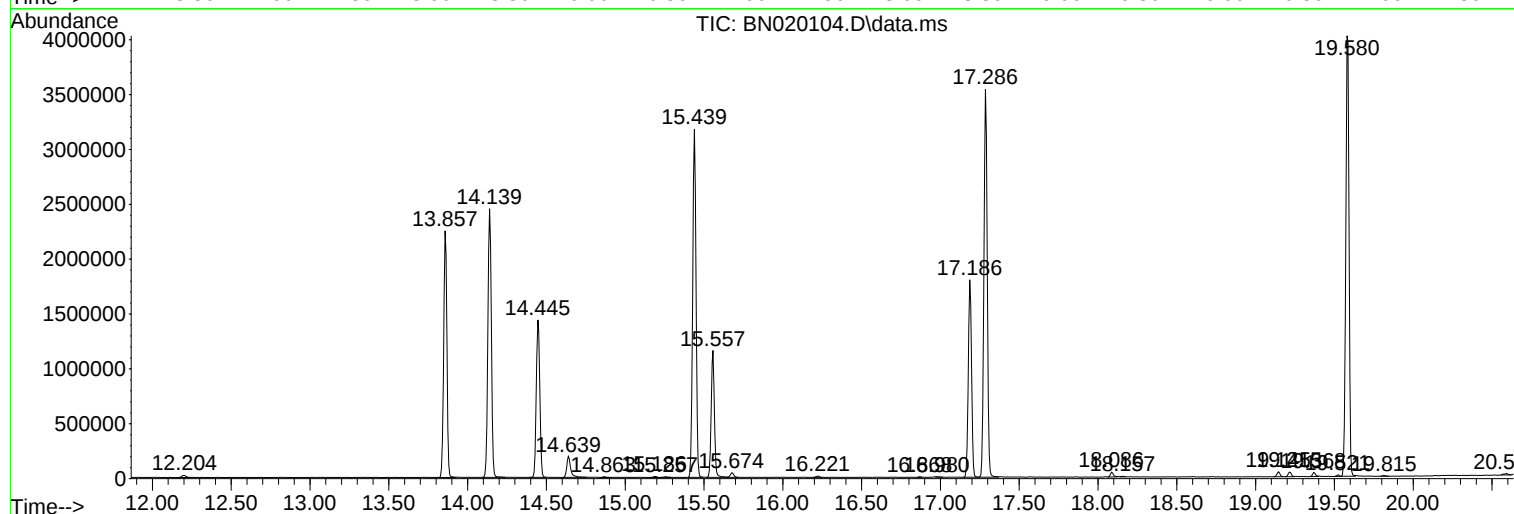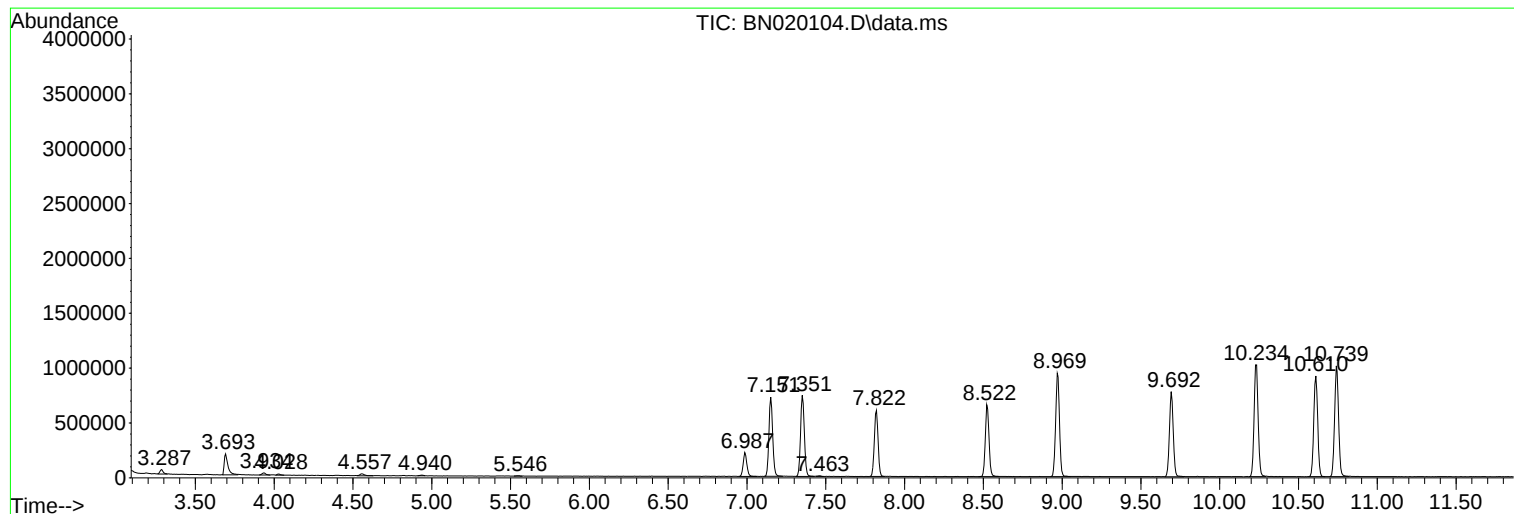

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020104.D
Acq On : 10 Jun 2022 17:19
Operator : CG/JU
Sample : N3250-22
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020104.D
Acq On : 10 Jun 2022 17:19
Operator : CG/JU
Sample : N3250-22
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
