

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020105.D
 Acq On : 10 Jun 2022 17:56
 Operator : CG/JU
 Sample : N3250-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYW2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020105.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	31	rBV	29808	41681	0.87%	0.092%
2	3.281	31	33	40	rVB	36450	45010	0.94%	0.099%
3	3.693	99	103	118	rBV	129802	224604	4.68%	0.495%
4	3.934	140	144	150	rVB	15161	25452	0.53%	0.056%
5	4.028	156	160	164	rVB	10271	14521	0.30%	0.032%
6	4.558	246	250	260	rVB8	10434	21619	0.45%	0.048%
7	4.934	309	314	319	rBV4	6839	12329	0.26%	0.027%
8	4.975	319	321	327	rVB6	3411	5352	0.11%	0.012%
9	5.540	414	417	423	rVB4	5003	8414	0.18%	0.019%
10	6.316	542	549	560	rVB3	28765	61837	1.29%	0.136%
11	6.811	628	633	639	rVB	22105	35849	0.75%	0.079%
12	6.987	657	663	672	rBV	151289	252444	5.26%	0.556%
13	7.152	683	691	700	rBV	564335	919310	19.15%	2.026%
14	7.222	700	703	709	rVB	11737	18604	0.39%	0.041%
15	7.352	718	725	734	rBV	565738	922917	19.23%	2.033%
16	7.458	741	743	748	rVB4	4261	5326	0.11%	0.012%
17	7.699	779	784	785	rBV2	7114	10387	0.22%	0.023%
18	7.728	785	789	795	rVB	23725	36034	0.75%	0.079%
19	7.816	798	804	812	rBV	528404	886686	18.47%	1.954%
20	7.887	813	816	822	rVB3	4980	8867	0.18%	0.020%
21	8.140	854	859	860	rBV5	3637	5143	0.11%	0.011%
22	8.193	860	868	874	rVV2	26930	61524	1.28%	0.136%
23	8.252	875	878	882	rVB3	3430	4823	0.10%	0.011%
24	8.316	884	889	894	rBV2	20699	32019	0.67%	0.071%
25	8.469	910	915	918	rBV2	20109	31448	0.66%	0.069%
26	8.522	918	924	938	rVB	487562	791983	16.50%	1.745%
27	8.969	988	1000	1016	rBV	733439	1291729	26.91%	2.846%
28	9.099	1016	1022	1028	rVV2	14290	26069	0.54%	0.057%
29	9.181	1028	1036	1041	rVB10	6520	17558	0.37%	0.039%
30	9.275	1044	1052	1056	rBV2	4226	7512	0.16%	0.017%
31	9.428	1076	1078	1087	rVB7	2726	5631	0.12%	0.012%
32	9.693	1115	1123	1133	rBV	593230	1003110	20.90%	2.210%
33	9.816	1136	1144	1148	rBV7	6351	12610	0.26%	0.028%
34	9.869	1148	1153	1157	rBV4	4521	7704	0.16%	0.017%
35	10.010	1171	1177	1185	rVB2	19274	34340	0.72%	0.076%
36	10.228	1207	1214	1227	rBV	812469	1419834	29.58%	3.128%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020105.D
 Acq On : 10 Jun 2022 17:56
 Operator : CG/JU
 Sample : N3250-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYW2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	10.610	1269	1279	1285	rBV	844738	1443476	30.07%	3.180%
38	10.657	1285	1287	1293	rVB	38163	56804	1.18%	0.125%
39	10.740	1293	1301	1312	rBV	804536	1399859	29.16%	3.084%
40	11.987	1506	1513	1515	rBV4	4234	6558	0.14%	0.014%

41	12.199	1540	1549	1556	rVV3	16423	33961	0.71%	0.075%
42	12.275	1556	1562	1567	rVB3	6074	10160	0.21%	0.022%
43	12.487	1593	1598	1606	rBV4	5737	9881	0.21%	0.022%
44	12.957	1672	1678	1682	rBV3	9780	17482	0.36%	0.039%
45	13.163	1709	1713	1722	rVB5	5854	11373	0.24%	0.025%

46	13.287	1729	1734	1738	rVB3	6646	10171	0.21%	0.022%
47	13.469	1759	1765	1774	rVB	47089	79271	1.65%	0.175%
48	13.857	1820	1831	1846	rBV	1801360	2528444	52.68%	5.571%
49	14.140	1870	1879	1893	rBV	1899896	2886032	60.12%	6.359%
50	14.363	1912	1917	1921	rVB4	3678	6061	0.13%	0.013%

51	14.445	1924	1931	1943	rBV	1276703	1999013	41.65%	4.404%
52	14.640	1956	1964	1974	rBV	139293	250719	5.22%	0.552%
53	14.722	1974	1978	1984	rVB2	15600	26368	0.55%	0.058%
54	14.863	1999	2002	2006	rVV3	7851	10250	0.21%	0.023%
55	14.981	2017	2022	2028	rVB2	2807	5484	0.11%	0.012%

56	15.104	2040	2043	2048	rVB4	3665	5863	0.12%	0.013%
57	15.192	2052	2058	2064	rVV	26059	35513	0.74%	0.078%
58	15.269	2064	2071	2074	rBV4	3801	6446	0.13%	0.014%
59	15.440	2093	2100	2112	rBV	2508023	3739434	77.90%	8.239%
60	15.557	2114	2120	2132	rVV	902681	1308252	27.25%	2.882%

61	15.663	2133	2138	2149	rVB2	65529	128351	2.67%	0.283%
62	16.004	2193	2196	2204	rBV5	2772	5575	0.12%	0.012%
63	16.169	2220	2224	2229	rVV4	5451	9270	0.19%	0.020%
64	16.222	2229	2233	2238	rVB3	11531	15853	0.33%	0.035%
65	16.869	2340	2343	2348	rVB6	4831	7063	0.15%	0.016%

66	16.969	2356	2360	2368	rVB6	4786	9991	0.21%	0.022%
67	17.186	2390	2397	2407	rBV	1657696	2355478	49.07%	5.190%
68	17.286	2407	2414	2426	rVV2	2866499	4225119	88.02%	9.309%
69	17.569	2456	2462	2467	rBV	65399	88584	1.85%	0.195%
70	17.869	2509	2513	2519	rVB6	10381	14939	0.31%	0.033%

71	18.086	2546	2550	2558	rBV	90723	142254	2.96%	0.313%
72	18.157	2560	2562	2566	rVB	10365	14024	0.29%	0.031%
73	19.145	2725	2730	2737	rBV	40877	61453	1.28%	0.135%
74	19.216	2737	2742	2746	rBV	37070	54997	1.15%	0.121%
75	19.369	2764	2768	2776	rBV3	43549	62391	1.30%	0.137%

76	19.522	2791	2794	2797	rBV4	16395	19986	0.42%	0.044%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020105.D
 Acq On : 10 Jun 2022 17:56
 Operator : CG/JU
 Sample : N3250-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYW2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

77	19.580	2797	2804	2811	rBV	3381276	4800076	100.00%	10.576%
78	20.139	2897	2899	2903	rVB5	7968	7910	0.16%	0.017%
79	20.569	2970	2972	2973	rBV2	8933	6988	0.15%	0.015%
80	21.098	3058	3062	3072	rBV	103101	192830	4.02%	0.425%
81	21.374	3103	3109	3118	rBV	1851964	2452731	51.10%	5.404%
82	21.986	3211	3213	3217	rVB2	17356	13043	0.27%	0.029%
83	22.469	3292	3295	3300	rBV2	30311	42422	0.88%	0.093%
84	22.533	3302	3306	3313	rVV2	59674	94105	1.96%	0.207%
85	23.004	3383	3386	3391	rVB	45702	69037	1.44%	0.152%
86	23.557	3471	3480	3487	rBV2	1987240	4094506	85.30%	9.021%
87	23.704	3497	3505	3515	rVB2	1017359	2096474	43.68%	4.619%
88	24.304	3602	3607	3614	rVB2	51050	103824	2.16%	0.229%




Sum of corrected areas: 45386429

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020105.D
Acq On : 10 Jun 2022 17:56
Operator : CG/JU
Sample : N3250-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

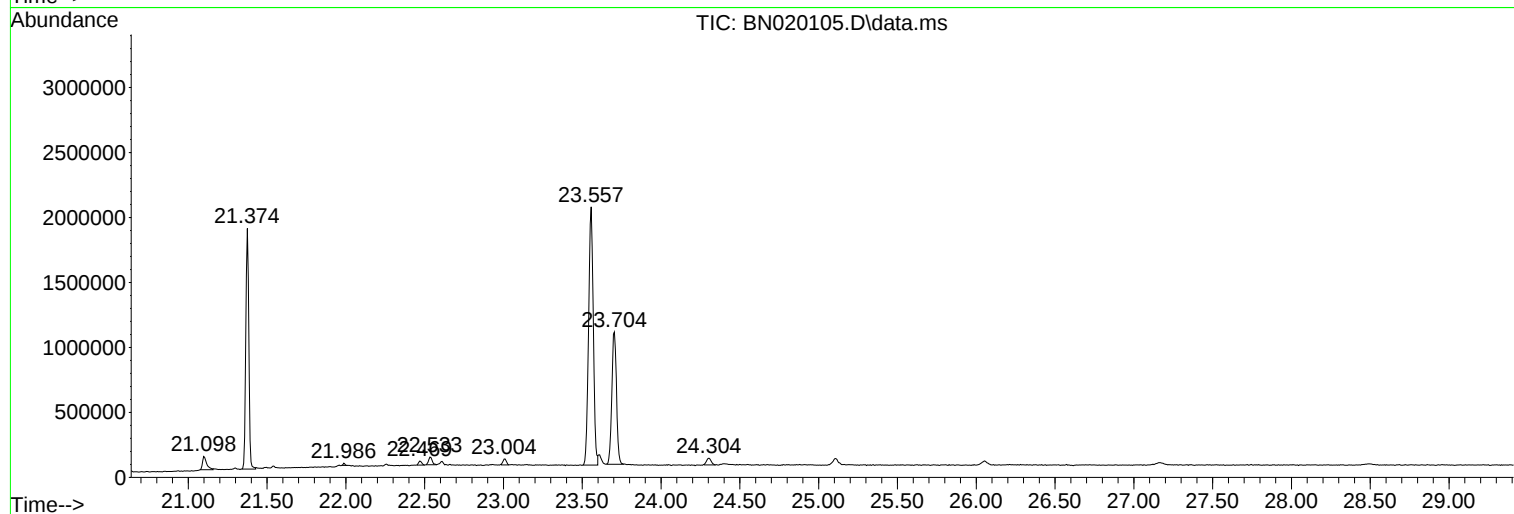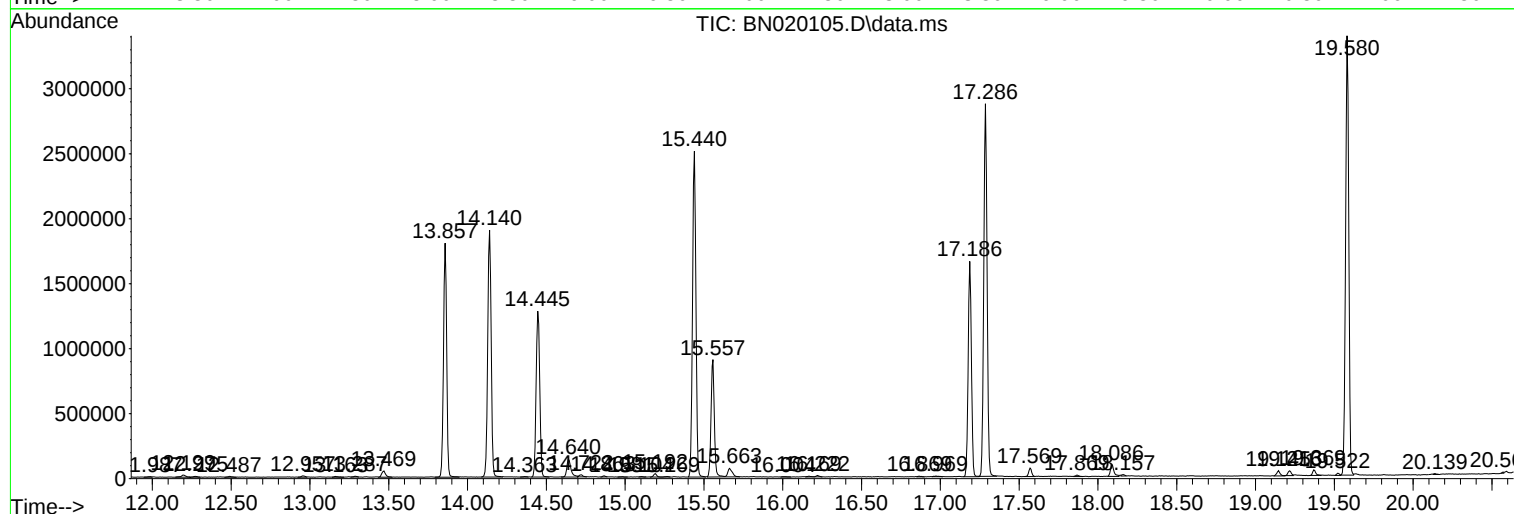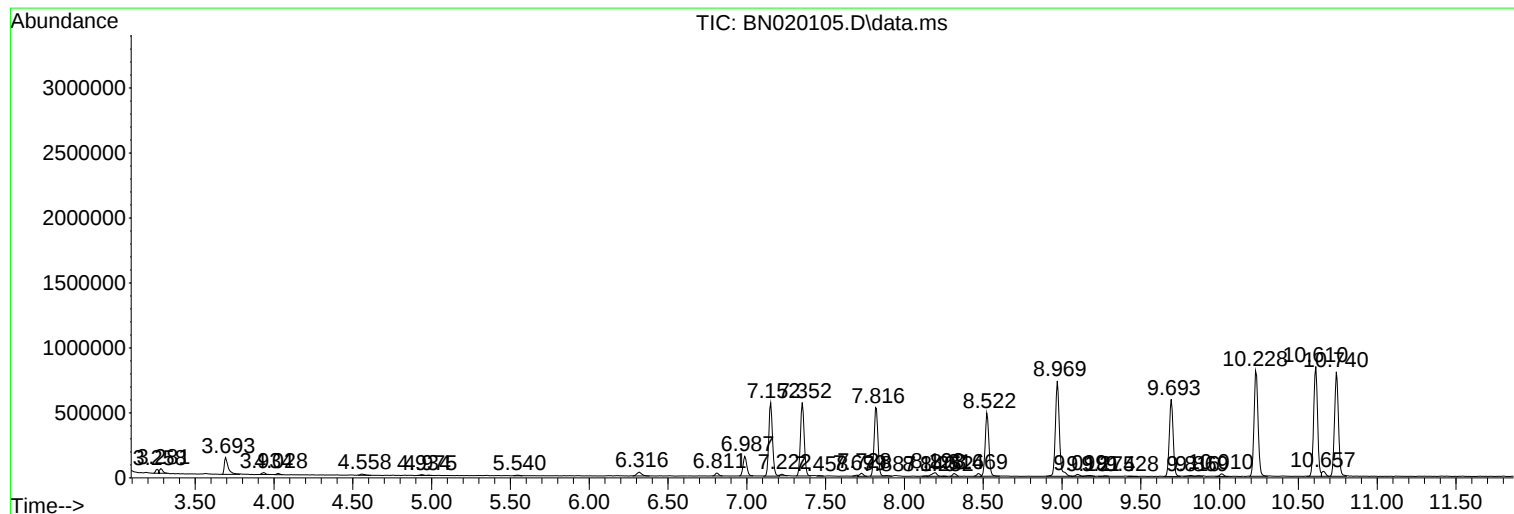

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020105.D
Acq On : 10 Jun 2022 17:56
Operator : CG/JU
Sample : N3250-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020105.D
Acq On : 10 Jun 2022 17:56
Operator : CG/JU
Sample : N3250-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc