

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020106.D
 Acq On : 10 Jun 2022 18:32
 Operator : CG/JU
 Sample : N3250-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYS7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020106.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	14	16	22	rVB5	5217	6062	0.12%	0.014%
2	3.281	29	33	41	rBV2	26749	38755	0.79%	0.092%
3	3.693	100	103	115	rBV	83876	145052	2.97%	0.343%
4	3.934	139	144	150	rVB2	13818	23253	0.48%	0.055%
5	4.028	155	160	169	rVB2	9808	16779	0.34%	0.040%
6	4.393	218	222	227	rVB5	4043	7315	0.15%	0.017%
7	4.934	311	314	320	rVB5	4410	6877	0.14%	0.016%
8	6.987	656	663	675	rBV	118057	196117	4.01%	0.464%
9	7.152	684	691	702	rBV	490926	810868	16.58%	1.920%
10	7.352	718	725	738	rVB	487666	792885	16.22%	1.877%
11	7.822	796	805	816	rBV	509055	859208	17.57%	2.035%
12	8.081	843	849	852	rVB5	3152	4961	0.10%	0.012%
13	8.522	916	924	939	rBV	387922	636824	13.02%	1.508%
14	8.734	954	960	963	rVB5	3649	6039	0.12%	0.014%
15	8.969	993	1000	1010	rBV	626502	1076859	22.02%	2.550%
16	9.099	1017	1022	1027	rBV4	16818	29984	0.61%	0.071%
17	9.146	1027	1030	1035	rVB5	10363	15349	0.31%	0.036%
18	9.693	1114	1123	1135	rBV	512336	872675	17.85%	2.066%
19	10.228	1207	1214	1225	rBV	691466	1215001	24.85%	2.877%
20	10.610	1270	1279	1289	rBV	787571	1385748	28.34%	3.281%
21	10.740	1293	1301	1315	rBV	630250	1127017	23.05%	2.669%
22	10.834	1315	1317	1327	rVB4	3134	6950	0.14%	0.016%
23	11.410	1412	1415	1422	rBV6	3137	6317	0.13%	0.015%
24	12.199	1543	1549	1557	rVB2	14240	25611	0.52%	0.061%
25	13.351	1742	1745	1753	rVB2	6696	11403	0.23%	0.027%
26	13.857	1824	1831	1845	rBV	1547572	2151676	44.00%	5.095%
27	14.087	1865	1870	1873	rBV	74646	101889	2.08%	0.241%
28	14.140	1873	1879	1891	rVB	1685485	2579848	52.76%	6.109%
29	14.446	1924	1931	1941	rVV	1236134	1928050	39.43%	4.565%
30	14.640	1958	1964	1977	rBV	102035	187176	3.83%	0.443%
31	14.869	1999	2003	2009	rVB4	4931	7548	0.15%	0.018%
32	15.134	2044	2048	2052	rVB4	5054	6923	0.14%	0.016%
33	15.257	2065	2069	2074	rVB5	4006	7175	0.15%	0.017%
34	15.310	2074	2078	2086	rBV3	9540	13114	0.27%	0.031%
35	15.440	2092	2100	2113	rBV	2135928	3314585	67.79%	7.849%
36	15.557	2113	2120	2131	rVV	893459	1241290	25.39%	2.939%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020106.D
 Acq On : 10 Jun 2022 18:32
 Operator : CG/JU
 Sample : N3250-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYS7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	15.681	2134	2141	2152	rVB2	26943	51877	1.06%	0.123%
38	15.816	2158	2164	2167	rVB6	3529	5679	0.12%	0.013%
39	16.169	2220	2224	2227	rBV2	18917	26398	0.54%	0.063%
40	16.222	2230	2233	2239	rVB5	10089	14171	0.29%	0.034%
41	16.516	2279	2283	2286	rBV6	3377	6298	0.13%	0.015%
42	16.875	2340	2344	2348	rVB6	3392	5068	0.10%	0.012%
43	16.963	2354	2359	2363	rBV2	25969	36281	0.74%	0.086%
44	17.010	2365	2367	2372	rVB3	5765	8578	0.18%	0.020%
45	17.187	2390	2397	2406	rBV	1563174	2309091	47.22%	5.468%
46	17.287	2407	2414	2428	rVV2	2930797	4310758	88.16%	10.208%
47	17.569	2457	2462	2465	rBV5	3796	6159	0.13%	0.015%
48	17.698	2480	2484	2489	rBV	25892	32815	0.67%	0.078%
49	17.863	2509	2512	2517	rVB7	7551	8647	0.18%	0.020%
50	18.028	2537	2540	2545	rVB5	9689	13499	0.28%	0.032%
51	18.086	2546	2550	2558	rBV	51107	81517	1.67%	0.193%
52	18.339	2591	2593	2598	rBV4	8253	11273	0.23%	0.027%
53	18.392	2598	2602	2607	rBV2	22200	30393	0.62%	0.072%
54	19.028	2706	2710	2716	rBV2	20536	26578	0.54%	0.063%
55	19.145	2725	2730	2736	rBV2	43561	61886	1.27%	0.147%
56	19.216	2738	2742	2746	rBV2	36878	49489	1.01%	0.117%
57	19.369	2764	2768	2779	rBV2	74623	117665	2.41%	0.279%
58	19.522	2791	2794	2797	rVB4	13044	16280	0.33%	0.039%
59	19.581	2797	2804	2811	rBV	3333480	4889695	100.00%	11.578%
60	20.139	2895	2899	2902	rBV2	23335	24377	0.50%	0.058%
61	20.586	2973	2975	2979	rVB3	12533	14176	0.29%	0.034%
62	20.633	2980	2983	2989	rVB	27092	30477	0.62%	0.072%
63	21.098	3059	3062	3066	rVB3	31745	34954	0.71%	0.083%
64	21.369	3103	3108	3121	rBV2	1761290	2453030	50.17%	5.809%
65	21.533	3133	3136	3142	rVB2	31751	39842	0.81%	0.094%
66	21.986	3210	3213	3219	rVB	36621	42841	0.88%	0.101%
67	22.469	3292	3295	3299	rVB2	40515	52622	1.08%	0.125%
68	23.004	3382	3386	3392	rVB	43450	68410	1.40%	0.162%
69	23.551	3471	3479	3487	rBV2	2181146	4291042	87.76%	10.161%
70	23.698	3497	3504	3514	rVB2	1052167	2110997	43.17%	4.999%
71	24.298	3602	3606	3613	rVB4	42071	84936	1.74%	0.201%


Sum of corrected areas: 42230982

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020106.D
Acq On : 10 Jun 2022 18:32
Operator : CG/JU
Sample : N3250-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYS7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

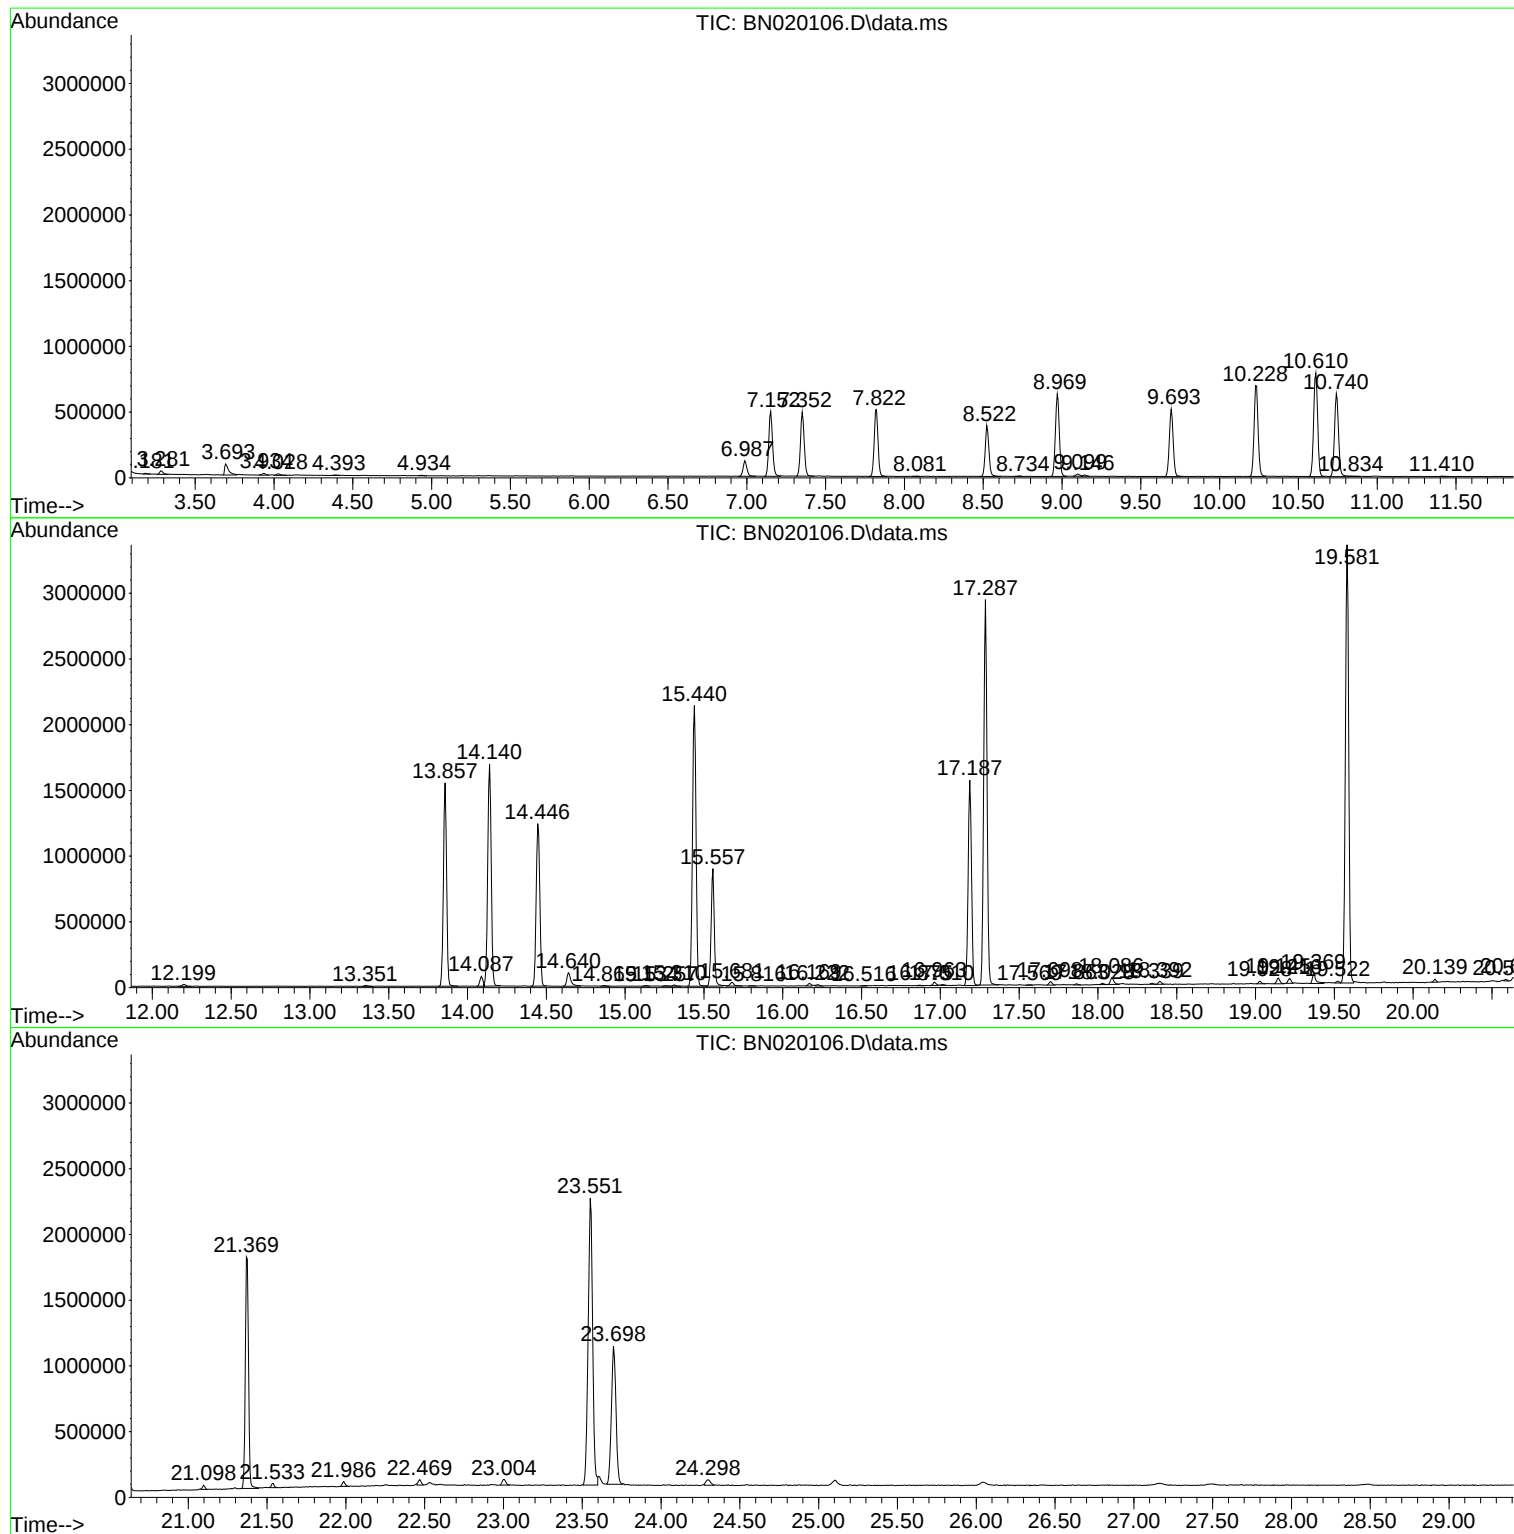

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020106.D
Acq On : 10 Jun 2022 18:32
Operator : CG/JU
Sample : N3250-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYS7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020106.D
Acq On : 10 Jun 2022 18:32
Operator : CG/JU
Sample : N3250-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYS7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc