

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020109.D
 Acq On : 10 Jun 2022 20:21
 Operator : CG/JU
 Sample : N3250-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYW9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020109.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	25	30	37	rBV2	390870	572453	12.03%	1.265%
2	3.317	37	39	46	rVB	30542	43146	0.91%	0.095%
3	3.687	100	102	120	rBV	221820	356400	7.49%	0.788%
4	3.934	140	144	149	rBV2	17461	27587	0.58%	0.061%
5	4.028	156	160	164	rVB3	11590	15844	0.33%	0.035%
6	4.123	172	176	184	rVB2	28916	44005	0.92%	0.097%
7	4.558	244	250	266	rVB	623246	979386	20.58%	2.165%
8	4.940	311	315	327	rVB2	22623	38049	0.80%	0.084%
9	5.540	415	417	422	rVB3	3504	5151	0.11%	0.011%
10	6.987	657	663	674	rVB	100481	165350	3.47%	0.365%
11	7.152	684	691	706	rBV	620008	1017305	21.37%	2.248%
12	7.352	719	725	734	rBV	385745	634487	13.33%	1.402%
13	7.458	739	743	749	rVB6	4853	7058	0.15%	0.016%
14	7.822	797	805	813	rBV	586903	1001699	21.04%	2.214%
15	8.522	915	924	941	rBV	381484	632077	13.28%	1.397%
16	8.969	993	1000	1015	rBV	772722	1323330	27.80%	2.925%
17	9.693	1116	1123	1136	rBV	376541	635209	13.34%	1.404%
18	10.228	1207	1214	1225	rBV	532758	943014	19.81%	2.084%
19	10.610	1269	1279	1292	rBV	884550	1541093	32.38%	3.406%
20	10.740	1293	1301	1321	rVV	864810	1514570	31.82%	3.347%
21	12.134	1531	1538	1545	rBV	208913	344863	7.25%	0.762%
22	12.199	1545	1549	1555	rVB3	18657	31734	0.67%	0.070%
23	13.769	1812	1816	1822	rVB2	12993	19868	0.42%	0.044%
24	13.857	1824	1831	1843	rBV	1834657	2628000	55.21%	5.808%
25	14.140	1871	1879	1898	rBV	2034207	3092475	64.97%	6.835%
26	14.446	1924	1931	1939	rBV	1339410	2050731	43.08%	4.532%
27	14.646	1954	1965	1979	rBV2	49165	109225	2.29%	0.241%
28	14.863	1997	2002	2012	rBV9	3152	5536	0.12%	0.012%
29	15.257	2064	2069	2075	rVB5	3445	6178	0.13%	0.014%
30	15.440	2093	2100	2113	rBV	2646673	3910847	82.16%	8.643%
31	15.551	2113	2119	2132	rVV	437062	627492	13.18%	1.387%
32	15.675	2135	2140	2146	rVB	31163	46260	0.97%	0.102%
33	16.222	2227	2233	2237	rVB2	8991	12032	0.25%	0.027%
34	16.975	2355	2361	2365	rBV5	4204	7814	0.16%	0.017%
35	17.187	2391	2397	2404	rBV	1578563	2340559	49.17%	5.173%
36	17.287	2407	2414	2425	rVV	2983759	4331952	91.01%	9.574%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020109.D
 Acq On : 10 Jun 2022 20:21
 Operator : CG/JU
 Sample : N3250-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYW9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	17.381	2426	2430	2435	rVB6	15116	22125	0.46%	0.049%
38	18.087	2546	2550	2558	rBV3	23232	34441	0.72%	0.076%
39	18.157	2558	2562	2568	rVB5	4040	7513	0.16%	0.017%
40	18.404	2599	2604	2609	rBV9	2263	5018	0.11%	0.011%
41	18.722	2655	2658	2663	rBV4	3762	5750	0.12%	0.013%
42	19.145	2725	2730	2735	rBV	36657	49702	1.04%	0.110%
43	19.216	2737	2742	2747	rBV	36350	53763	1.13%	0.119%
44	19.369	2765	2768	2774	rBV2	20158	29562	0.62%	0.065%
45	19.522	2790	2794	2797	rBV4	11642	12770	0.27%	0.028%
46	19.581	2797	2804	2812	rBV	3326521	4759920	100.00%	10.520%
47	20.145	2896	2900	2902	rBV3	4396	6028	0.13%	0.013%
48	20.575	2969	2973	2974	rBV4	11086	14175	0.30%	0.031%
49	20.592	2974	2976	2980	rVB3	10961	12068	0.25%	0.027%
50	21.375	3103	3109	3116	rBV	1797349	2328865	48.93%	5.147%
51	21.539	3135	3137	3140	rVB4	15087	13487	0.28%	0.030%
52	22.469	3292	3295	3302	rVB3	32431	45608	0.96%	0.101%
53	23.004	3382	3386	3392	rVB	51622	77587	1.63%	0.171%
54	23.557	3471	3480	3486	rBV	1982221	4046472	85.01%	8.943%
55	23.698	3497	3504	3516	rVB	971438	2056674	43.21%	4.546%
56	24.298	3602	3606	3614	rVB3	62800	129540	2.72%	0.286%
57	25.104	3738	3743	3752	rVB2	56381	133091	2.80%	0.294%
58	27.498	4144	4150	4164	rVB4	104439	339171	7.13%	0.750%




Sum of corrected areas: 45246109

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020109.D
Acq On : 10 Jun 2022 20:21
Operator : CG/JU
Sample : N3250-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

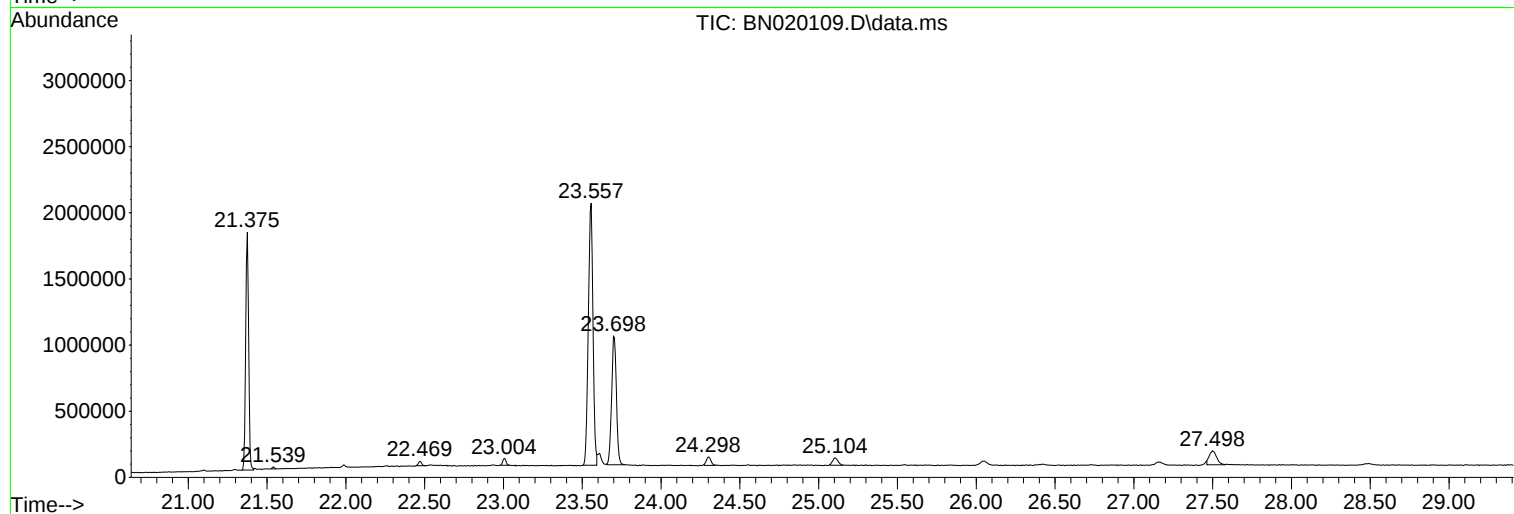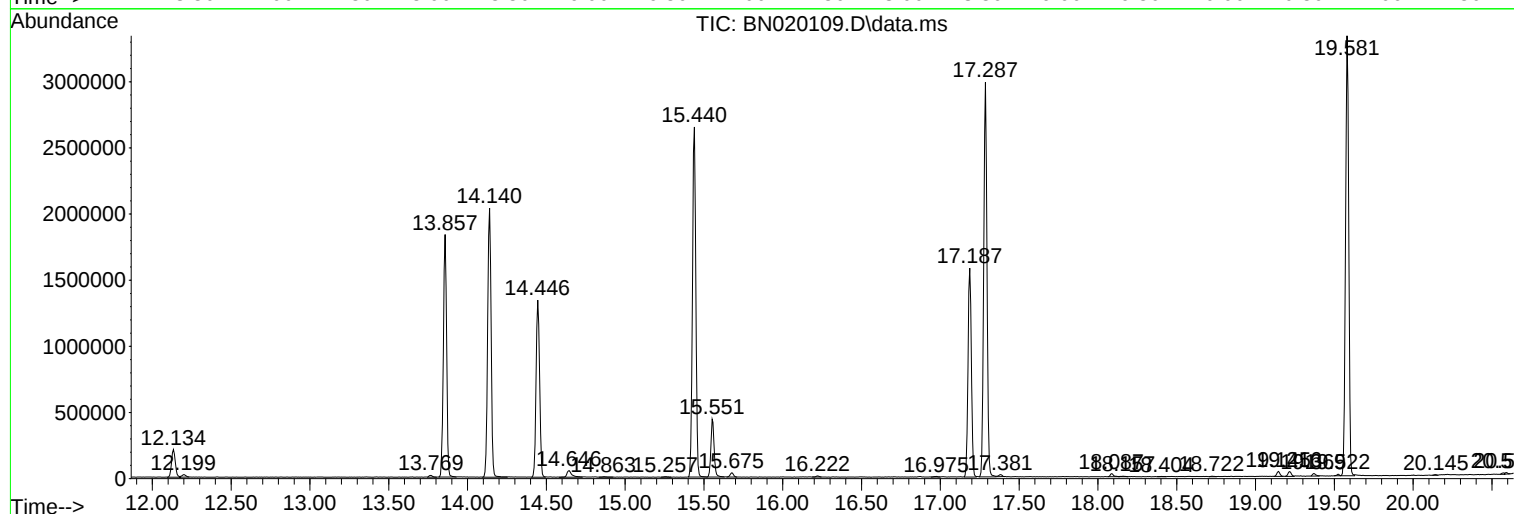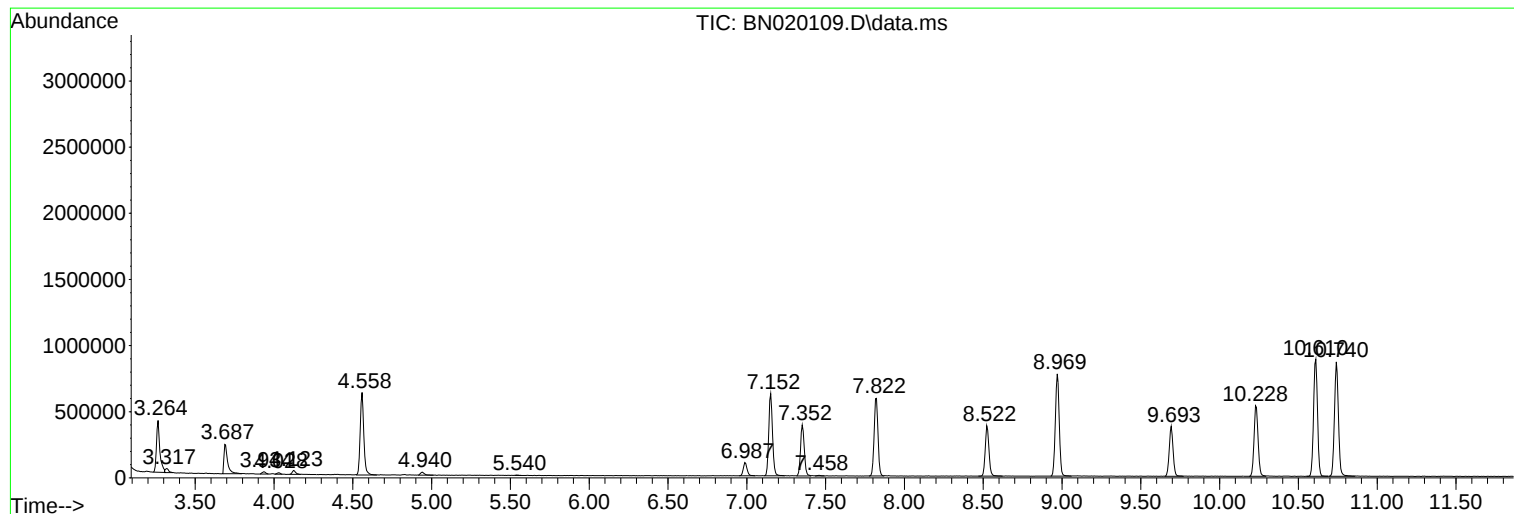

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020109.D
Acq On : 10 Jun 2022 20:21
Operator : CG/JU
Sample : N3250-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020109.D
Acq On : 10 Jun 2022 20:21
Operator : CG/JU
Sample : N3250-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc