

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020111.D
 Acq On : 10 Jun 2022 22:10
 Operator : CG/JU
 Sample : PB145446BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK446

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020111.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	41	rVB	44724	62884	1.37%	0.129%
2	3.687	98	102	118	rBV	606400	964725	21.05%	1.980%
3	4.028	156	160	169	rVB4	10825	19540	0.43%	0.040%
4	6.987	656	663	675	rBV	723563	1180442	25.76%	2.423%
5	7.152	684	691	705	rVB	579469	939080	20.49%	1.928%
6	7.352	718	725	737	rBV	744607	1222243	26.67%	2.509%
7	7.816	796	804	815	rBV	611247	1012319	22.09%	2.078%
8	8.522	917	924	941	rBV	947158	1570413	34.27%	3.223%
9	8.969	992	1000	1013	rBV	745568	1248531	27.25%	2.563%
10	9.693	1116	1123	1136	rBV	627479	1061224	23.16%	2.178%
11	10.228	1206	1214	1226	rBV	901068	1546245	33.75%	3.174%
12	10.604	1271	1278	1288	rBV	921664	1632135	35.62%	3.350%
13	10.740	1293	1301	1314	rBV	1004493	1742253	38.02%	3.576%
14	12.198	1542	1549	1557	rVB2	14470	27021	0.59%	0.055%
15	13.857	1824	1831	1844	rBV	1810763	2517296	54.94%	5.167%
16	14.139	1871	1879	1890	rBV	1875608	2894661	63.17%	5.942%
17	14.445	1924	1931	1941	rVB	1478187	2280581	49.77%	4.681%
18	14.639	1957	1964	1988	rBV	835070	1282600	27.99%	2.633%
19	15.439	2091	2100	2110	rBV	2344379	3607577	78.73%	7.405%
20	15.551	2113	2119	2128	rBV	820538	1180410	25.76%	2.423%
21	15.675	2136	2140	2145	rVB	30252	42591	0.93%	0.087%
22	16.216	2229	2232	2239	rVB3	9606	13371	0.29%	0.027%
23	16.869	2339	2343	2349	rBV6	4015	5741	0.13%	0.012%
24	16.969	2354	2360	2363	rBV5	4849	7826	0.17%	0.016%
25	17.186	2390	2397	2407	rBV	1877744	2698527	58.89%	5.539%
26	17.286	2407	2414	2427	rVV	2681794	4039635	88.16%	8.292%
27	18.086	2545	2550	2551	rBV4	4656	5032	0.11%	0.010%
28	19.145	2724	2730	2736	rBV	33679	48442	1.06%	0.099%
29	19.216	2736	2742	2749	rBV	30984	46607	1.02%	0.096%
30	19.522	2791	2794	2797	rVB3	7298	7649	0.17%	0.016%
31	19.580	2797	2804	2819	rBV	3243621	4582041	100.00%	9.405%
32	20.216	2905	2912	2917	rVV8	10672	33628	0.73%	0.069%
33	20.586	2968	2975	2979	rBV6	10976	25034	0.55%	0.051%
34	21.369	3103	3108	3119	rBV	2082757	2716611	59.29%	5.576%
35	22.463	3291	3294	3299	rBV3	29104	41863	0.91%	0.086%
36	22.998	3381	3385	3390	rVB2	45564	71130	1.55%	0.146%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020111.D
Acq On : 10 Jun 2022 22:10
Operator : CG/JU
Sample : PB145446BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK446

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Title : SVOA CALIBRATION

37	23.551	3470	3479	3485	rBV2	1842015	3734973	81.51%	7.666%
38	23.698	3496	3504	3515	rVB	1147417	2329928	50.85%	4.782%
39	24.298	3601	3606	3613	rVB	65730	131576	2.87%	0.270%
40	25.098	3737	3742	3750	rVB2	62004	144019	3.14%	0.296%




Sum of corrected areas: 48718404

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020111.D
Acq On : 10 Jun 2022 22:10
Operator : CG/JU
Sample : PB145446BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK446

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

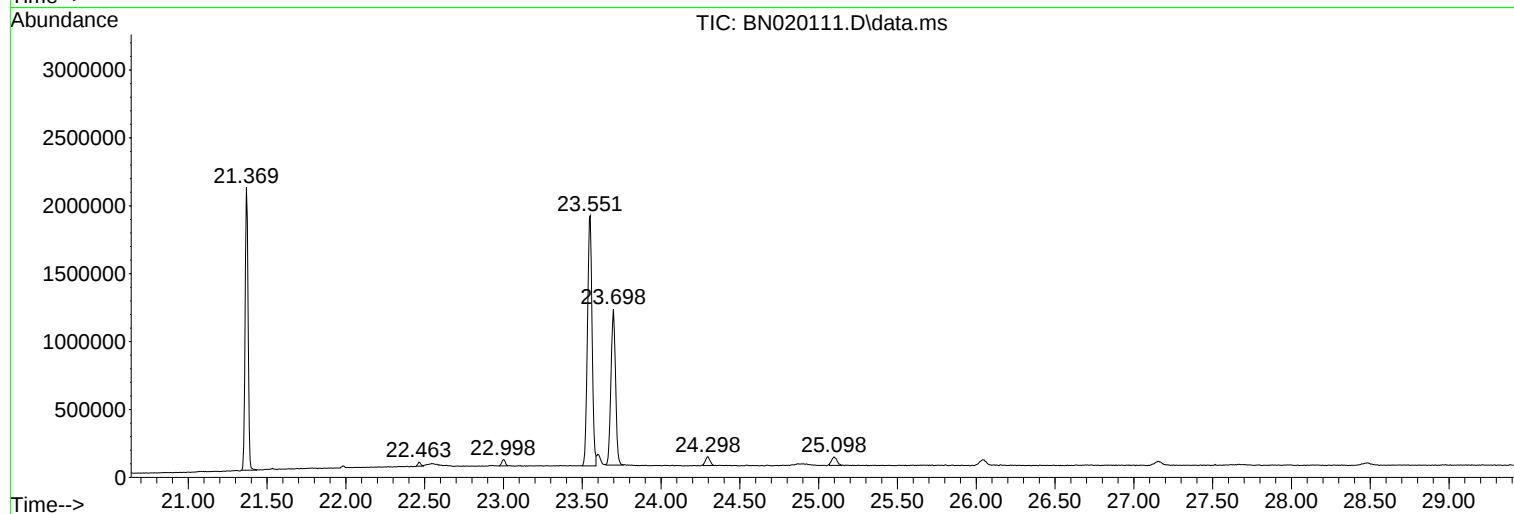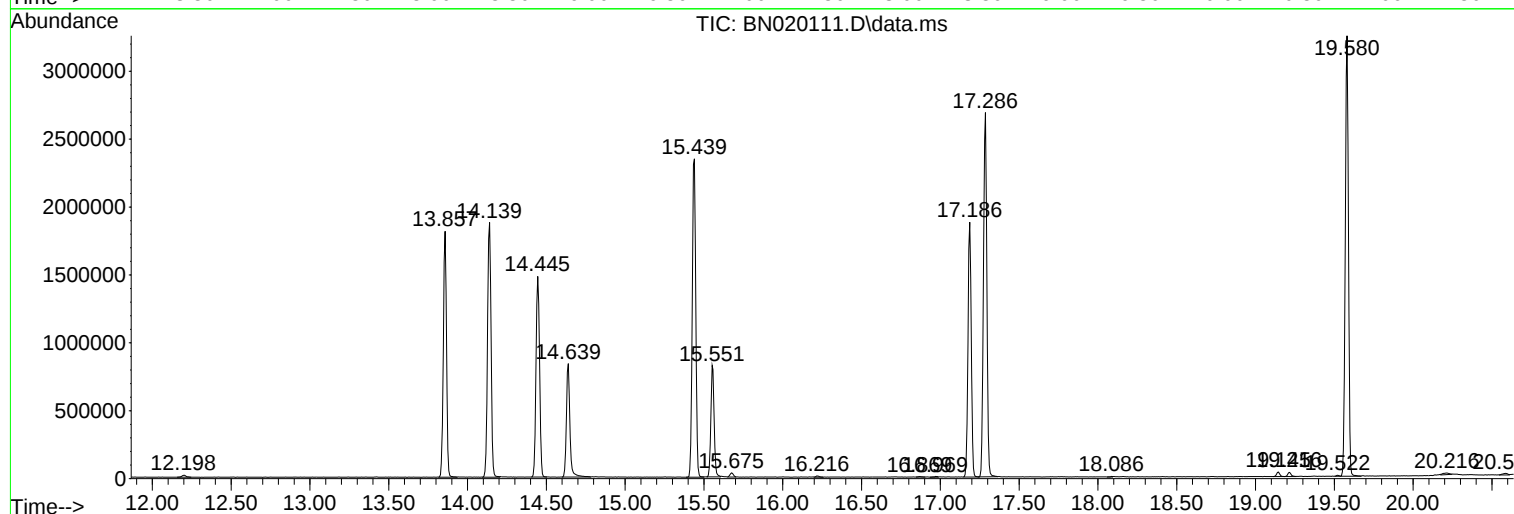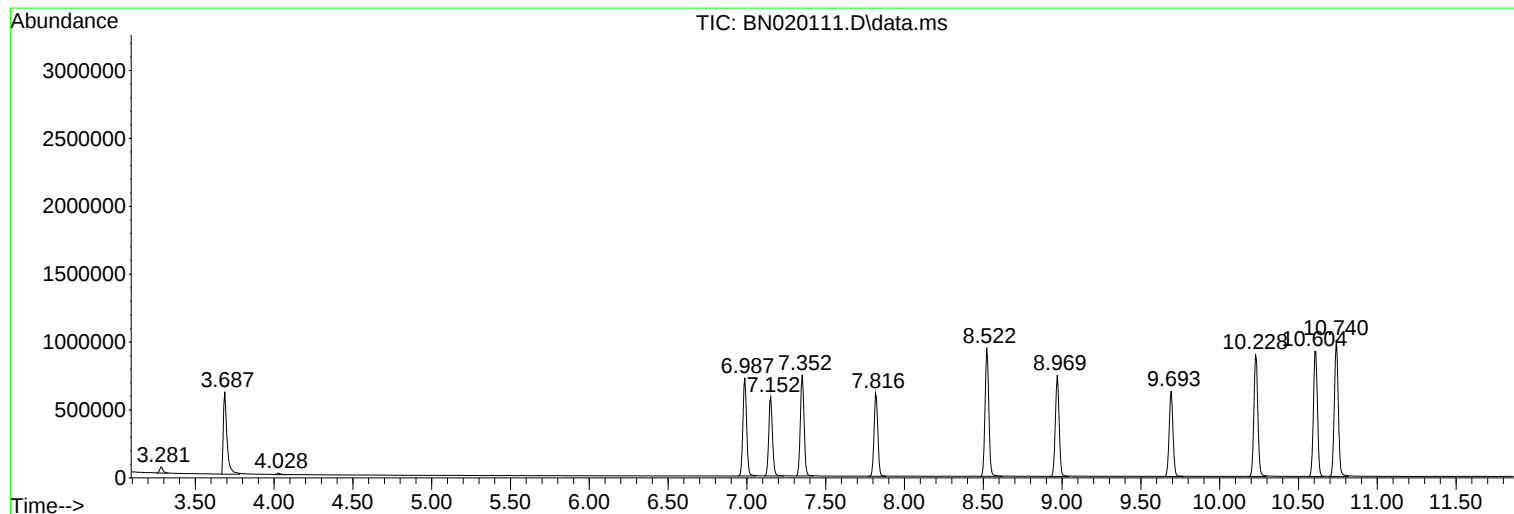

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020111.D
Acq On : 10 Jun 2022 22:10
Operator : CG/JU
Sample : PB145446BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK446

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020111.D
Acq On : 10 Jun 2022 22:10
Operator : CG/JU
Sample : PB145446BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK446

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------