

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020112.D
 Acq On : 10 Jun 2022 22:46
 Operator : CG/JU
 Sample : PB145447BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK447

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020112.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	40	rVB	43764	59978	1.29%	0.126%
2	3.687	98	102	117	rBV	595190	961223	20.75%	2.019%
3	4.028	156	160	164	rVB2	8324	11625	0.25%	0.024%
4	6.987	655	663	675	rBV	713072	1160408	25.05%	2.437%
5	7.151	684	691	707	rVB	563393	923930	19.95%	1.940%
6	7.351	717	725	735	rBV	725980	1200981	25.93%	2.522%
7	7.816	798	804	813	rBV	522000	866441	18.71%	1.820%
8	8.522	918	924	937	rBV	939083	1532189	33.08%	3.218%
9	8.969	992	1000	1015	rBV	720931	1214501	26.22%	2.551%
10	9.692	1115	1123	1133	rBV	605962	1023445	22.10%	2.149%
11	10.228	1207	1214	1231	rBV	874486	1514625	32.70%	3.181%
12	10.604	1271	1278	1287	rVB	797275	1378499	29.76%	2.895%
13	10.739	1293	1301	1315	rBV	973990	1696424	36.63%	3.563%
14	12.198	1541	1549	1556	rBV2	13830	24663	0.53%	0.052%
15	13.857	1824	1831	1842	rBV	1688147	2425951	52.38%	5.095%
16	14.139	1871	1879	1892	rBV	1866053	2826310	61.02%	5.936%
17	14.445	1924	1931	1941	rBV	1265639	1913047	41.30%	4.018%
18	14.639	1957	1964	1982	rBV	855155	1298635	28.04%	2.727%
19	15.439	2092	2100	2113	rBV	2313166	3530804	76.23%	7.415%
20	15.551	2113	2119	2130	rBV	839294	1202357	25.96%	2.525%
21	15.674	2136	2140	2147	rVB2	28998	43728	0.94%	0.092%
22	16.221	2227	2233	2240	rVB4	8702	12657	0.27%	0.027%
23	16.868	2338	2343	2346	rBV4	3655	5181	0.11%	0.011%
24	16.974	2356	2361	2363	rBV4	3547	5445	0.12%	0.011%
25	17.186	2388	2397	2407	rBV	1596585	2334295	50.40%	4.902%
26	17.286	2407	2414	2429	rVV	2685453	3997733	86.32%	8.396%
27	18.098	2546	2552	2557	rBV7	3083	6090	0.13%	0.013%
28	19.145	2726	2730	2735	rVB3	30957	43392	0.94%	0.091%
29	19.215	2735	2742	2747	rBV	34241	47441	1.02%	0.100%
30	19.521	2791	2794	2797	rBV3	7711	7951	0.17%	0.017%
31	19.580	2797	2804	2813	rBV2	3271279	4631534	100.00%	9.727%
32	20.574	2969	2973	2974	rBV3	8232	10994	0.24%	0.023%
33	20.592	2974	2976	2981	rVB6	11364	13744	0.30%	0.029%
34	21.374	3103	3109	3120	rBV	1839292	2497834	53.93%	5.246%
35	22.468	3292	3295	3300	rVB3	35549	50836	1.10%	0.107%
36	23.003	3382	3386	3391	rBV	58952	90636	1.96%	0.190%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020112.D
Acq On : 10 Jun 2022 22:46
Operator : CG/JU
Sample : PB145447BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK447

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Title : SVOA CALIBRATION

37	23.556	3471	3480	3486	rBV2	2053500	4161416	89.85%	8.740%
38	23.703	3497	3505	3516	rVB2	1086841	2223157	48.00%	4.669%
39	24.297	3601	3606	3614	rVB	86823	182588	3.94%	0.383%
40	25.103	3737	3743	3751	rVB	82180	194464	4.20%	0.408%
41	26.050	3898	3904	3915	rVB3	64854	171342	3.70%	0.360%
42	27.162	4087	4093	4101	rVB4	41010	117408	2.53%	0.247%




Sum of corrected areas: 47615902

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020112.D
Acq On : 10 Jun 2022 22:46
Operator : CG/JU
Sample : PB145447BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK447

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

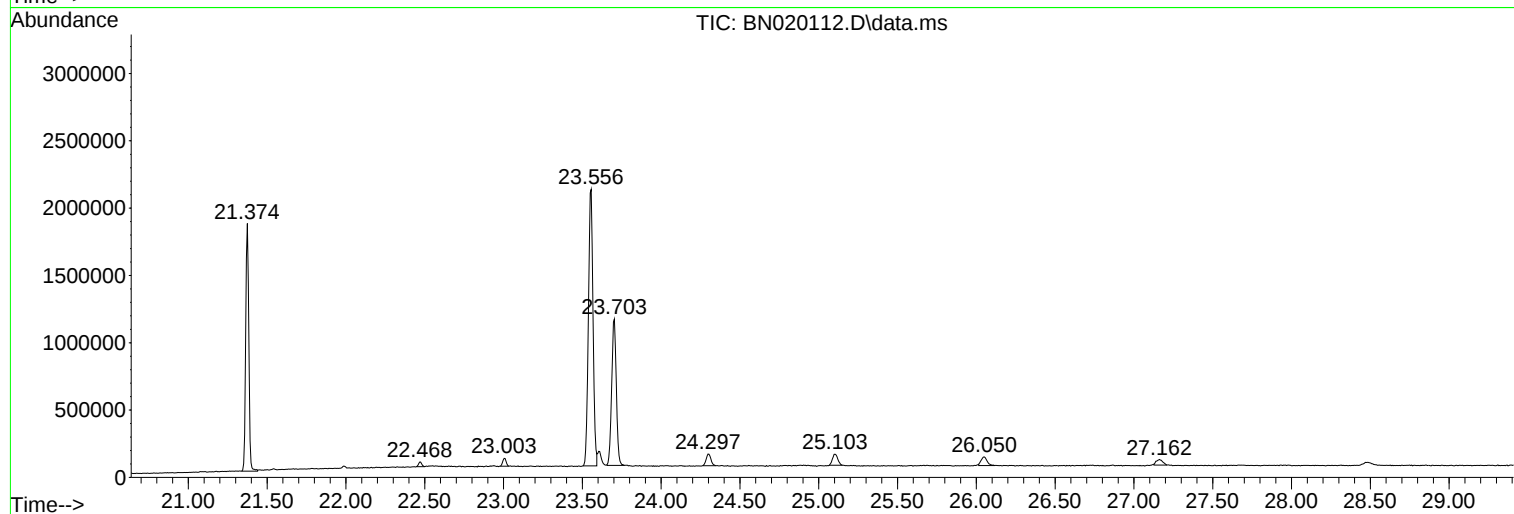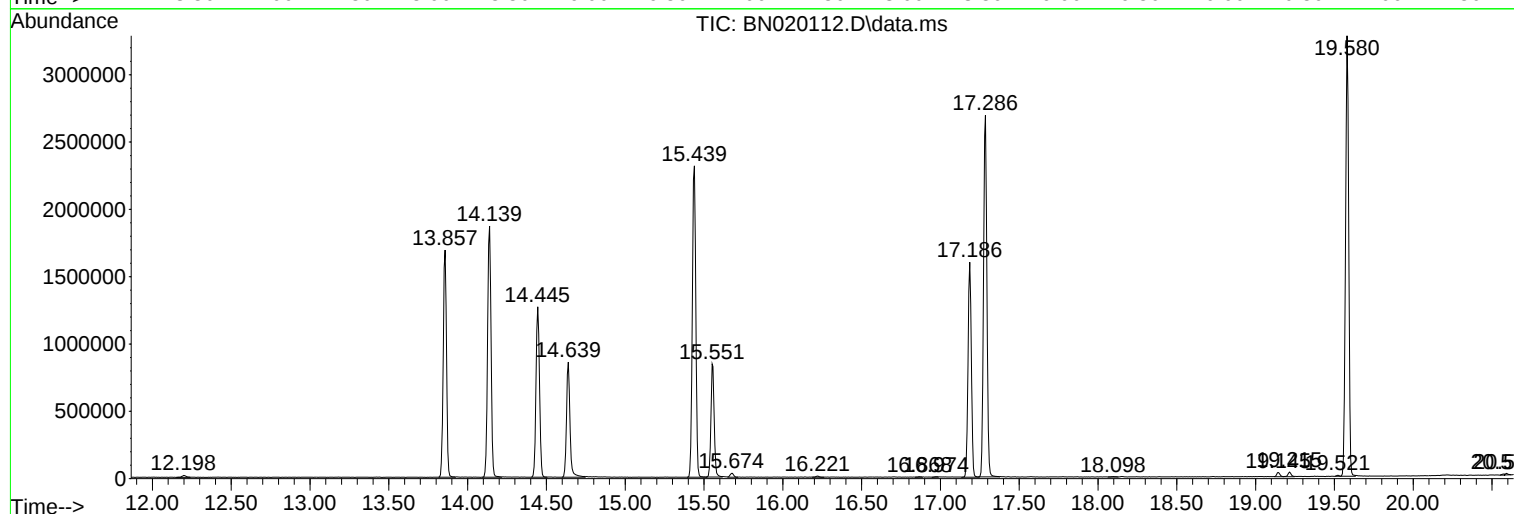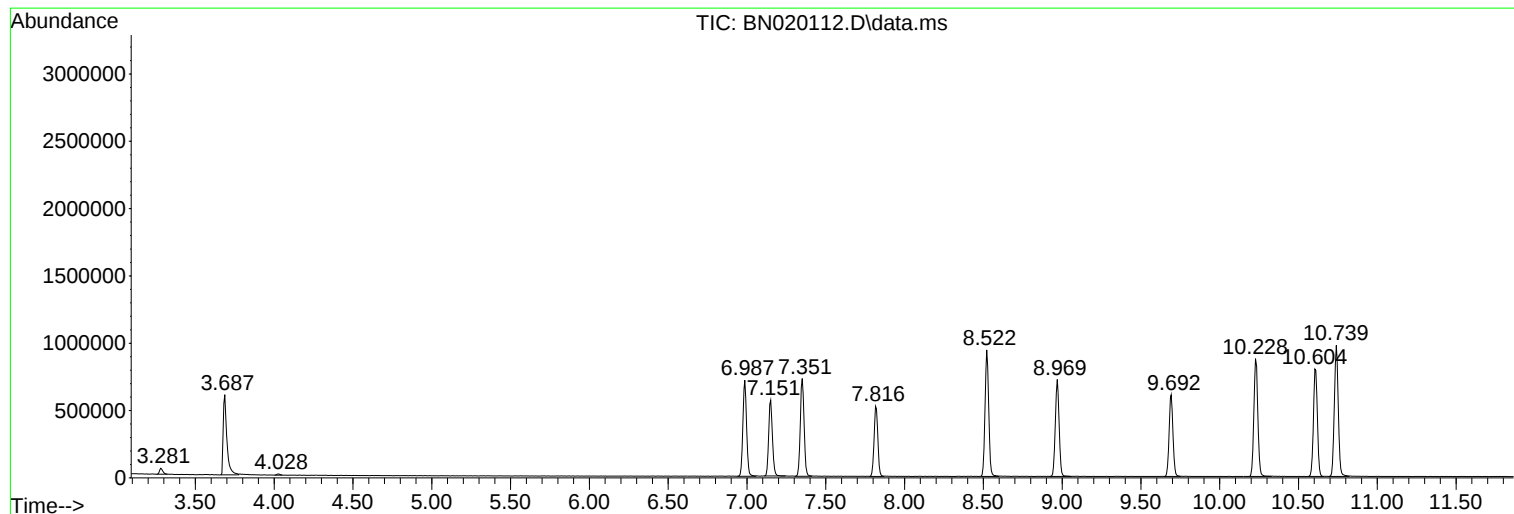

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020112.D
Acq On : 10 Jun 2022 22:46
Operator : CG/JU
Sample : PB145447BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK447

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020112.D
Acq On : 10 Jun 2022 22:46
Operator : CG/JU
Sample : PB145447BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK447

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc