

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020114.D
 Acq On : 10 Jun 2022 23:58
 Operator : CG/JU
 Sample : N3250-09
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYW7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020114.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	24	29	38	rBV2	151438	285360	5.29%	0.572%
2	3.570	78	82	90	rVB4	7440	15852	0.29%	0.032%
3	3.693	99	103	114	rBV	132252	223745	4.14%	0.448%
4	3.934	139	144	150	rVB	16398	27286	0.51%	0.055%
5	4.028	156	160	166	rVB2	11777	16316	0.30%	0.033%
6	4.117	172	175	182	rVB2	18800	28913	0.54%	0.058%
7	4.552	243	249	263	rVB	583518	966829	17.91%	1.938%
8	4.934	309	314	321	rVB4	6717	11218	0.21%	0.022%
9	6.987	657	663	675	rBV	146488	244385	4.53%	0.490%
10	7.146	684	690	699	rBV	528419	900149	16.67%	1.804%
11	7.222	699	703	716	rVB	13506	29987	0.56%	0.060%
12	7.352	716	725	733	rBV	545491	906776	16.80%	1.818%
13	7.458	739	743	749	rVB6	3956	7276	0.13%	0.015%
14	7.816	797	804	812	rBV	580187	971141	17.99%	1.947%
15	7.887	812	816	822	rVB3	5922	11089	0.21%	0.022%
16	8.522	917	924	937	rBV	466837	769574	14.25%	1.543%
17	8.969	992	1000	1011	rBV	726682	1212333	22.46%	2.430%
18	9.093	1017	1021	1028	rBV6	5657	12352	0.23%	0.025%
19	9.428	1075	1078	1083	rVB4	4073	6771	0.13%	0.014%
20	9.693	1113	1123	1134	rBV	568511	980235	18.16%	1.965%
21	10.228	1207	1214	1227	rBV	801713	1377186	25.51%	2.761%
22	10.399	1237	1243	1247	rBV5	3259	6374	0.12%	0.013%
23	10.610	1271	1279	1289	rBV	888839	1579744	29.26%	3.167%
24	10.740	1294	1301	1318	rBV	748917	1314653	24.35%	2.635%
25	12.199	1544	1549	1557	rVB3	14533	25621	0.47%	0.051%
26	13.287	1728	1734	1738	rVB3	6853	9386	0.17%	0.019%
27	13.857	1824	1831	1843	rBV	1767243	2561777	47.45%	5.135%
28	14.140	1870	1879	1893	rBV	1905384	2895303	53.63%	5.804%
29	14.445	1924	1931	1941	rVV	1453338	2206678	40.87%	4.423%
30	14.640	1958	1964	1976	rBV	151855	257819	4.78%	0.517%
31	14.863	1997	2002	2008	rBV5	10733	16638	0.31%	0.033%
32	15.257	2064	2069	2074	rVV4	6482	11038	0.20%	0.022%
33	15.434	2092	2099	2112	rBV	2482206	3842430	71.17%	7.702%
34	15.551	2113	2119	2134	rVV	1077334	1509326	27.96%	3.025%
35	15.675	2136	2140	2148	rVB2	34776	51678	0.96%	0.104%
36	16.128	2213	2217	2222	rBV2	8664	12338	0.23%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020114.D
 Acq On : 10 Jun 2022 23:58
 Operator : CG/JU
 Sample : N3250-09
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYW7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	16.222	2228	2233	2237	rVB3	10358	15824	0.29%	0.032%
38	16.969	2354	2360	2362	rBV5	5740	9564	0.18%	0.019%
39	17.186	2390	2397	2407	rBV	1784472	2618399	48.50%	5.248%
40	17.286	2407	2414	2429	rVV	3165184	4717061	87.37%	9.455%
41	17.869	2508	2513	2517	rVB4	9112	13931	0.26%	0.028%
42	18.086	2545	2550	2559	rBV2	99365	152570	2.83%	0.306%
43	18.151	2559	2561	2567	rVB	8200	13258	0.25%	0.027%
44	18.398	2598	2603	2609	rBV6	5696	10857	0.20%	0.022%
45	19.028	2708	2710	2715	rVB6	4547	5979	0.11%	0.012%
46	19.145	2725	2730	2735	rBV2	44510	64078	1.19%	0.128%
47	19.216	2737	2742	2746	rBV	50896	72335	1.34%	0.145%
48	19.251	2746	2748	2751	rVB3	5407	6209	0.12%	0.012%
49	19.369	2763	2768	2777	rBV	73340	109968	2.04%	0.220%
50	19.522	2790	2794	2797	rBV3	24678	29707	0.55%	0.060%
51	19.580	2797	2804	2811	rVV	3775715	5398798	100.00%	10.822%
52	19.639	2811	2814	2821	rVB5	17919	27166	0.50%	0.054%
53	20.139	2895	2899	2903	rVB	22190	26823	0.50%	0.054%
54	20.510	2959	2962	2968	rVB2	26051	31207	0.58%	0.063%
55	20.569	2968	2972	2974	rBV3	19781	26662	0.49%	0.053%
56	20.633	2979	2983	2986	rVV	42096	45235	0.84%	0.091%
57	21.098	3058	3062	3073	rBV	116214	197414	3.66%	0.396%
58	21.292	3092	3095	3100	rVB3	18067	21447	0.40%	0.043%
59	21.369	3103	3108	3120	rVV	1984723	2727481	50.52%	5.467%
60	21.533	3133	3136	3145	rVB	62990	75319	1.40%	0.151%
61	21.986	3209	3213	3217	rBV	66281	82161	1.52%	0.165%
62	22.469	3291	3295	3299	rVB	78245	107864	2.00%	0.216%
63	23.004	3381	3386	3394	rVB	92205	155029	2.87%	0.311%
64	23.551	3471	3479	3486	rBV2	2326212	4712489	87.29%	9.446%
65	23.698	3496	3504	3517	rVB2	1135384	2346580	43.46%	4.704%
66	24.298	3600	3606	3614	rVB	92799	192824	3.57%	0.387%
67	25.098	3737	3742	3750	rVB2	76362	171247	3.17%	0.343%
68	27.492	4142	4149	4162	rVB2	127970	397711	7.37%	0.797%




Sum of corrected areas: 49888773

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020114.D
Acq On : 10 Jun 2022 23:58
Operator : CG/JU
Sample : N3250-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

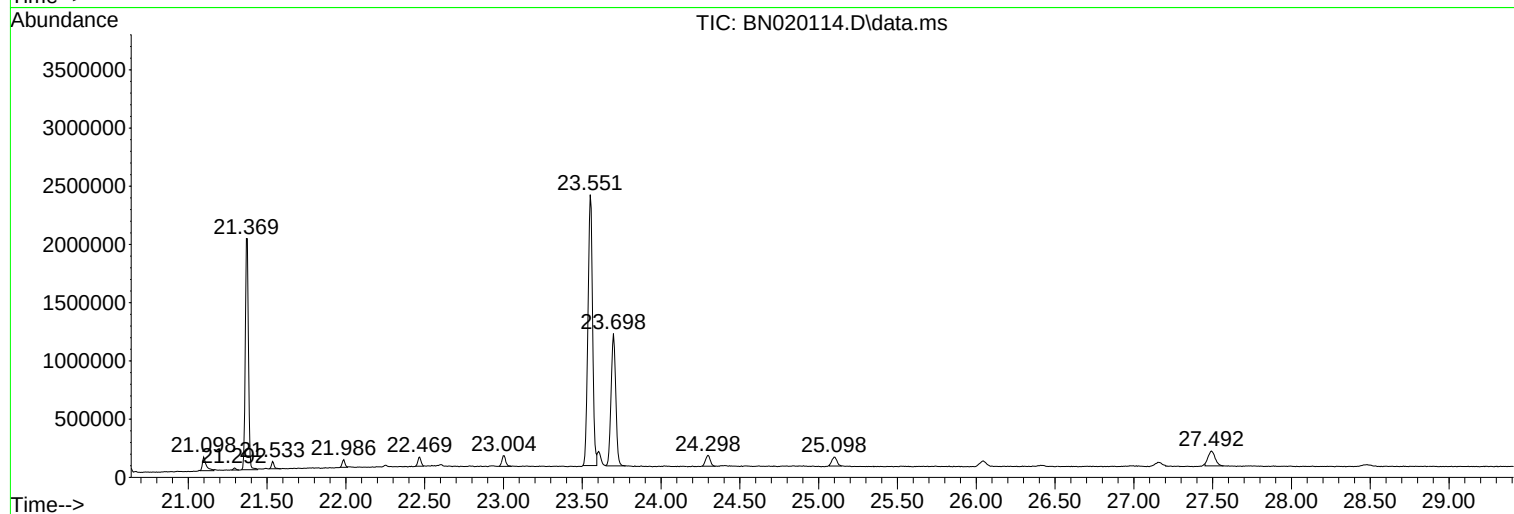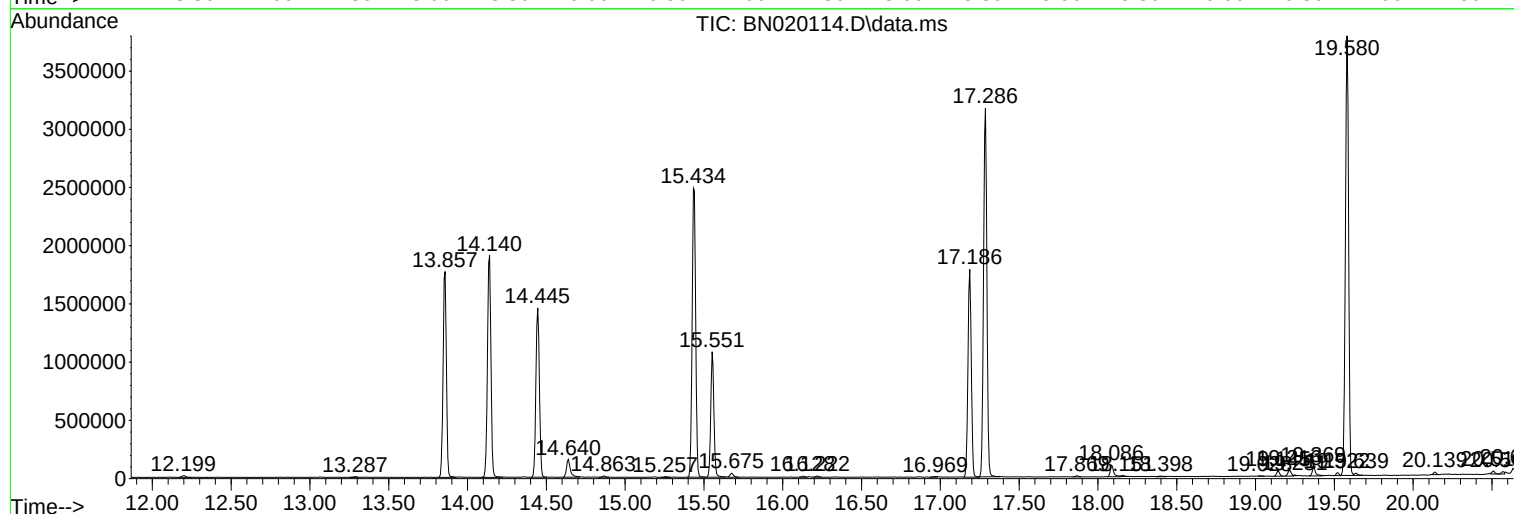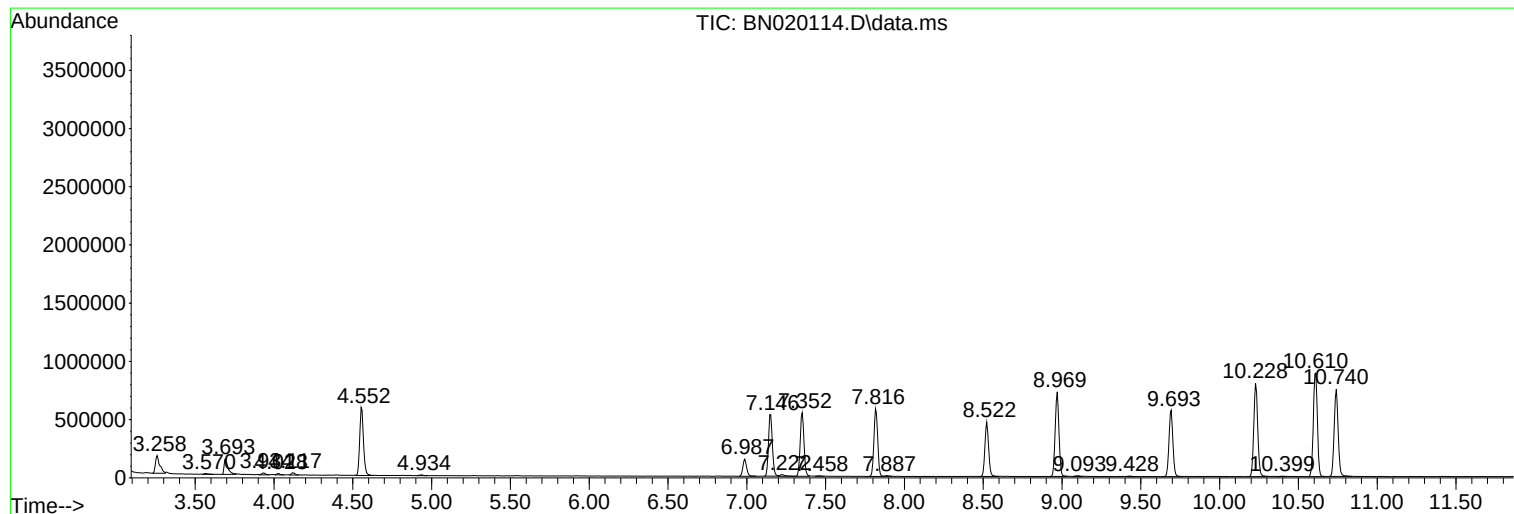

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020114.D
Acq On : 10 Jun 2022 23:58
Operator : CG/JU
Sample : N3250-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020114.D
Acq On : 10 Jun 2022 23:58
Operator : CG/JU
Sample : N3250-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc