

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020116.D
 Acq On : 11 Jun 2022 01:10
 Operator : CG/JU
 Sample : N3250-08
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020116.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	30	33	43	rVB	32316	49494	0.99%	0.107%
2	3.687	99	102	114	rBV2	152263	317356	6.34%	0.686%
3	3.934	139	144	150	rVB2	16372	28607	0.57%	0.062%
4	4.022	156	159	168	rVB	10859	19922	0.40%	0.043%
5	4.558	244	250	258	rVB	65993	111633	2.23%	0.241%
6	4.928	309	313	319	rBV2	7674	12348	0.25%	0.027%
7	5.546	414	418	424	rVB5	3665	7399	0.15%	0.016%
8	6.987	656	663	674	rBV	157192	265671	5.31%	0.575%
9	7.152	682	691	699	rBV	555317	928847	18.57%	2.009%
10	7.228	702	704	709	rVB2	6190	8500	0.17%	0.018%
11	7.352	718	725	737	rBV	570059	939814	18.78%	2.033%
12	7.452	740	742	749	rVB4	4821	7413	0.15%	0.016%
13	7.816	797	804	813	rBV	608618	996867	19.93%	2.156%
14	8.522	916	924	935	rBV	495894	815826	16.31%	1.765%
15	8.969	993	1000	1011	rBV	738962	1237660	24.74%	2.677%
16	9.693	1116	1123	1133	rBV	591848	993578	19.86%	2.149%
17	10.228	1207	1214	1228	rBV	816527	1402782	28.04%	3.034%
18	10.604	1270	1278	1288	rBV	918106	1608088	32.14%	3.479%
19	10.740	1294	1301	1314	rBV	802907	1406076	28.10%	3.042%
20	12.199	1543	1549	1554	rBV3	14972	25253	0.50%	0.055%
21	13.063	1692	1696	1701	rVB5	3169	5478	0.11%	0.012%
22	13.287	1730	1734	1739	rVB4	3508	6130	0.12%	0.013%
23	13.857	1824	1831	1838	rBV	1680705	2419838	48.37%	5.234%
24	14.140	1871	1879	1889	rBV	1883966	2866776	57.30%	6.201%
25	14.445	1924	1931	1943	rBV	1485369	2233454	44.64%	4.831%
26	14.640	1957	1964	1982	rBV	140039	257400	5.14%	0.557%
27	14.863	1999	2002	2007	rBV4	7409	9887	0.20%	0.021%
28	15.257	2064	2069	2074	rVB5	5324	9888	0.20%	0.021%
29	15.434	2092	2099	2111	rBV	2445058	3685828	73.67%	7.973%
30	15.551	2113	2119	2133	rVV	986915	1375708	27.50%	2.976%
31	15.675	2136	2140	2145	rVB	30095	43363	0.87%	0.094%
32	15.998	2190	2195	2202	rVB7	2540	5352	0.11%	0.012%
33	16.216	2229	2232	2239	rVB3	9576	12955	0.26%	0.028%
34	16.969	2355	2360	2364	rBV3	5031	9015	0.18%	0.020%
35	17.186	2390	2397	2406	rBV	1825414	2656480	53.10%	5.746%
36	17.286	2407	2414	2427	rVV	2966801	4443840	88.82%	9.613%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020116.D
 Acq On : 11 Jun 2022 01:10
 Operator : CG/JU
 Sample : N3250-08
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	17.869	2509	2513	2518	rVB5	7417	11874	0.24%	0.026%
38	18.086	2545	2550	2559	rBV2	53239	84124	1.68%	0.182%
39	18.157	2559	2562	2567	rVB2	7576	10412	0.21%	0.023%
40	19.139	2723	2729	2735	rBV3	36979	56605	1.13%	0.122%
41	19.216	2738	2742	2746	rBV2	36052	53309	1.07%	0.115%
42	19.369	2764	2768	2773	rBV3	26517	33131	0.66%	0.072%
43	19.522	2790	2794	2797	rBV2	14286	15445	0.31%	0.033%
44	19.580	2797	2804	2812	rBV	3486035	5003052	100.00%	10.822%
45	20.569	2969	2972	2974	rBV3	11357	16129	0.32%	0.035%
46	20.627	2980	2982	2987	rVB5	6687	8862	0.18%	0.019%
47	21.098	3057	3062	3071	rBV3	59527	125269	2.50%	0.271%
48	21.369	3103	3108	3118	rBV	2024620	2685317	53.67%	5.809%
49	21.986	3210	3213	3215	rBV4	15188	18066	0.36%	0.039%
50	22.469	3292	3295	3300	rVB3	32398	40191	0.80%	0.087%
51	22.998	3381	3385	3390	rBV3	48661	80970	1.62%	0.175%
52	23.551	3470	3479	3486	rBV2	2101628	4202750	84.00%	9.091%
53	23.698	3496	3504	3515	rVB	1144334	2334156	46.65%	5.049%
54	24.298	3601	3606	3613	rVB3	56345	115808	2.31%	0.251%
55	25.098	3738	3742	3750	rVB	51963	109349	2.19%	0.237%




Sum of corrected areas: 46229345

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020116.D
Acq On : 11 Jun 2022 01:10
Operator : CG/JU
Sample : N3250-08
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

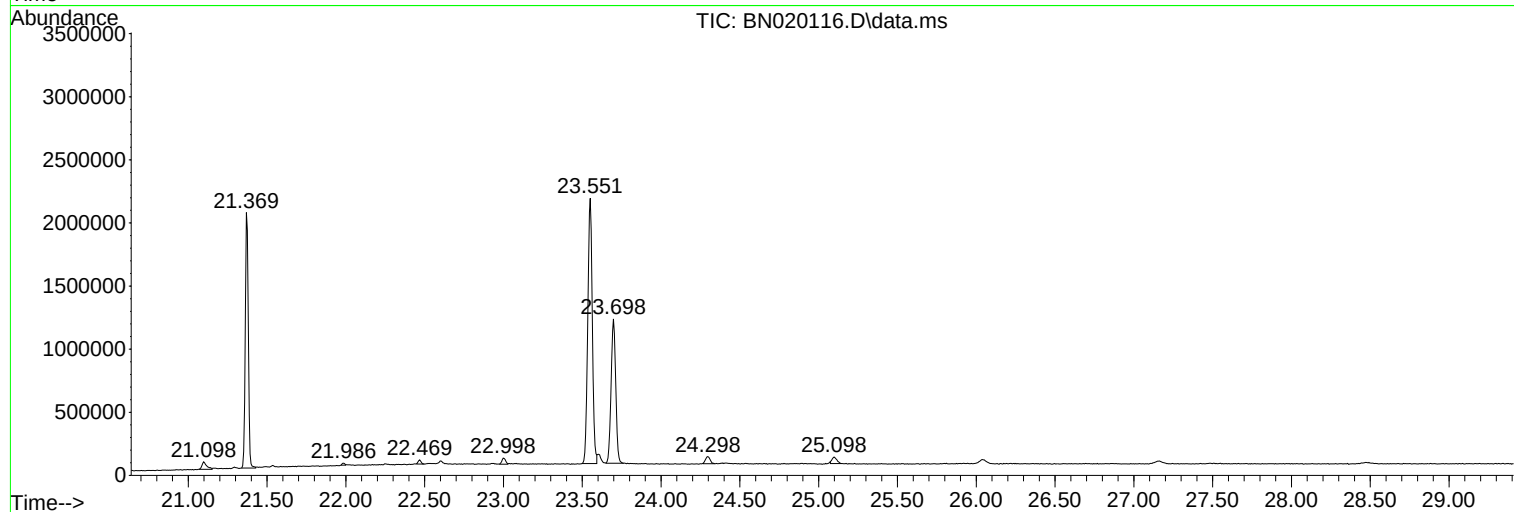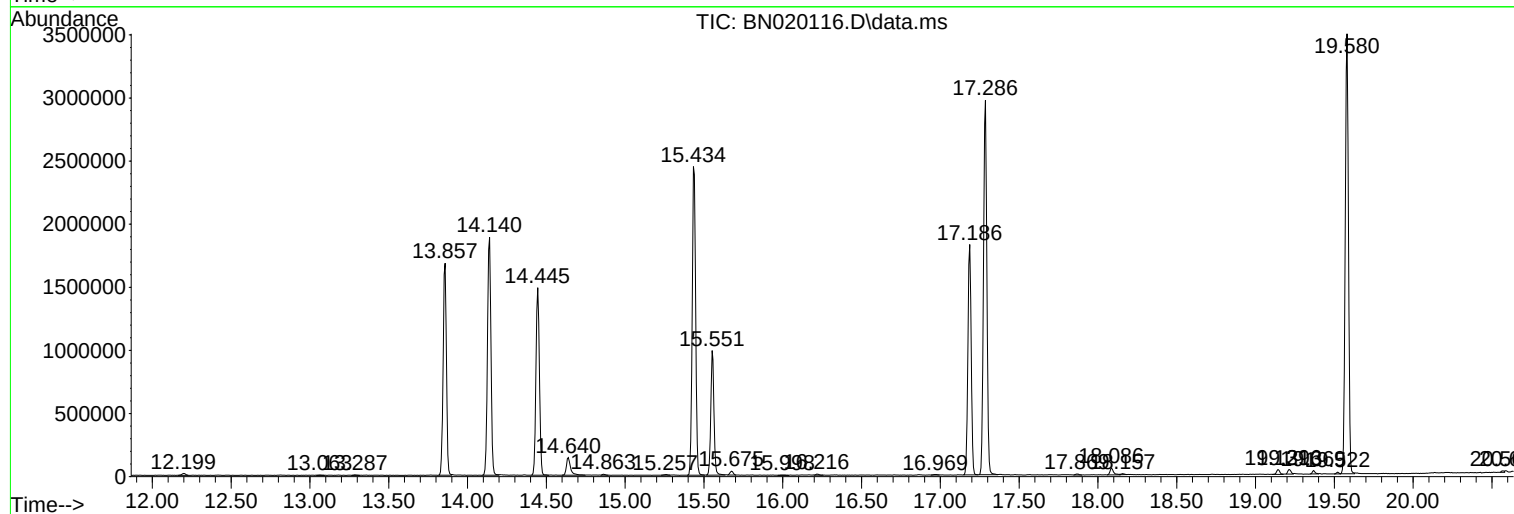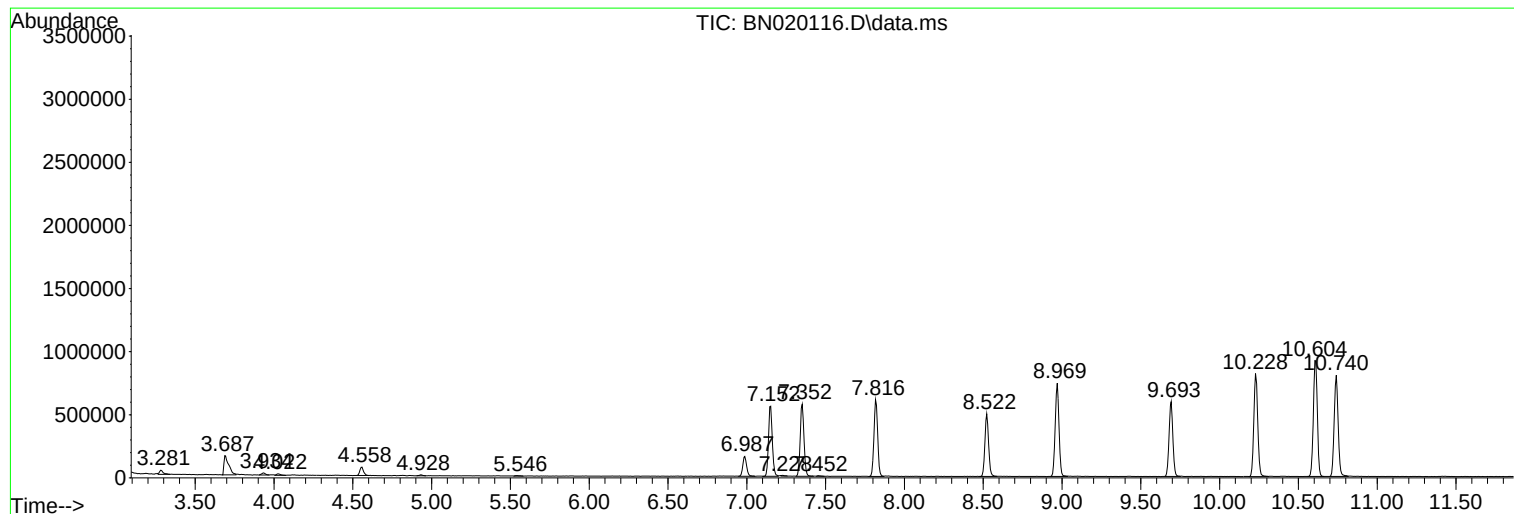

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020116.D
Acq On : 11 Jun 2022 01:10
Operator : CG/JU
Sample : N3250-08
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW6









Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.558	2.24 ng/ul	111633	1,4-Dichlorobenzene-d4	7.816

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	32

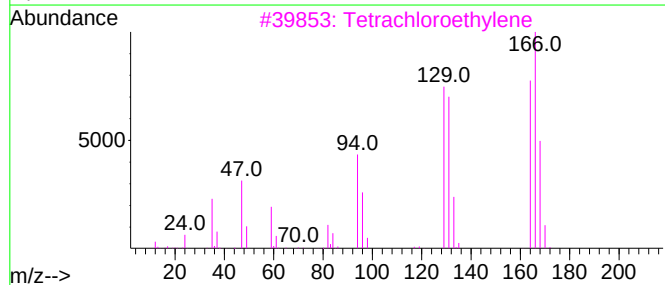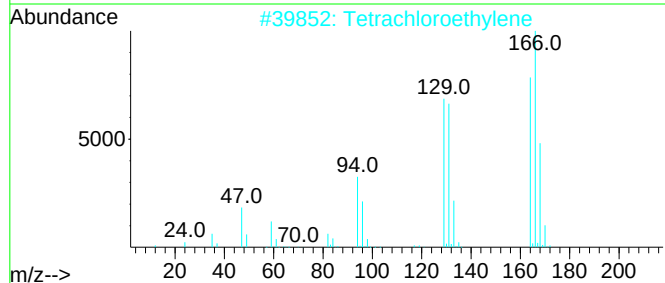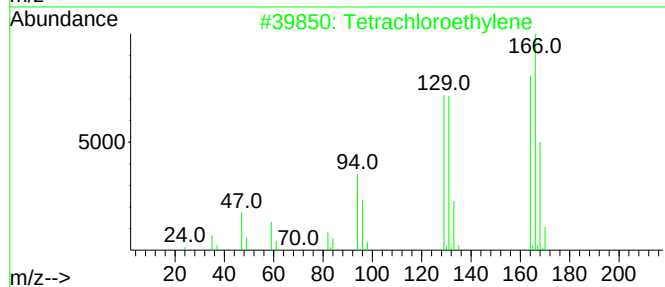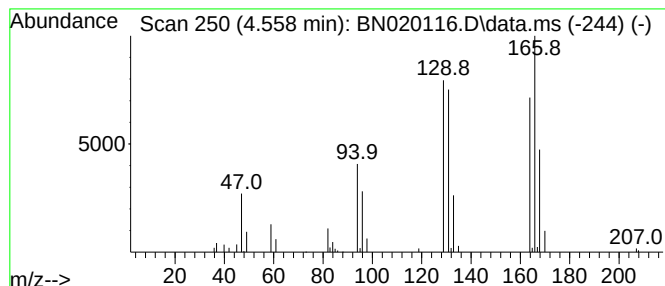

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020116.D
Acq On : 11 Jun 2022 01:10
Operator : CG/JU
Sample : N3250-08
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.558	2.2	ng/u1	111633	1	7.816	996867	20.0