

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020118.D
 Acq On : 11 Jun 2022 02:22
 Operator : CG/JU
 Sample : N3250-13
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020118.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	36	rBV	30799	41919	0.85%	0.086%
2	3.316	36	39	45	rVB	31316	46236	0.93%	0.095%
3	3.693	100	103	117	rBV2	128764	267359	5.39%	0.549%
4	3.928	140	143	150	rVB2	14734	23130	0.47%	0.047%
5	4.028	156	160	166	rVB3	10356	16858	0.34%	0.035%
6	4.934	310	314	321	rVB3	6274	12080	0.24%	0.025%
7	6.987	657	663	674	rBV	128558	218190	4.40%	0.448%
8	7.146	683	690	700	rBV	531194	888529	17.92%	1.823%
9	7.352	717	725	736	rBV	531659	878712	17.72%	1.803%
10	7.816	793	804	813	rBV	577305	947460	19.11%	1.944%
11	7.893	813	817	822	rVB7	5693	8728	0.18%	0.018%
12	8.257	873	879	890	rVB7	10812	28696	0.58%	0.059%
13	8.446	904	911	917	rBV5	5459	9426	0.19%	0.019%
14	8.522	917	924	936	rBV	443323	746824	15.06%	1.532%
15	8.616	936	940	951	rVB8	8690	22053	0.44%	0.045%
16	8.728	951	959	965	rBV5	13974	30003	0.61%	0.062%
17	8.834	971	977	983	rBV4	18961	41081	0.83%	0.084%
18	8.969	992	1000	1008	rBV	718412	1228223	24.77%	2.520%
19	9.193	1034	1038	1045	rVB9	5084	10734	0.22%	0.022%
20	9.587	1101	1105	1110	rVB6	4477	7764	0.16%	0.016%
21	9.693	1115	1123	1132	rBV	572591	988493	19.94%	2.028%
22	10.098	1187	1192	1194	rBV5	4309	7236	0.15%	0.015%
23	10.228	1207	1214	1221	rBV	818682	1410655	28.45%	2.894%
24	10.293	1221	1225	1235	rVV3	34748	79545	1.60%	0.163%
25	10.481	1252	1257	1263	rVB6	9600	20306	0.41%	0.042%
26	10.604	1270	1278	1289	rBV	878994	1538556	31.03%	3.157%
27	10.740	1293	1301	1315	rBV	749743	1331815	26.86%	2.733%
28	10.869	1319	1323	1324	rBV4	6313	8606	0.17%	0.018%
29	11.022	1343	1349	1354	rBV9	4349	9226	0.19%	0.019%
30	11.228	1377	1384	1398	rBV10	30490	94514	1.91%	0.194%
31	11.416	1411	1416	1420	rBV7	14457	28928	0.58%	0.059%
32	11.510	1428	1432	1436	rBV4	8100	12523	0.25%	0.026%
33	11.581	1439	1444	1448	rVV7	14958	27938	0.56%	0.057%
34	11.634	1448	1453	1461	rVB4	27908	55814	1.13%	0.115%
35	11.745	1466	1472	1476	rVB5	15434	24867	0.50%	0.051%
36	11.863	1481	1492	1498	rBV10	20097	69113	1.39%	0.142%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020118.D
 Acq On : 11 Jun 2022 02:22
 Operator : CG/JU
 Sample : N3250-13
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	11.928	1498	1503	1507	rVV4	19762	38424	0.77%	0.079%
38	11.975	1507	1511	1520	rVB8	24094	60988	1.23%	0.125%
39	12.063	1520	1526	1531	rBV3	20558	36142	0.73%	0.074%
40	12.192	1545	1548	1555	rVB	13507	20194	0.41%	0.041%
41	12.410	1579	1585	1589	rBV8	4053	7296	0.15%	0.015%
42	12.487	1594	1598	1603	rBV6	9515	14438	0.29%	0.030%
43	12.598	1611	1617	1624	rBV4	19560	39633	0.80%	0.081%
44	13.022	1682	1689	1694	rVB	25723	46934	0.95%	0.096%
45	13.169	1710	1714	1721	rVB8	7538	13762	0.28%	0.028%
46	13.287	1730	1734	1741	rBV4	9327	15464	0.31%	0.032%
47	13.445	1758	1761	1770	rVB5	14158	30739	0.62%	0.063%
48	13.651	1790	1796	1801	rBV8	6645	13802	0.28%	0.028%
49	13.734	1804	1810	1817	rBV9	8990	21704	0.44%	0.045%
50	13.857	1824	1831	1837	rBV	1782664	2512344	50.67%	5.155%
51	13.987	1848	1853	1858	rVB6	6463	13332	0.27%	0.027%
52	14.139	1870	1879	1886	rBV	1858966	2887989	58.24%	5.926%
53	14.210	1888	1891	1897	rVB2	19510	31623	0.64%	0.065%
54	14.363	1910	1917	1920	rBV3	18305	28730	0.58%	0.059%
55	14.445	1924	1931	1940	rVV	1447110	2136539	43.09%	4.384%
56	14.522	1940	1944	1948	rVV2	19554	31823	0.64%	0.065%
57	14.575	1948	1953	1957	rVV	26987	51868	1.05%	0.106%
58	14.639	1957	1964	1980	rVB2	156914	309901	6.25%	0.636%
59	14.804	1986	1992	1998	rVB2	6007	10645	0.21%	0.022%
60	14.863	1998	2002	2007	rBV7	12848	18896	0.38%	0.039%
61	14.975	2015	2021	2024	rBV7	11131	17881	0.36%	0.037%
62	15.069	2027	2037	2046	rBV3	29004	60784	1.23%	0.125%
63	15.257	2064	2069	2073	rBV7	6040	10024	0.20%	0.021%
64	15.310	2073	2078	2084	rVB	30455	41053	0.83%	0.084%
65	15.439	2091	2100	2109	rBV	2416485	3717559	74.97%	7.628%
66	15.551	2113	2119	2132	rBV	1032272	1465632	29.56%	3.007%
67	15.675	2134	2140	2145	rBV3	30707	54722	1.10%	0.112%
68	15.816	2159	2164	2169	rBV7	6521	14034	0.28%	0.029%
69	15.945	2179	2186	2191	rBV3	21046	37326	0.75%	0.077%
70	16.169	2220	2224	2227	rBV	50707	70648	1.42%	0.145%
71	16.457	2269	2273	2276	rVB3	8439	12742	0.26%	0.026%
72	16.575	2291	2293	2299	rVB6	8029	7578	0.15%	0.016%
73	16.957	2354	2358	2363	rBV3	51378	71645	1.44%	0.147%
74	17.016	2365	2368	2373	rVB3	22444	30015	0.61%	0.062%
75	17.186	2390	2397	2406	rBV	1690280	2540254	51.23%	5.212%
76	17.286	2407	2414	2425	rVV2	2851703	4328259	87.29%	8.881%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020118.D
 Acq On : 11 Jun 2022 02:22
 Operator : CG/JU
 Sample : N3250-13
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYZ3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

77	17.563	2458	2461	2466	rBV	23128	31197	0.63%	0.064%
78	17.698	2481	2484	2488	rVB	52012	62126	1.25%	0.127%
79	18.086	2546	2550	2557	rBV	129573	193074	3.89%	0.396%
80	18.392	2598	2602	2610	rBV	48651	64134	1.29%	0.132%
81	19.022	2706	2709	2714	rBV	44444	61373	1.24%	0.126%
82	19.139	2726	2729	2734	rVB2	43939	58916	1.19%	0.121%
83	19.216	2738	2742	2745	rBV	42251	58077	1.17%	0.119%
84	19.369	2764	2768	2779	rBV	105480	183007	3.69%	0.376%
85	19.522	2791	2794	2797	rVB4	22947	25174	0.51%	0.052%
86	19.580	2797	2804	2811	rBV	3492493	4958495	100.00%	10.174%
87	20.133	2896	2898	2902	rVB	32471	34010	0.69%	0.070%
88	20.633	2980	2983	2986	rVB	35508	38739	0.78%	0.079%
89	21.098	3058	3062	3072	rVB	65289	105684	2.13%	0.217%
90	21.368	3103	3108	3117	rBV	1942088	2569491	51.82%	5.272%
91	21.533	3133	3136	3140	rVB	52255	54888	1.11%	0.113%
92	21.980	3209	3212	3217	rBV	55476	72268	1.46%	0.148%
93	22.468	3290	3295	3301	rBV	332980	486490	9.81%	0.998%
94	22.998	3381	3385	3393	rVB	114219	180605	3.64%	0.371%
95	23.551	3470	3479	3485	rBV2	2080604	4260000	85.91%	8.741%
96	23.598	3485	3487	3496	rVV	147490	271949	5.48%	0.558%
97	23.698	3496	3504	3515	rVB2	1128133	2293364	46.25%	4.706%
98	24.292	3600	3605	3614	rVB	113709	241664	4.87%	0.496%
99	25.098	3737	3742	3752	rVB2	96822	220463	4.45%	0.452%
100	26.039	3897	3902	3914	rVB2	59444	155984	3.15%	0.320%




Sum of corrected areas: 48736678

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020118.D
Acq On : 11 Jun 2022 02:22
Operator : CG/JU
Sample : N3250-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYZ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

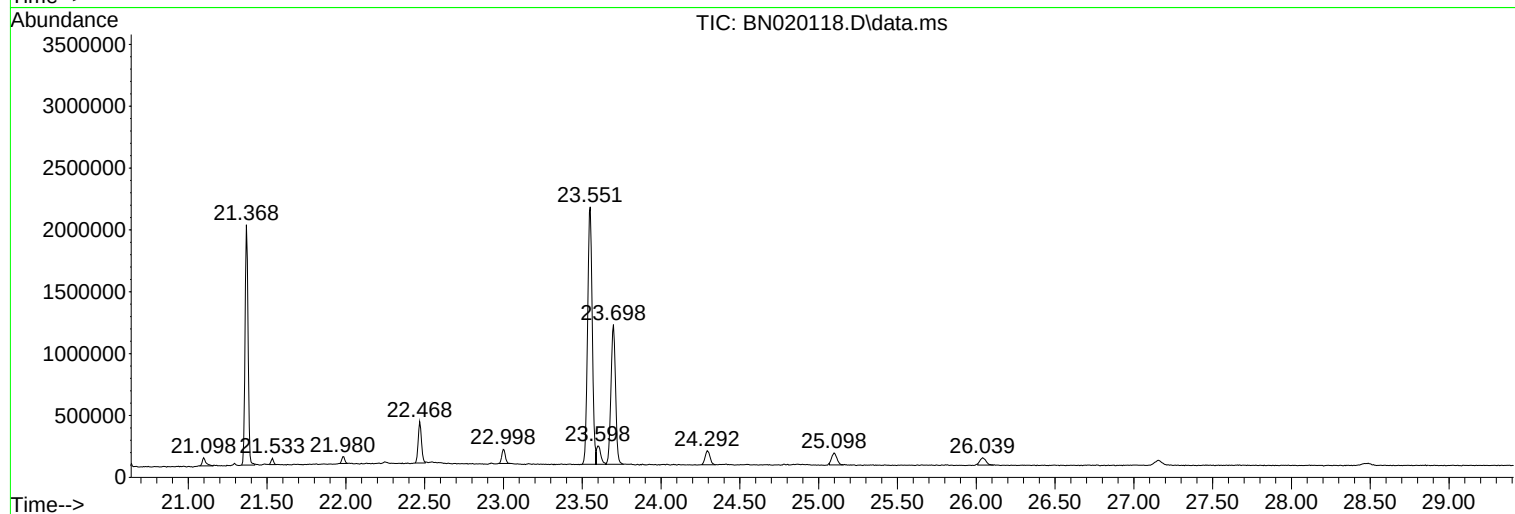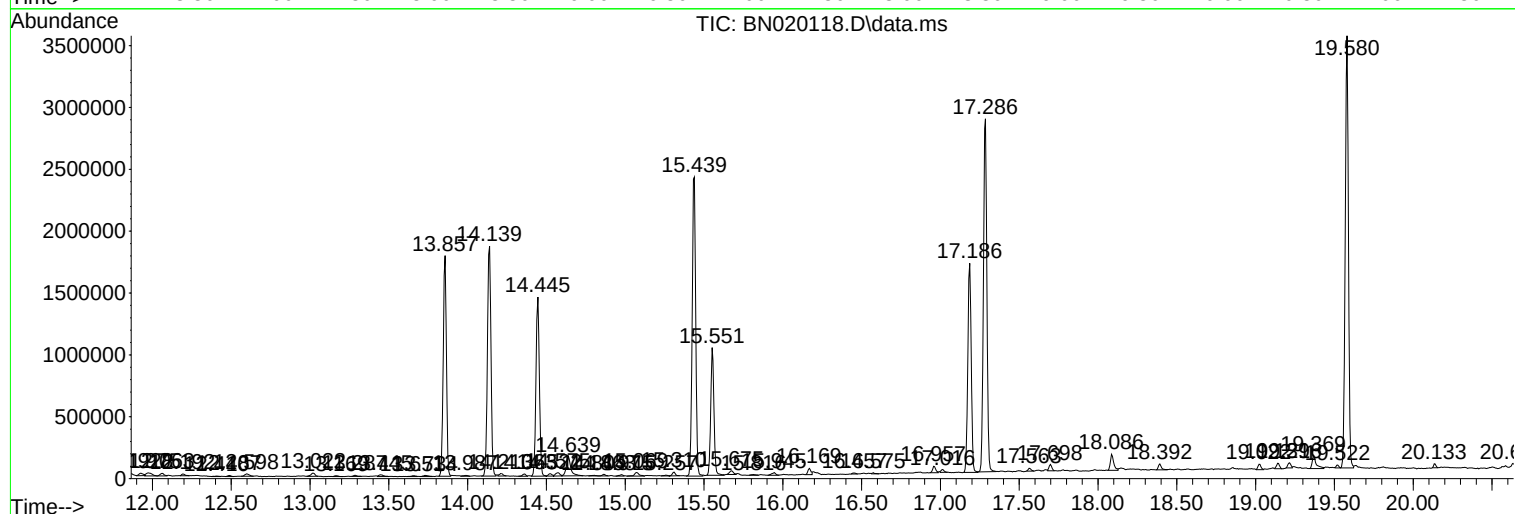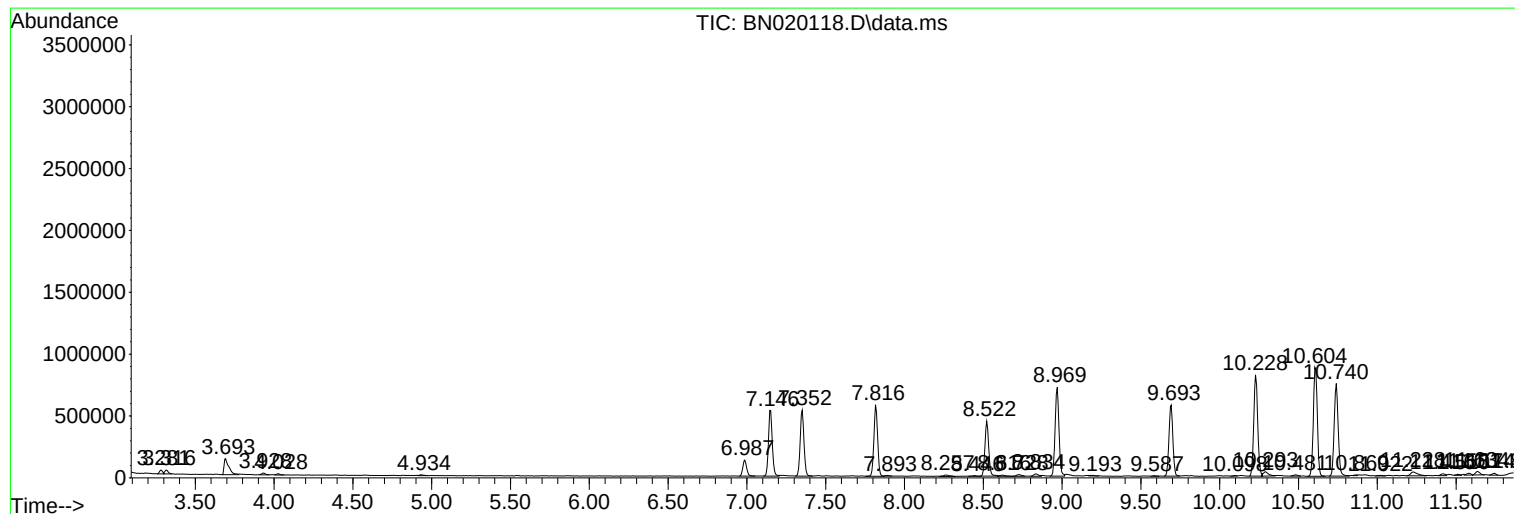

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020118.D
Acq On : 11 Jun 2022 02:22
Operator : CG/JU
Sample : N3250-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYZ3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Decanedioic acid, bis(2-eth... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
22.468	3.79 ng/ul	486490	Chrysene-d12	21.368

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Decanedioic acid, bis(2-ethylhex...	426	C26H50O4	000122-62-3	62
2			Decanedioic acid, bis(2-ethylhex...	426	C26H50O4	000122-62-3	62
3			Sebacic acid, isobutyl 2-methylp...	342	C20H38O4	1000355-45-0	46
4			Sebacic acid, isobutyl 4-methylp...	342	C20H38O4	1010355-34-9	43
5			Sebacic acid, isobutyl 3-methylb...	328	C19H36O4	1000355-55-9	38

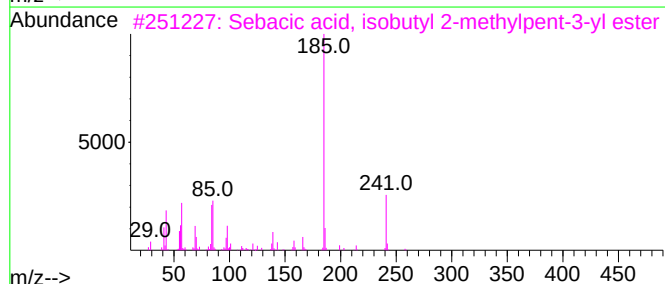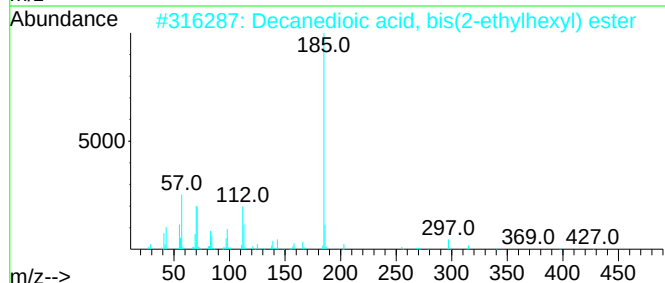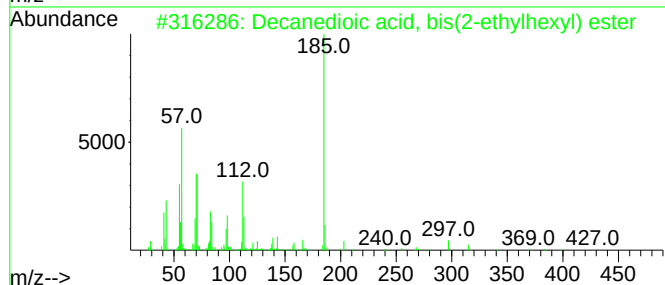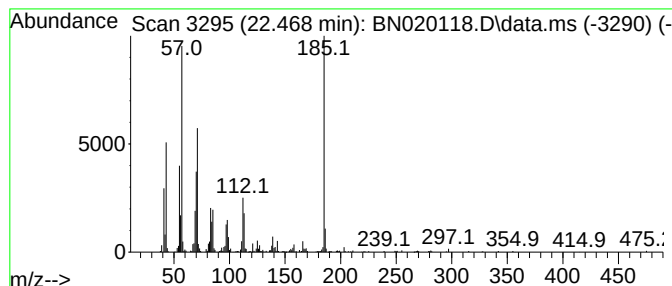

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020118.D
Acq On : 11 Jun 2022 02:22
Operator : CG/JU
Sample : N3250-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYZ3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
24.292	2.11 ng/ul	241664	Perylene-d12	23.698

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Heneicosane	296	C21H44	000629-94-7	95
2		Heneicosane	296	C21H44	000629-94-7	93
3		Hexacosane	366	C26H54	000630-01-3	93
4		Heneicosane	296	C21H44	000629-94-7	90
5		Octacosane	394	C28H58	000630-02-4	90

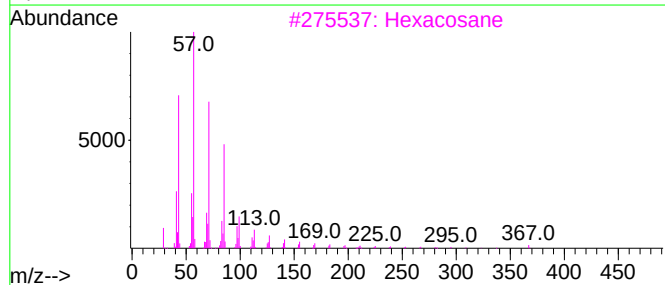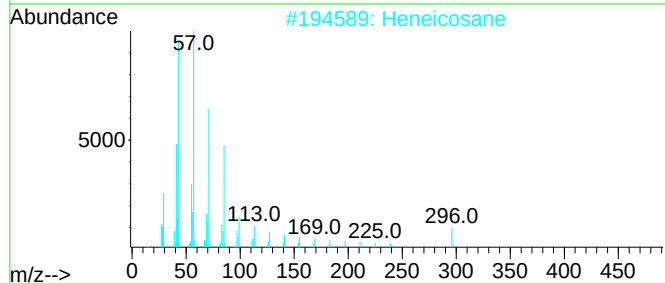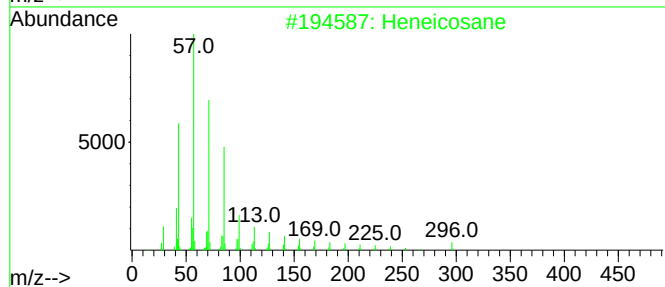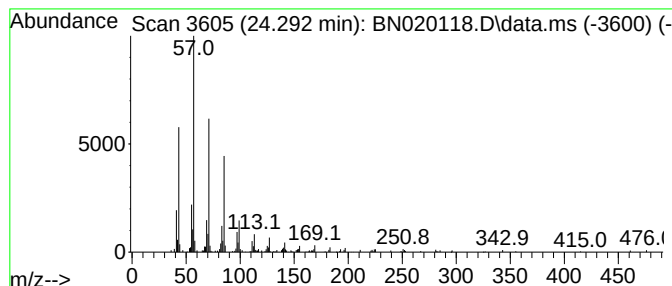

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020118.D
Acq On : 11 Jun 2022 02:22
Operator : CG/JU
Sample : N3250-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYZ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Decanedioic aci...	22.468	3.8	ng/ul	486490	5	21.368	2569490	20.0
(DEL) Alkane: S...	24.292	2.1	ng/ul	241664	6	23.698	2293360	20.0