

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020121.D
 Acq On : 11 Jun 2022 04:10
 Operator : CG/JU
 Sample : N3250-10
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYS6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020121.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	30	33	40	rVB	34517	48526	0.93%	0.099%
2	3.693	100	103	113	rBV	77836	129265	2.47%	0.264%
3	3.934	140	144	151	rVB2	17221	27357	0.52%	0.056%
4	4.028	156	160	166	rVB2	12002	17628	0.34%	0.036%
5	4.393	216	222	228	rVB8	6833	15577	0.30%	0.032%
6	4.934	310	314	321	rVB6	5134	8259	0.16%	0.017%
7	6.987	656	663	674	rBV	149351	248344	4.75%	0.507%
8	7.152	684	691	701	rBV	620641	1043619	19.97%	2.131%
9	7.352	718	725	734	rBV	614760	1015849	19.44%	2.074%
10	7.816	797	804	813	rBV	683217	1125608	21.54%	2.298%
11	8.522	917	924	936	rBV	489458	803310	15.37%	1.640%
12	8.728	953	959	966	rVB3	4491	7774	0.15%	0.016%
13	8.969	990	1000	1008	rBV	842201	1396495	26.73%	2.851%
14	9.146	1026	1030	1037	rVB5	9943	16328	0.31%	0.033%
15	9.693	1115	1123	1135	rBV	659160	1129401	21.62%	2.306%
16	10.228	1207	1214	1229	rBV	893390	1539593	29.47%	3.143%
17	10.604	1271	1278	1290	rVB	1013115	1776821	34.01%	3.628%
18	10.740	1293	1301	1313	rVV	775994	1378601	26.38%	2.815%
19	10.840	1316	1318	1324	rVB5	3782	5955	0.11%	0.012%
20	10.981	1338	1342	1347	rBV5	4955	9166	0.18%	0.019%
21	12.004	1511	1516	1524	rBV4	3628	5530	0.11%	0.011%
22	12.198	1543	1549	1555	rBV	17296	27958	0.54%	0.057%
23	13.857	1824	1831	1843	rBV	1903389	2697557	51.63%	5.508%
24	14.087	1865	1870	1873	rBV	81507	117807	2.25%	0.241%
25	14.139	1873	1879	1890	rVB	2050808	3223328	61.69%	6.581%
26	14.445	1924	1931	1940	rBV	1627031	2426700	46.44%	4.955%
27	14.639	1958	1964	1978	rBV	123089	220176	4.21%	0.450%
28	14.863	1998	2002	2007	rVB5	5206	7299	0.14%	0.015%
29	15.134	2042	2048	2053	rBV3	8084	13397	0.26%	0.027%
30	15.186	2053	2057	2064	rVB	32198	43306	0.83%	0.088%
31	15.257	2064	2069	2073	rBV5	5338	8446	0.16%	0.017%
32	15.439	2092	2100	2107	rBV	2573330	4031463	77.16%	8.231%
33	15.551	2113	2119	2131	rBV	1009862	1409722	26.98%	2.878%
34	15.675	2135	2140	2145	rVB2	34170	50389	0.96%	0.103%
35	15.998	2192	2195	2199	rBV5	4034	6736	0.13%	0.014%
36	16.222	2225	2233	2238	rVB3	10156	17014	0.33%	0.035%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020121.D
 Acq On : 11 Jun 2022 04:10
 Operator : CG/JU
 Sample : N3250-10
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYS6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	16.869	2339	2343	2347	rBV4	3881	5545	0.11%	0.011%
38	16.969	2353	2360	2364	rBV3	4876	9276	0.18%	0.019%
39	17.186	2390	2397	2406	rBV	1934515	2840234	54.36%	5.799%
40	17.286	2407	2414	2428	rVV	3213041	4775117	91.39%	9.750%
41	17.863	2509	2512	2517	rVB4	5327	5938	0.11%	0.012%
42	18.027	2535	2540	2545	rBV5	9558	12630	0.24%	0.026%
43	18.086	2545	2550	2557	rVV2	26031	39978	0.77%	0.082%
44	18.157	2560	2562	2568	rVB5	3870	5484	0.10%	0.011%
45	18.339	2589	2593	2599	rVB7	7562	10594	0.20%	0.022%
46	19.145	2725	2730	2735	rBV	39262	55335	1.06%	0.113%
47	19.216	2737	2742	2748	rBV	37535	55091	1.05%	0.112%
48	19.369	2764	2768	2774	rBV6	16050	24293	0.46%	0.050%
49	19.522	2790	2794	2797	rBV2	16350	19431	0.37%	0.040%
50	19.580	2797	2804	2812	rBV	3716671	5224989	100.00%	10.668%
51	20.139	2896	2899	2902	rBV4	5404	6473	0.12%	0.013%
52	20.504	2959	2961	2965	rBV4	8793	10501	0.20%	0.021%
53	20.592	2969	2976	2980	rBV5	19202	37505	0.72%	0.077%
54	20.633	2981	2983	2986	rVB3	9926	10818	0.21%	0.022%
55	21.374	3103	3109	3118	rBV	2046858	2691091	51.50%	5.494%
56	21.539	3134	3137	3140	rVB	16979	18228	0.35%	0.037%
57	21.986	3210	3213	3217	rVB2	29316	34849	0.67%	0.071%
58	22.468	3291	3295	3301	rVB	51088	68283	1.31%	0.139%
59	22.533	3302	3306	3312	rVB	74683	100140	1.92%	0.204%
60	23.004	3382	3386	3391	rVB	74909	110165	2.11%	0.225%
61	23.551	3471	3479	3486	rBV2	2022213	4007293	76.69%	8.182%
62	23.698	3497	3504	3521	rVB2	1127936	2271790	43.48%	4.638%
63	24.298	3601	3606	3613	rVB	87897	172903	3.31%	0.353%
64	25.098	3737	3742	3751	rVB2	78780	180598	3.46%	0.369%
65	26.045	3898	3903	3912	rVB2	49426	123191	2.36%	0.252%




Sum of corrected areas: 48978067

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020121.D
Acq On : 11 Jun 2022 04:10
Operator : CG/JU
Sample : N3250-10
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYS6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

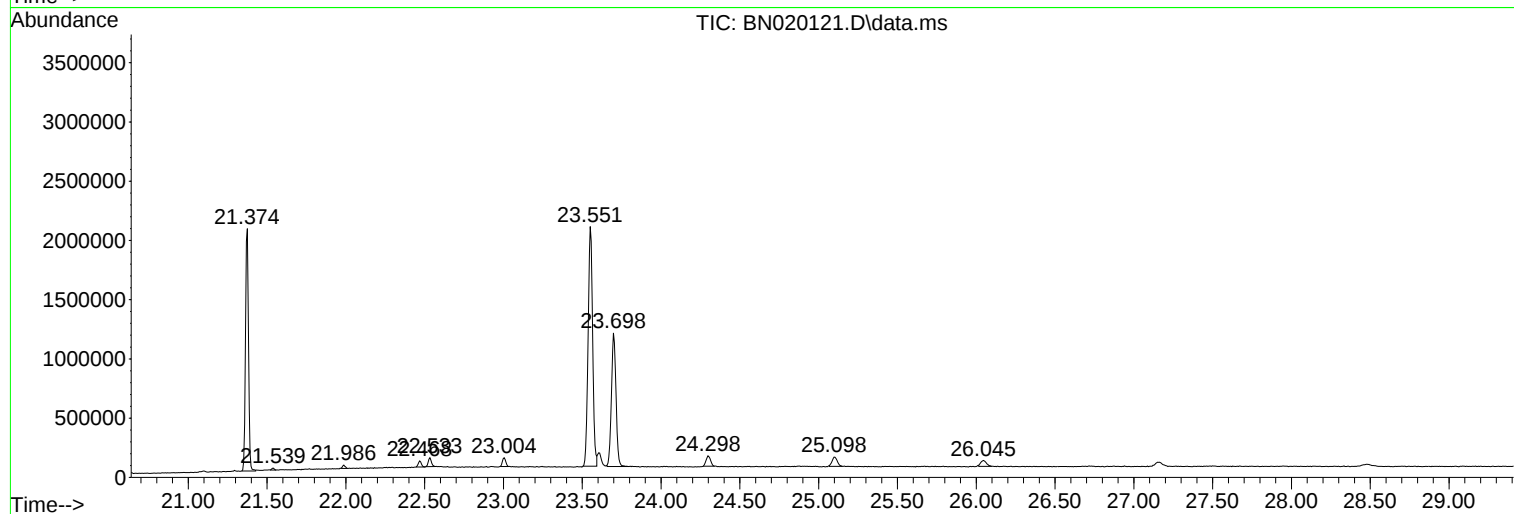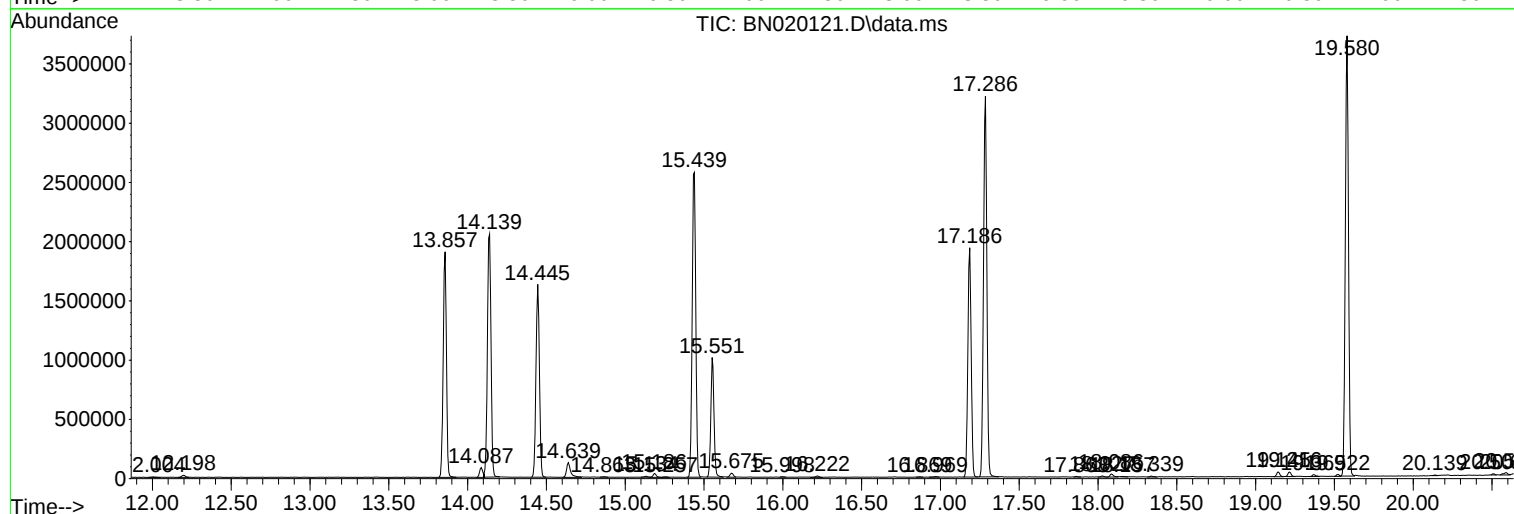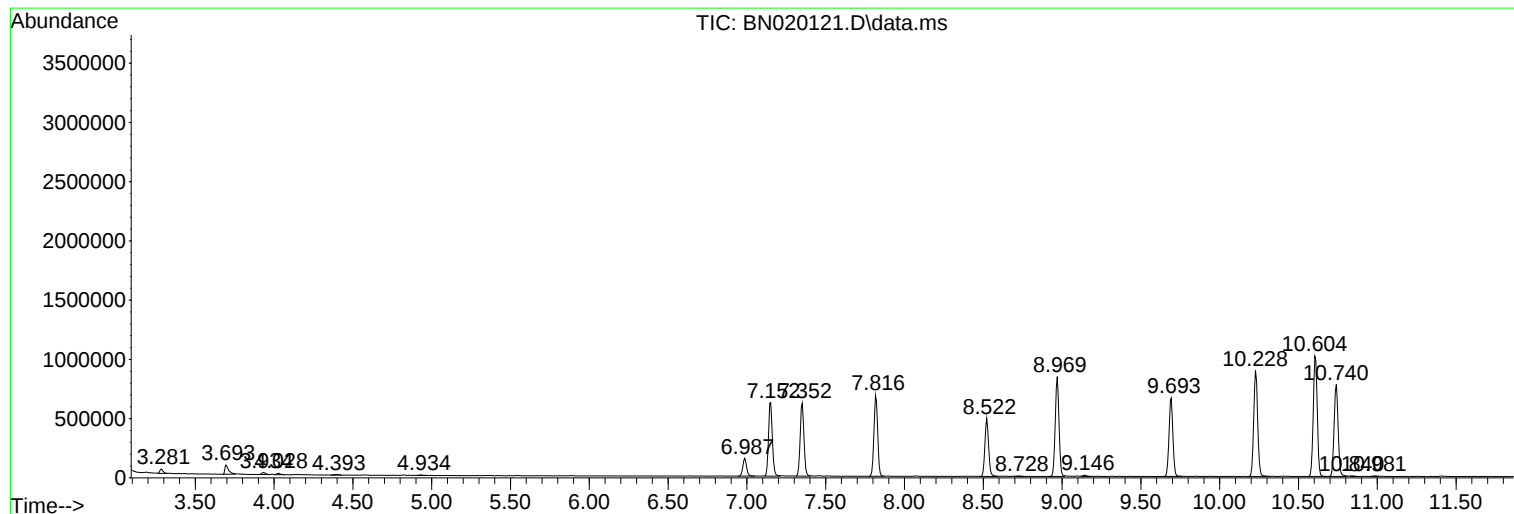

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020121.D
Acq On : 11 Jun 2022 04:10
Operator : CG/JU
Sample : N3250-10
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYS6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020121.D
Acq On : 11 Jun 2022 04:10
Operator : CG/JU
Sample : N3250-10
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYS6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc