

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020127.D
 Acq On : 11 Jun 2022 08:20
 Operator : CG/JU
 Sample : PB145456BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK456

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020127.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	40	rVB	36804	53253	1.32%	0.125%
2	3.681	98	101	119	rBV	505331	851385	21.10%	1.999%
3	4.028	157	160	165	rVB	8702	12042	0.30%	0.028%
4	6.981	655	662	678	rVB	626501	1019652	25.27%	2.394%
5	7.146	684	690	702	rBV	499172	811872	20.12%	1.906%
6	7.352	718	725	736	rBV	621080	1055023	26.15%	2.477%
7	7.816	796	804	813	rBV	519878	864581	21.43%	2.030%
8	8.522	916	924	936	rBV	823617	1367474	33.89%	3.211%
9	8.969	992	1000	1013	rBV	647247	1082856	26.84%	2.542%
10	9.687	1115	1122	1137	rBV	537104	923002	22.88%	2.167%
11	10.228	1205	1214	1228	rBV	784071	1352249	33.51%	3.175%
12	10.605	1270	1278	1287	rBV	804353	1383239	34.28%	3.248%
13	10.740	1293	1301	1316	rBV	844414	1533614	38.01%	3.601%
14	12.199	1542	1549	1555	rBV2	13695	23509	0.58%	0.055%
15	13.851	1824	1830	1840	rBV	1541151	2233978	55.37%	5.245%
16	14.134	1871	1878	1889	rBV	1677263	2529322	62.69%	5.939%
17	14.445	1924	1931	1938	rBV	1240678	1934312	47.94%	4.542%
18	14.634	1957	1963	1979	rBV	714930	1103147	27.34%	2.590%
19	15.434	2092	2099	2108	rBV	2168732	3204741	79.43%	7.524%
20	15.551	2113	2119	2134	rVV	719296	1016253	25.19%	2.386%
21	15.675	2134	2140	2145	rVB2	24891	37151	0.92%	0.087%
22	16.216	2228	2232	2238	rVB2	7289	10037	0.25%	0.024%
23	16.969	2356	2360	2365	rBV5	3876	6467	0.16%	0.015%
24	17.181	2390	2396	2406	rBV	1526914	2331856	57.79%	5.475%
25	17.281	2406	2413	2425	rBV2	2433315	3604282	89.33%	8.462%
26	17.775	2493	2497	2502	rBV3	2196	4501	0.11%	0.011%
27	17.863	2507	2512	2515	rBV3	2972	4752	0.12%	0.011%
28	18.098	2546	2552	2553	rBV5	2313	4456	0.11%	0.010%
29	18.733	2652	2660	2663	rBV6	2610	6633	0.16%	0.016%
30	19.145	2724	2730	2734	rVB2	27539	37708	0.93%	0.089%
31	19.216	2737	2742	2747	rBV	26494	37851	0.94%	0.089%
32	19.522	2791	2794	2797	rVB3	6221	5788	0.14%	0.014%
33	19.575	2797	2803	2812	rBV	2789877	4034839	100.00%	9.473%
34	20.586	2971	2975	2980	rBV5	7775	11223	0.28%	0.026%
35	21.375	3103	3109	3119	rBV	1819495	2386750	59.15%	5.604%
36	22.998	3382	3385	3392	rVB	36852	59677	1.48%	0.140%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020127.D
Acq On : 11 Jun 2022 08:20
Operator : CG/JU
Sample : PB145456BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK456

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Title : SVOA CALIBRATION

37	23.551	3471	3479	3486	rBV2	1612229	3386673	83.94%	7.952%
38	23.698	3496	3504	3521	rVB2	1007852	2045246	50.69%	4.802%
39	24.298	3600	3606	3614	rVB	52296	102550	2.54%	0.241%
40	25.104	3737	3743	3750	rVB3	50799	117583	2.91%	0.276%




Sum of corrected areas: 42591527

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020127.D
Acq On : 11 Jun 2022 08:20
Operator : CG/JU
Sample : PB145456BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK456

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

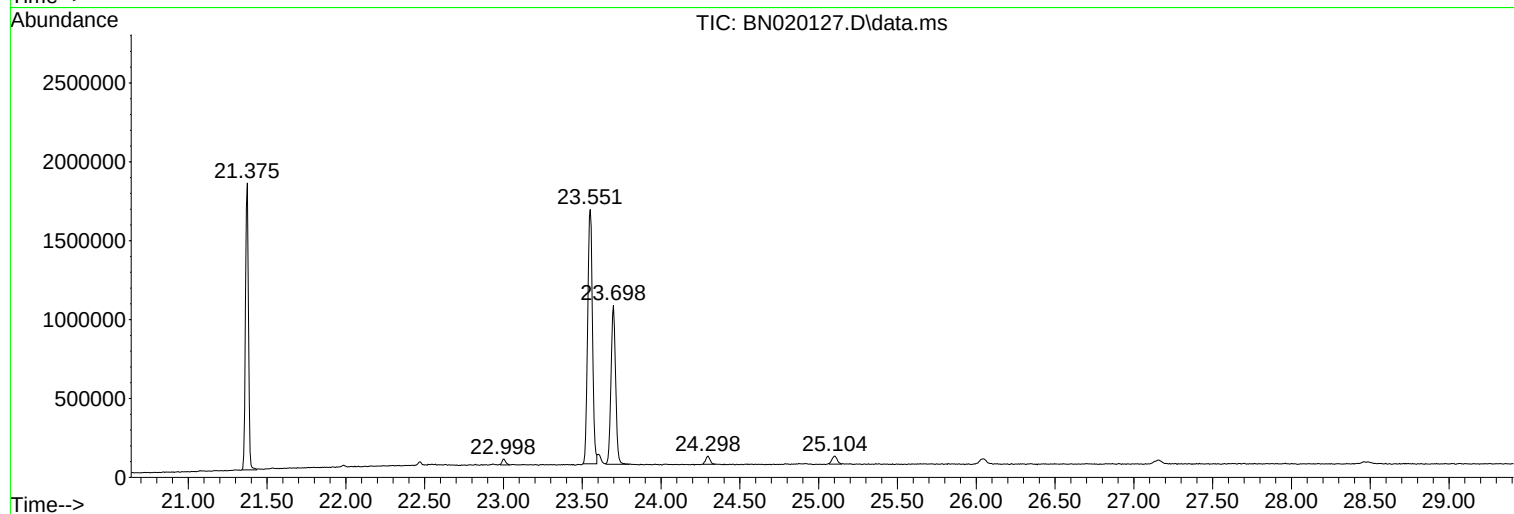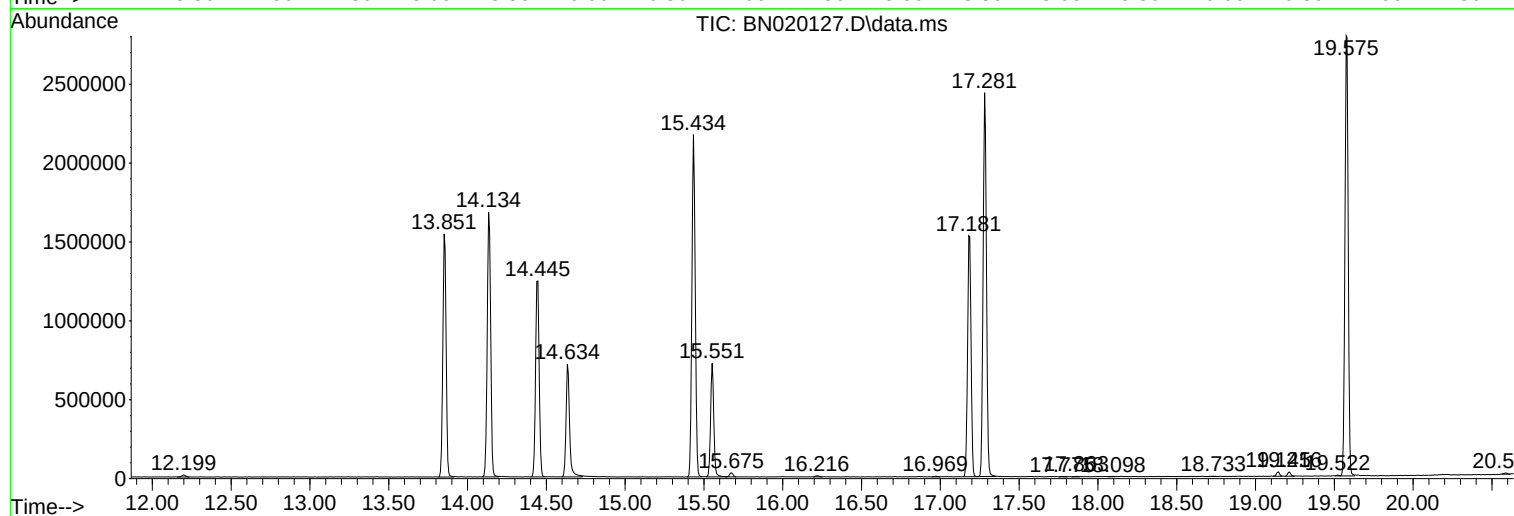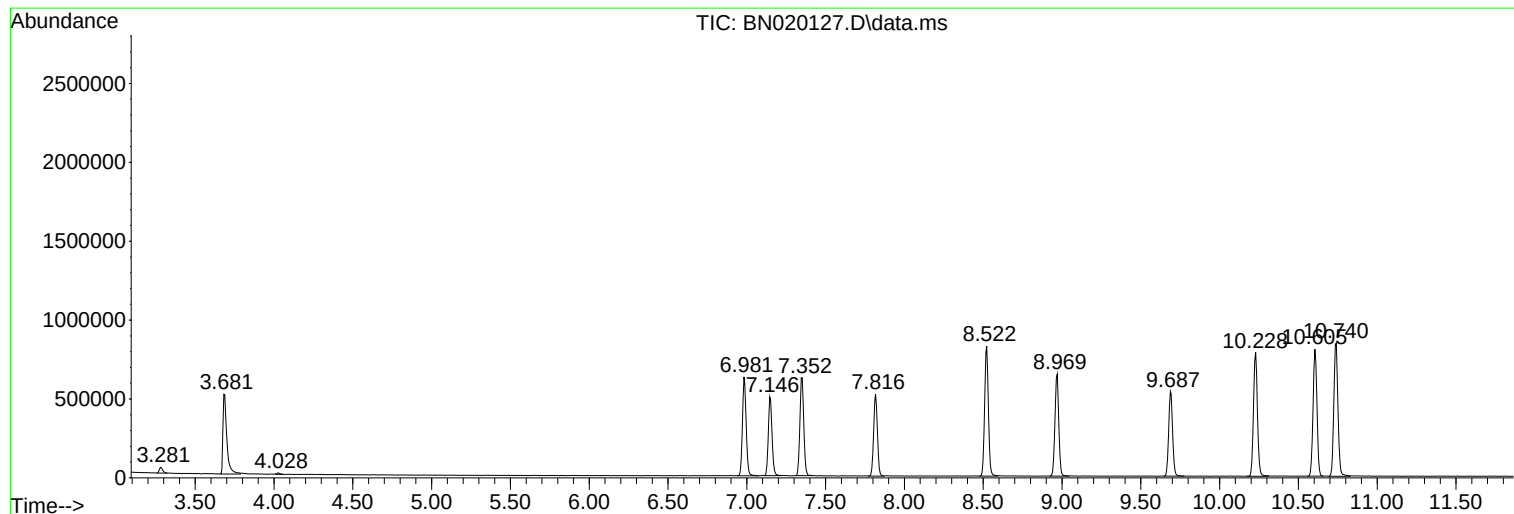

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020127.D
Acq On : 11 Jun 2022 08:20
Operator : CG/JU
Sample : PB145456BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK456

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020127.D
Acq On : 11 Jun 2022 08:20
Operator : CG/JU
Sample : PB145456BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK456

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------