

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020130.D
 Acq On : 11 Jun 2022 10:07
 Operator : CG/JU
 Sample : N3284-01
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020130.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	35	rBV	33897	42125	0.85%	0.093%
2	3.317	35	39	50	rVB	110807	170552	3.43%	0.375%
3	3.693	99	103	118	rBV	111128	201322	4.05%	0.442%
4	3.928	139	143	150	rVB	16961	30256	0.61%	0.066%
5	4.023	157	159	164	rVB2	9964	10806	0.22%	0.024%
6	4.393	218	222	226	rBV5	3362	5350	0.11%	0.012%
7	4.928	309	313	318	rBV2	6673	10154	0.20%	0.022%
8	6.987	656	663	672	rBV	137278	233310	4.70%	0.513%
9	7.146	682	690	703	rBV	538543	885848	17.84%	1.946%
10	7.346	717	724	738	rVB	518296	885770	17.83%	1.946%
11	7.816	797	804	814	rBV	562892	911155	18.35%	2.002%
12	7.893	814	817	825	rVB5	3542	5811	0.12%	0.013%
13	8.522	916	924	935	rBV	436821	751098	15.12%	1.650%
14	8.969	992	1000	1012	rBV	693542	1191006	23.98%	2.617%
15	9.422	1072	1077	1083	rBV3	4341	8092	0.16%	0.018%
16	9.687	1115	1122	1135	rBV	569975	978730	19.71%	2.150%
17	10.228	1206	1214	1232	rBV	795324	1364295	27.47%	2.998%
18	10.605	1270	1278	1287	rBV	842234	1482185	29.84%	3.257%
19	10.740	1292	1301	1320	rBV	754177	1376120	27.71%	3.024%
20	12.199	1540	1549	1556	rBV2	14239	25822	0.52%	0.057%
21	13.287	1729	1734	1739	rVB2	4993	7478	0.15%	0.016%
22	13.851	1824	1830	1846	rBV	1719550	2456210	49.45%	5.397%
23	14.134	1870	1878	1892	rBV	1841960	2791616	56.21%	6.134%
24	14.446	1924	1931	1943	rVB	1316542	2065088	41.58%	4.537%
25	14.634	1958	1963	1978	rBV	131073	239296	4.82%	0.526%
26	14.863	1996	2002	2007	rBV6	8315	12967	0.26%	0.028%
27	15.251	2063	2068	2074	rVB3	6591	12113	0.24%	0.027%
28	15.434	2092	2099	2112	rBV	2479528	3720797	74.91%	8.175%
29	15.551	2112	2119	2130	rBV	973197	1361899	27.42%	2.992%
30	15.675	2135	2140	2147	rVB2	30956	46634	0.94%	0.102%
31	16.222	2228	2233	2239	rVB6	9219	14557	0.29%	0.032%
32	16.869	2338	2343	2345	rBV5	3498	5288	0.11%	0.012%
33	16.969	2355	2360	2365	rBV5	4631	10532	0.21%	0.023%
34	17.181	2390	2396	2403	rBV	1672979	2473142	49.79%	5.434%
35	17.281	2406	2413	2427	rVV	2979976	4393277	88.45%	9.653%
36	17.375	2427	2429	2435	rVB5	4497	5274	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020130.D
 Acq On : 11 Jun 2022 10:07
 Operator : CG/JU
 Sample : N3284-01
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	17.775	2493	2497	2500	rBV5	3732	5840	0.12%	0.013%
38	17.863	2508	2512	2515	rBV5	4874	6319	0.13%	0.014%
39	17.957	2524	2528	2531	rBV4	2968	5080	0.10%	0.011%
40	18.087	2545	2550	2558	rVV	69459	112891	2.27%	0.248%
41	18.151	2559	2561	2567	rVB2	7253	12001	0.24%	0.026%
42	19.139	2724	2729	2735	rBV	44524	63309	1.27%	0.139%
43	19.216	2737	2742	2746	rBV	38330	57757	1.16%	0.127%
44	19.369	2764	2768	2777	rBV2	54317	83585	1.68%	0.184%
45	19.522	2791	2794	2797	rVB2	17775	17732	0.36%	0.039%
46	19.581	2797	2804	2811	rBV	3409729	4966737	100.00%	10.913%
47	20.139	2896	2899	2902	rBV4	6026	5743	0.12%	0.013%
48	20.569	2969	2972	2974	rBV2	14528	17334	0.35%	0.038%
49	20.633	2981	2983	2985	rVB2	8915	5935	0.12%	0.013%
50	21.098	3058	3062	3070	rBV4	35071	58744	1.18%	0.129%
51	21.375	3103	3109	3122	rBV	1914681	2640413	53.16%	5.801%
52	22.469	3292	3295	3301	rVB3	42967	54379	1.09%	0.119%
53	22.604	3314	3318	3324	rVB	77009	109323	2.20%	0.240%
54	23.004	3382	3386	3392	rVB2	67390	98087	1.97%	0.216%
55	23.551	3470	3479	3486	rBV2	2140655	4366672	87.92%	9.594%
56	23.698	3496	3504	3520	rVB	1125241	2307708	46.46%	5.070%
57	24.298	3600	3606	3616	rVB	78811	169163	3.41%	0.372%
58	25.104	3738	3743	3750	rVB3	73915	162384	3.27%	0.357%




Sum of corrected areas: 45513111

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020130.D
Acq On : 11 Jun 2022 10:07
Operator : CG/JU
Sample : N3284-01
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYT1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

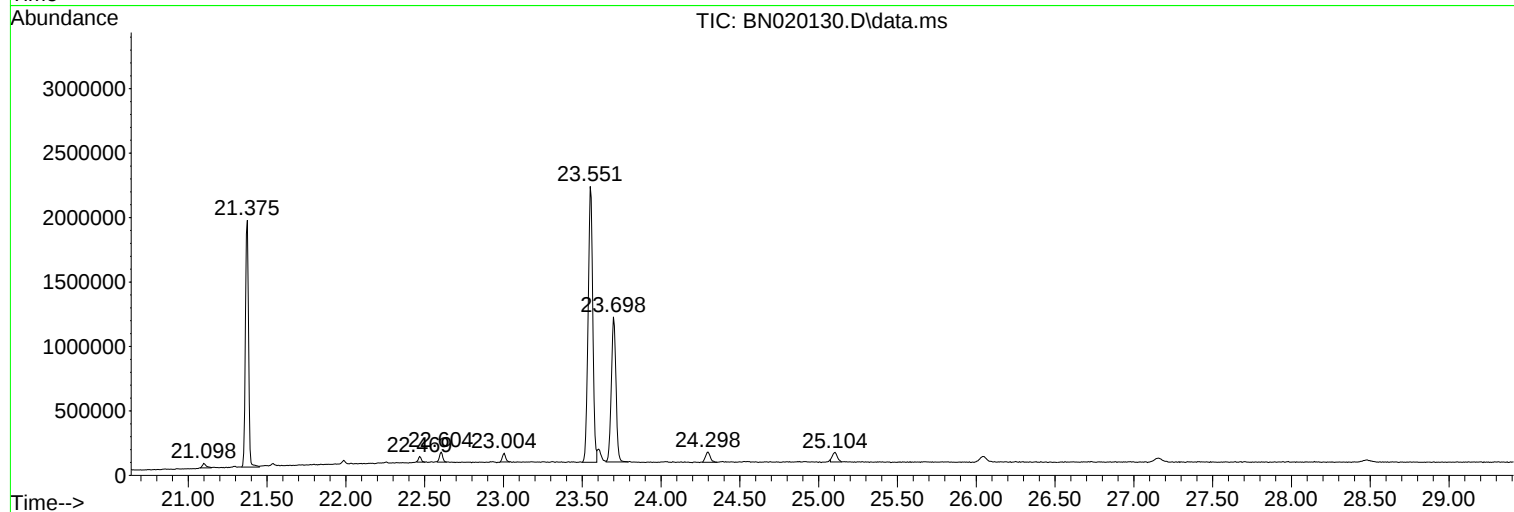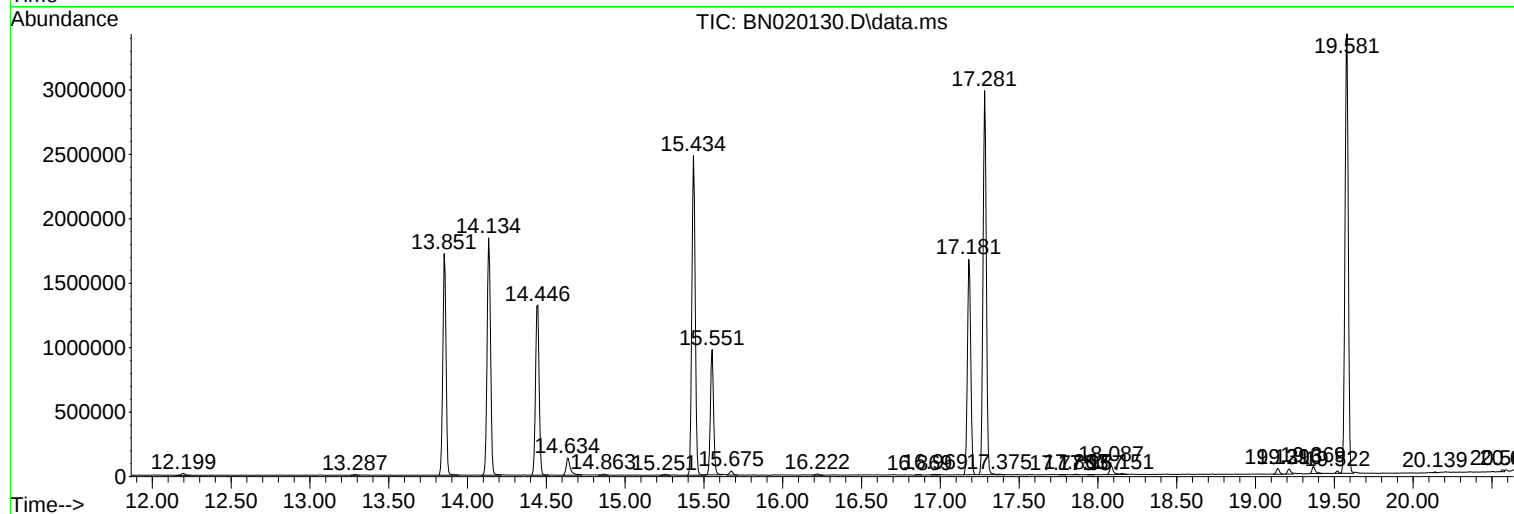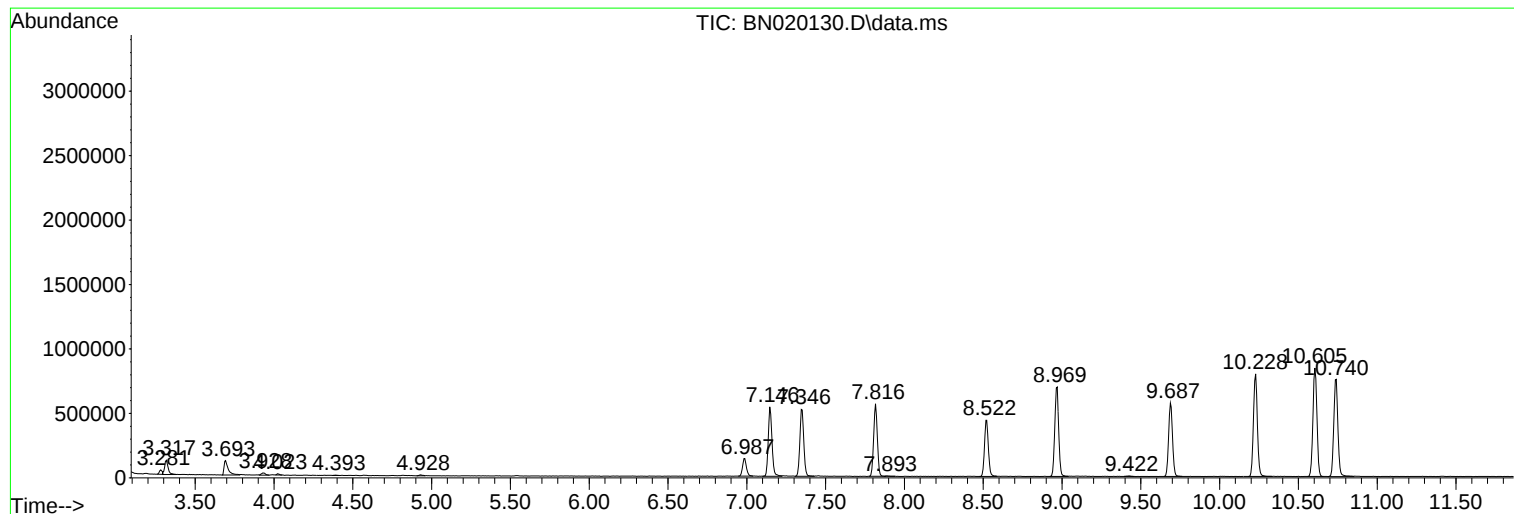

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020130.D
Acq On : 11 Jun 2022 10:07
Operator : CG/JU
Sample : N3284-01
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYT1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020130.D
Acq On : 11 Jun 2022 10:07
Operator : CG/JU
Sample : N3284-01
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYT1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc