

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020135.D
 Acq On : 11 Jun 2022 13:06
 Operator : CG/JU
 Sample : N3284-11
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYS9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020135.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	37	rBV	30212	41541	0.78%	0.088%
2	3.687	100	102	119	rBV	116122	210115	3.94%	0.443%
3	3.928	139	143	150	rVB2	15035	27648	0.52%	0.058%
4	4.028	156	160	168	rVB2	9788	16336	0.31%	0.034%
5	4.934	308	314	320	rBV6	6975	15165	0.28%	0.032%
6	5.475	401	406	407	rBV4	5849	7608	0.14%	0.016%
7	6.981	656	662	672	rBV	154559	264259	4.95%	0.558%
8	7.146	684	690	710	rBV	560983	948770	17.79%	2.003%
9	7.346	718	724	736	rVV	565346	939184	17.61%	1.982%
10	7.469	739	745	750	rVB4	7694	13002	0.24%	0.027%
11	7.816	797	804	814	rBV	559420	918415	17.22%	1.938%
12	8.522	917	924	935	rBV	450830	768280	14.40%	1.622%
13	8.969	992	1000	1007	rBV	725181	1250754	23.45%	2.640%
14	9.093	1018	1021	1025	rBV5	3765	5773	0.11%	0.012%
15	9.428	1074	1078	1086	rVB4	5166	9079	0.17%	0.019%
16	9.687	1115	1122	1132	rBV	616435	1043090	19.56%	2.202%
17	10.228	1207	1214	1231	rBV	835925	1434785	26.90%	3.028%
18	10.605	1268	1278	1293	rBV	877640	1516313	28.43%	3.200%
19	10.734	1293	1300	1312	rBV	734726	1319285	24.73%	2.785%
20	11.422	1410	1417	1426	rBV3	15135	27995	0.52%	0.059%
21	11.981	1507	1512	1518	rVB2	44563	70157	1.32%	0.148%
22	12.128	1533	1537	1540	rVB2	4795	5788	0.11%	0.012%
23	12.193	1543	1548	1554	rVB2	16384	27475	0.52%	0.058%
24	12.463	1589	1594	1601	rBV3	56551	94601	1.77%	0.200%
25	13.287	1727	1734	1743	rBV5	7359	13286	0.25%	0.028%
26	13.851	1824	1830	1843	rBV	1796478	2596825	48.68%	5.481%
27	14.134	1871	1878	1890	rBV	1969854	3012508	56.48%	6.358%
28	14.357	1909	1916	1919	rVB5	2749	5953	0.11%	0.013%
29	14.440	1924	1930	1938	rBV	1343153	2105670	39.48%	4.444%
30	14.640	1958	1964	1974	rBV	166266	303768	5.69%	0.641%
31	14.857	1997	2001	2011	rVB10	6329	10899	0.20%	0.023%
32	15.434	2092	2099	2112	rBV	2637007	3932274	73.72%	8.300%
33	15.551	2113	2119	2134	rVV	1101465	1532846	28.74%	3.235%
34	15.675	2134	2140	2146	rVB	35945	54515	1.02%	0.115%
35	15.945	2181	2186	2191	rVB4	6323	10892	0.20%	0.023%
36	16.216	2226	2232	2239	rVB7	9795	15665	0.29%	0.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020135.D
 Acq On : 11 Jun 2022 13:06
 Operator : CG/JU
 Sample : N3284-11
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYS9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	16.734	2317	2320	2323	rVB5	4764	5647	0.11%	0.012%
38	16.863	2339	2342	2345	rBV5	4350	5682	0.11%	0.012%
39	16.969	2356	2360	2366	rBV6	4036	8043	0.15%	0.017%
40	17.181	2390	2396	2406	rBV	1698188	2533489	47.50%	5.347%
41	17.281	2406	2413	2426	rVV2	3181395	4743054	88.92%	10.011%
42	17.369	2426	2428	2436	rVB8	5319	9585	0.18%	0.020%
43	17.863	2508	2512	2518	rBV2	28354	38368	0.72%	0.081%
44	18.051	2538	2544	2545	rBV6	4519	6472	0.12%	0.014%
45	18.086	2545	2550	2558	rVV3	53234	85495	1.60%	0.180%
46	18.151	2560	2561	2565	rVB3	6464	6562	0.12%	0.014%
47	19.039	2705	2712	2715	rBV9	7553	11437	0.21%	0.024%
48	19.139	2724	2729	2737	rBV2	44343	63893	1.20%	0.135%
49	19.210	2737	2741	2750	rBV	45879	72133	1.35%	0.152%
50	19.310	2755	2758	2764	rVB8	12833	16860	0.32%	0.036%
51	19.369	2764	2768	2780	rBV3	29463	53824	1.01%	0.114%
52	19.522	2790	2794	2797	rBV2	15949	17440	0.33%	0.037%
53	19.581	2797	2804	2811	rVV	3829340	5334032	100.00%	11.258%
54	19.633	2811	2813	2818	rVB6	10691	15534	0.29%	0.033%
55	19.804	2840	2842	2847	rVB4	3892	5839	0.11%	0.012%
56	20.563	2969	2971	2972	rBV2	10363	7938	0.15%	0.017%
57	21.063	3052	3056	3057	rBV3	14808	20096	0.38%	0.042%
58	21.092	3057	3061	3073	rVV3	81138	160628	3.01%	0.339%
59	21.375	3103	3109	3119	rBV	1865057	2594238	48.64%	5.475%
60	21.539	3134	3137	3140	rBV3	17260	17865	0.33%	0.038%
61	21.986	3210	3213	3223	rVB4	29790	47807	0.90%	0.101%
62	23.004	3382	3386	3391	rVB	57647	80665	1.51%	0.170%
63	23.551	3470	3479	3486	rBV	2180782	4449175	83.41%	9.391%
64	23.698	3496	3504	3513	rBV	1099546	2152427	40.35%	4.543%
65	24.292	3601	3605	3613	rVB4	62647	129808	2.43%	0.274%
66	25.098	3738	3742	3750	rVB2	51929	114488	2.15%	0.242%




Sum of corrected areas: 47379043

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020135.D
Acq On : 11 Jun 2022 13:06
Operator : CG/JU
Sample : N3284-11
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYS9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

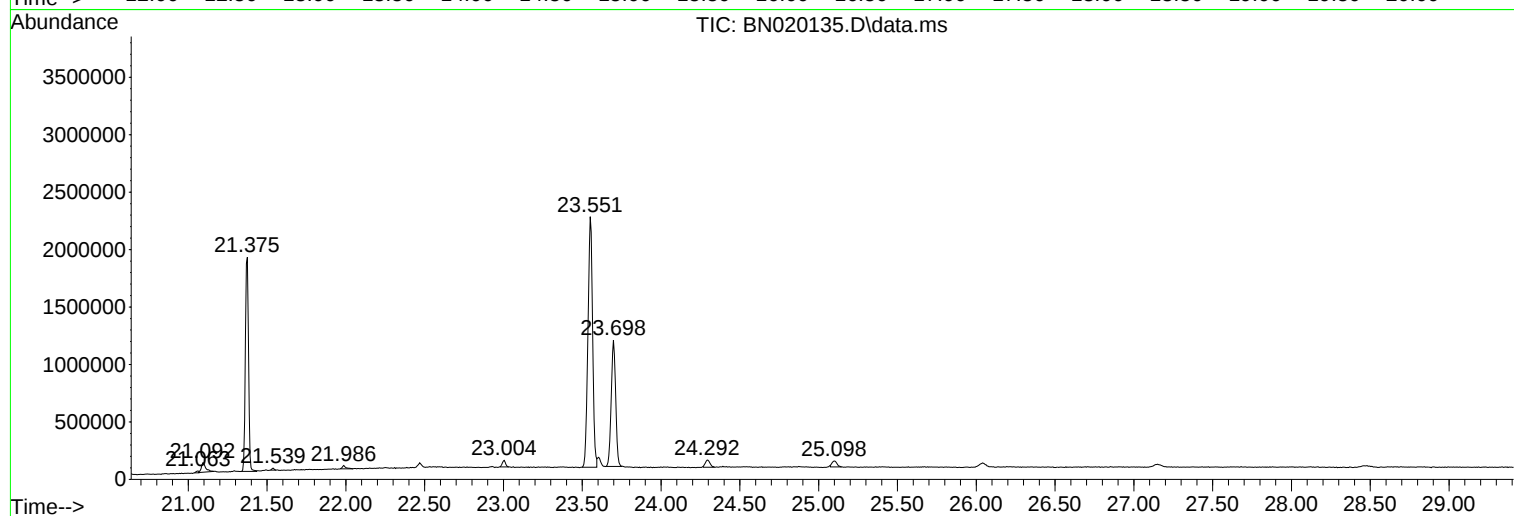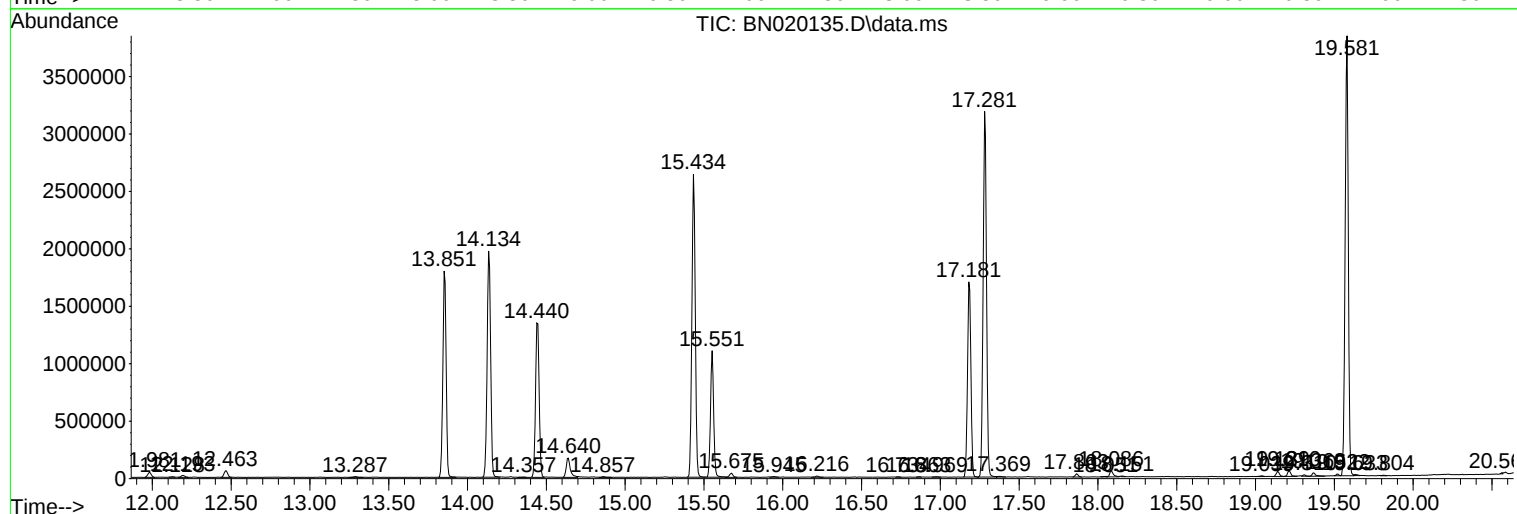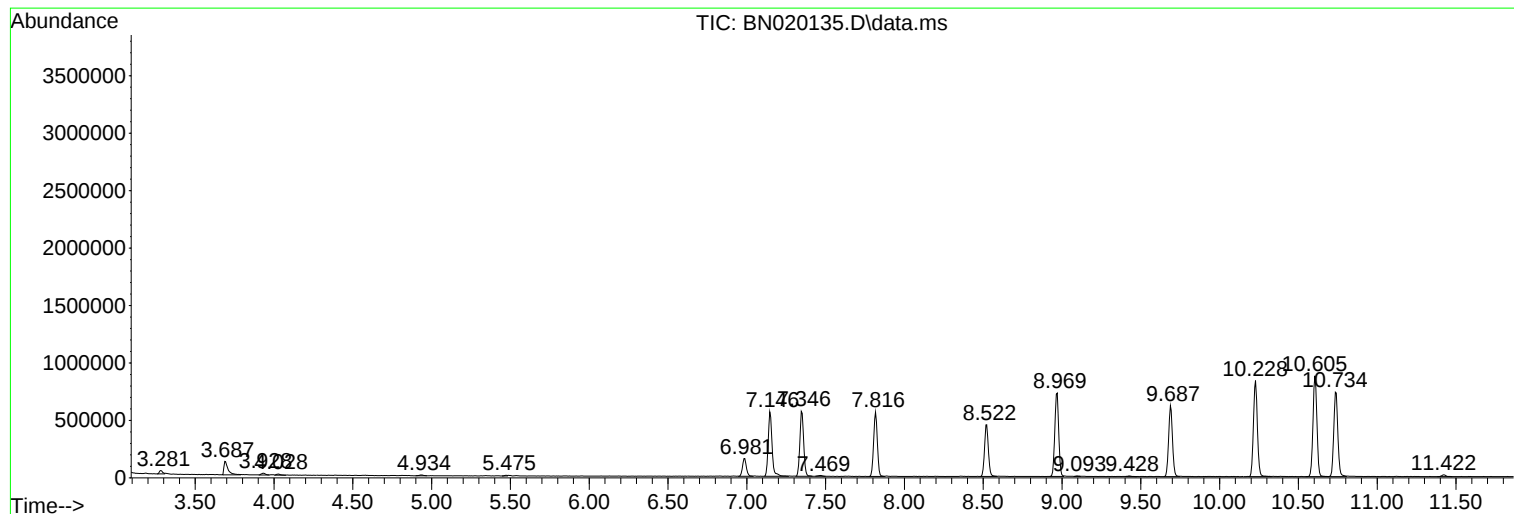

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020135.D
Acq On : 11 Jun 2022 13:06
Operator : CG/JU
Sample : N3284-11
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYS9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020135.D
Acq On : 11 Jun 2022 13:06
Operator : CG/JU
Sample : N3284-11
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYS9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc