

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020137.D
 Acq On : 11 Jun 2022 14:18
 Operator : CG/JU
 Sample : N3284-05
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYT5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020137.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	30	rBV	15769	18807	0.33%	0.036%
2	3.281	30	33	42	rVB	41245	60207	1.04%	0.114%
3	3.687	99	102	119	rBV	256253	419988	7.27%	0.793%
4	3.934	138	144	149	rVB2	19563	32940	0.57%	0.062%
5	4.028	156	160	167	rVB	10547	16787	0.29%	0.032%
6	4.552	245	249	259	rVB5	15260	30564	0.53%	0.058%
7	4.928	310	313	318	rVB	7510	10685	0.18%	0.020%
8	6.334	546	552	557	rVB6	8858	15583	0.27%	0.029%
9	6.469	571	575	579	rVB5	3711	6716	0.12%	0.013%
10	6.810	627	633	637	rBV2	14627	25895	0.45%	0.049%
11	6.916	646	651	656	rBV4	5799	8589	0.15%	0.016%
12	6.981	656	662	669	rVV	237230	397425	6.88%	0.751%
13	7.046	669	673	678	rVB	25536	38278	0.66%	0.072%
14	7.146	683	690	698	rBV	621486	1025002	17.74%	1.936%
15	7.210	698	701	711	rVB	20858	34596	0.60%	0.065%
16	7.346	717	724	734	rBV	644638	1080330	18.70%	2.040%
17	7.469	739	745	751	rBV	45888	73468	1.27%	0.139%
18	7.722	785	788	796	rVB	8795	15057	0.26%	0.028%
19	7.816	797	804	811	rBV	562016	925340	16.01%	1.747%
20	7.940	819	825	834	rVB3	19538	42204	0.73%	0.080%
21	8.181	860	866	872	rVB6	5906	13875	0.24%	0.026%
22	8.310	883	888	893	rBV2	9193	14122	0.24%	0.027%
23	8.369	893	898	904	rVV	20157	31976	0.55%	0.060%
24	8.463	907	914	918	rVV2	35900	61959	1.07%	0.117%
25	8.522	918	924	934	rVV	607962	1005727	17.41%	1.899%
26	8.622	936	941	952	rVB2	15041	30381	0.53%	0.057%
27	8.775	962	967	972	rBV3	10945	17147	0.30%	0.032%
28	8.822	972	975	981	rVB	13030	20340	0.35%	0.038%
29	8.969	993	1000	1016	rVB	806875	1412250	24.44%	2.667%
30	9.110	1016	1024	1031	rBV2	87653	171254	2.96%	0.323%
31	9.169	1031	1034	1040	rVB6	10657	22458	0.39%	0.042%
32	9.257	1045	1049	1055	rVV4	6420	12242	0.21%	0.023%
33	9.316	1055	1059	1065	rVB4	4311	8790	0.15%	0.017%
34	9.446	1076	1081	1086	rVV3	11389	18800	0.33%	0.036%
35	9.504	1086	1091	1098	rVB3	16891	27123	0.47%	0.051%
36	9.687	1114	1122	1131	rBV	688161	1171456	20.27%	2.212%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020137.D
 Acq On : 11 Jun 2022 14:18
 Operator : CG/JU
 Sample : N3284-05
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYT5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	9.810	1139	1143	1146	rBV4	6567	9511	0.16%	0.018%
38	10.016	1173	1178	1184	rVB4	21830	38843	0.67%	0.073%
39	10.081	1184	1189	1193	rBV6	3809	6959	0.12%	0.013%
40	10.228	1206	1214	1226	rBV	942825	1637375	28.34%	3.092%
41	10.316	1226	1229	1234	rVB3	5171	7477	0.13%	0.014%
42	10.399	1238	1243	1248	rBV4	2981	7276	0.13%	0.014%
43	10.604	1269	1278	1285	rBV	867172	1508157	26.10%	2.848%
44	10.657	1285	1287	1294	rVB	20294	25465	0.44%	0.048%
45	10.740	1294	1301	1313	rBV	916558	1642509	28.43%	3.102%
46	11.404	1407	1414	1415	rBV4	3643	5898	0.10%	0.011%
47	11.804	1475	1482	1487	rBV7	2963	5846	0.10%	0.011%
48	12.193	1544	1548	1555	rVB3	17895	30475	0.53%	0.058%
49	12.269	1555	1561	1568	rVB	23118	39060	0.68%	0.074%
50	12.487	1592	1598	1605	rVB2	14859	26264	0.45%	0.050%
51	13.281	1729	1733	1738	rBV6	5064	8369	0.14%	0.016%
52	13.469	1762	1765	1769	rBV5	4136	6658	0.12%	0.013%
53	13.616	1784	1790	1797	rBV8	3789	10844	0.19%	0.020%
54	13.769	1811	1816	1821	rVB4	7991	12224	0.21%	0.023%
55	13.851	1821	1830	1841	rBV	2062977	3010453	52.10%	5.685%
56	14.134	1869	1878	1893	rBV	2105455	3336969	57.75%	6.302%
57	14.445	1922	1931	1938	rBV	1364102	2080706	36.01%	3.929%
58	14.634	1958	1963	1974	rBV	245827	435125	7.53%	0.822%
59	14.798	1985	1991	1997	rVV9	3586	8819	0.15%	0.017%
60	14.863	1997	2002	2008	rVB6	14450	22762	0.39%	0.043%
61	15.257	2062	2069	2073	rBV3	6939	11910	0.21%	0.022%
62	15.304	2073	2077	2084	rVB3	10740	14550	0.25%	0.027%
63	15.434	2092	2099	2107	rBV	2991035	4421254	76.52%	8.349%
64	15.551	2113	2119	2133	rBV	1222945	1711886	29.63%	3.233%
65	15.675	2133	2140	2150	rVB3	39454	80965	1.40%	0.153%
66	15.863	2168	2172	2177	rBV7	3028	6923	0.12%	0.013%
67	16.163	2220	2223	2227	rBV2	16791	22500	0.39%	0.042%
68	16.216	2229	2232	2237	rVB5	13193	19375	0.34%	0.037%
69	16.863	2339	2342	2346	rBV5	6099	7215	0.12%	0.014%
70	16.957	2354	2358	2362	rBV3	19844	27806	0.48%	0.053%
71	17.181	2389	2396	2406	rBV	1674234	2507937	43.40%	4.736%
72	17.281	2406	2413	2424	rVV2	3367394	5084279	87.99%	9.602%
73	17.375	2427	2429	2436	rVB6	5573	9610	0.17%	0.018%
74	17.563	2456	2461	2466	rBV	51339	72667	1.26%	0.137%
75	17.692	2479	2483	2489	rBV	15722	20442	0.35%	0.039%
76	17.863	2509	2512	2515	rVB5	4305	5910	0.10%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
 Data File : BN020137.D
 Acq On : 11 Jun 2022 14:18
 Operator : CG/JU
 Sample : N3284-05
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYT5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

77	18.080	2545	2549	2557	rBV	60511	92179	1.60%	0.174%
78	18.157	2559	2562	2567	rVB2	13291	18617	0.32%	0.035%
79	18.386	2596	2601	2611	rBV4	11986	23650	0.41%	0.045%
80	19.022	2707	2709	2713	rVB4	10112	11839	0.20%	0.022%
81	19.139	2724	2729	2736	rBV2	49269	68497	1.19%	0.129%
82	19.210	2737	2741	2745	rVV	45741	62985	1.09%	0.119%
83	19.369	2763	2768	2774	rBV2	47769	68459	1.18%	0.129%
84	19.516	2790	2793	2797	rVB2	17483	19168	0.33%	0.036%
85	19.580	2797	2804	2819	rBV	3854917	5778176	100.00%	10.912%
86	20.139	2896	2899	2902	rVB4	11088	12463	0.22%	0.024%
87	20.569	2969	2972	2974	rBV2	12482	16957	0.29%	0.032%
88	20.633	2981	2983	2987	rVB3	13858	12876	0.22%	0.024%
89	21.098	3059	3062	3069	rVB2	25022	30542	0.53%	0.058%
90	21.369	3103	3108	3119	rBV	1926503	2589346	44.81%	4.890%
91	21.533	3134	3136	3141	rVB2	20664	22757	0.39%	0.043%
92	21.986	3209	3213	3217	rBV4	33103	43616	0.75%	0.082%
93	22.468	3291	3295	3300	rVB	52531	71477	1.24%	0.135%
94	22.604	3314	3318	3324	rVB	38535	57039	0.99%	0.108%
95	23.004	3381	3386	3393	rVB	75224	126195	2.18%	0.238%
96	23.551	3470	3479	3486	rBV2	2404420	4949387	85.66%	9.347%
97	23.698	3496	3504	3516	rVB	1135684	2222277	38.46%	4.197%
98	24.298	3600	3606	3615	rVB	93481	201810	3.49%	0.381%
99	25.098	3737	3742	3749	rVB2	87376	185000	3.20%	0.349%




Sum of corrected areas: 52952946

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020137.D
Acq On : 11 Jun 2022 14:18
Operator : CG/JU
Sample : N3284-05
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYT5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

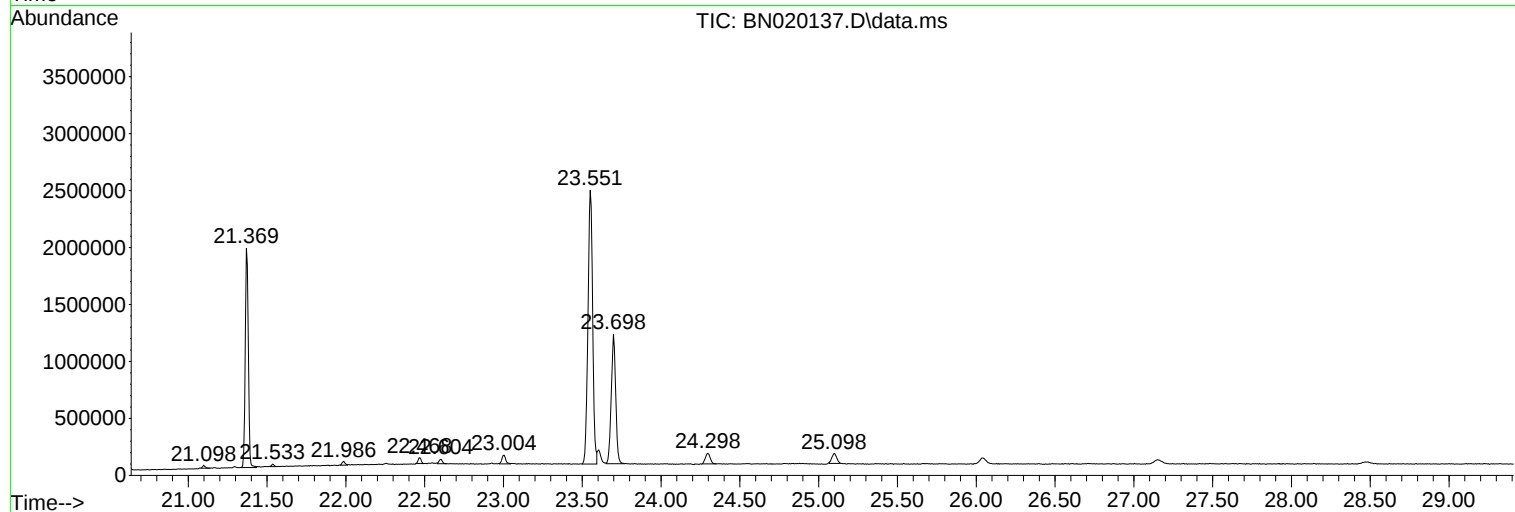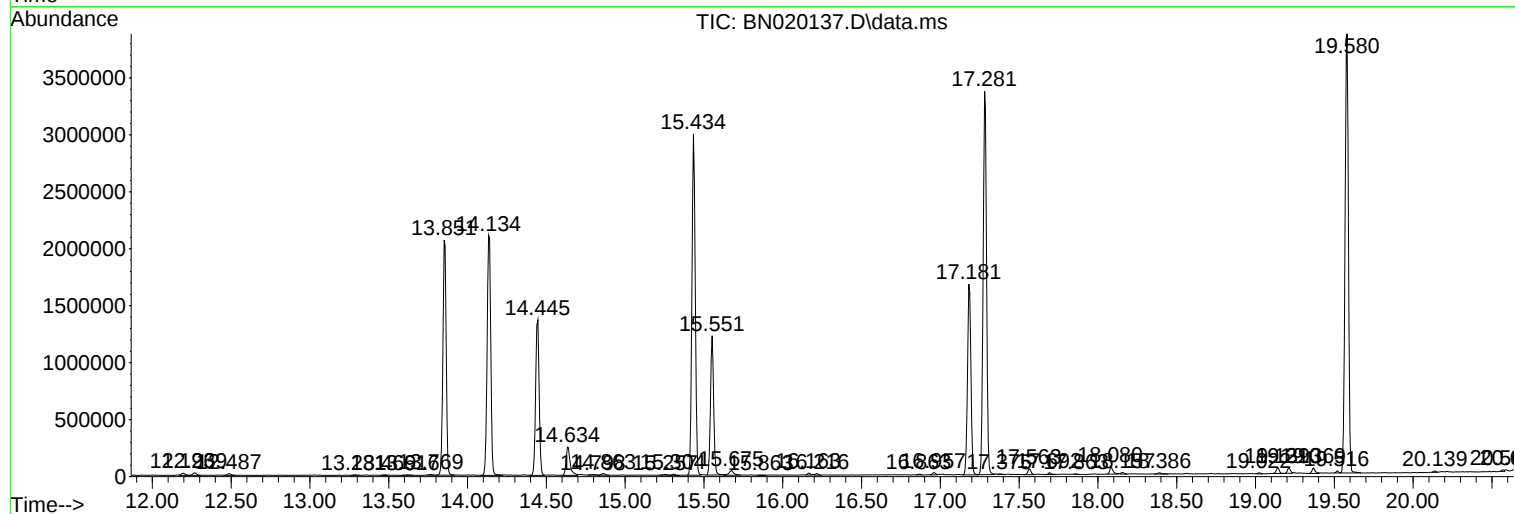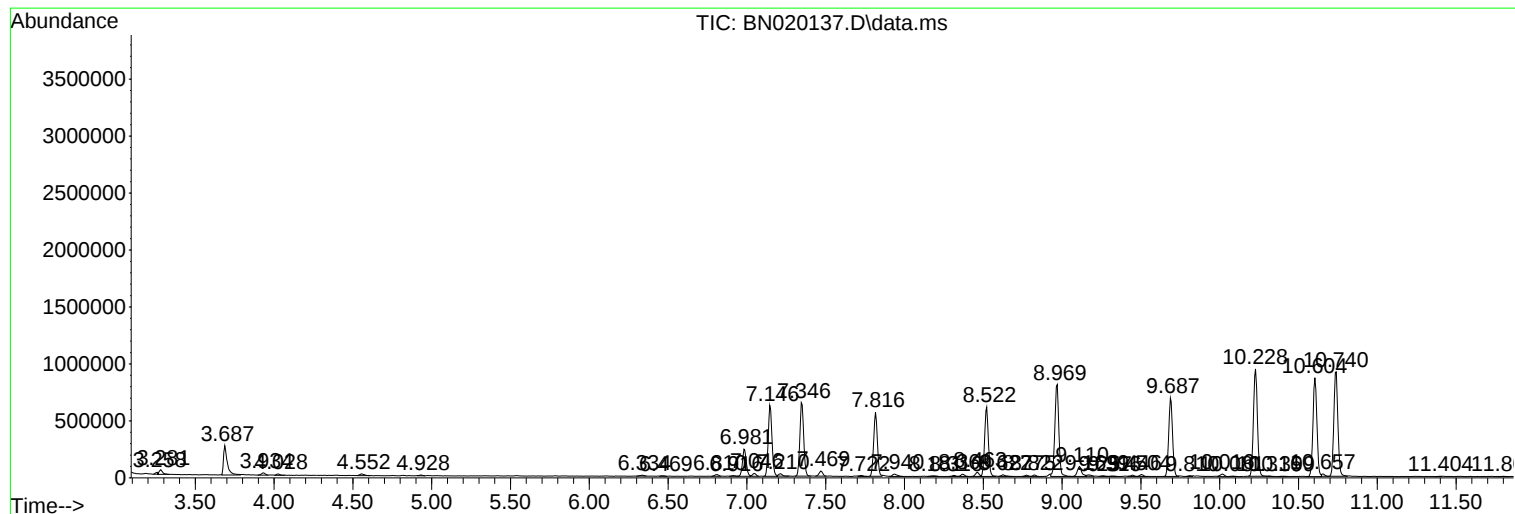

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020137.D
Acq On : 11 Jun 2022 14:18
Operator : CG/JU
Sample : N3284-05
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYT5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexanoic acid, 2-ethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.110	3.70 ng/ul	171254	1,4-Dichlorobenzene-d4	7.816

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	86
2			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	86
3			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	86
4			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	78
5			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	78

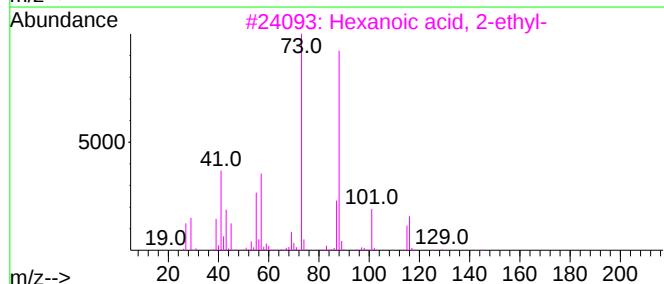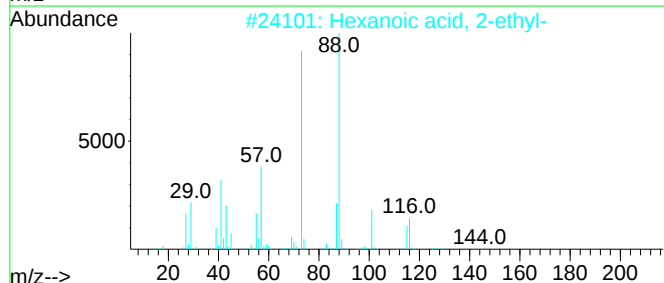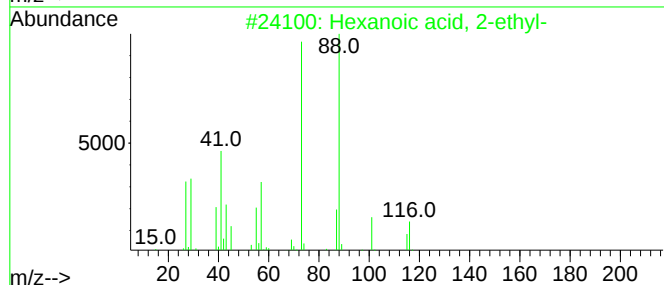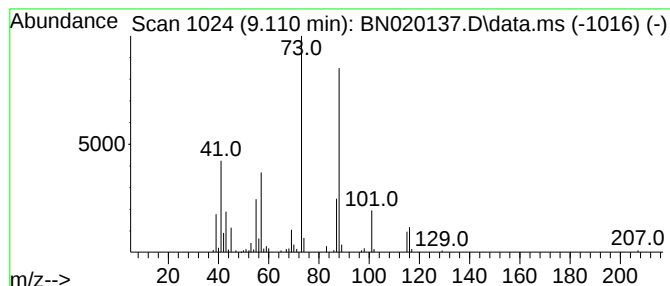

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061122\
Data File : BN020137.D
Acq On : 11 Jun 2022 14:18
Operator : CG/JU
Sample : N3284-05
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYT5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexanoic acid, ...	9.110	3.7	ng/ul	171254	1	7.816	925340	20.0