

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN061122\  
 Data File : BN020138.D  
 Acq On : 11 Jun 2022 14:53  
 Operator : CG/JU  
 Sample : N3284-07  
 Misc :  
 ALS Vial : 47 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 EXYS8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN060622.M  
 Title : SVOA CALIBRATION

Signal : TIC: BN020138.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.281       | 29            | 33          | 36           | rBV      | 29132          | 37964         | 0.80%           | 0.089%        |
| 2         | 3.317       | 36            | 39          | 48           | rVB      | 30354          | 45406         | 0.96%           | 0.107%        |
| 3         | 3.687       | 99            | 102         | 114          | rBV      | 142492         | 244889        | 5.16%           | 0.575%        |
| 4         | 3.934       | 139           | 144         | 149          | rVB2     | 16127          | 27104         | 0.57%           | 0.064%        |
| 5         | 4.022       | 156           | 159         | 165          | rVB3     | 9967           | 15013         | 0.32%           | 0.035%        |
| 6         | 4.822       | 291           | 295         | 298          | rVB4     | 3636           | 5787          | 0.12%           | 0.014%        |
| 7         | 4.928       | 309           | 313         | 321          | rBV5     | 6547           | 11933         | 0.25%           | 0.028%        |
| 8         | 5.534       | 413           | 416         | 424          | rVB4     | 3184           | 5654          | 0.12%           | 0.013%        |
| 9         | 6.981       | 657           | 662         | 676          | rVB      | 135144         | 230704        | 4.86%           | 0.542%        |
| 10        | 7.146       | 684           | 690         | 701          | rBV      | 493944         | 816999        | 17.22%          | 1.919%        |
| 11        | 7.346       | 718           | 724         | 735          | rBV      | 492012         | 829919        | 17.49%          | 1.950%        |
| 12        | 7.816       | 797           | 804         | 812          | rBV      | 498917         | 822318        | 17.33%          | 1.932%        |
| 13        | 8.522       | 917           | 924         | 934          | rBV      | 425102         | 719468        | 15.16%          | 1.690%        |
| 14        | 8.969       | 991           | 1000        | 1014         | rBV      | 647112         | 1101614       | 23.22%          | 2.588%        |
| 15        | 9.140       | 1025          | 1029        | 1034         | rVB5     | 3390           | 5598          | 0.12%           | 0.013%        |
| 16        | 9.687       | 1114          | 1122        | 1130         | rBV      | 531921         | 893628        | 18.83%          | 2.099%        |
| 17        | 10.228      | 1206          | 1214        | 1225         | rBV      | 726293         | 1273584       | 26.84%          | 2.992%        |
| 18        | 10.604      | 1270          | 1278        | 1290         | rBV      | 763936         | 1326370       | 27.95%          | 3.116%        |
| 19        | 10.734      | 1292          | 1300        | 1316         | rBV      | 718814         | 1307766       | 27.56%          | 3.072%        |
| 20        | 12.198      | 1540          | 1549        | 1556         | rBV4     | 14952          | 27907         | 0.59%           | 0.066%        |
| 21        | 13.351      | 1741          | 1745        | 1752         | rVB4     | 5982           | 9133          | 0.19%           | 0.021%        |
| 22        | 13.851      | 1824          | 1830        | 1838         | rBV      | 1725074        | 2383982       | 50.24%          | 5.600%        |
| 23        | 14.134      | 1871          | 1878        | 1891         | rBV      | 1818726        | 2724569       | 57.42%          | 6.400%        |
| 24        | 14.228      | 1891          | 1894        | 1900         | rVB4     | 3345           | 5737          | 0.12%           | 0.013%        |
| 25        | 14.445      | 1924          | 1931        | 1943         | rVB      | 1181876        | 1857551       | 39.15%          | 4.364%        |
| 26        | 14.634      | 1956          | 1963        | 1978         | rBV      | 119174         | 228139        | 4.81%           | 0.536%        |
| 27        | 14.869      | 1998          | 2003        | 2007         | rVB5     | 6160           | 10285         | 0.22%           | 0.024%        |
| 28        | 15.257      | 2065          | 2069        | 2074         | rBV6     | 4629           | 6655          | 0.14%           | 0.016%        |
| 29        | 15.434      | 2092          | 2099        | 2110         | rBV      | 2465474        | 3586887       | 75.59%          | 8.426%        |
| 30        | 15.551      | 2113          | 2119        | 2130         | rVV      | 917200         | 1245757       | 26.25%          | 2.926%        |
| 31        | 15.675      | 2135          | 2140        | 2146         | rVB2     | 28419          | 44827         | 0.94%           | 0.105%        |
| 32        | 16.222      | 2228          | 2233        | 2237         | rVB3     | 7395           | 10266         | 0.22%           | 0.024%        |
| 33        | 16.863      | 2335          | 2342        | 2348         | rVB7     | 4853           | 8443          | 0.18%           | 0.020%        |
| 34        | 16.981      | 2355          | 2362        | 2370         | rBV4     | 9806           | 22537         | 0.47%           | 0.053%        |
| 35        | 17.181      | 2390          | 2396        | 2406         | rVB      | 1538121        | 2232840       | 47.05%          | 5.245%        |
| 36        | 17.281      | 2406          | 2413        | 2425         | rBV      | 2819447        | 4223863       | 89.01%          | 9.922%        |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN061122\  
 Data File : BN020138.D  
 Acq On : 11 Jun 2022 14:53  
 Operator : CG/JU  
 Sample : N3284-07  
 Misc :  
 ALS Vial : 47 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 EXYS8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN060622.M  
 Title : SVOA CALIBRATION

|    |        |      |      |      |      |         |         |         |         |
|----|--------|------|------|------|------|---------|---------|---------|---------|
| 37 | 17.375 | 2427 | 2429 | 2434 | rVB4 | 6267    | 9601    | 0.20%   | 0.023%  |
| 38 | 17.863 | 2508 | 2512 | 2515 | rBV4 | 5656    | 7827    | 0.16%   | 0.018%  |
| 39 | 18.086 | 2545 | 2550 | 2558 | rBV  | 115253  | 169830  | 3.58%   | 0.399%  |
| 40 | 18.151 | 2560 | 2561 | 2566 | rVB2 | 7008    | 8626    | 0.18%   | 0.020%  |
| 41 | 18.722 | 2653 | 2658 | 2662 | rBV4 | 3390    | 5363    | 0.11%   | 0.013%  |
| 42 | 19.139 | 2725 | 2729 | 2734 | rVB  | 34943   | 47614   | 1.00%   | 0.112%  |
| 43 | 19.210 | 2737 | 2741 | 2745 | rBV2 | 34389   | 47259   | 1.00%   | 0.111%  |
| 44 | 19.245 | 2745 | 2747 | 2751 | rVB3 | 4125    | 4934    | 0.10%   | 0.012%  |
| 45 | 19.369 | 2763 | 2768 | 2774 | rBV  | 53533   | 78313   | 1.65%   | 0.184%  |
| 46 | 19.516 | 2788 | 2793 | 2797 | rBV4 | 16938   | 24440   | 0.52%   | 0.057%  |
| 47 | 19.580 | 2797 | 2804 | 2811 | rBV  | 3137811 | 4745197 | 100.00% | 11.147% |
| 48 | 20.569 | 2969 | 2972 | 2974 | rBV2 | 11797   | 16084   | 0.34%   | 0.038%  |
| 49 | 20.633 | 2980 | 2983 | 2988 | rVB4 | 10010   | 11862   | 0.25%   | 0.028%  |
| 50 | 21.098 | 3057 | 3062 | 3073 | rBV  | 89975   | 189903  | 4.00%   | 0.446%  |
| 51 | 21.369 | 3103 | 3108 | 3123 | rBV  | 1666075 | 2313285 | 48.75%  | 5.434%  |
| 52 | 21.539 | 3134 | 3137 | 3141 | rVB3 | 20626   | 22272   | 0.47%   | 0.052%  |
| 53 | 21.986 | 3209 | 3213 | 3216 | rBV  | 32389   | 42607   | 0.90%   | 0.100%  |
| 54 | 22.469 | 3291 | 3295 | 3302 | rBV2 | 53294   | 75389   | 1.59%   | 0.177%  |
| 55 | 23.004 | 3381 | 3386 | 3392 | rVB  | 71854   | 113283  | 2.39%   | 0.266%  |
| 56 | 23.551 | 3471 | 3479 | 3486 | rBV  | 1933844 | 3979518 | 83.86%  | 9.348%  |
| 57 | 23.698 | 3496 | 3504 | 3514 | rVB  | 984133  | 1976999 | 41.66%  | 4.644%  |
| 58 | 24.292 | 3600 | 3605 | 3613 | rVB2 | 84437   | 175651  | 3.70%   | 0.413%  |
| 59 | 25.098 | 3737 | 3742 | 3749 | rVB3 | 67610   | 152244  | 3.21%   | 0.358%  |




Sum of corrected areas: 42569197

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN061122\  
Data File : BN020138.D  
Acq On : 11 Jun 2022 14:53  
Operator : CG/JU  
Sample : N3284-07  
Misc :  
ALS Vial : 47 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
EXYS8

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN060622.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

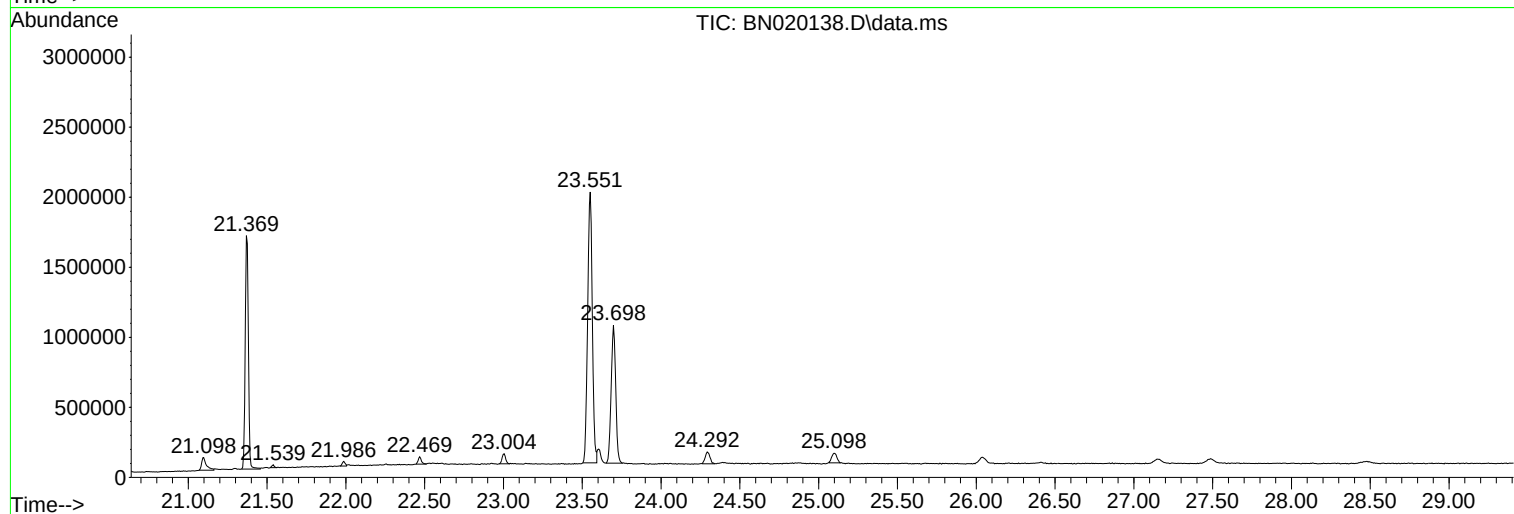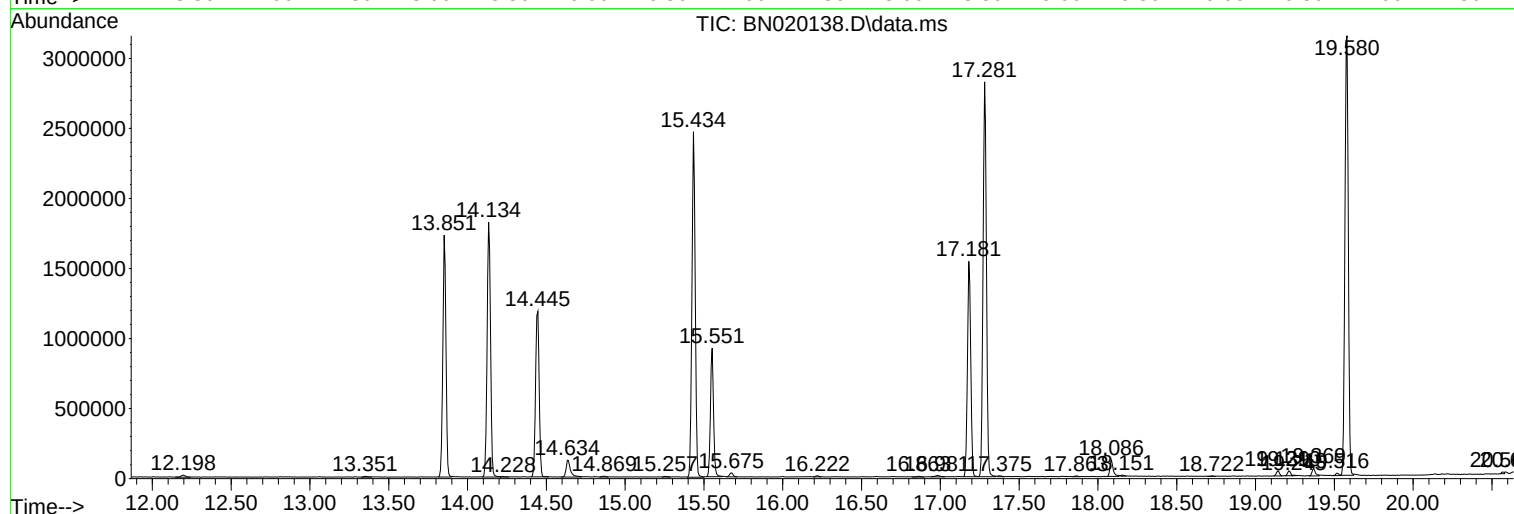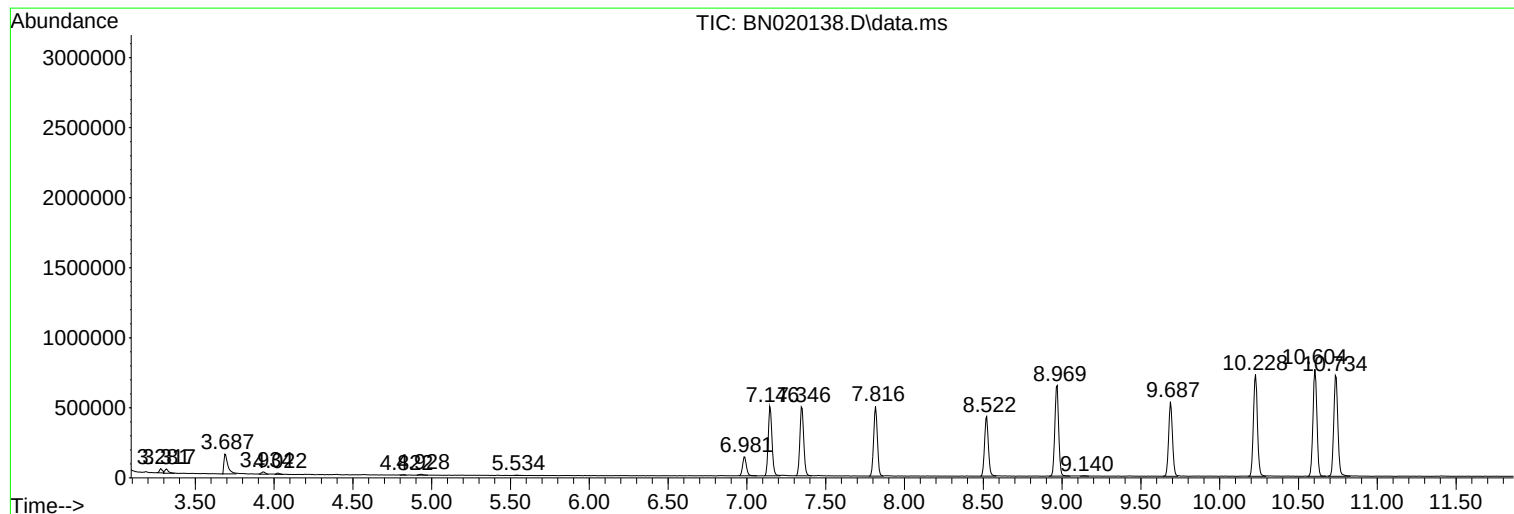

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN061122\  
Data File : BN020138.D  
Acq On : 11 Jun 2022 14:53  
Operator : CG/JU  
Sample : N3284-07  
Misc :  
ALS Vial : 47 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
EXYS8

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN060622.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN061122\  
Data File : BN020138.D  
Acq On : 11 Jun 2022 14:53  
Operator : CG/JU  
Sample : N3284-07  
Misc :  
ALS Vial : 47 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
EXYS8

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN060622.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

---