
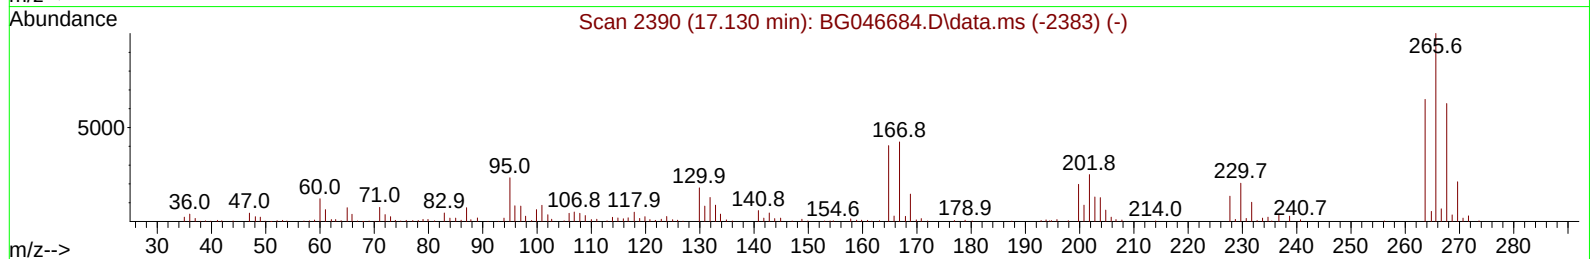
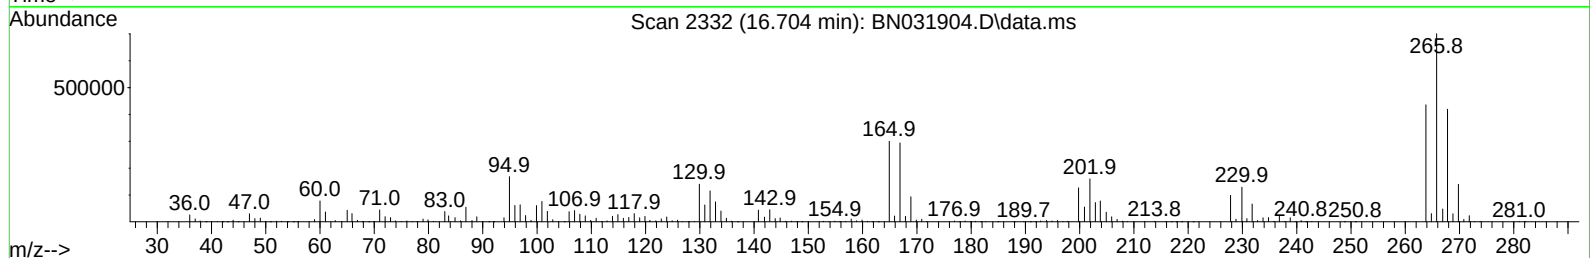


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061124\
Data File : BN031904.D
Acq On : 11 Jun 2024 10:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 11:32:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 11 01:48:18 2024
Response via : Initial Calibration

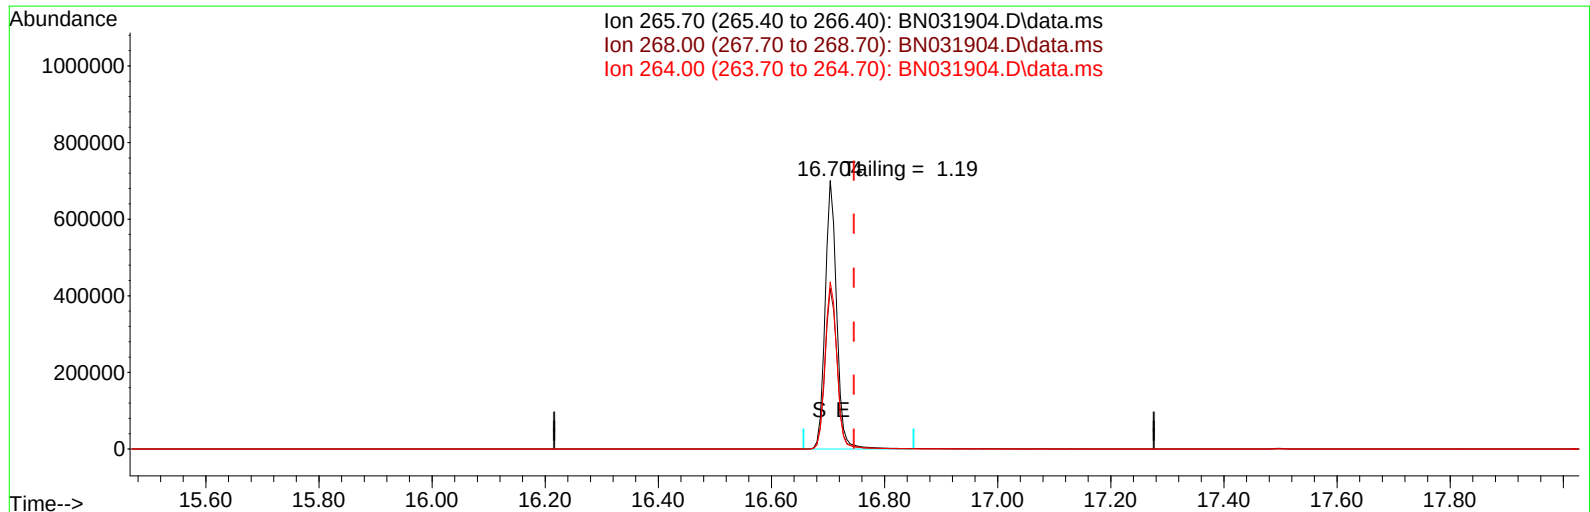

TIC: BN031904.D\data.ms

(70) Pentachlorophenol (C)




16.704min (-0.042) 26326.14 ng

response 997056

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.82
264.00	61.60	62.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061124\
Data File : BN031904.D
Acq On : 11 Jun 2024 10:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 11:32:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 11 01:48:18 2024
Response via : Initial Calibration

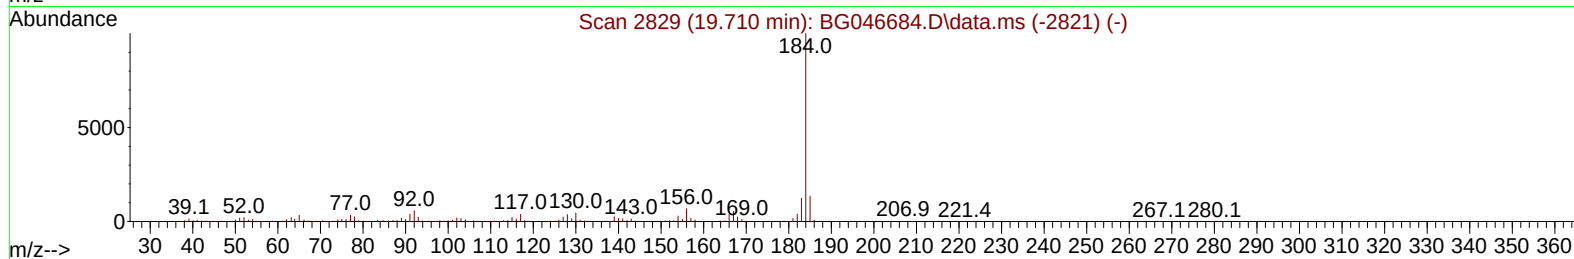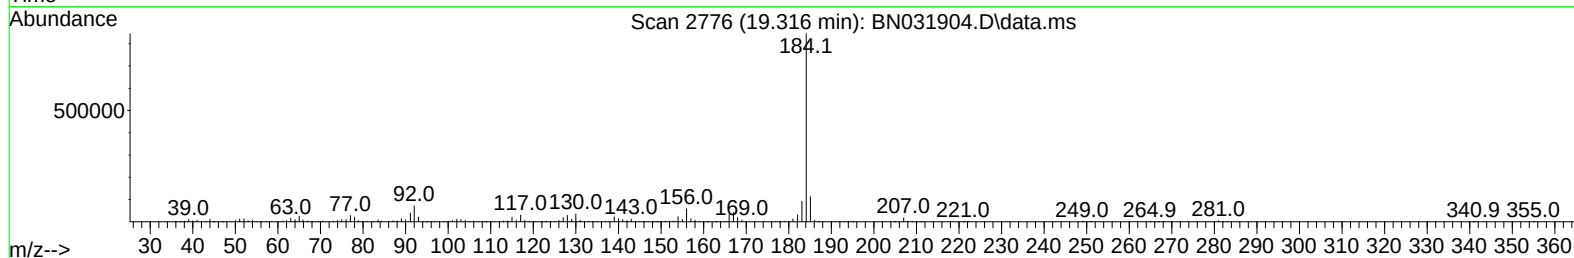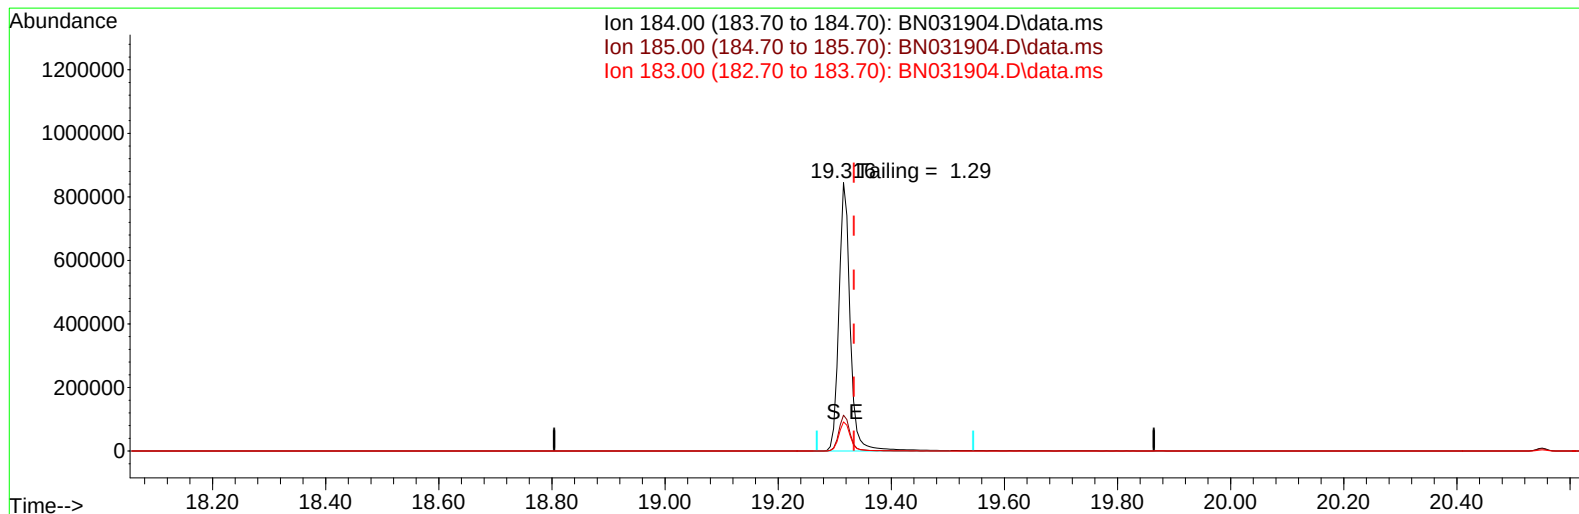

TIC: BN031904.D\data.ms

(77) Benzidine

19.316min (-0.018) 0.00 ng

response 1177088

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.39
183.00	13.20	10.88
0.00	0.00	0.00