
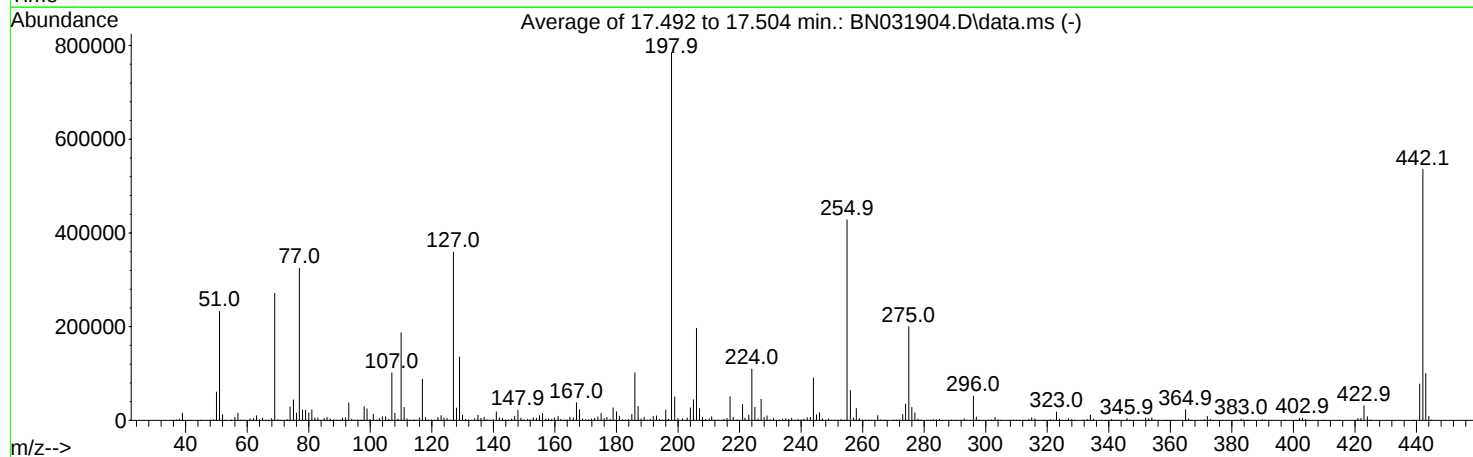


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061124\
Data File : BN031904.D
Acq On : 11 Jun 2024 10:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN061024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 10 15:47:32 2024

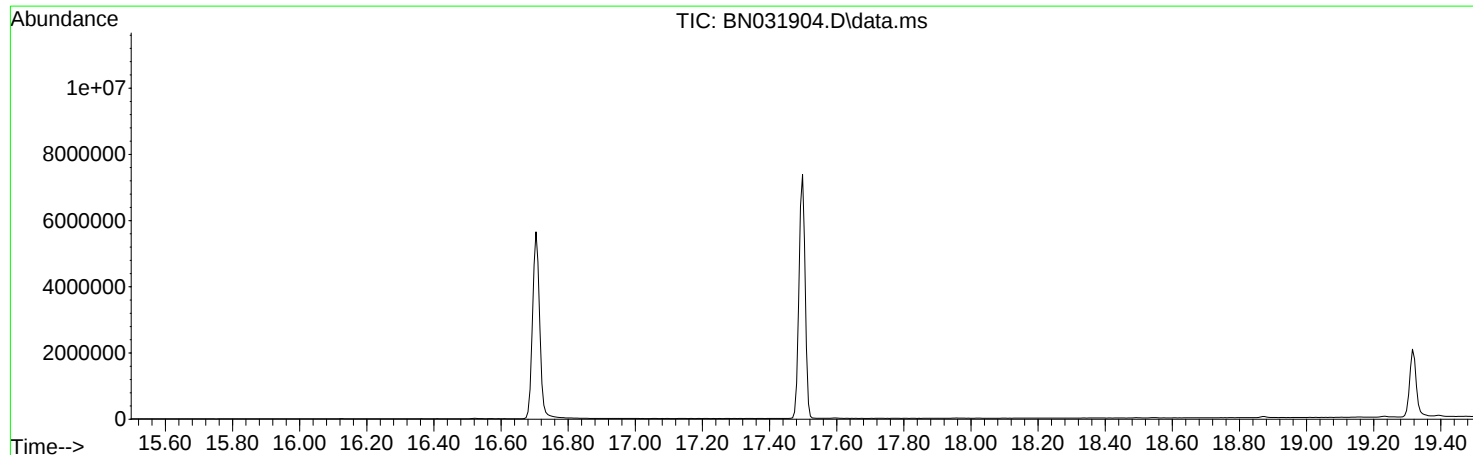




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.6	232724	PASS
68	69	0.00	2	1.6	4287	PASS
69	198	0.00	100	34.5	271125	PASS
70	69	0.00	2	0.6	1528	PASS
127	198	10	80	45.7	359083	PASS
197	198	0.00	2	0.3	2466	PASS
198	198	100	100	100.0	785067	PASS
199	198	5	9	6.4	50235	PASS
275	198	10	60	25.5	199808	PASS
365	198	1	100	2.9	23013	PASS
441	198	0.01	100	9.9	77701	PASS
442	442	50	100	100.0	535445	PASS
443	442	15	24	18.7	100027	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061124\
Data File : BN031904.D
Acq On : 11 Jun 2024 10:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 11 11:32:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 11 01:48:18 2024
Response via : Initial Calibration

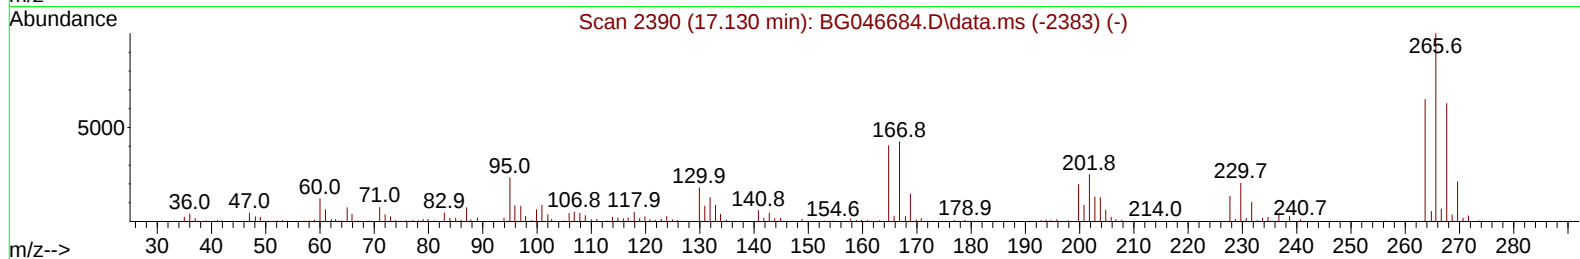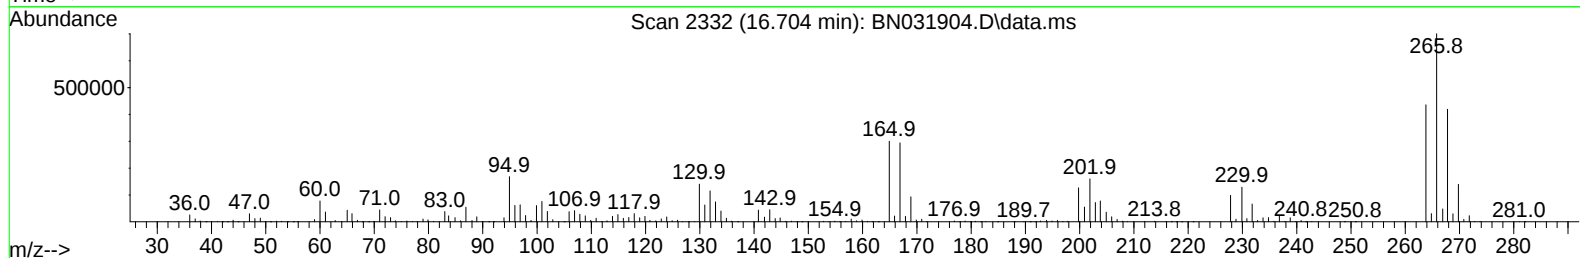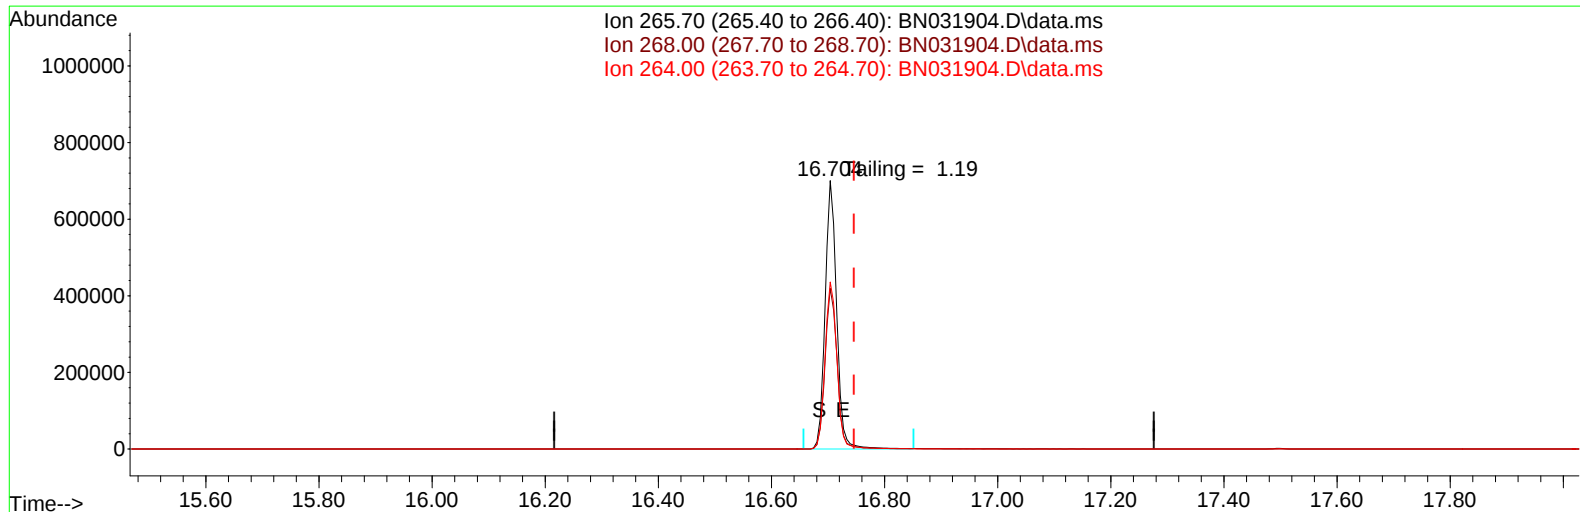

TIC: BN031904.D\data.ms

(70) Pentachlorophenol (C)

16.704min (-0.042) 26326.14 ng




response 997056

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.82
264.00	61.60	62.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061124\
Data File : BN031904.D
Acq On : 11 Jun 2024 10:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 11 11:32:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 11 01:48:18 2024
Response via : Initial Calibration

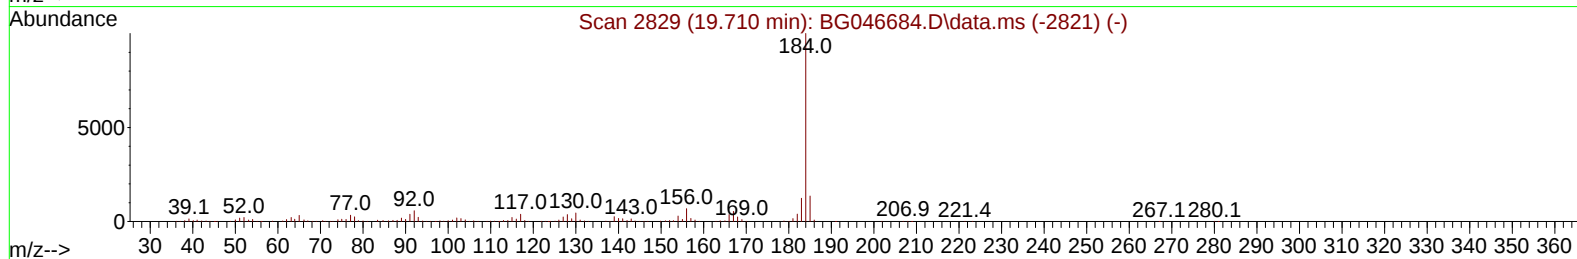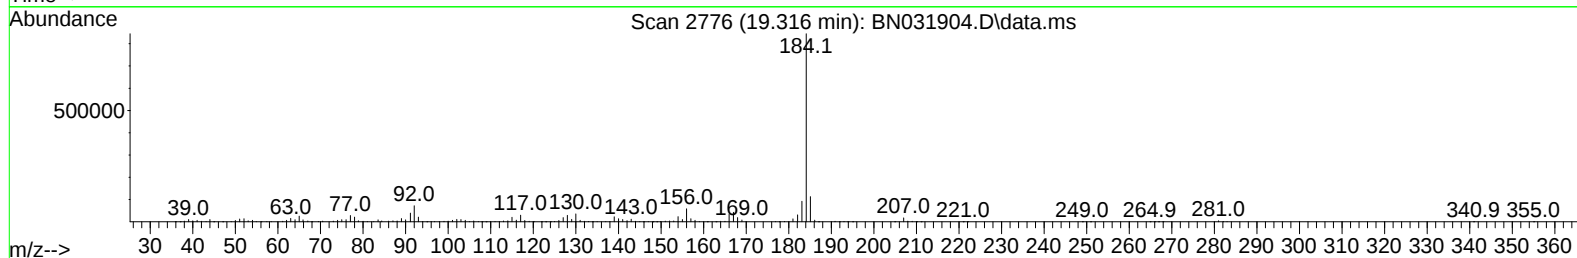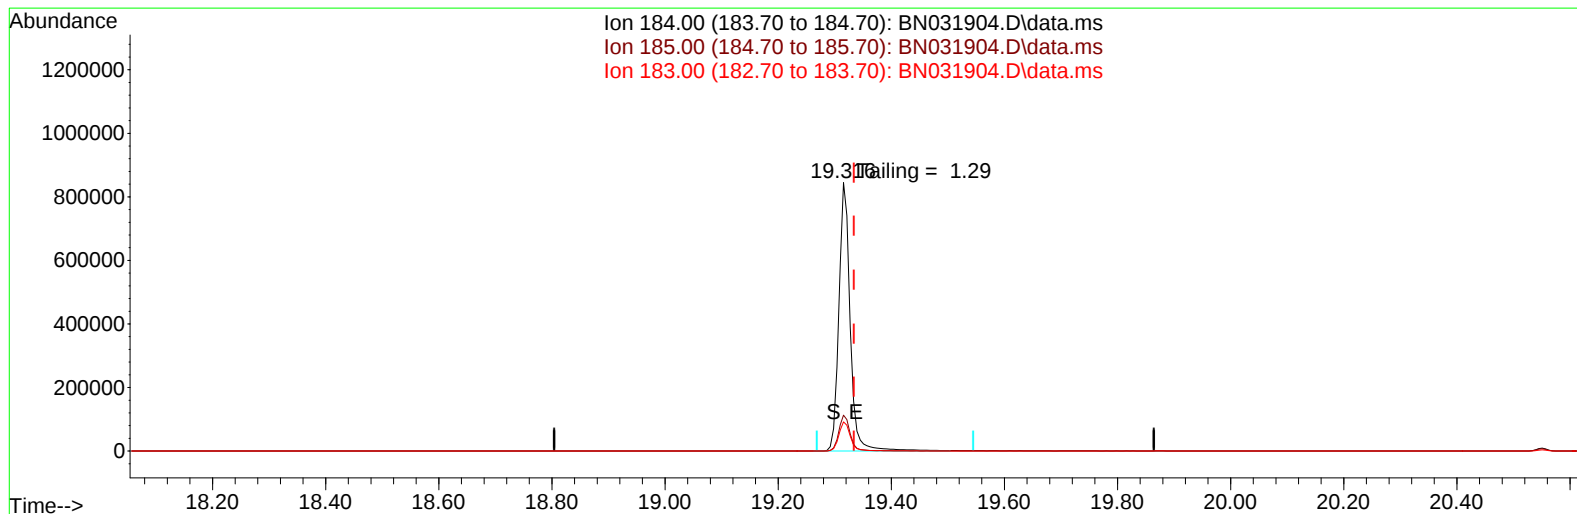

TIC: BN031904.D\data.ms

(77) Benzidine

19.316min (-0.018) 0.00 ng

response 1177088

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.39
183.00	13.20	10.88
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/11/2024	BNA_N	<u>BN031904.D</u>
Compound Name	Response	Retention Time
DDT	2688079	20.551
DDD	30854	20.157
DDE	2169	19.598
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
33023	2721102	1.21

Instrument :
BNA_N
ClientSampleId :
DFTPP